

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060920\
 Data File : PS010744.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2020 00:37
 Operator : DD\AJ
 Sample : PB129418BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 03:20:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.921	568.4E6	410.6E6	718.712	752.739
Target Compounds							
1) T	Dalapon	2.995	2.585	31109700	110.8E6	31.641	151.294 #
2) T	3,5-DICHL...	0.000	6.101	0	50544346	N.D.	61.666
3) T	4-Nitroph...	7.005	0.000	7227429	0	19.495	N.D. #
7) T	MCPA	7.778	7.385	56077480	44092497	16.041	16.224
8) T	DICHLORPROP	0.000	7.740	0	7865635	N.D.	13.641
10) T	Pentachlo...	8.711	0.000	10125181	0	<MDL	N.D. #
12) T	2,4,5-T	9.431	0.000	34727919	0	8.539	N.D. #
14) T	DINOSEB	11.171	10.029	17018134	12938923	5.267	6.014
15) T	Picloram	10.996	0.000	23984772	0	4.698	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060920\
Data File : PS010744.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2020 00:37
Operator : DD\AJ
Sample : PB129418BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 03:20:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

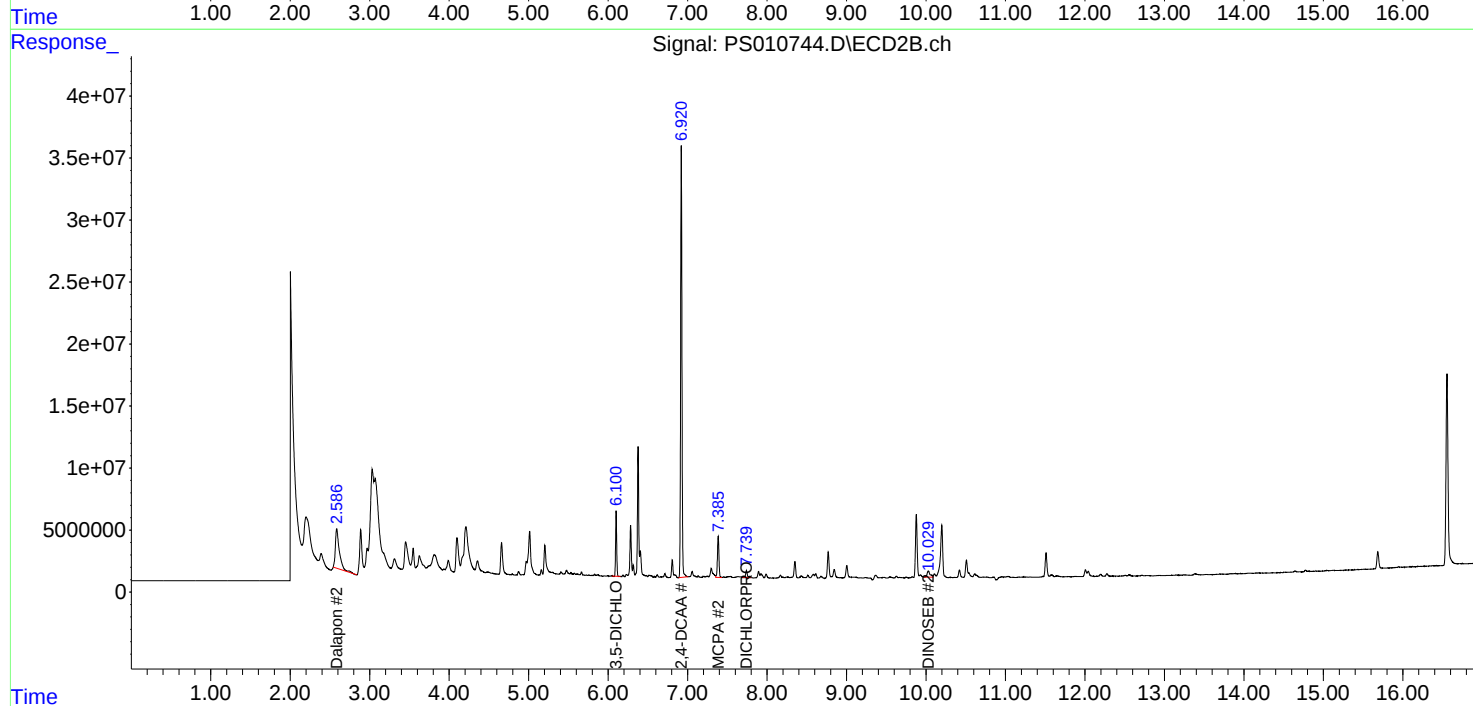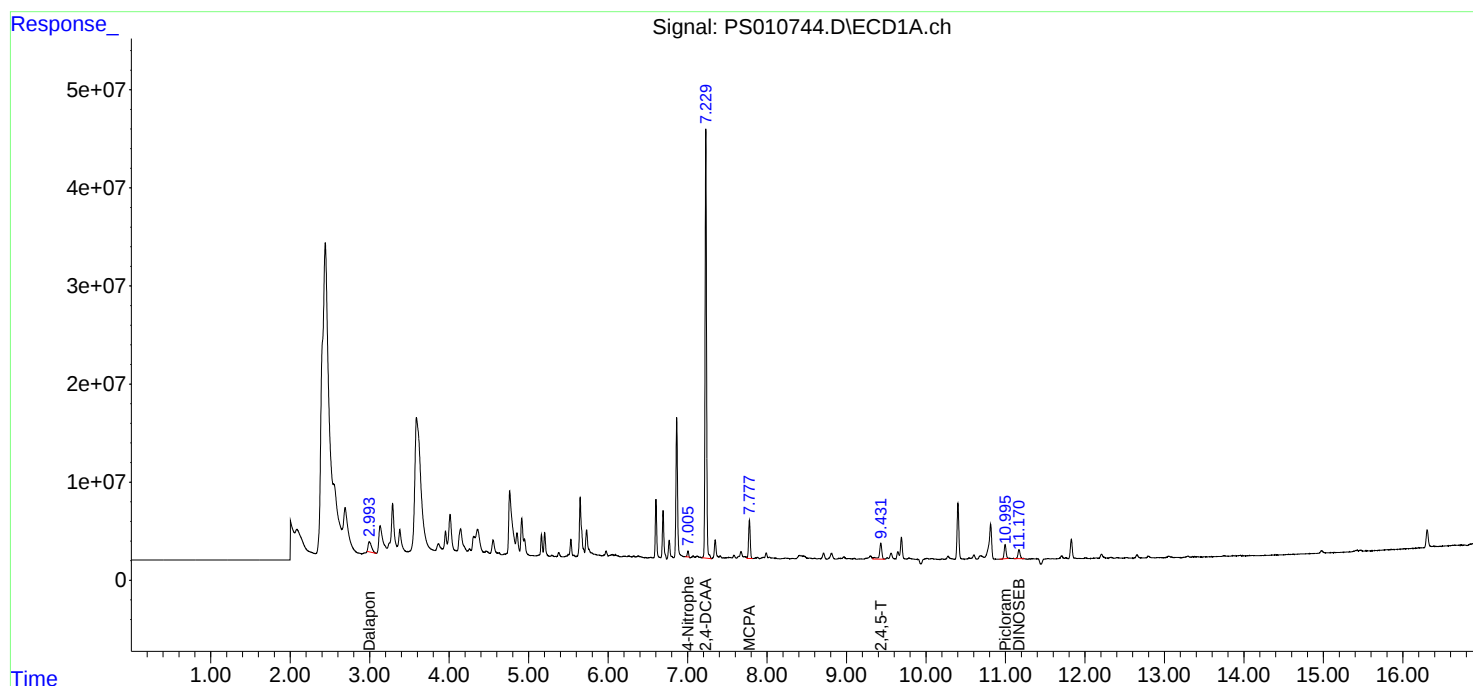


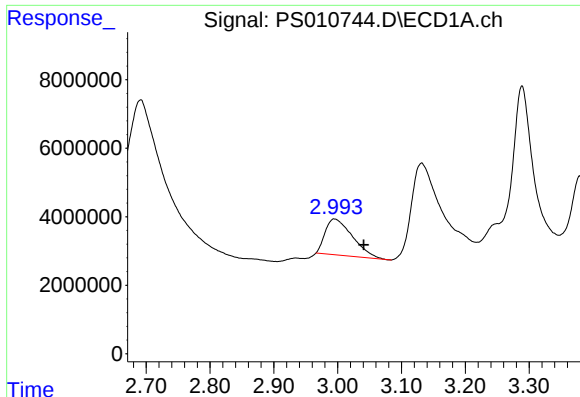

#1 Dalapon


R.T.: 2.995 min
Delta R.T.: -0.046 min
Response: 31109700
Conc: 31.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

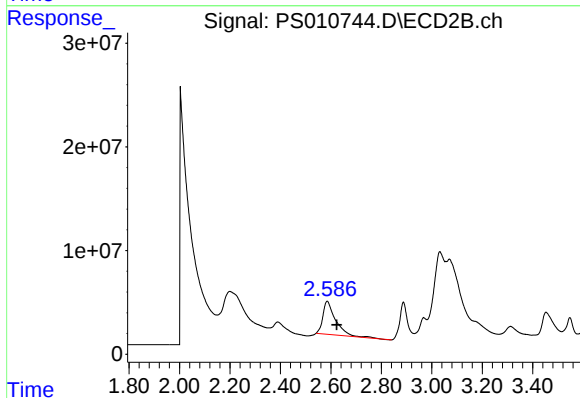


#1 Dalapon

R.T.: 2.585 min
Delta R.T.: -0.038 min
Response: 110769283
Conc: 151.29 ng/ml

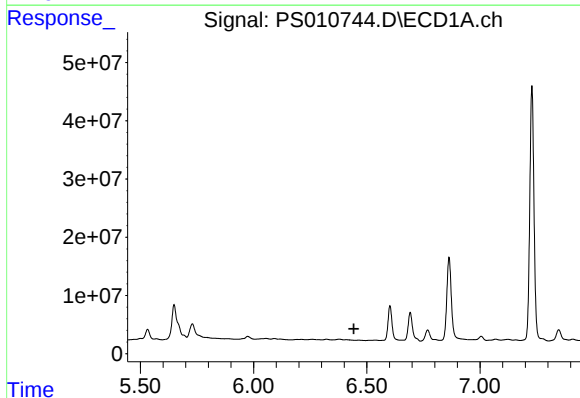


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

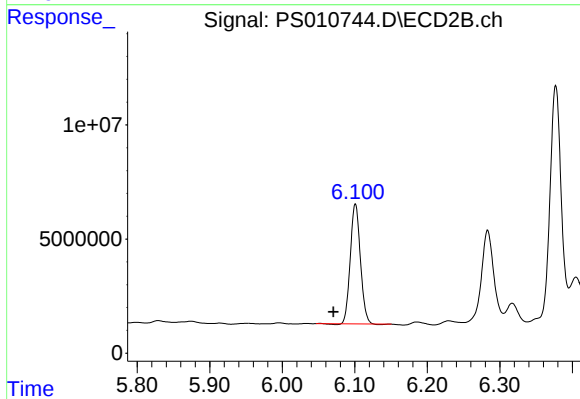

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.101 min
Delta R.T.: 0.031 min
Response: 50544346
Conc: 61.67 ng/ml

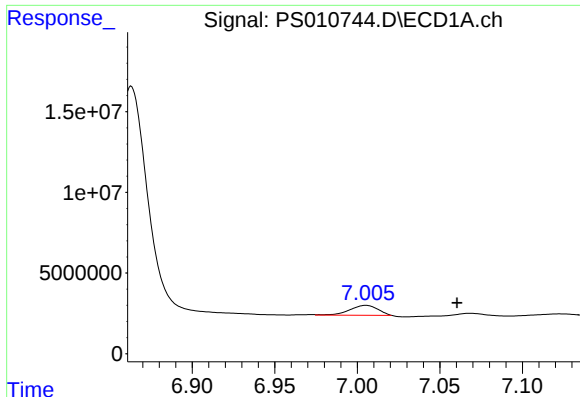

#3 4-Nitrophenol


R.T.: 7.005 min
Delta R.T.: -0.055 min
Response: 7227429
Conc: 19.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

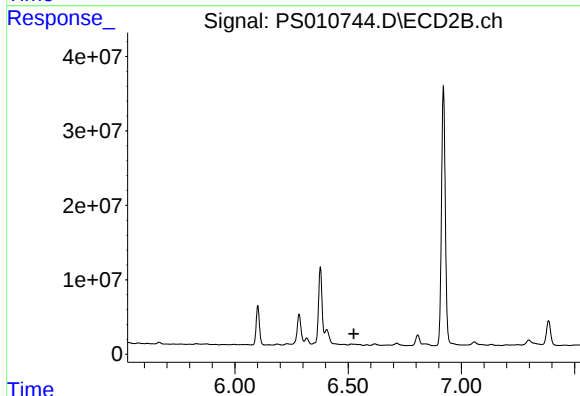


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.525 min
Response: 0
Conc: N.D.

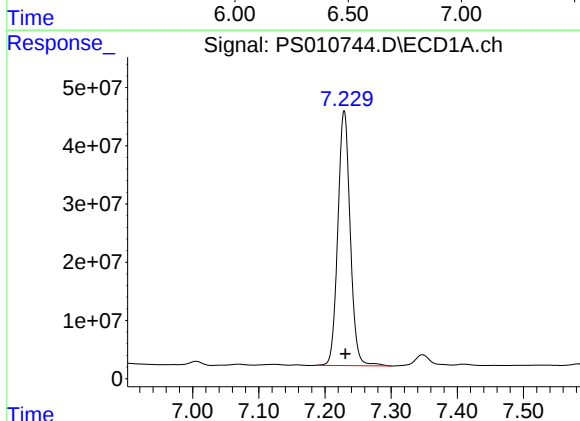


#4 2,4-DCAA

R.T.: 7.229 min
Delta R.T.: -0.002 min
Response: 568401598
Conc: 718.71 ng/ml

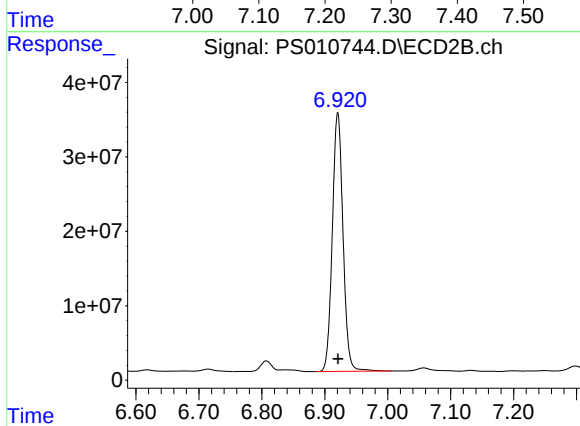

#4 2,4-DCAA


R.T.: 6.921 min
Delta R.T.: 0.000 min
Response: 410555701
Conc: 752.74 ng/ml

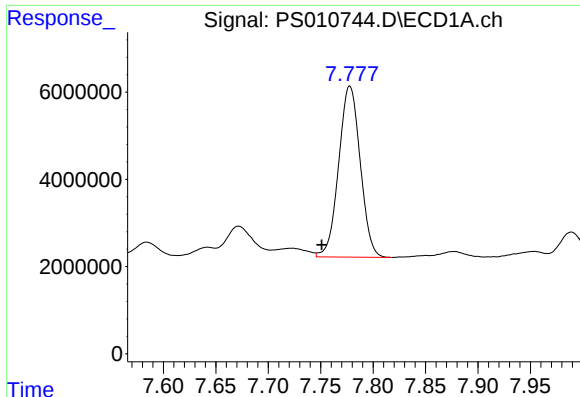

#7 MCPA


R.T.: 7.778 min
Delta R.T.: 0.027 min
Response: 56077480
Conc: 16.04 ug/ml

Instrument :
ECD_S
ClientSampleId :

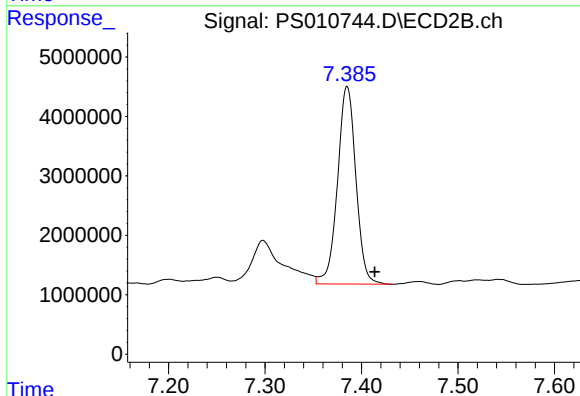


#7 MCPA

R.T.: 7.385 min
Delta R.T.: -0.029 min
Response: 44092497
Conc: 16.22 ug/ml

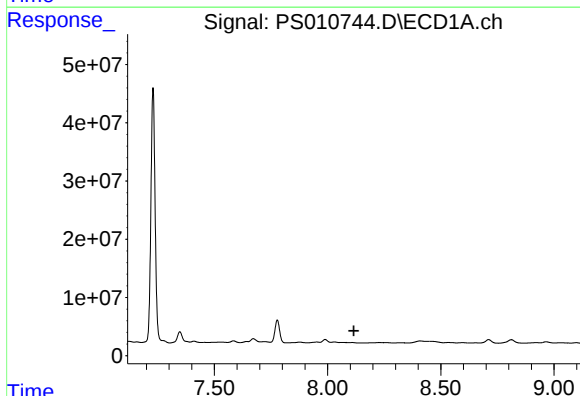


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.116 min
Response: 0
Conc: N.D.

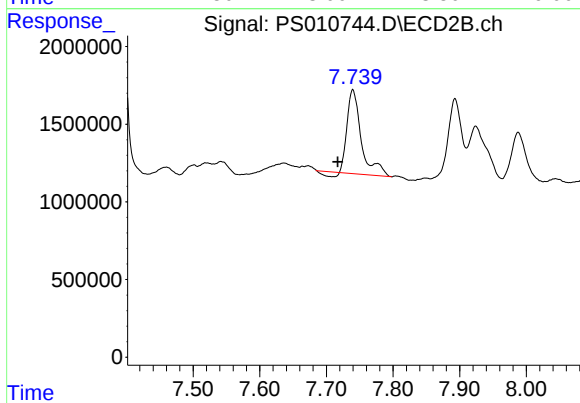

#8 DICHLORPROP


R.T.: 7.740 min
Delta R.T.: 0.023 min
Response: 7865635
Conc: 13.64 ng/ml

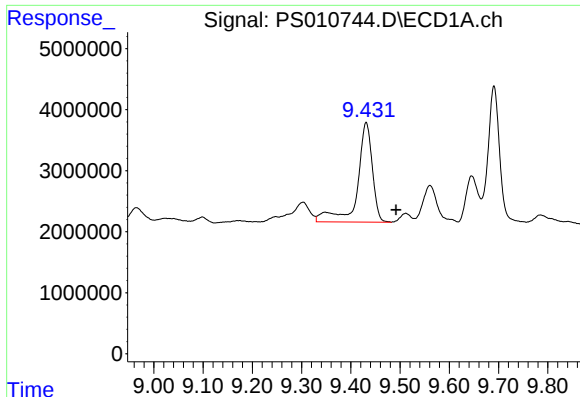

#12 2,4,5-T


R.T.: 9.431 min
Delta R.T.: -0.061 min
Response: 34727919
Conc: 8.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

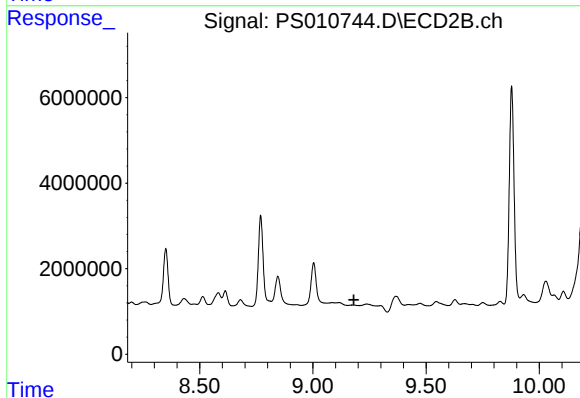


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.181 min
Response: 0
Conc: N.D.

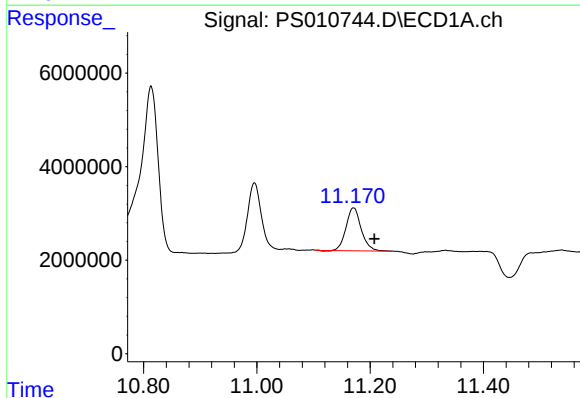


#14 DINOSEB

R.T.: 11.171 min
Delta R.T.: -0.037 min
Response: 17018134
Conc: 5.27 ng/ml

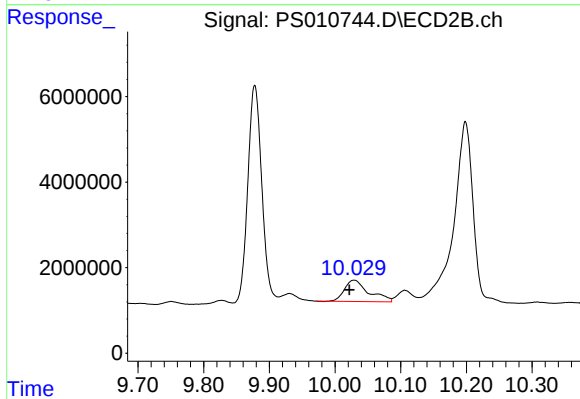

#14 DINOSEB


R.T.: 10.029 min
Delta R.T.: 0.007 min
Response: 12938923
Conc: 6.01 ng/ml

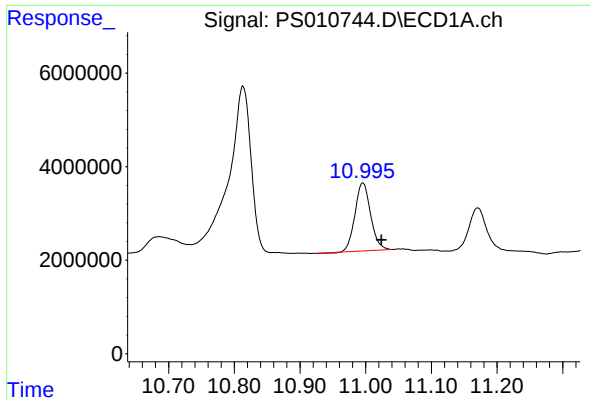

#15 Picloram

R.T.: 10.996 min
Delta R.T.: -0.028 min
Response: 23984772
Conc: 4.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

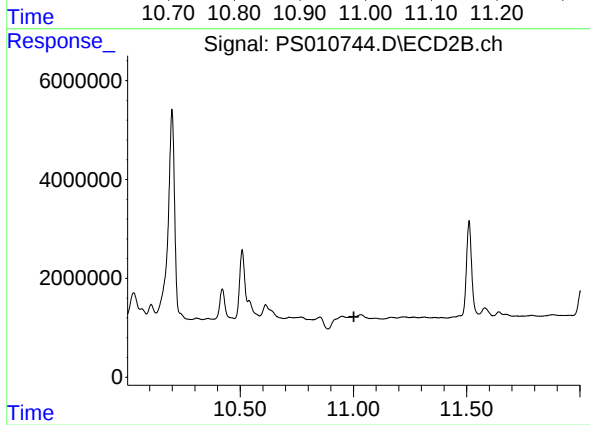

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.