

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060920\
 Data File : PS010732.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2020 20:01
 Operator : DD\AJ
 Sample : L2886-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 GEN

Manual Integrations
 APPROVED

Sohil
 6/10/2020 2:24:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 03:48:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.920	305.6E6	204.4E6	386.371m	374.732m
Target Compounds							
5) T	DICAMBA	7.420	7.089	138.2E6	129.4E6	43.961	57.476 #
9) T	2,4-D	8.343	8.010	1778.9E6	1374.3E6	2256.665	1812.510
15) T	Picloram	11.021	11.001	411.1E6	321.0E6	80.519m	77.789m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060920\
Data File : PS010732.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2020 20:01
Operator : DD\AJ
Sample : L2886-03
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
GEN


Manual Integrations
APPROVED

Sohil
6/10/2020 2:24:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 03:48:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

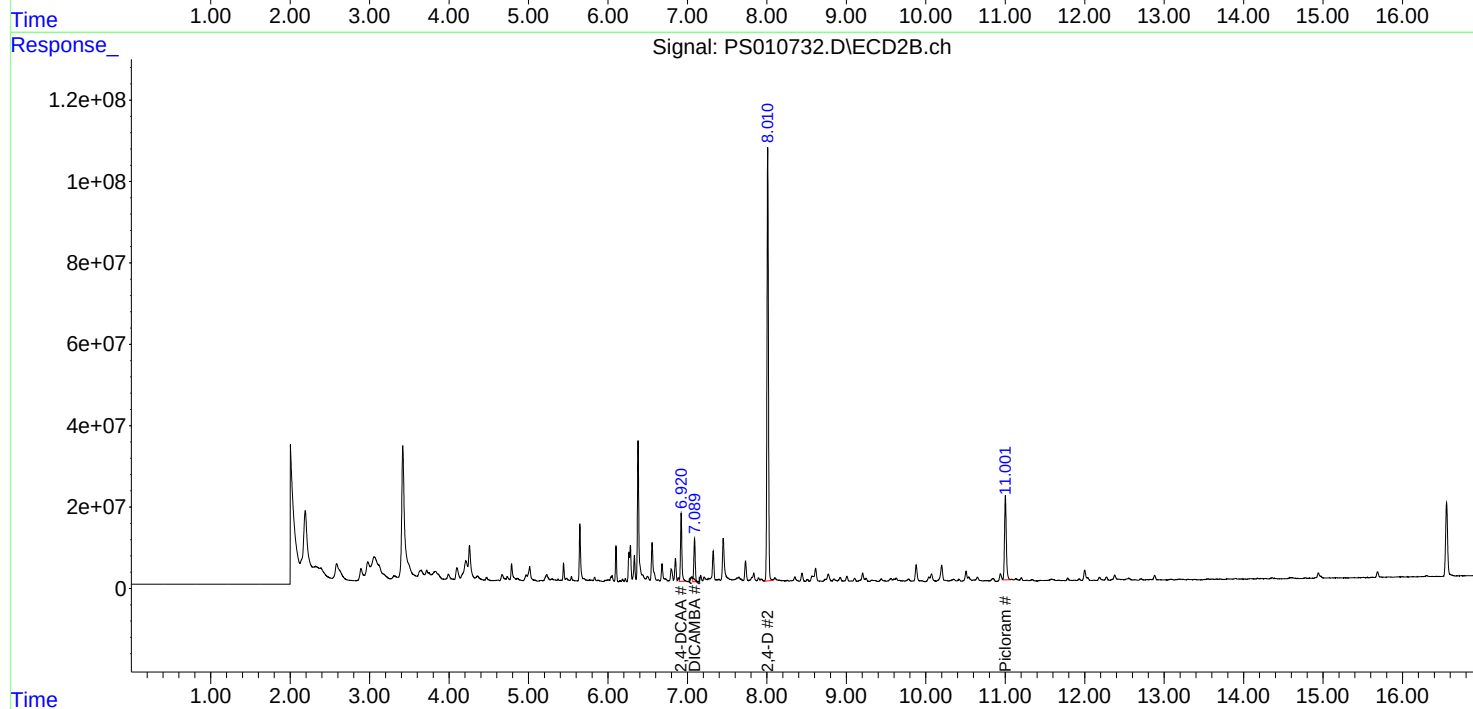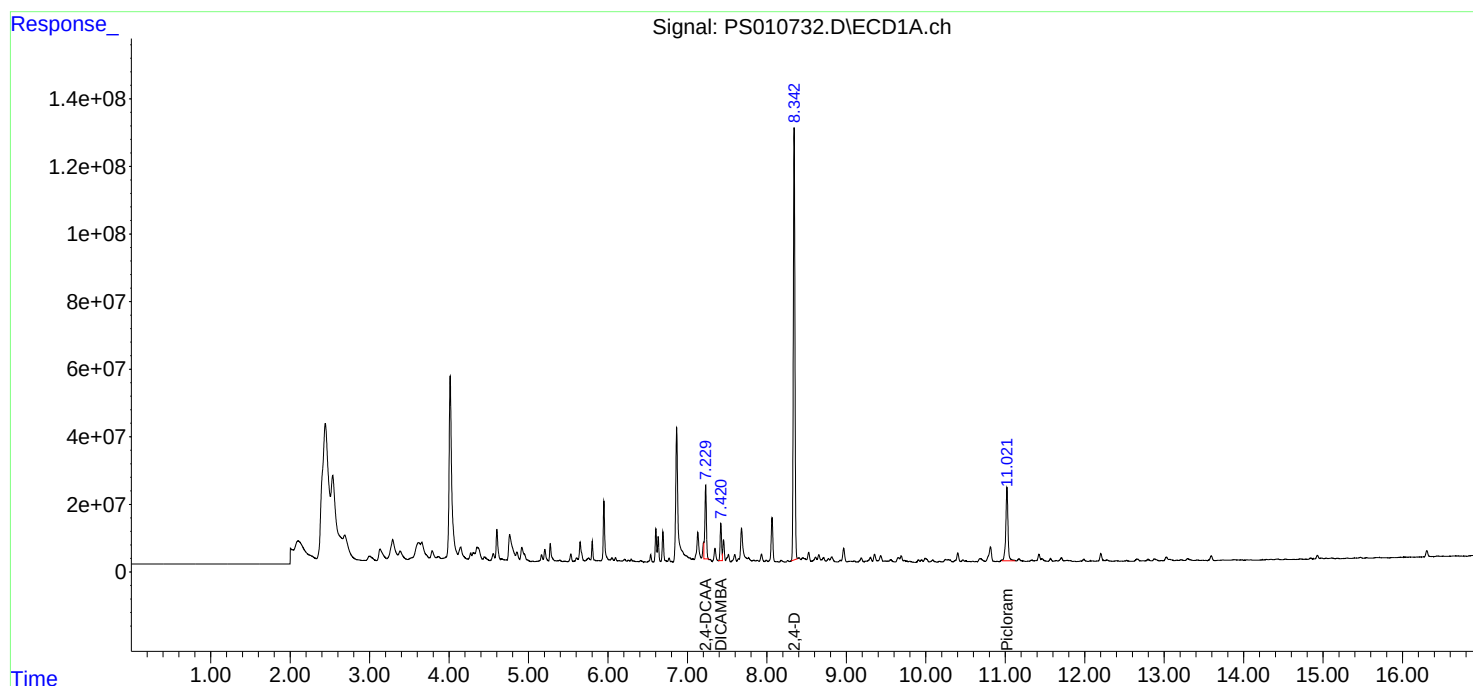

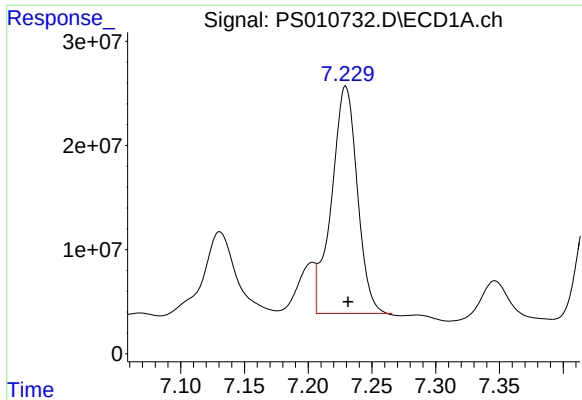


#4 2,4-DCAA

R.T.: 7.229 min
Delta R.T.: -0.002 min
Response: 305566207
Conc: 386.37 ng/ml m

Instrument :
ECD_S
ClientSampleId :
GEN


Manual Integrations
APPROVED

Sohil
6/10/2020 2:24:42 PM

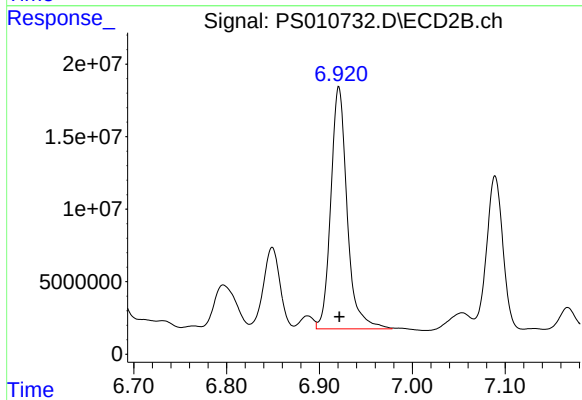


#4 2,4-DCAA

R.T.: 6.920 min
Delta R.T.: -0.001 min
Response: 204384723
Conc: 374.73 ng/ml m

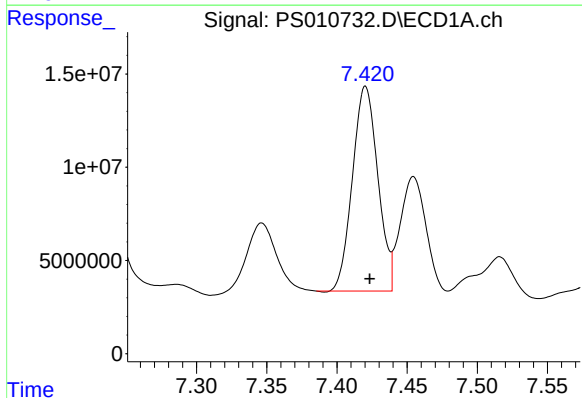


#5 DICAMBA

R.T.: 7.420 min
Delta R.T.: -0.003 min
Response: 138235253
Conc: 43.96 ng/ml

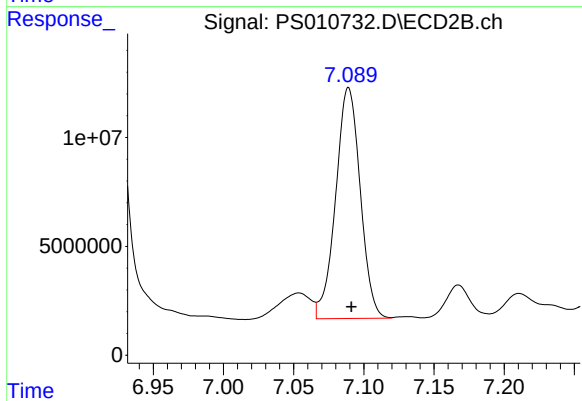

#5 DICAMBA

R.T.: 7.089 min
Delta R.T.: -0.002 min
Response: 129368513
Conc: 57.48 ng/ml

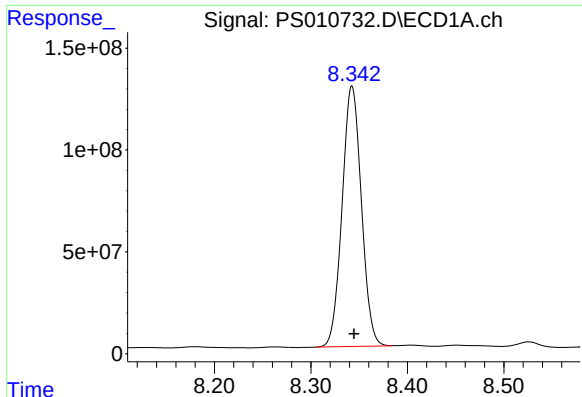


#9 2,4-D

R.T.: 8.343 min
Delta R.T.: -0.002 min
Response: 1778872564
Conc: 2256.66 ng/ml

Instrument :
ECD_S
ClientSampleId :
GEN


Manual Integrations
APPROVED

Sohil
6/10/2020 2:24:42 PM

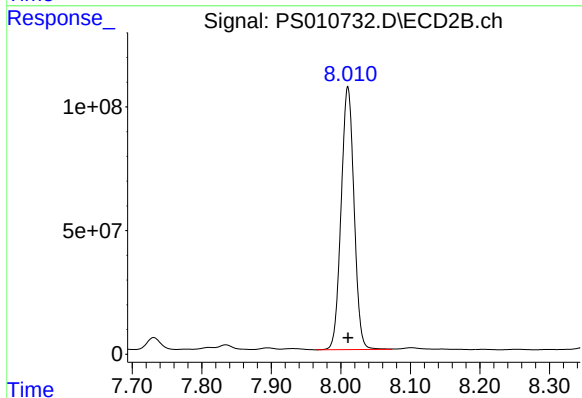


#9 2,4-D

R.T.: 8.010 min
Delta R.T.: 0.000 min
Response: 1374345760
Conc: 1812.51 ng/ml

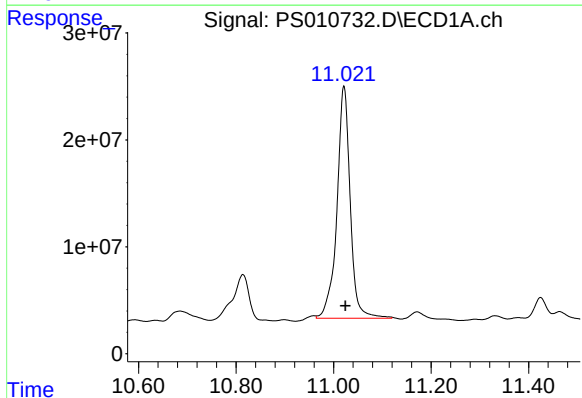

#15 Picloram

R.T.: 11.021 min
Delta R.T.: -0.003 min
Response: 411058596
Conc: 80.52 ng/ml m

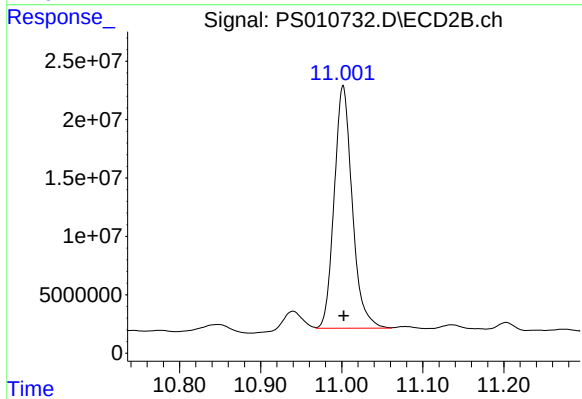

#15 Picloram

R.T.: 11.001 min
Delta R.T.: 0.000 min
Response: 320955283
Conc: 77.79 ng/ml m