

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060921\
 Data File : PS015304.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2021 08:03
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 14:46:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.227	0.000	2675568	0	1.062	N.D.	#
Target Compounds								
5) T	DICAMBA	7.421	0.000	9258639	0	<MDL	N.D.	#
6) T	MCPD	7.617	0.000	6907593	0	<MDL	N.D.	#
7) T	MCPA	7.762	0.000	2150779	0	<MDL	N.D.	#
8) T	DICHLORPROP	8.115	0.000	2877323	0	1.249	N.D.	#
9) T	2,4-D	8.345	0.000	5609563	0	2.201	N.D.	#
10) T	Pentachlo...	8.656	8.289	17640056	4226009	<MDL	<MDL	#
11) T	2,4,5-TP ...	9.209	8.651	13321608	3241561	1.073	1.117	
12) T	2,4,5-T	9.491	9.029	27059253	6157700	2.253	2.127	
13) T	2,4-DB	10.031	0.000	16735871	0	6.572	N.D.	#
14) T	DINOSEB	11.205	9.865	15627594	3394992	1.956	1.859	
15) T	Picloram	11.020	10.843	496.6E6	125.4E6	29.976	30.187	
16) T	DCPA	11.473	10.798	28352063	6263971	1.681	1.453	



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060921\
Data File : PS015304.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2021 08:03
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 14:46:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

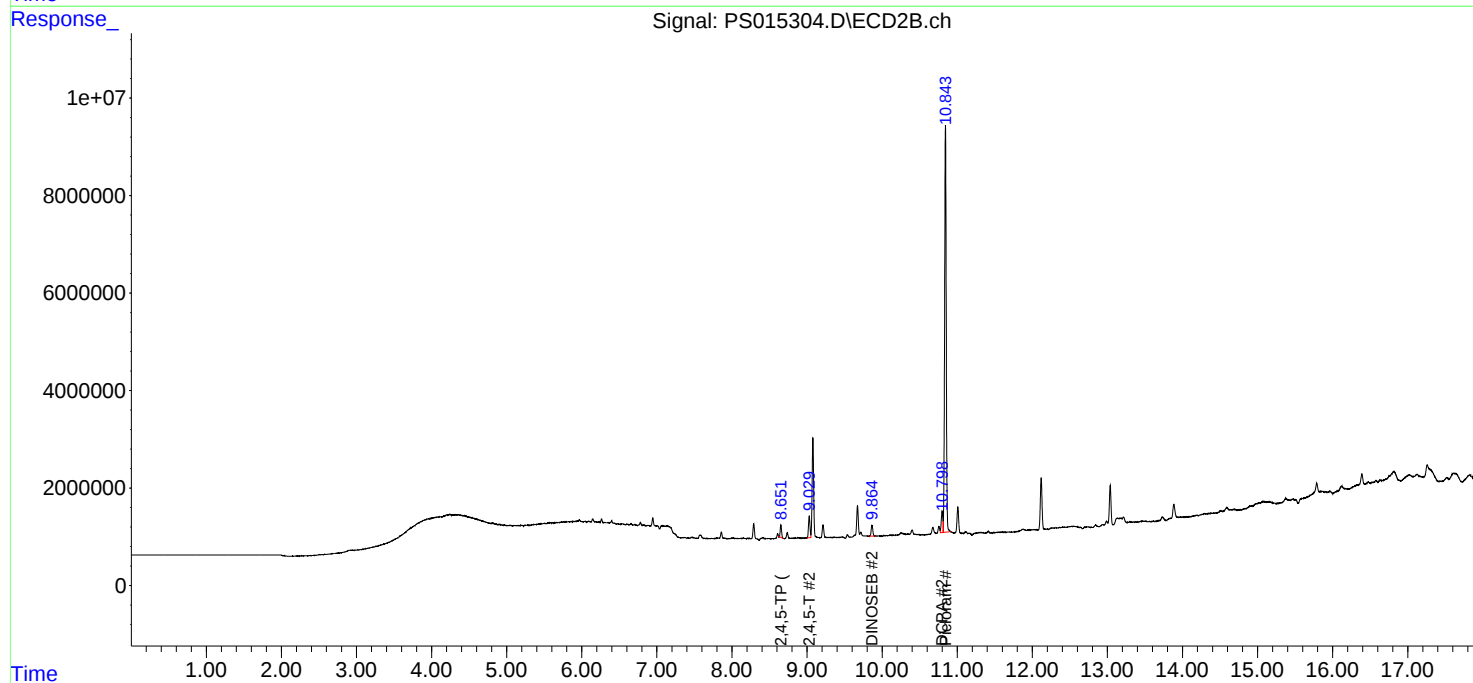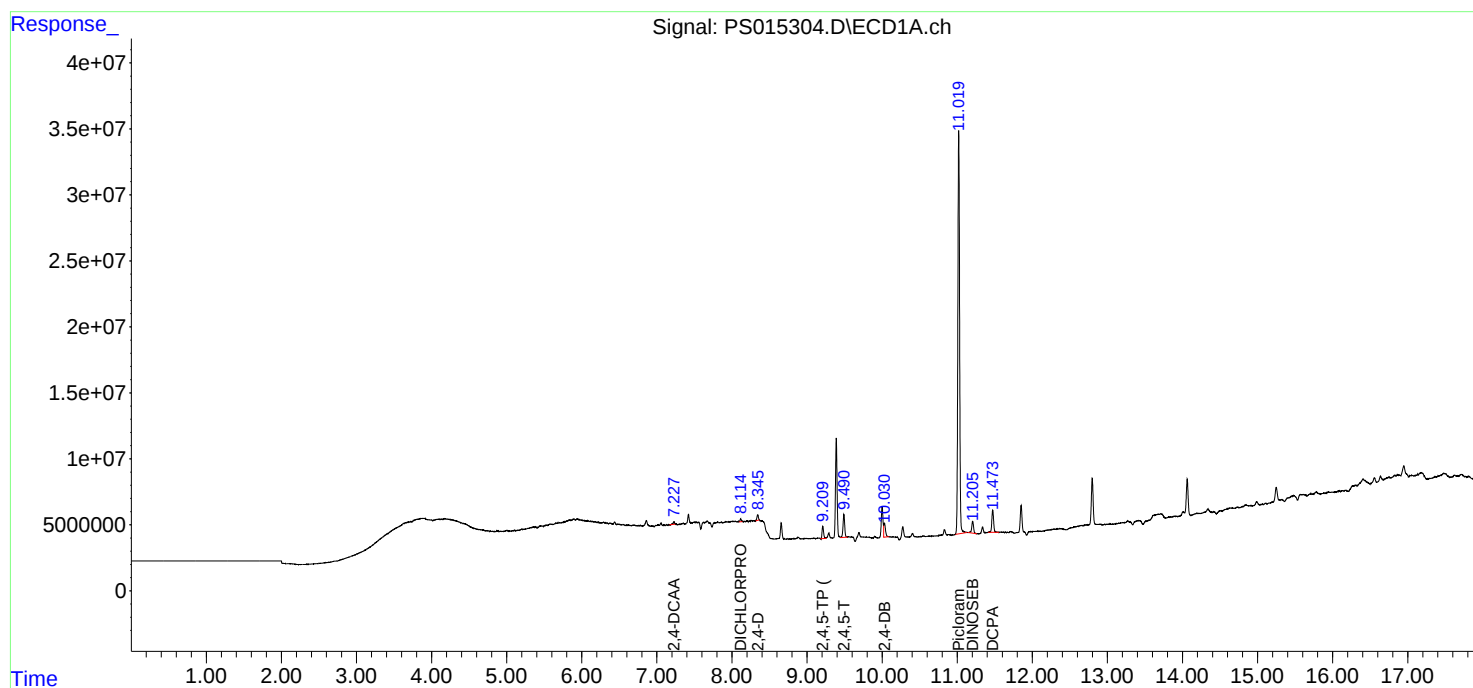


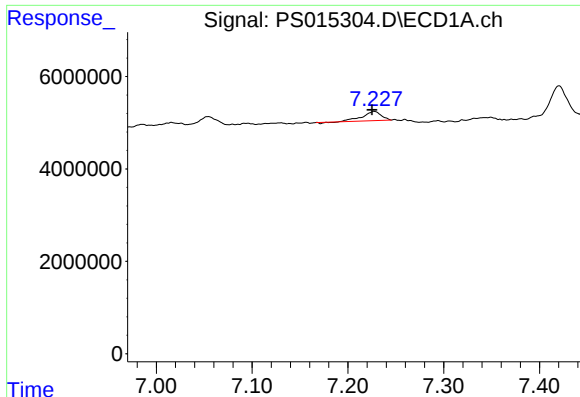

#4 2,4-DCAA


R.T.: 7.227 min
Delta R.T.: 0.002 min
Response: 2675568
Conc: 1.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

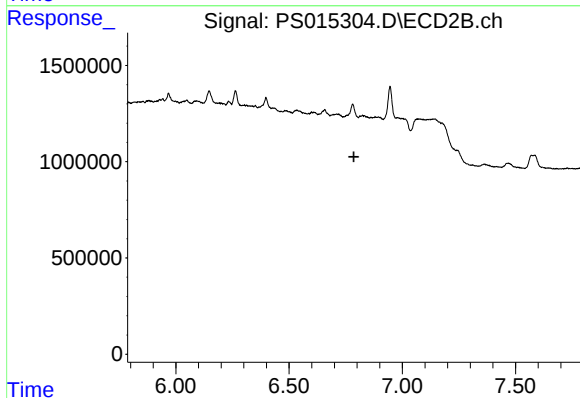


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.786 min
Response: 0
Conc: N.D.

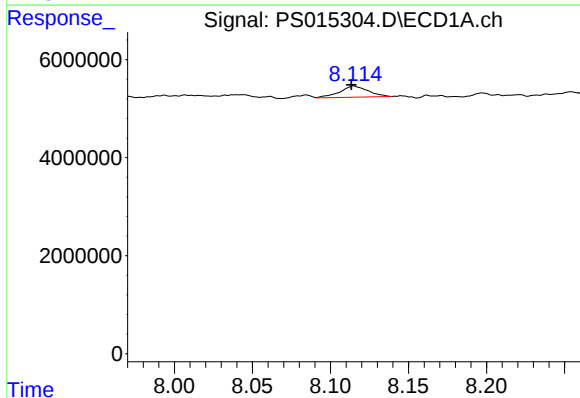


#8 DICHLORPROP

R.T.: 8.115 min
Delta R.T.: 0.001 min
Response: 2877323
Conc: 1.25 ng/ml

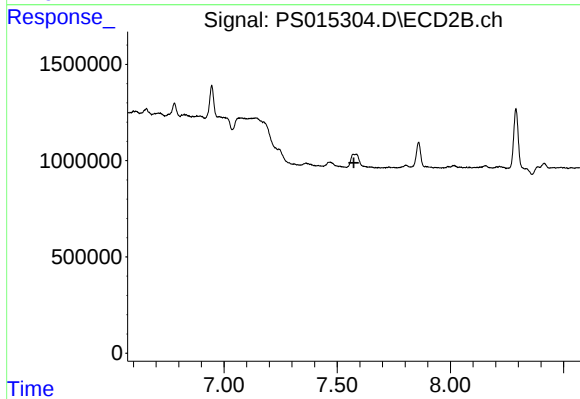

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 7.574 min
Response: 0
Conc: N.D.

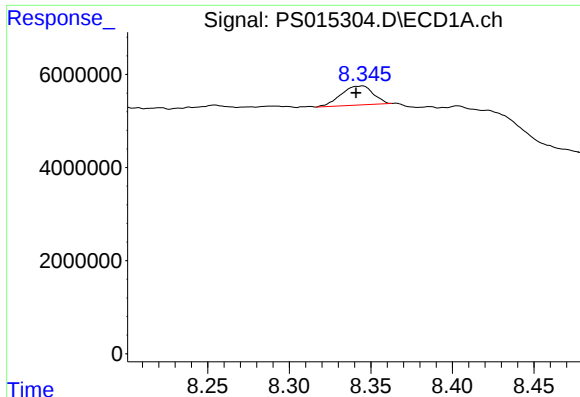

#9 2,4-D


R.T.: 8.345 min
Delta R.T.: 0.004 min
Response: 5609563
Conc: 2.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

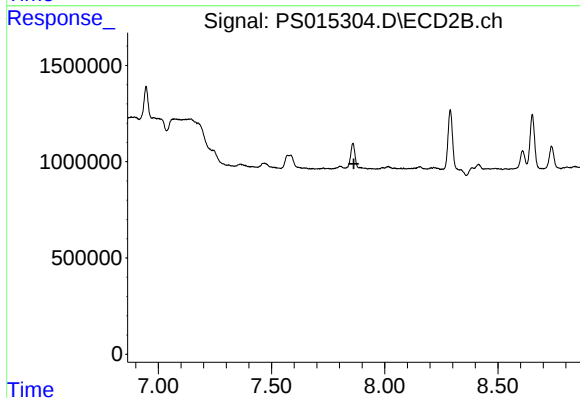


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.864 min
Response: 0
Conc: N.D.

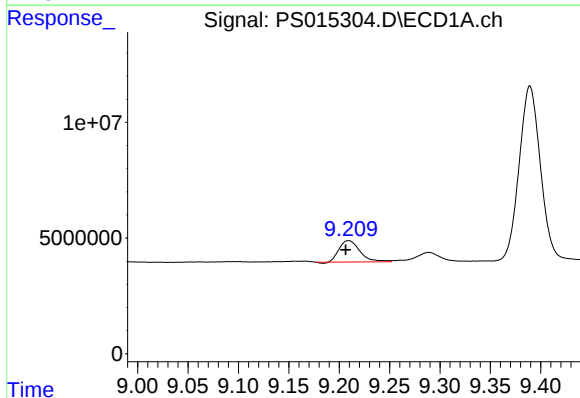


#11 2,4,5-TP (SILVEX)

R.T.: 9.209 min
Delta R.T.: 0.003 min
Response: 13321608
Conc: 1.07 ng/ml

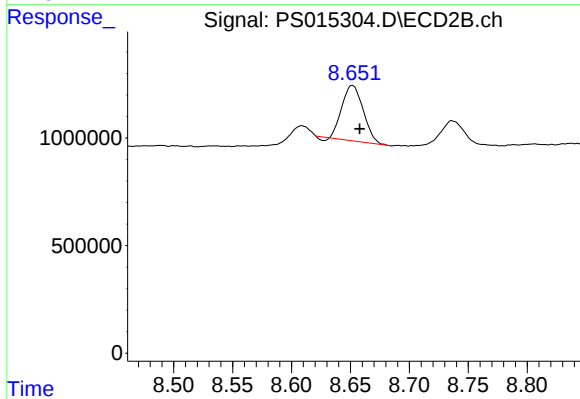

#11 2,4,5-TP (SILVEX)


R.T.: 8.651 min
Delta R.T.: -0.007 min
Response: 3241561
Conc: 1.12 ng/ml

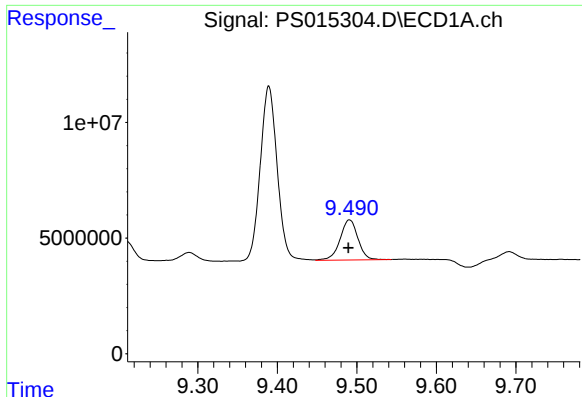

#12 2,4,5-T


R.T.: 9.491 min
Delta R.T.: 0.001 min
Response: 27059253
Conc: 2.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

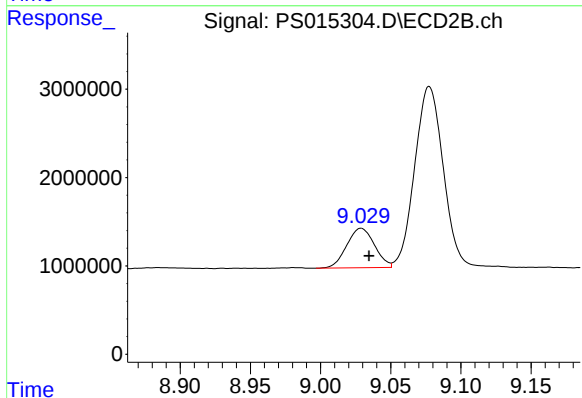


#12 2,4,5-T

R.T.: 9.029 min
Delta R.T.: -0.006 min
Response: 6157700
Conc: 2.13 ng/ml

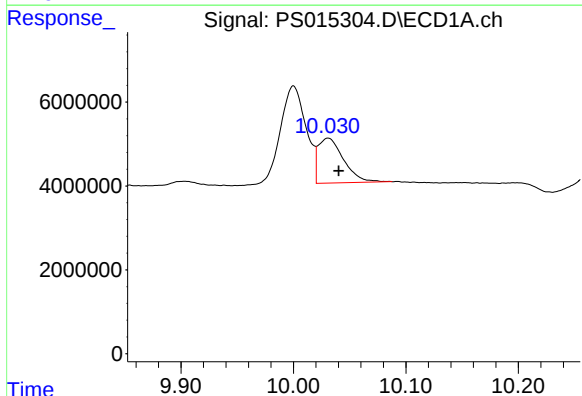


#13 2,4-DB

R.T.: 10.031 min
Delta R.T.: -0.009 min
Response: 16735871
Conc: 6.57 ng/ml

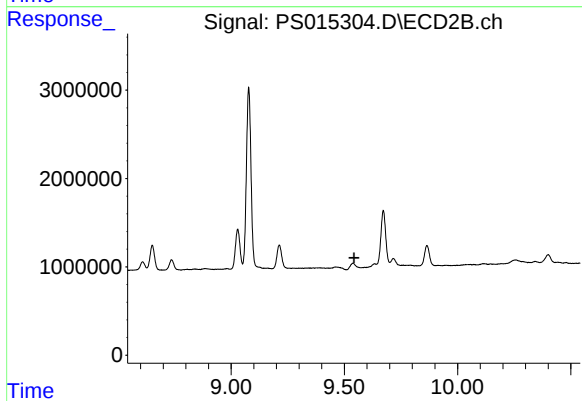

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.542 min
Response: 0
Conc: N.D.

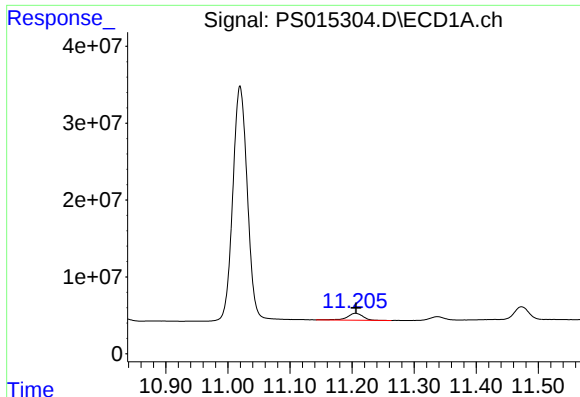

#14 DINOSEB


R.T.: 11.205 min
Delta R.T.: -0.001 min
Response: 15627594
Conc: 1.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

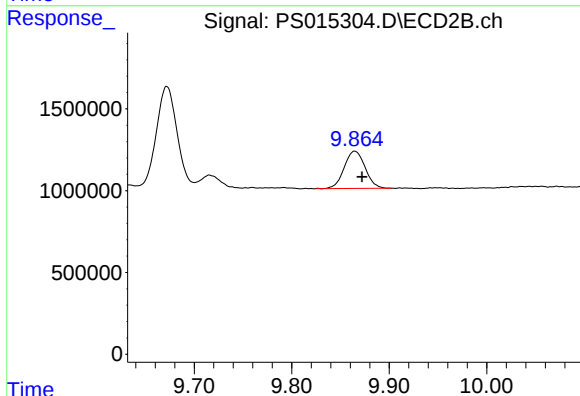


#14 DINOSEB

R.T.: 9.865 min
Delta R.T.: -0.008 min
Response: 3394992
Conc: 1.86 ng/ml

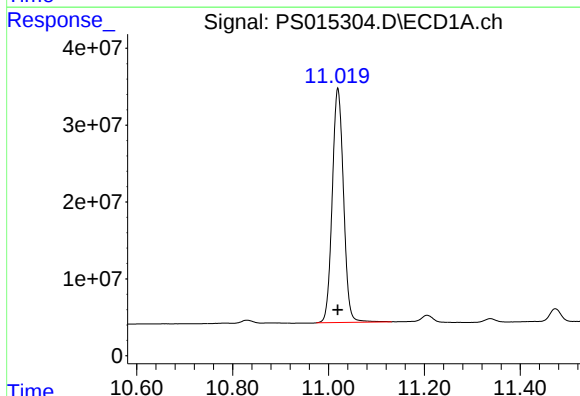


#15 Picloram

R.T.: 11.020 min
Delta R.T.: 0.000 min
Response: 496611399
Conc: 29.98 ng/ml

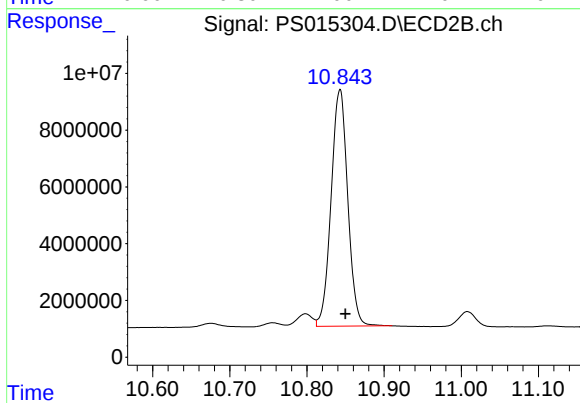

#15 Picloram


R.T.: 10.843 min
Delta R.T.: -0.007 min
Response: 125364788
Conc: 30.19 ng/ml

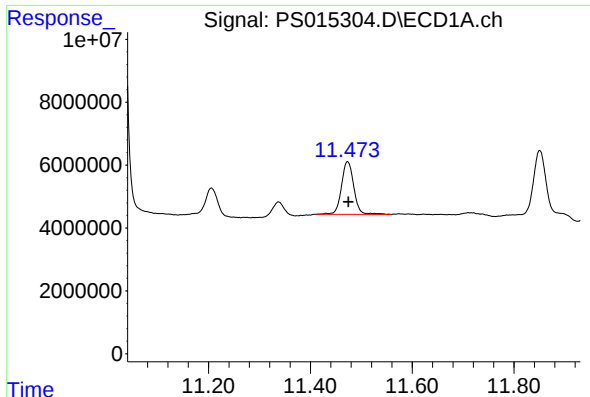

#16 DCPA

R.T.: 11.473 min
Delta R.T.: -0.002 min
Response: 28352063
Conc: 1.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

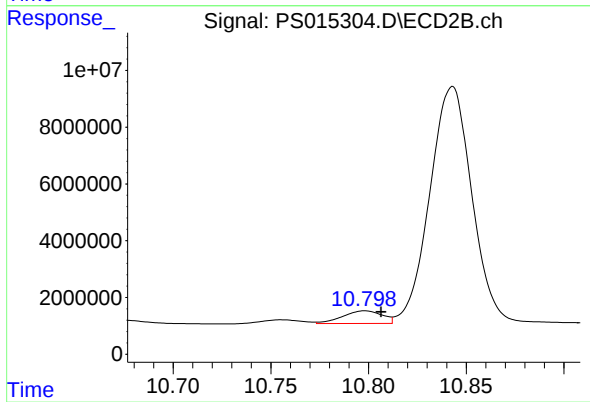

#16 DCPA

R.T.: 10.798 min
Delta R.T.: -0.008 min
Response: 6263971
Conc: 1.45 ng/ml