

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060921\
 Data File : PS015305.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2021 08:27
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 14:47:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.225	6.782	1105.7E6	280.4E6	438.723	523.425
Target Compounds							
3) T	4-Nitroph...	7.025	0.000	4858190	0	3.446	N.D. #
7) T	MCPA	7.670f	0.000	15639130	0	1.558	N.D. #
9) T	2,4-D	8.341	0.000	5899519	0	2.315	N.D. #
11) T	2,4,5-TP ...	9.204	0.000	3282293	0	<MDL	N.D. #
12) T	2,4,5-T	9.487	9.030	15506743	3373880	1.291	1.165
13) T	2,4-DB	10.029	0.000	11530281	0	4.528	N.D. #
14) T	DINOSEB	11.201	0.000	6909546	0	<MDL	N.D. #
15) T	Picloram	11.016	10.843	366.0E6	91313483	22.090	21.988
16) T	DCPA	11.469	10.843	6435673	91313483	<MDL	21.182 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060921\
Data File : PS015305.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2021 08:27
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 14:47:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

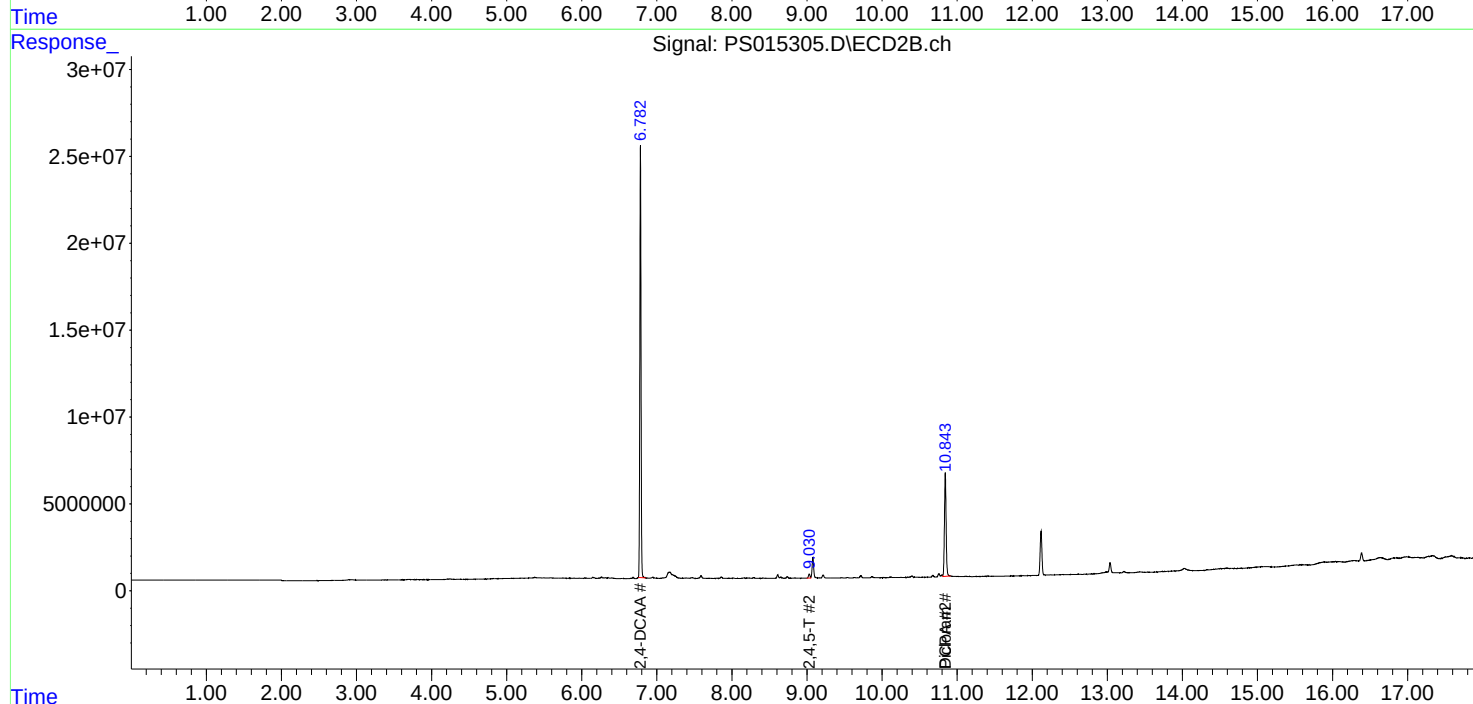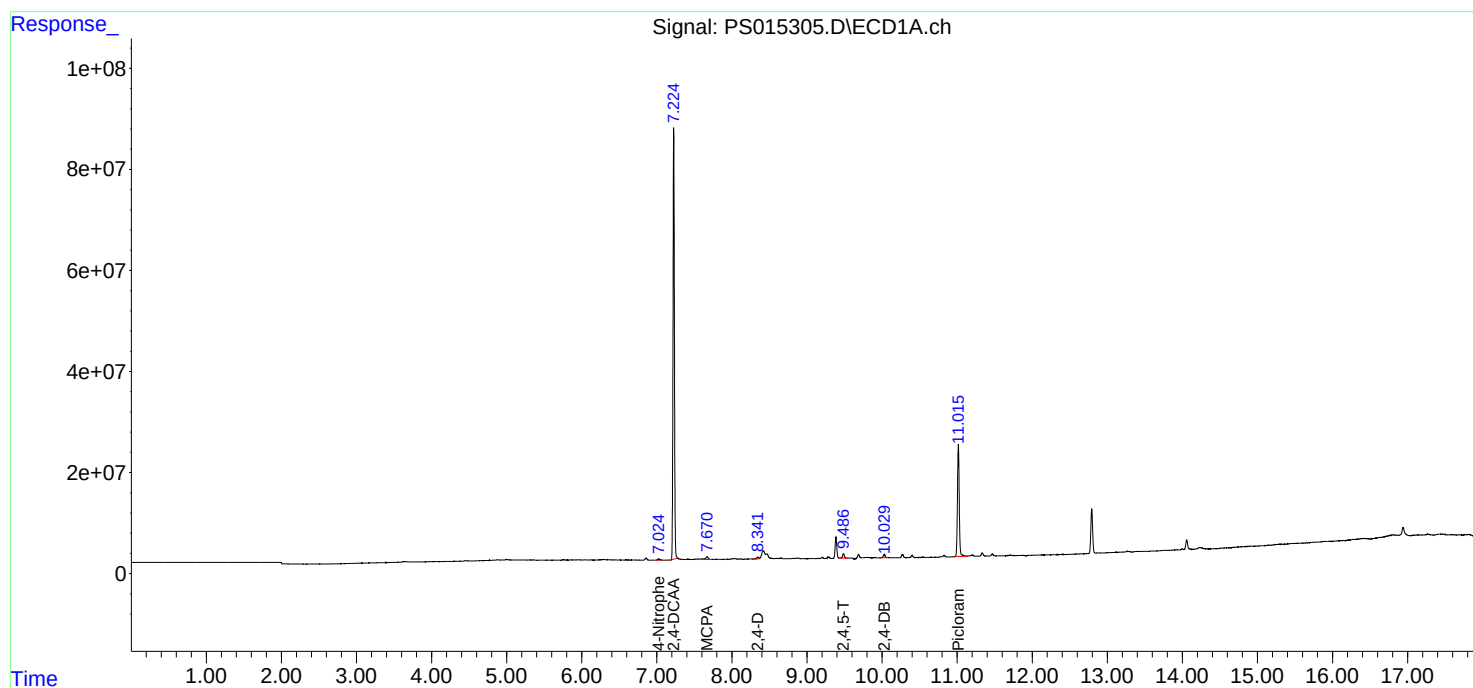


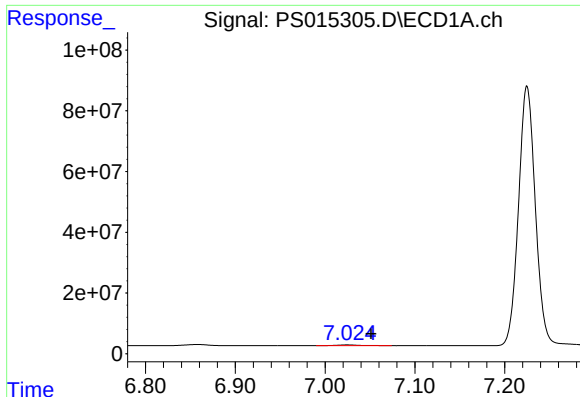

#3 4-Nitrophenol


R.T.: 7.025 min
Delta R.T.: -0.026 min
Response: 4858190
Conc: 3.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

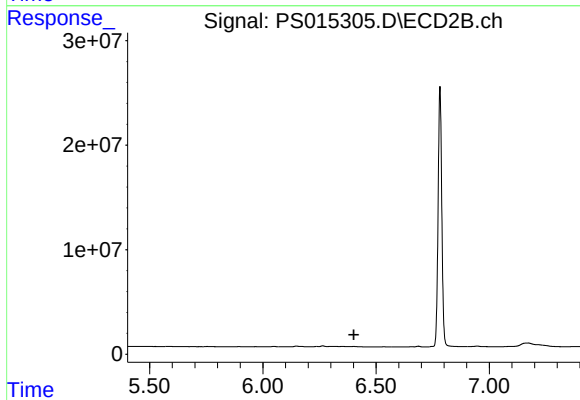


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

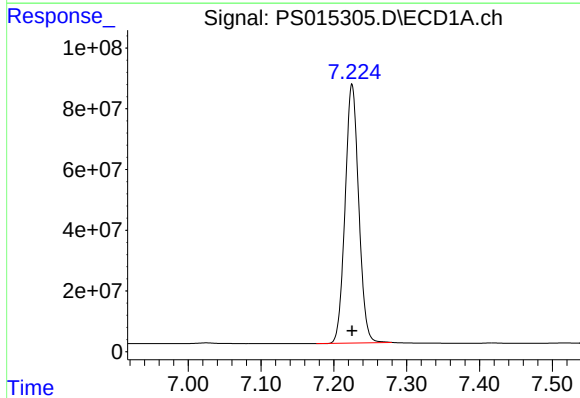


#4 2,4-DCAA

R.T.: 7.225 min
Delta R.T.: 0.000 min
Response: 1105745267
Conc: 438.72 ng/ml

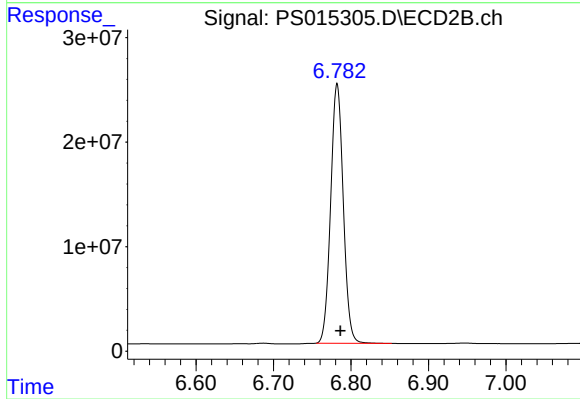

#4 2,4-DCAA


R.T.: 6.782 min
Delta R.T.: -0.004 min
Response: 280436100
Conc: 523.43 ng/ml

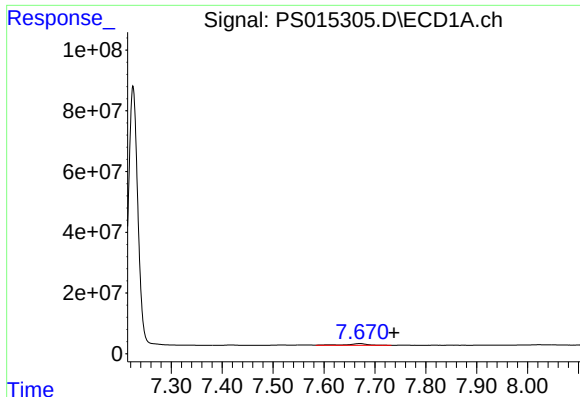

#7 MCPA


R.T.: 7.670 min
Delta R.T.: -0.068 min
Response: 15639130
Conc: 1.56 ug/ml

Instrument :
ECD_S
ClientSampleId :

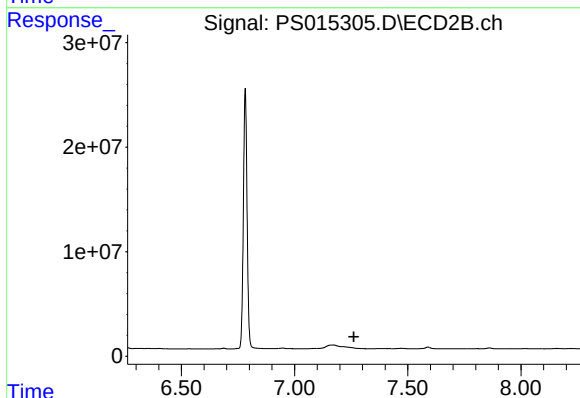


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.262 min
Response: 0
Conc: N.D.

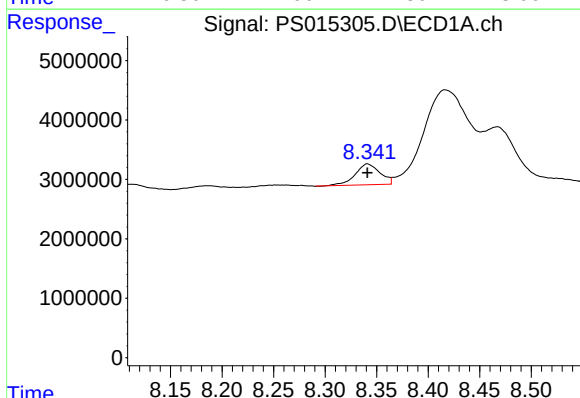


#9 2,4-D

R.T.: 8.341 min
Delta R.T.: 0.000 min
Response: 5899519
Conc: 2.32 ng/ml

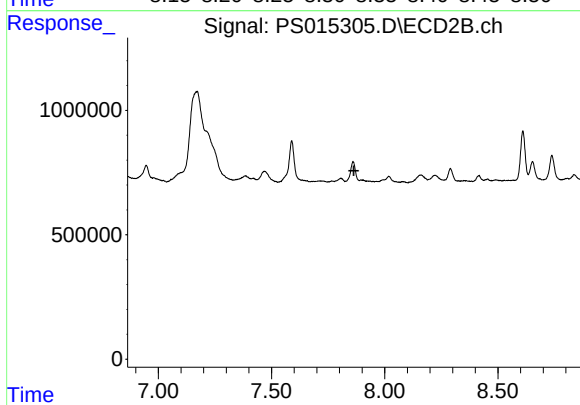

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.864 min
Response: 0
Conc: N.D.

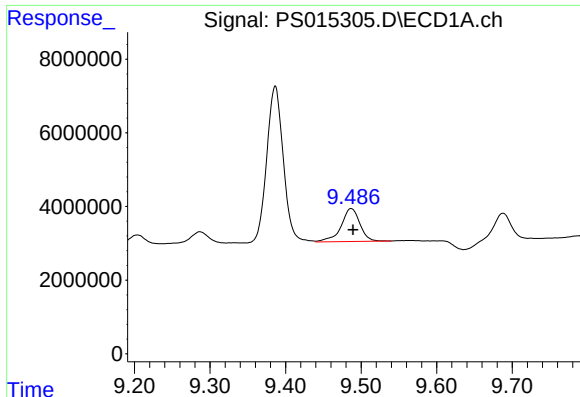

#12 2,4,5-T


R.T.: 9.487 min
Delta R.T.: -0.003 min
Response: 15506743
Conc: 1.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

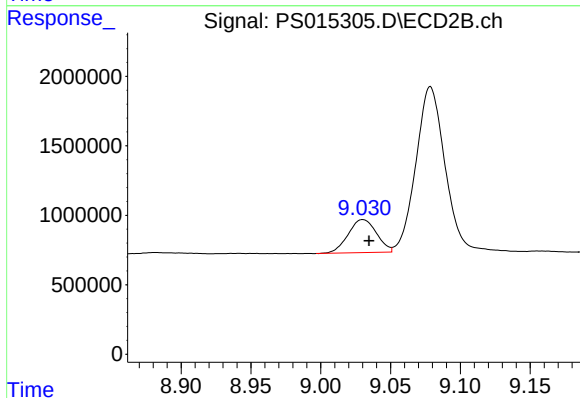


#12 2,4,5-T

R.T.: 9.030 min
Delta R.T.: -0.005 min
Response: 3373880
Conc: 1.17 ng/ml

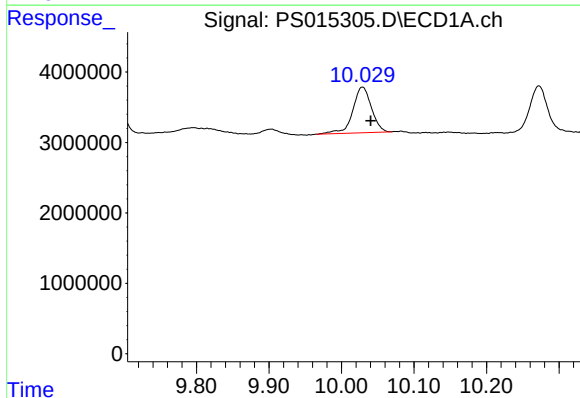


#13 2,4-DB

R.T.: 10.029 min
Delta R.T.: -0.011 min
Response: 11530281
Conc: 4.53 ng/ml

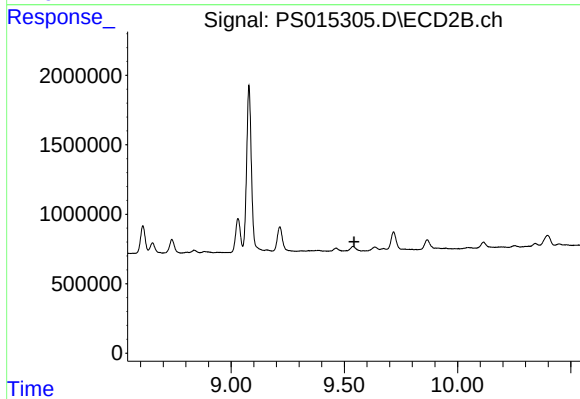

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.542 min
Response: 0
Conc: N.D.

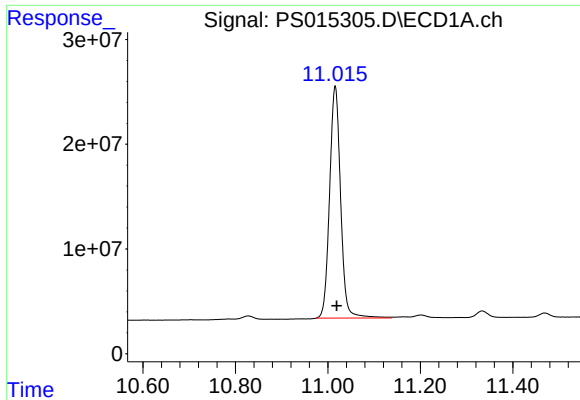

#15 Picloram


R.T.: 11.016 min
Delta R.T.: -0.003 min
Response: 365963088
Conc: 22.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

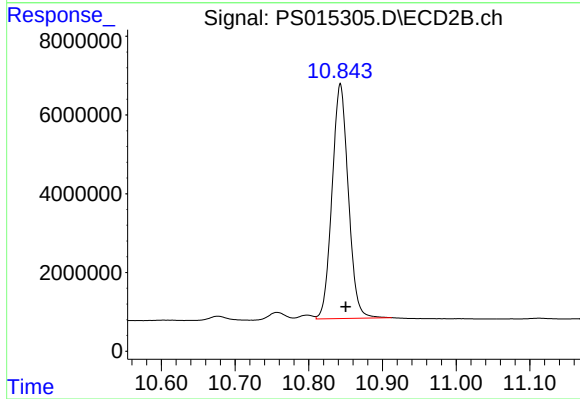


#15 Picloram

R.T.: 10.843 min
Delta R.T.: -0.007 min
Response: 91313483
Conc: 21.99 ng/ml

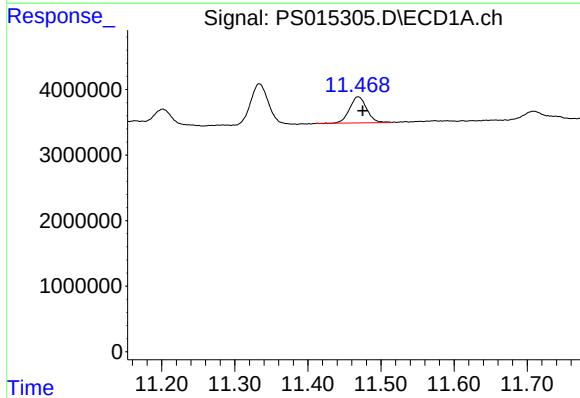

#16 DCPA

R.T.: 11.469 min
Delta R.T.: -0.006 min
Response: 6435673
Conc: N.D.

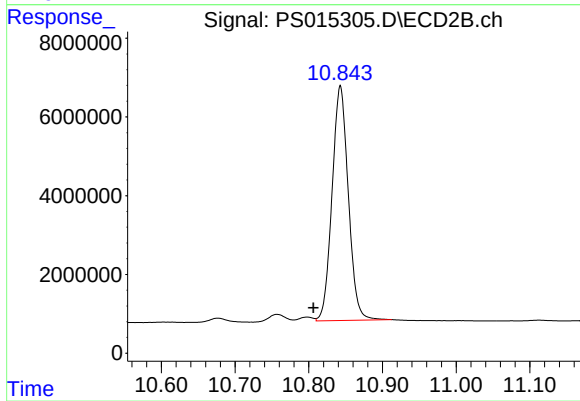

#16 DCPA

R.T.: 10.843 min
Delta R.T.: 0.036 min
Response: 91313483
Conc: 21.18 ng/ml