

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060921\
 Data File : PS015317.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2021 13:54
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 14:49:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.224	6.783	1126.5E6	286.5E6	446.943	534.753
Target Compounds							
3) T	4-Nitroph...	7.023	0.000	5388462	0	3.822	N.D. #
5) T	DICAMBA	7.417	0.000	4119832	0	<MDL	N.D. #
9) T	2,4-D	8.341	0.000	10607508	0	4.163	N.D. #
10) T	Pentachlo...	8.652	0.000	10496447	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.203	0.000	6356388	0	<MDL	N.D. #
12) T	2,4,5-T	9.485	9.079f	10779742	4818348	<MDL	1.664 #
14) T	DINOSEB	11.199	0.000	7414529	0	<MDL	N.D. #
15) T	Picloram	11.014	10.842	32824522	8769840	1.981	2.112
16) T	DCPA	11.467	10.842	9606573	8769840	<MDL	2.034 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060921\
Data File : PS015317.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2021 13:54
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 14:49:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

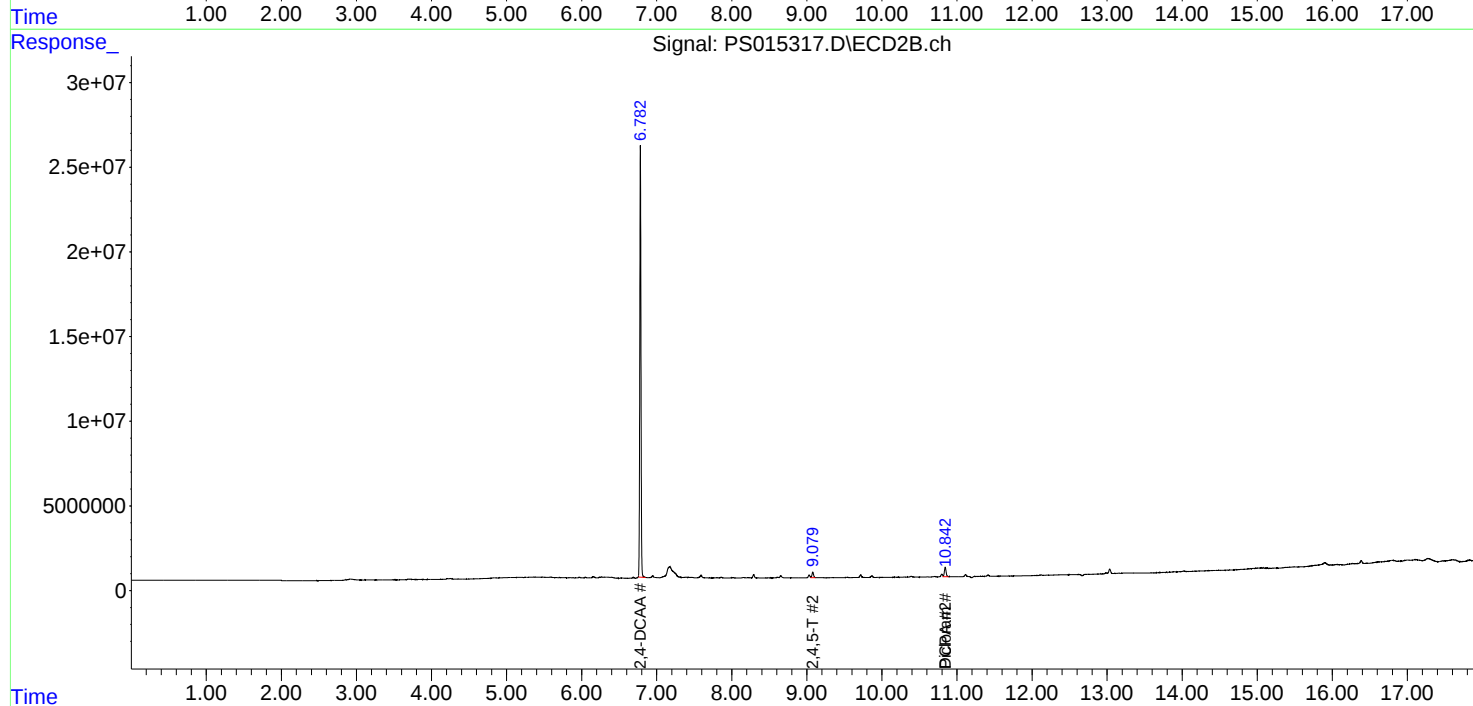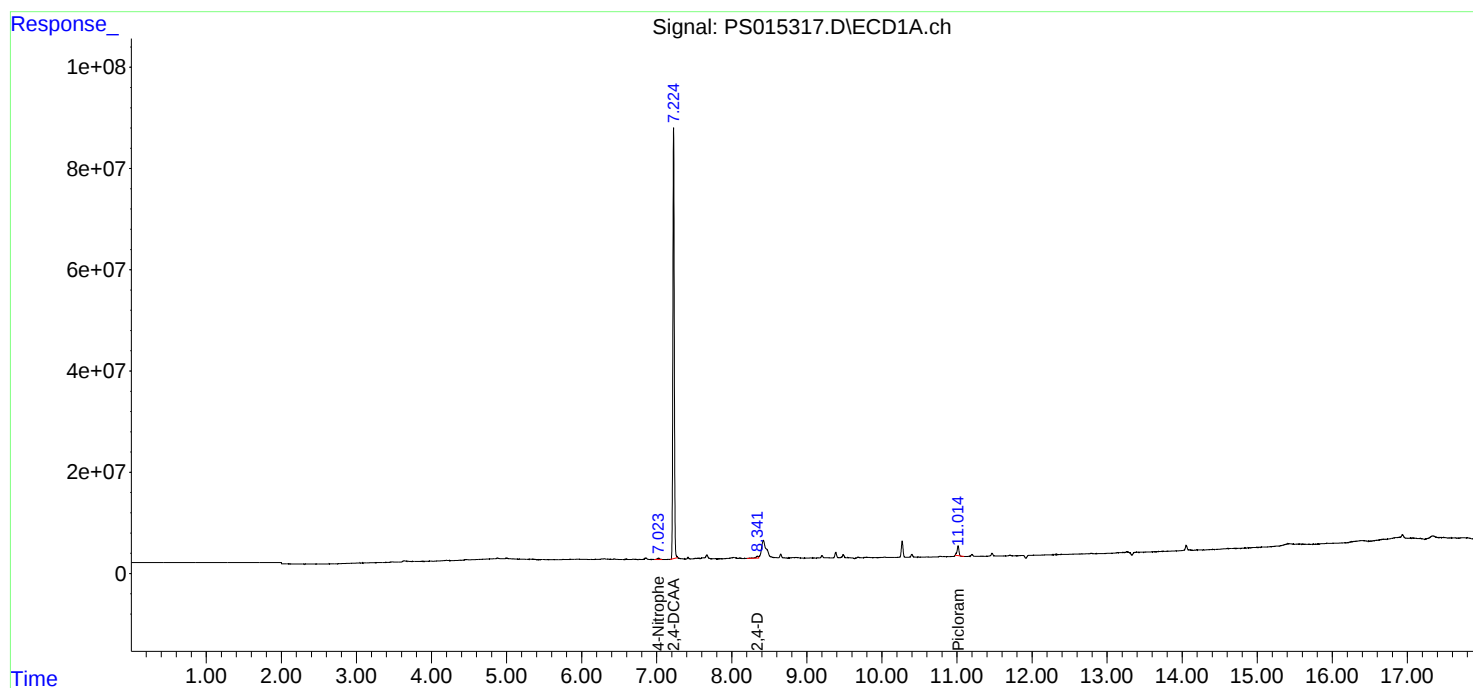


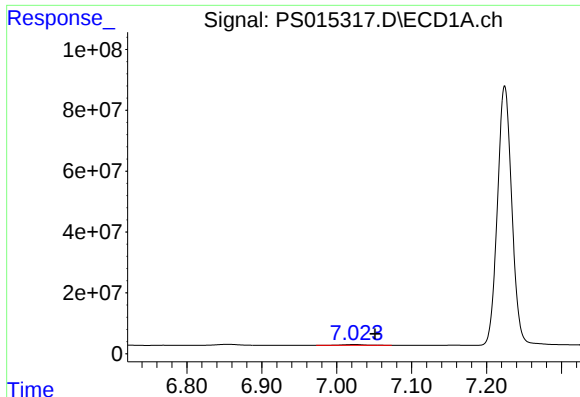

#3 4-Nitrophenol


R.T.: 7.023 min
Delta R.T.: -0.028 min
Response: 5388462
Conc: 3.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

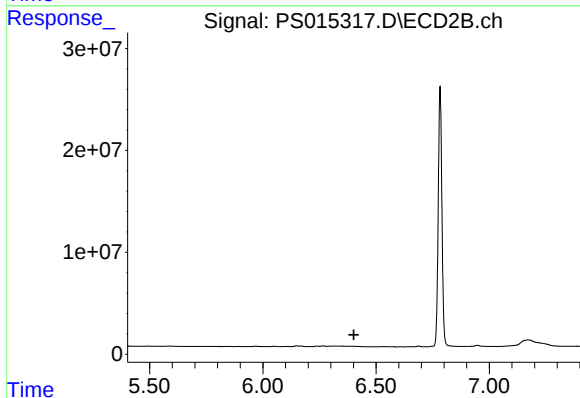


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

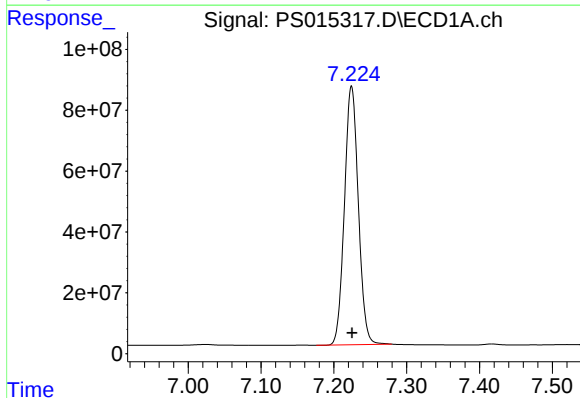


#4 2,4-DCAA

R.T.: 7.224 min
Delta R.T.: 0.000 min
Response: 1126463808
Conc: 446.94 ng/ml

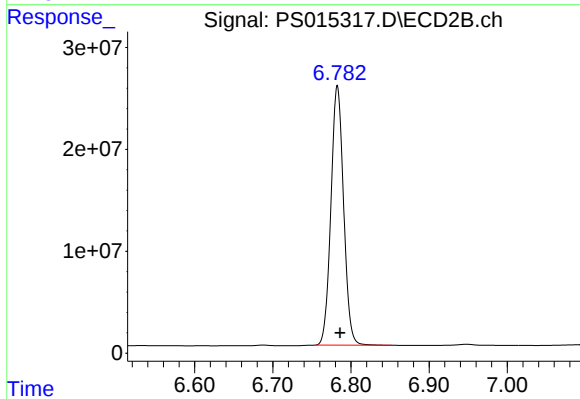

#4 2,4-DCAA


R.T.: 6.783 min
Delta R.T.: -0.004 min
Response: 286505091
Conc: 534.75 ng/ml

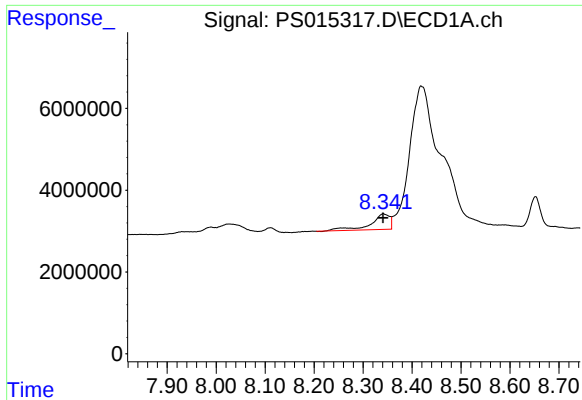

#9 2,4-D


R.T.: 8.341 min
Delta R.T.: 0.000 min
Response: 10607508
Conc: 4.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

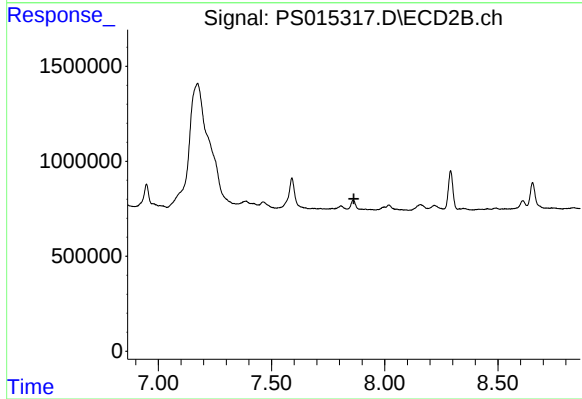


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.864 min
Response: 0
Conc: N.D.

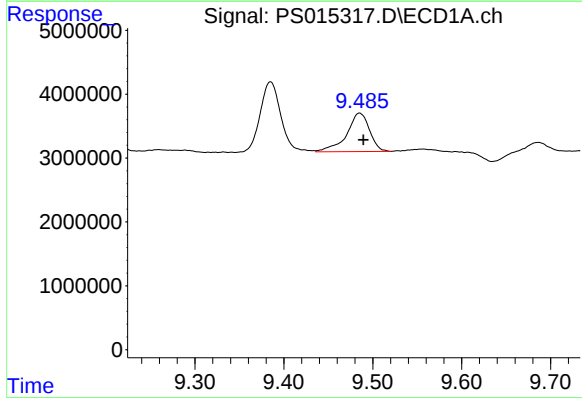


#12 2,4,5-T

R.T.: 9.485 min
Delta R.T.: -0.004 min
Response: 10779742
Conc: N.D.

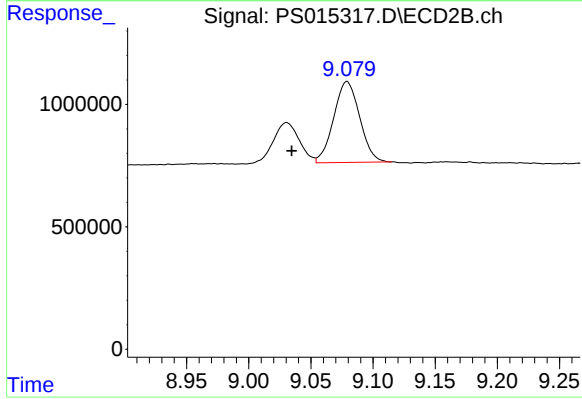

#12 2,4,5-T


R.T.: 9.079 min
Delta R.T.: 0.044 min
Response: 4818348
Conc: 1.66 ng/ml

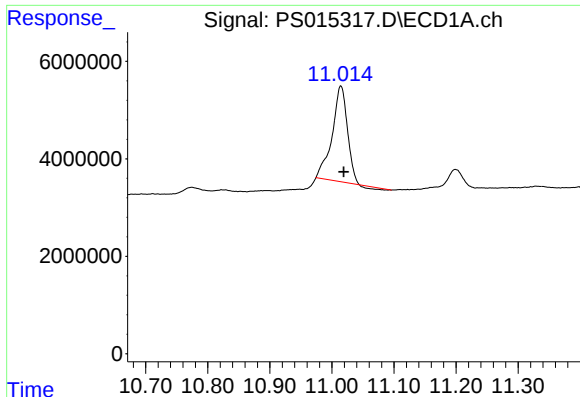

#15 Picloram


R.T.: 11.014 min
Delta R.T.: -0.005 min
Response: 32824522
Conc: 1.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

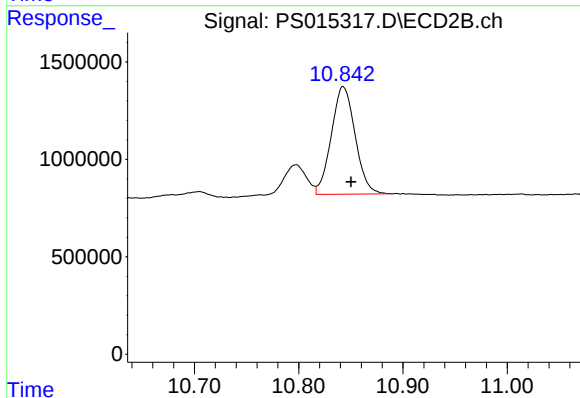


#15 Picloram

R.T.: 10.842 min
Delta R.T.: -0.008 min
Response: 8769840
Conc: 2.11 ng/ml

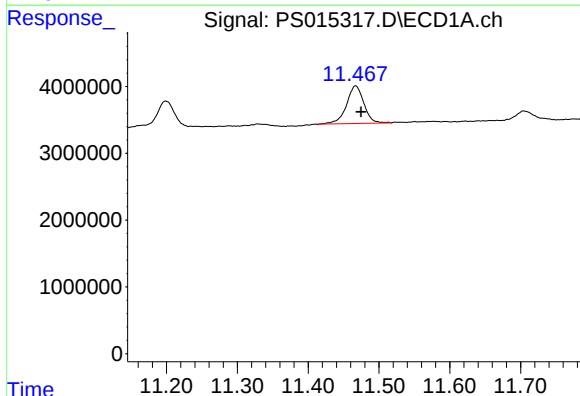

#16 DCPA

R.T.: 11.467 min
Delta R.T.: -0.008 min
Response: 9606573
Conc: N.D.

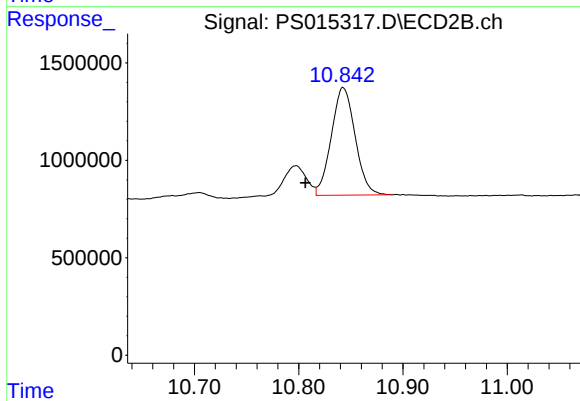

#16 DCPA

R.T.: 10.842 min
Delta R.T.: 0.036 min
Response: 8769840
Conc: 2.03 ng/ml