

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060921\
 Data File : PS015345.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2021 03:17
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 05:45:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.224	6.782	1156.8E6	288.7E6	458.988	538.835
Target Compounds							
2) T	3,5-DICHL...	6.473	5.965	2912421	1968095	<MDL	2.436 #
3) T	4-Nitroph...	7.014	0.000	11789521	0	8.363	N.D. #
5) T	DICAMBA	7.416	0.000	2987325	0	<MDL	N.D. #
7) T	MCPA	7.718	0.000	78106174	0	7.782	N.D. #
9) T	2,4-D	8.410f	0.000	85881711	0	33.704	N.D. #
13) T	2,4-DB	10.051	0.000	3929062	0	1.543	N.D. #
15) T	Picloram	11.014	10.842	16625022	4437480	1.004	1.069
16) T	DCPA	0.000	10.842	0	4437480	N.D.	1.029



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060921\
Data File : PS015345.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2021 03:17
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 05:45:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

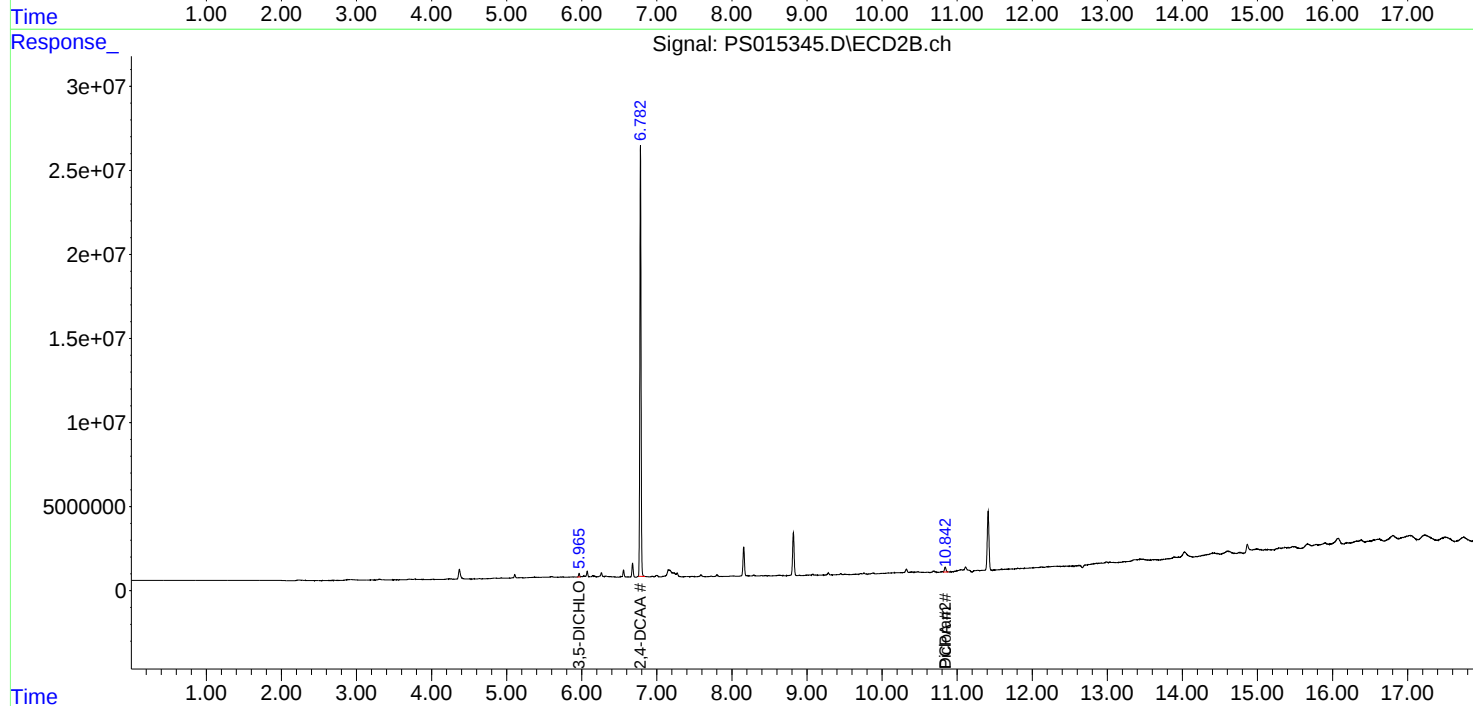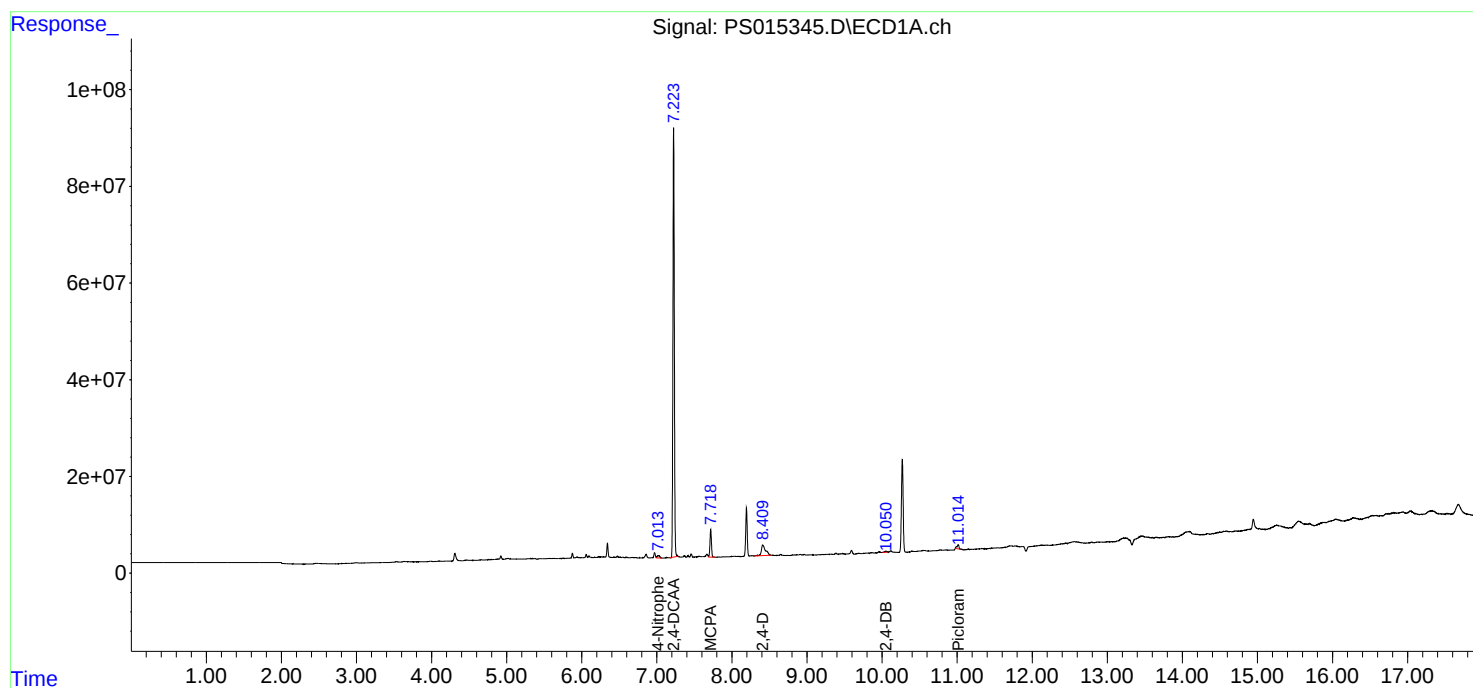


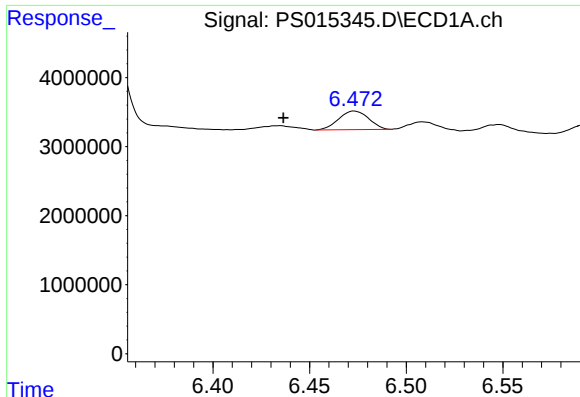

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.473 min
Delta R.T.: 0.037 min
Response: 2912421
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

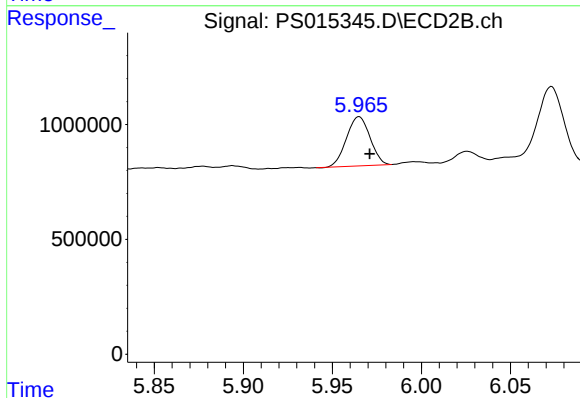


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.965 min
Delta R.T.: -0.006 min
Response: 1968095
Conc: 2.44 ng/ml

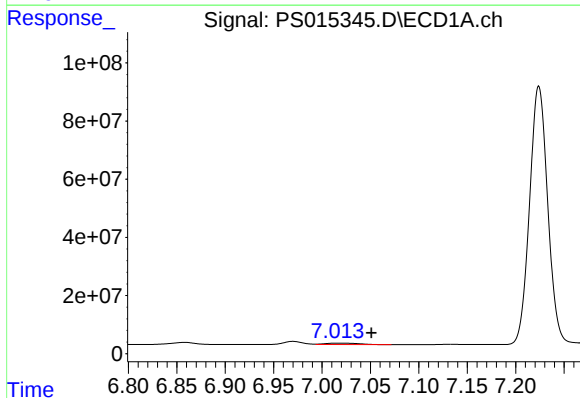


#3 4-Nitrophenol

R.T.: 7.014 min
Delta R.T.: -0.037 min
Response: 11789521
Conc: 8.36 ng/ml

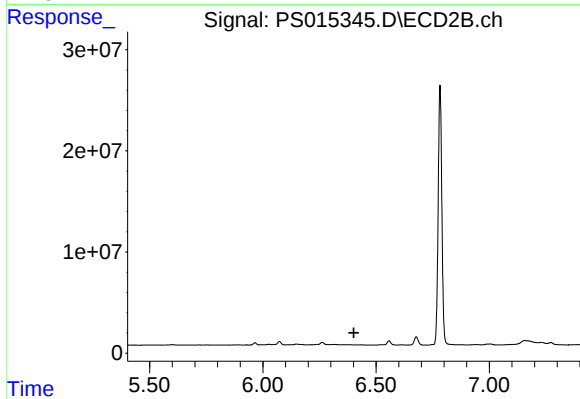

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.402 min
Response: 0
Conc: N.D.

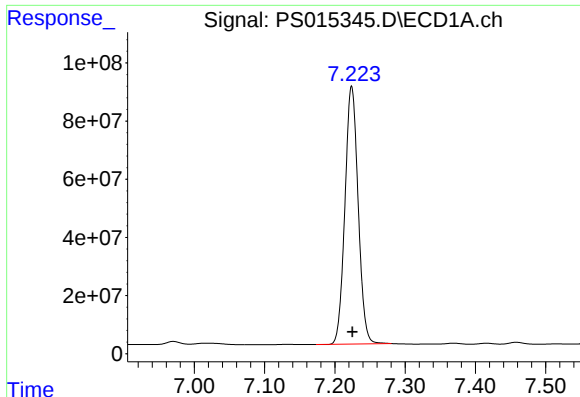

#4 2,4-DCAA


R.T.: 7.224 min
Delta R.T.: -0.001 min
Response: 1156822131
Conc: 458.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

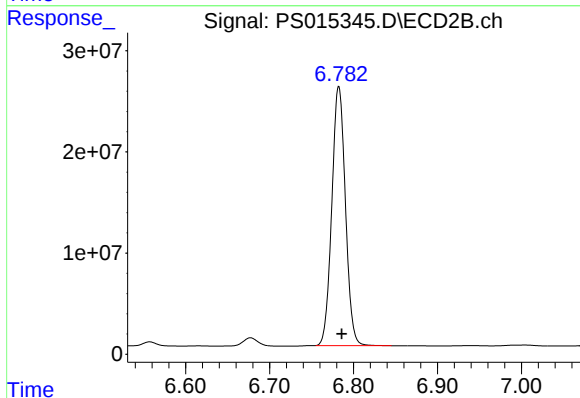


#4 2,4-DCAA

R.T.: 6.782 min
Delta R.T.: -0.004 min
Response: 288692376
Conc: 538.84 ng/ml

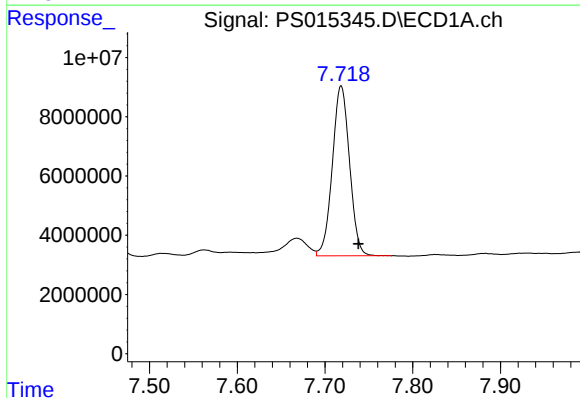


#7 MCPA

R.T.: 7.718 min
Delta R.T.: -0.020 min
Response: 78106174
Conc: 7.78 ug/ml

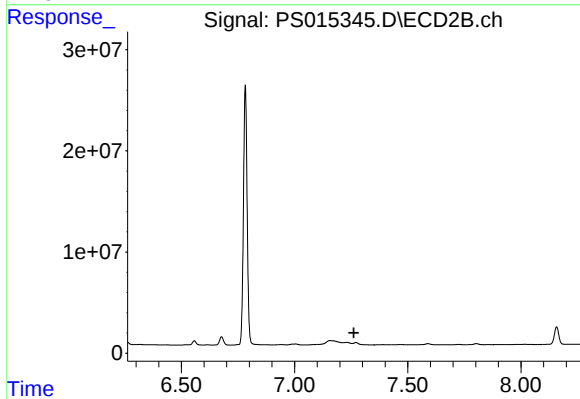

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.262 min
Response: 0
Conc: N.D.

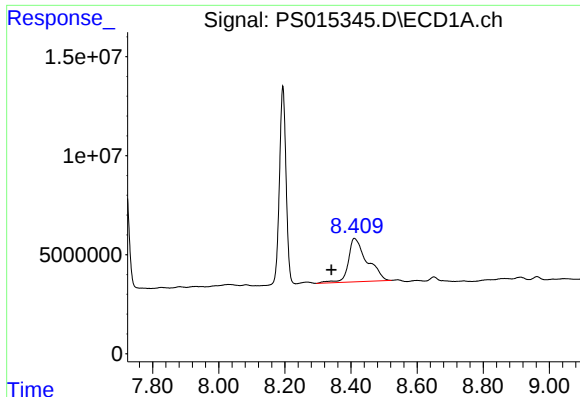

#9 2,4-D


R.T.: 8.410 min
Delta R.T.: 0.069 min
Response: 85881711
Conc: 33.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

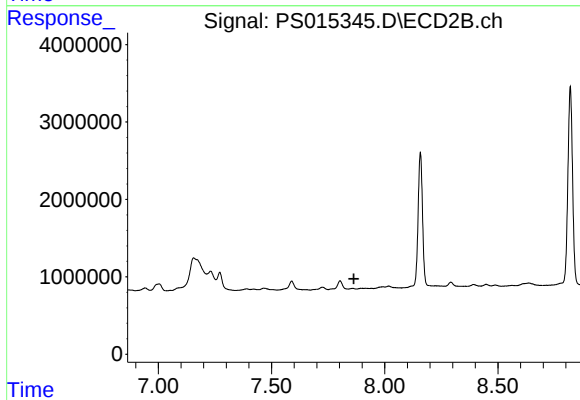


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.864 min
Response: 0
Conc: N.D.

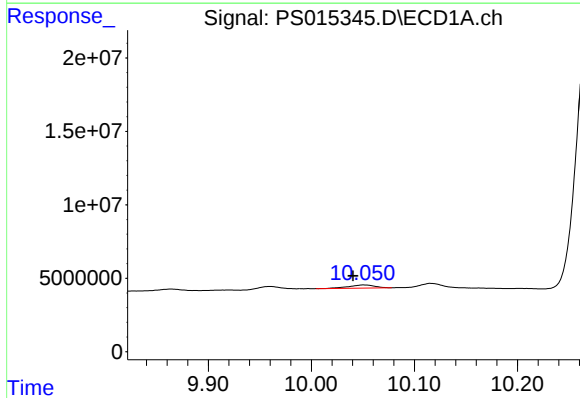


#13 2,4-DB

R.T.: 10.051 min
Delta R.T.: 0.011 min
Response: 3929062
Conc: 1.54 ng/ml

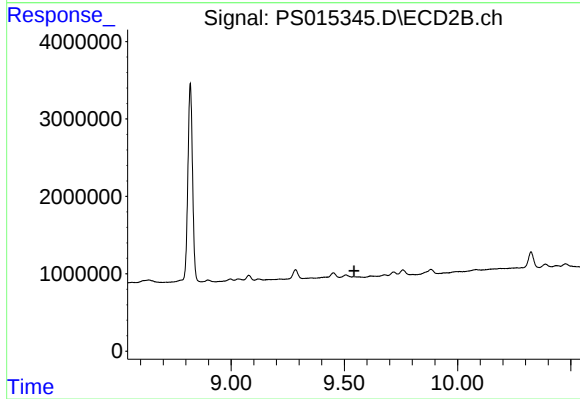

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.542 min
Response: 0
Conc: N.D.

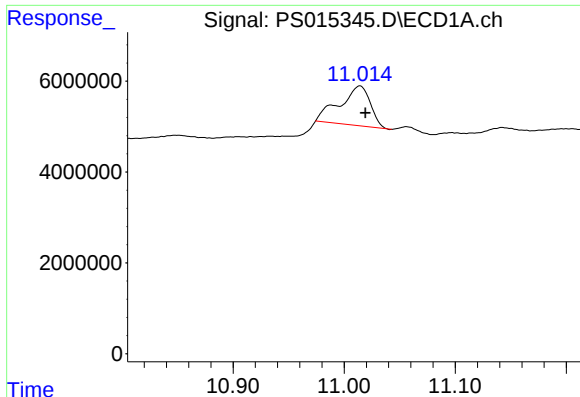

#15 Picloram


R.T.: 11.014 min
Delta R.T.: -0.005 min
Response: 16625022
Conc: 1.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

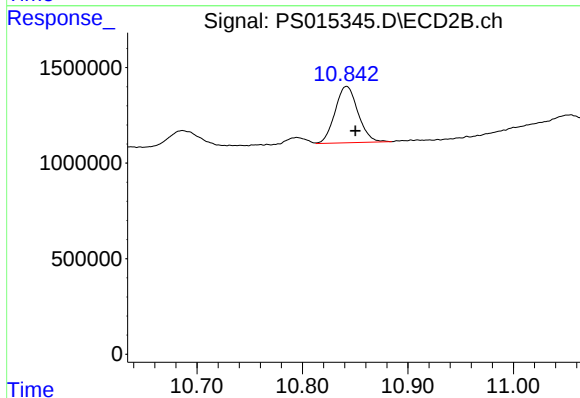


#15 Picloram

R.T.: 10.842 min
Delta R.T.: -0.008 min
Response: 4437480
Conc: 1.07 ng/ml

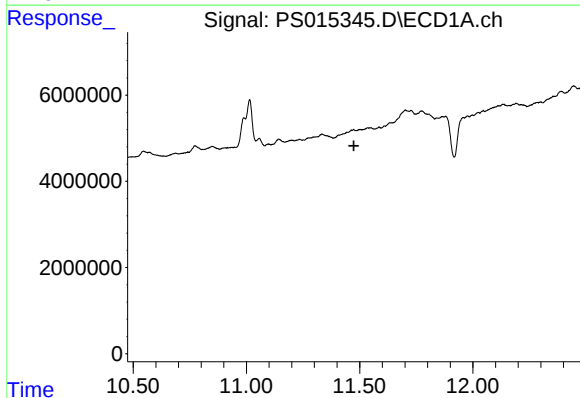

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.475 min
Response: 0
Conc: N.D.

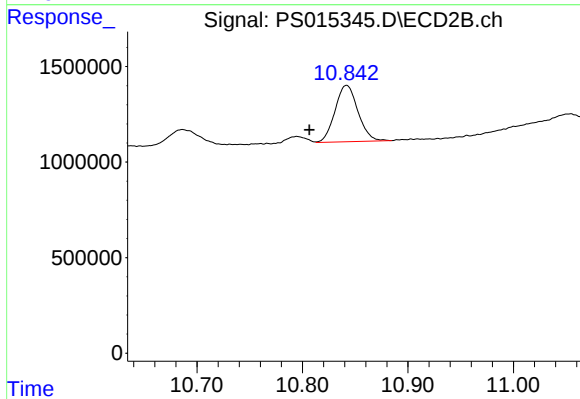

#16 DCPA

R.T.: 10.842 min
Delta R.T.: 0.035 min
Response: 4437480
Conc: 1.03 ng/ml