

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060922\
 Data File : PS019663.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2022 09:50
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 11:17:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.201	6.784	1013.1E6	425.7E6	422.275	549.348 #
Target Compounds							
3) T	4-Nitroph...	0.000	6.387	0	518264	N.D.	1.211
6) T	MCP	0.000	7.068	0	471259	N.D.	<MDL
7) T	MCPA	7.668	0.000	171932	0	<MDL	N.D. #
10) T	Pentachlo...	8.625	8.285	496430	630093	<MDL	<MDL #
11) T	2,4,5-TP ...	9.129	0.000	1302864	0	<MDL	N.D. #
12) T	2,4,5-T	9.475	0.000	7606401	0	<MDL	N.D. #
13) T	2,4-DB	9.996	0.000	760612	0	<MDL	N.D. #
14) T	DINOSEB	11.087f	0.000	56742657	0	3.669	N.D. #
15) T	Picloram	10.995	10.785f	13334833	741372	<MDL	<MDL #
16) T	DCPA	11.427	10.785	1463639	741372	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060922\
Data File : PS019663.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2022 09:50
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 11:17:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

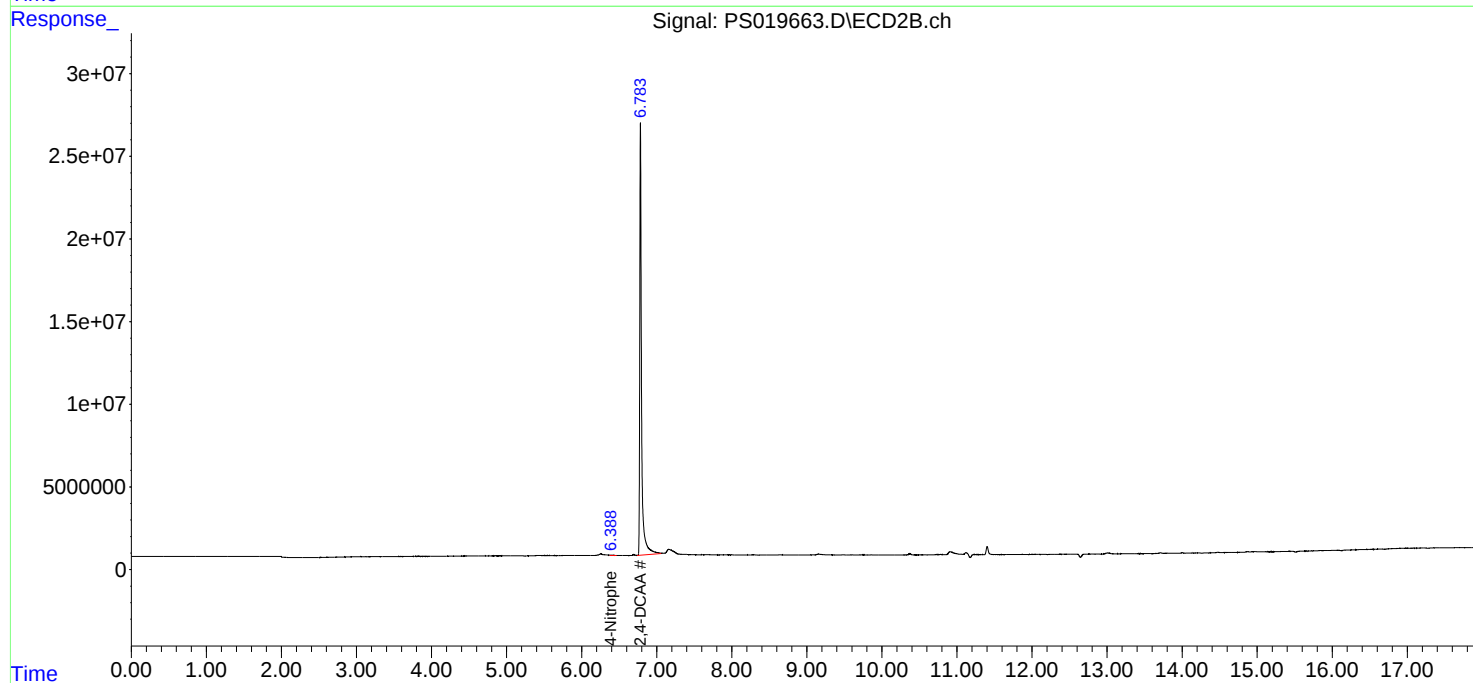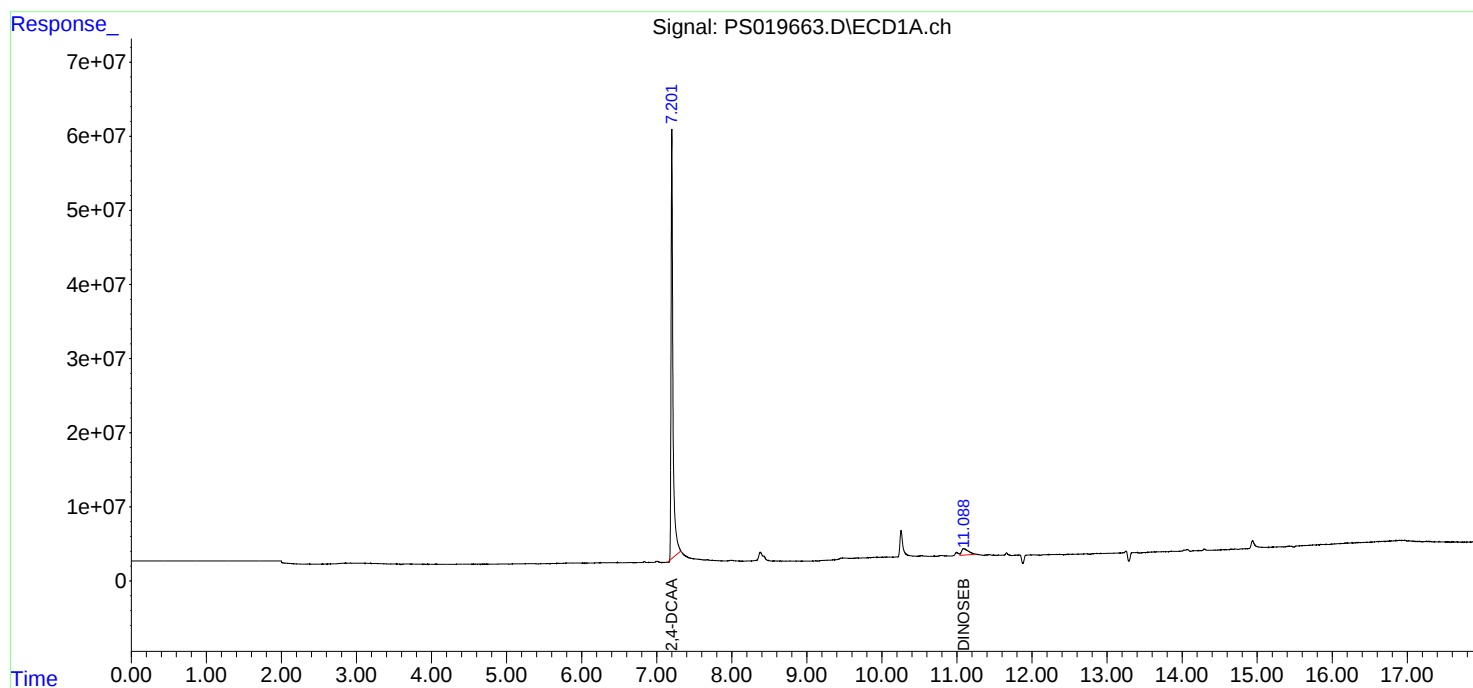


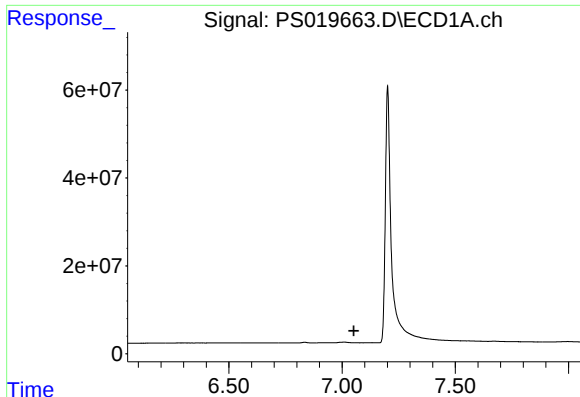

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.052 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

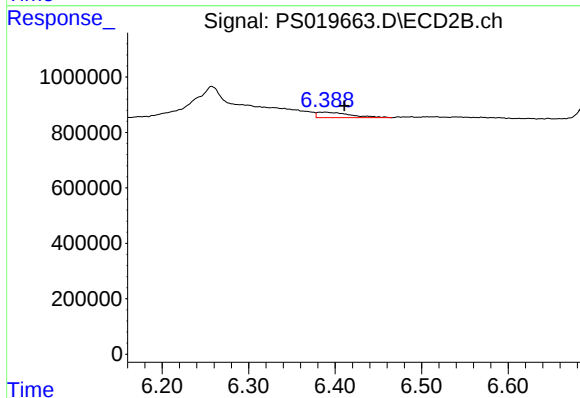


#3 4-Nitrophenol

R.T.: 6.387 min
Delta R.T.: -0.023 min
Response: 518264
Conc: 1.21 ng/ml

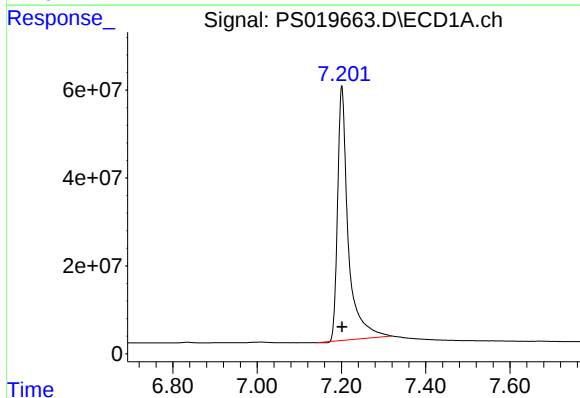


#4 2,4-DCAA

R.T.: 7.201 min
Delta R.T.: 0.000 min
Response: 1013107674
Conc: 422.27 ng/ml

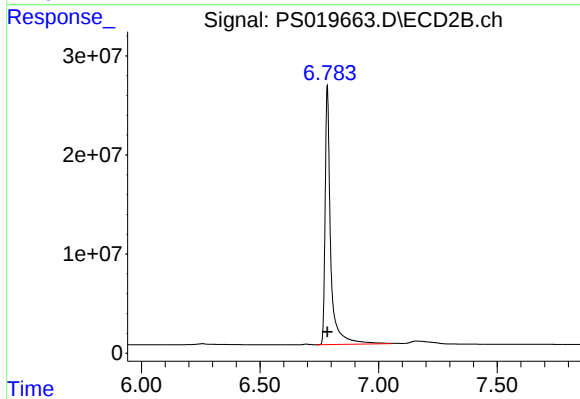

#4 2,4-DCAA


R.T.: 6.784 min
Delta R.T.: 0.000 min
Response: 425673295
Conc: 549.35 ng/ml

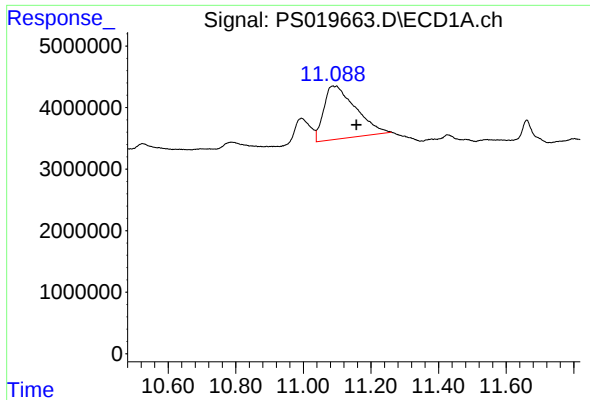

#14 DINOSEB

R.T.: 11.087 min
Delta R.T.: -0.069 min
Response: 56742657
Conc: 3.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

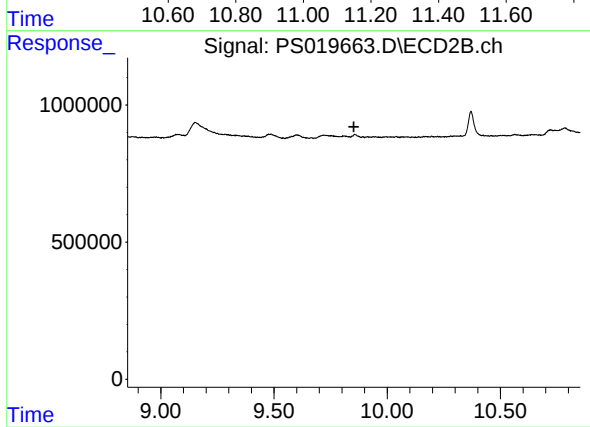

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.853 min
Response: 0
Conc: N.D.