

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060922\
 Data File : PS019674.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2022 14:21
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 14:53:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.200	6.783	1051.0E6	425.8E6	438.057	549.510 #
Target Compounds							
1) T	Dalapon	3.003	0.000	562114	0	<MDL	N.D. #
2) T	3,5-DICHL...	0.000	5.911f	0	337111	N.D.	<MDL
7) T	MCPA	7.661	0.000	1475658	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.630f	0	1631161	N.D.	1.847
10) T	Pentachlo...	8.618	8.289	578991	777970	<MDL	<MDL #
11) T	2,4,5-TP ...	9.126f	8.616	2084863	1101403	<MDL	<MDL #
12) T	2,4,5-T	9.442	9.058	5434430	307019	<MDL	<MDL #
13) T	2,4-DB	10.005	9.469f	4993525	1701541	1.234	2.753 #
14) T	DINOSEB	11.143	0.000	13423622	0	<MDL	N.D. #
15) T	Picloram	10.972	10.887f	47384473	2962431	1.597	<MDL #
16) T	DCPA	11.429	10.785	1712631	545278	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060922\
Data File : PS019674.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2022 14:21
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 14:53:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

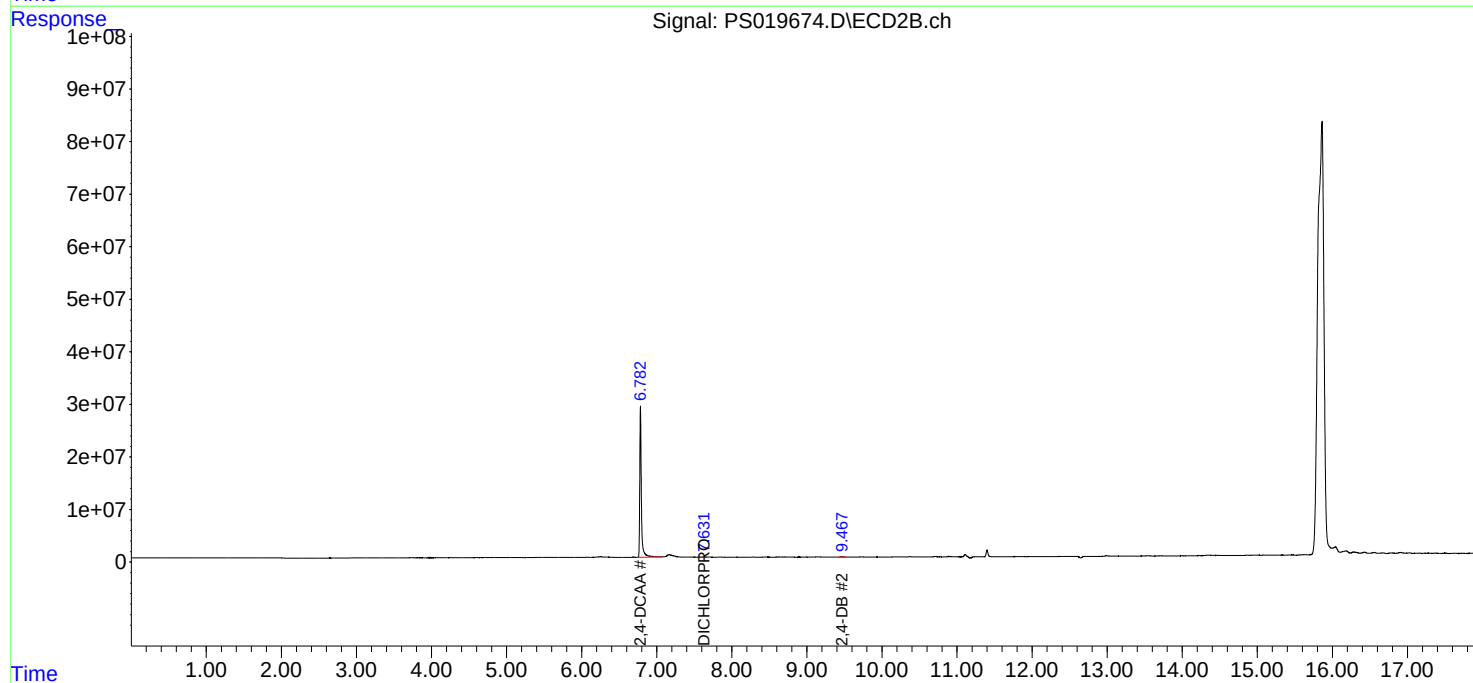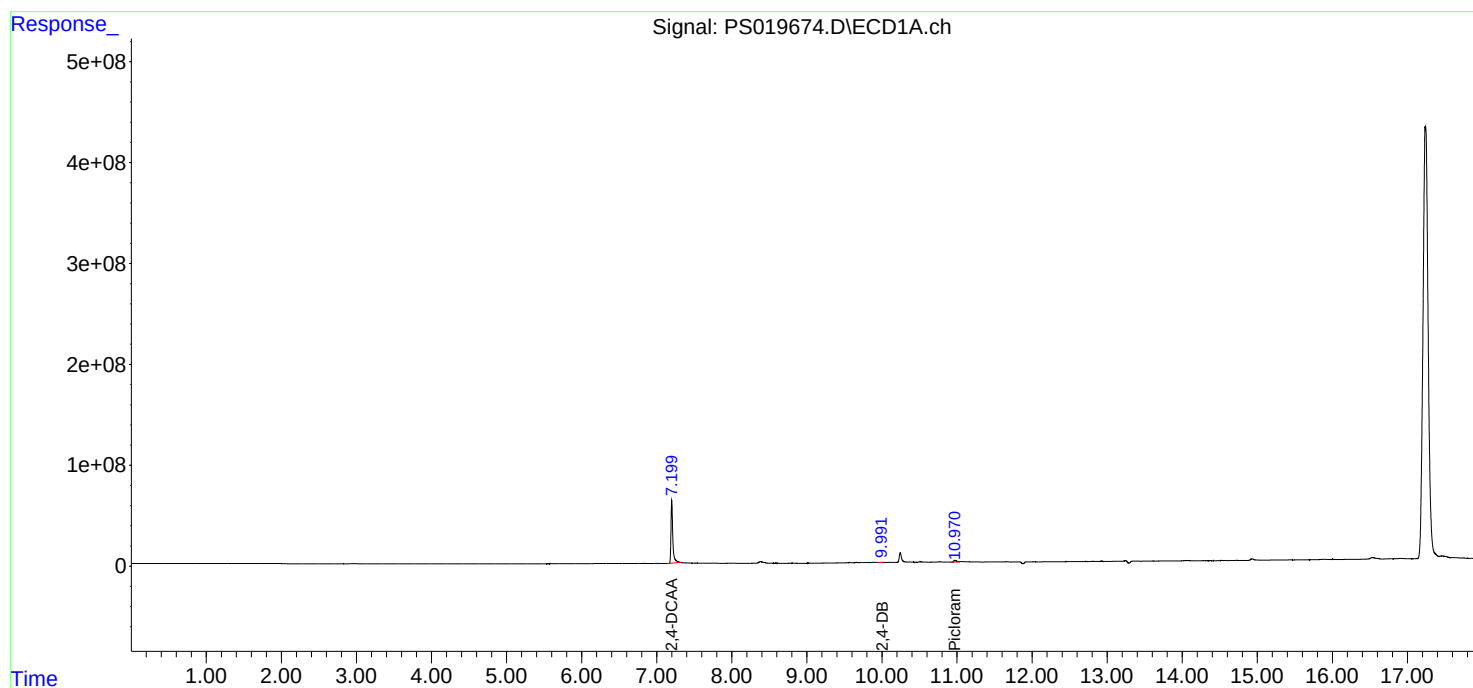


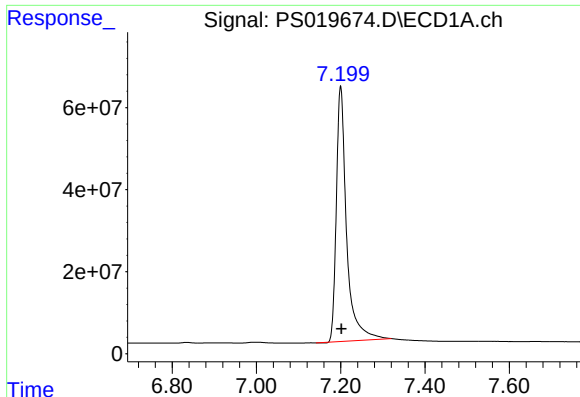

#4 2,4-DCAA


R.T.: 7.200 min
Delta R.T.: -0.002 min
Response: 1050971353
Conc: 438.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

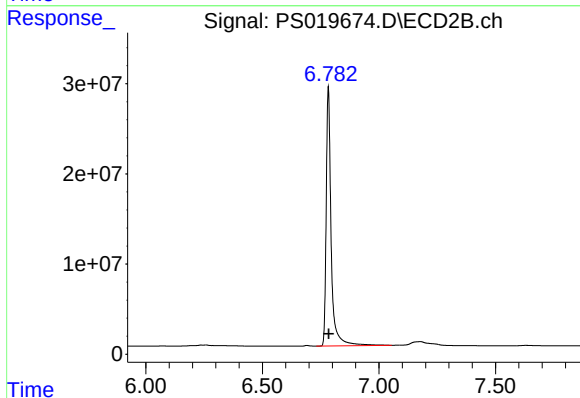


#4 2,4-DCAA

R.T.: 6.783 min
Delta R.T.: -0.002 min
Response: 425799339
Conc: 549.51 ng/ml

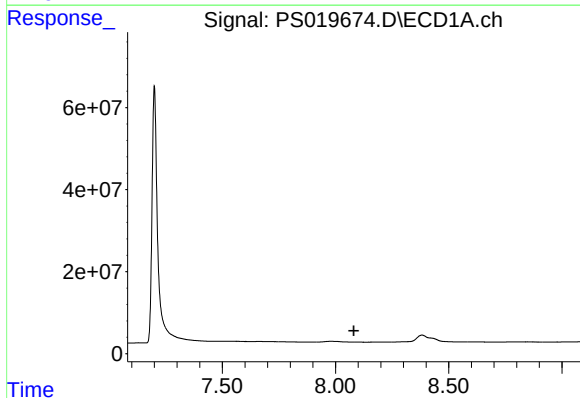


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.081 min
Response: 0
Conc: N.D.

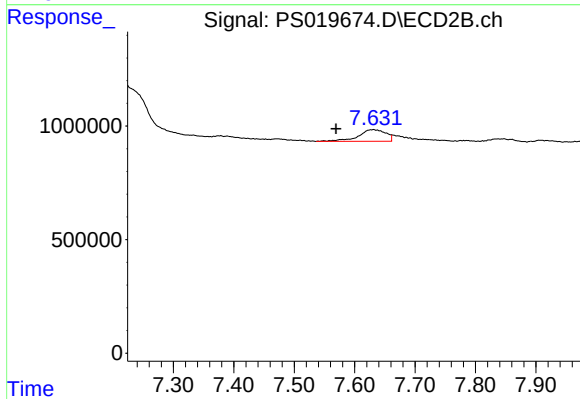

#8 DICHLORPROP


R.T.: 7.630 min
Delta R.T.: 0.061 min
Response: 1631161
Conc: 1.85 ng/ml

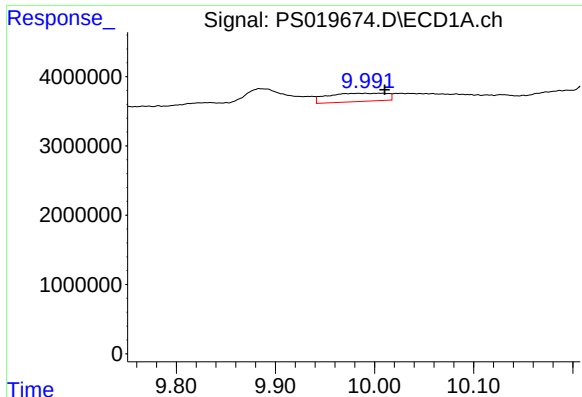

#13 2,4-DB


R.T.: 10.005 min
Delta R.T.: -0.005 min
Response: 4993525
Conc: 1.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

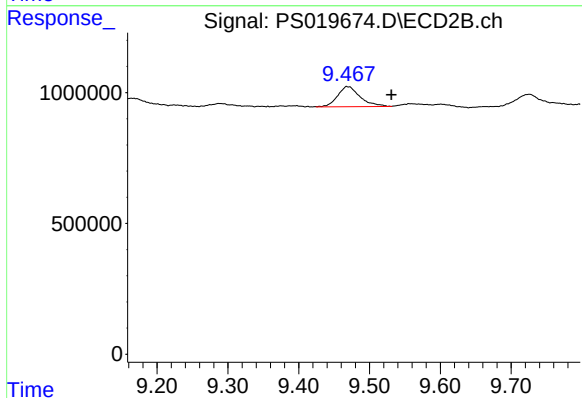


#13 2,4-DB

R.T.: 9.469 min
Delta R.T.: -0.061 min
Response: 1701541
Conc: 2.75 ng/ml

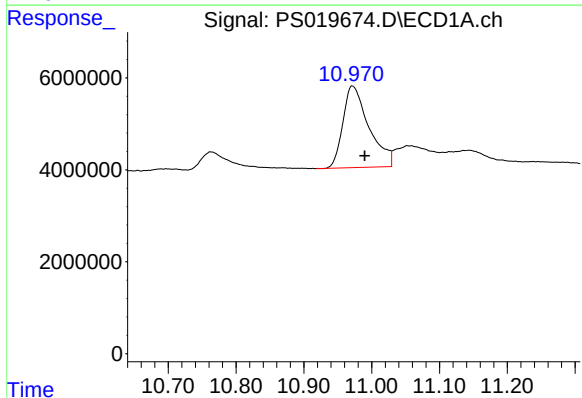

#15 Picloram

R.T.: 10.972 min
Delta R.T.: -0.018 min
Response: 47384473
Conc: 1.60 ng/ml

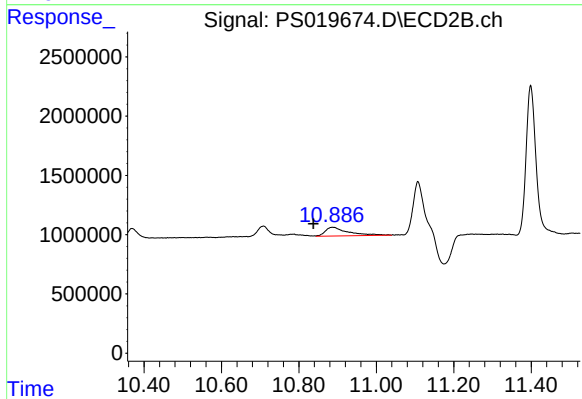

#15 Picloram

R.T.: 10.887 min
Delta R.T.: 0.050 min
Response: 2962431
Conc: N.D.