

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060922\
 Data File : PS019684.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2022 19:09
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 04:11:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.200	6.782	1088.8E6	434.9E6	453.815	561.256
Target Compounds							
1) T	Dalapon	2.989	0.000	396295	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.468f	5.916f	1804318	98237	<MDL	<MDL #
3) T	4-Nitroph...	6.991f	0.000	946144	0	<MDL	N.D. #
5) T	DICAMBA	0.000	7.007f	0	1672478	N.D.	<MDL
6) T	MCP	0.000	7.007	0	1672478	N.D.	<MDL
7) T	MCPA	7.701	0.000	2904170	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.625f	0	2860670	N.D.	3.238
9) T	2,4-D	0.000	7.843	0	488327	N.D.	<MDL
10) T	Pentachlo...	8.621	8.286	740828	1215238	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	8.614	0	1447494	N.D.	<MDL
12) T	2,4,5-T	0.000	9.052	0	707995	N.D.	<MDL
13) T	2,4-DB	9.991	9.561	17124866	409225	4.233	<MDL #
14) T	DINOSEB	11.138	9.857	18224965	601349	1.178	<MDL #
15) T	Picloram	10.964	10.883f	184.2E6	3145810	6.207	<MDL #
16) T	DCPA	11.430	10.782	3037478	1148644	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060922\
Data File : PS019684.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2022 19:09
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 04:11:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

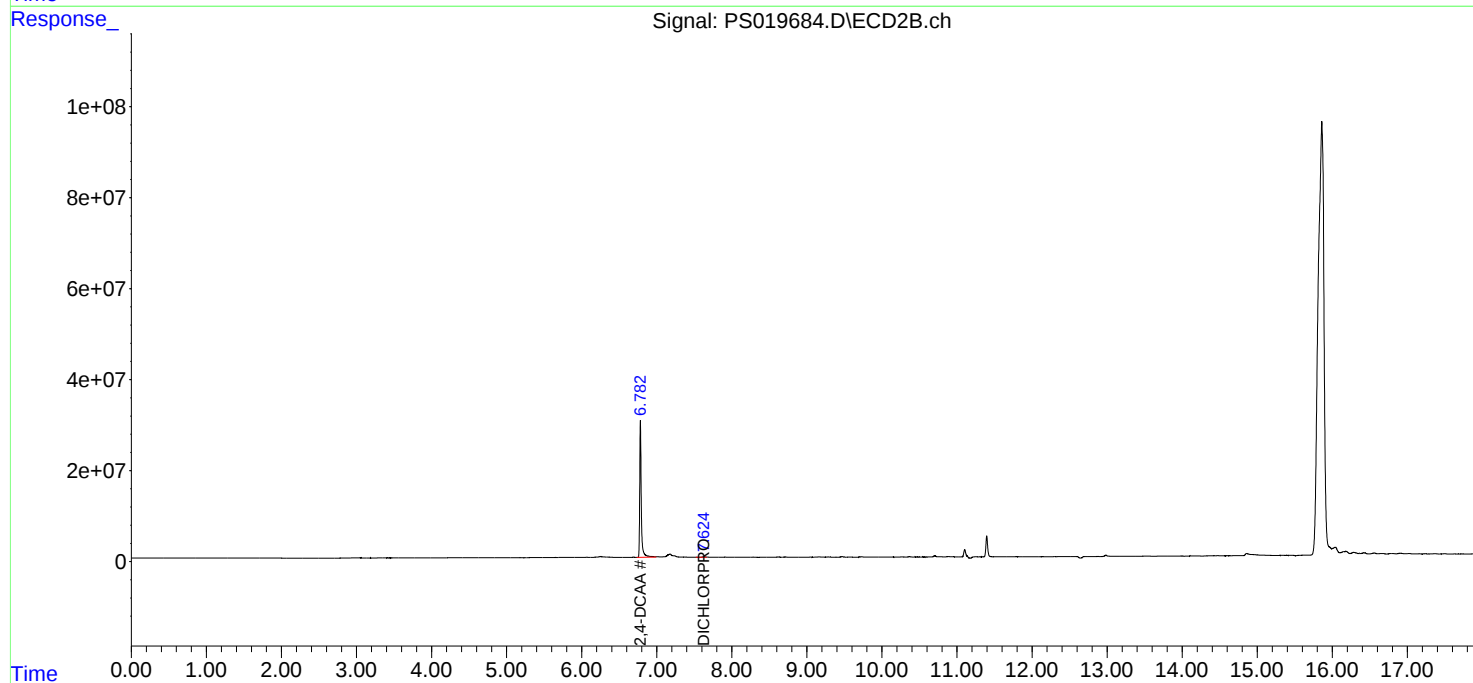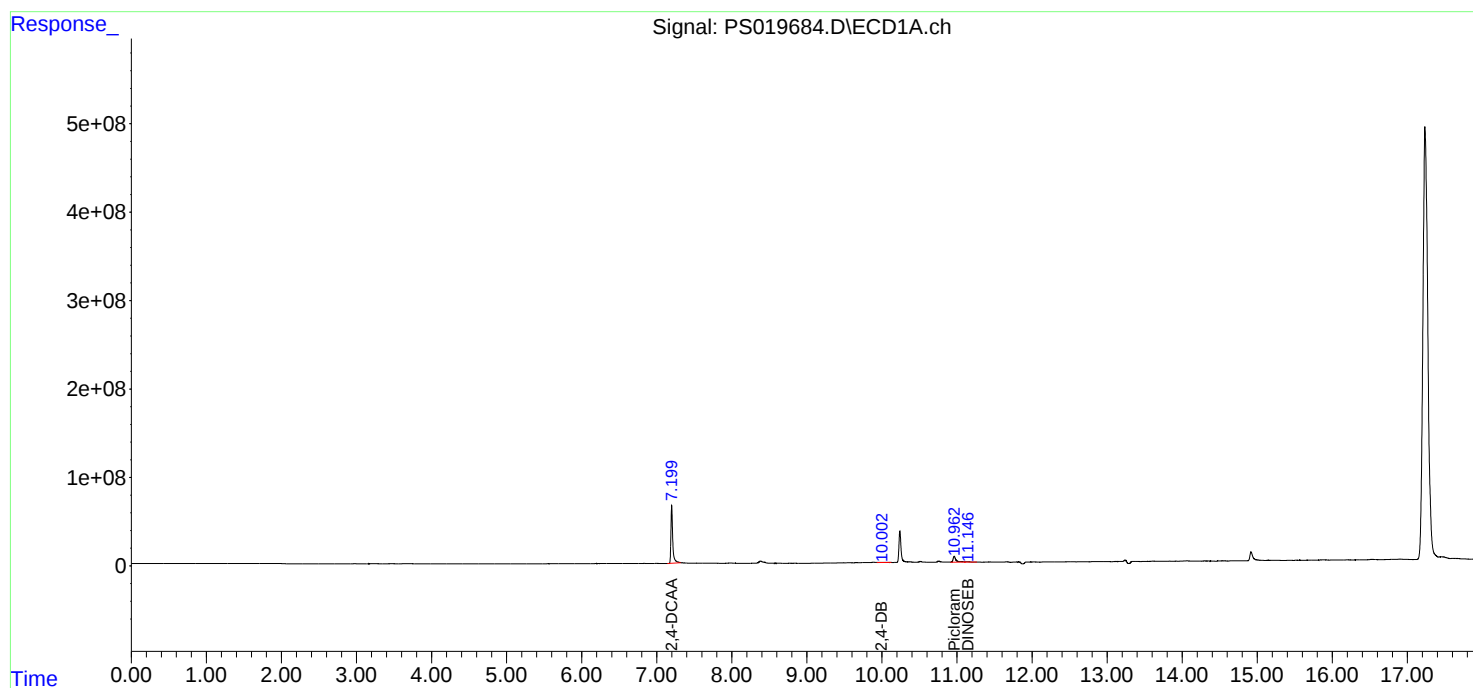


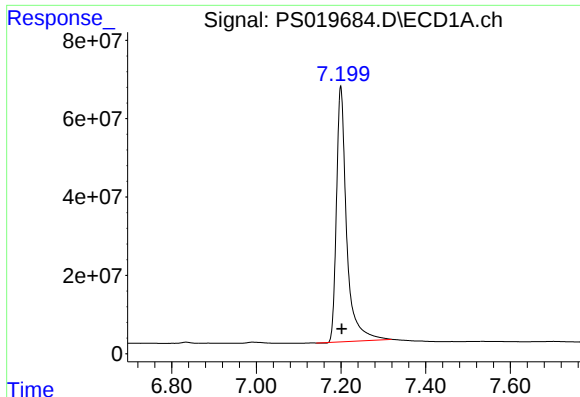

#4 2,4-DCAA


R.T.: 7.200 min
Delta R.T.: -0.002 min
Response: 1088777451
Conc: 453.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

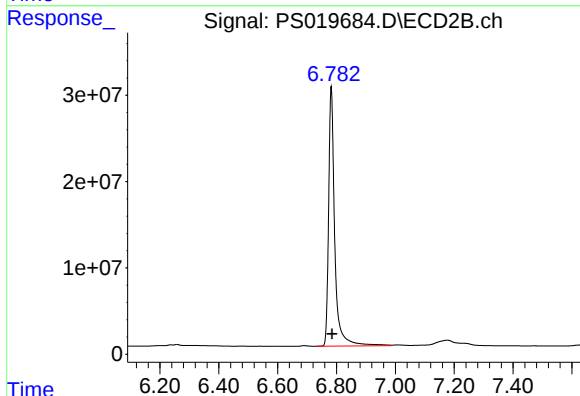


#4 2,4-DCAA

R.T.: 6.782 min
Delta R.T.: -0.003 min
Response: 434900324
Conc: 561.26 ng/ml

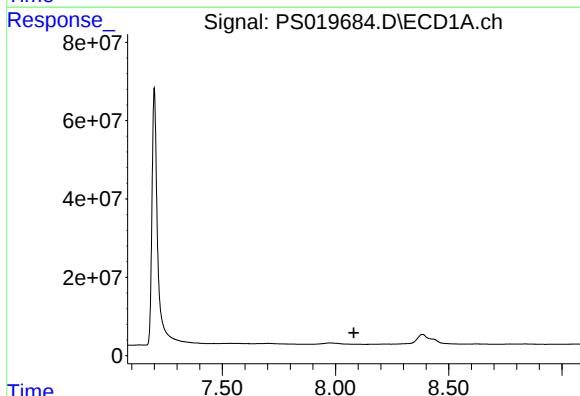


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.081 min
Response: 0
Conc: N.D.

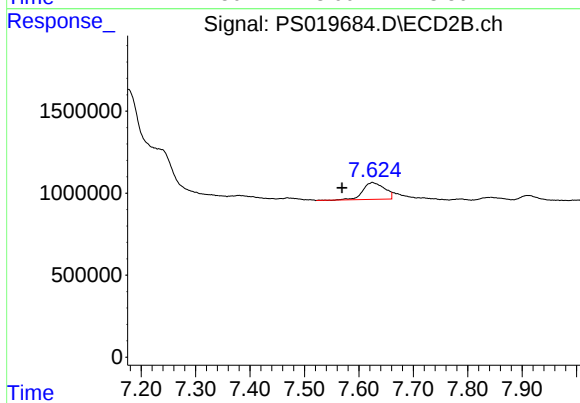

#8 DICHLORPROP


R.T.: 7.625 min
Delta R.T.: 0.056 min
Response: 2860670
Conc: 3.24 ng/ml

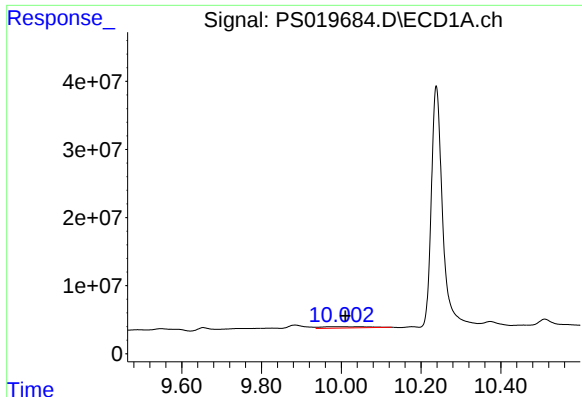

#13 2,4-DB


R.T.: 9.991 min
Delta R.T.: -0.020 min
Response: 17124866
Conc: 4.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

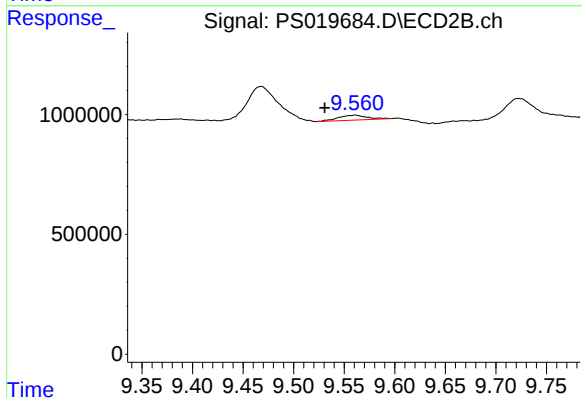


#13 2,4-DB

R.T.: 9.561 min
Delta R.T.: 0.030 min
Response: 409225
Conc: N.D.

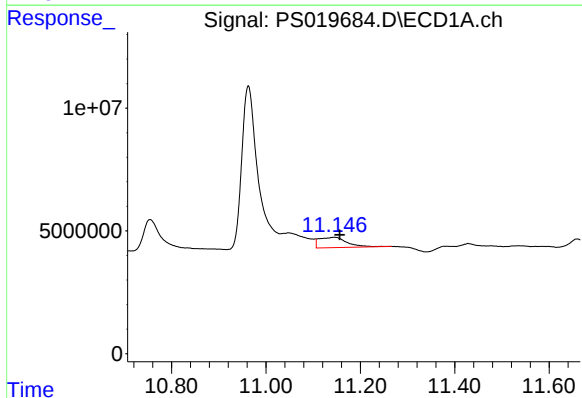


#14 DINOSEB

R.T.: 11.138 min
Delta R.T.: -0.018 min
Response: 18224965
Conc: 1.18 ng/ml

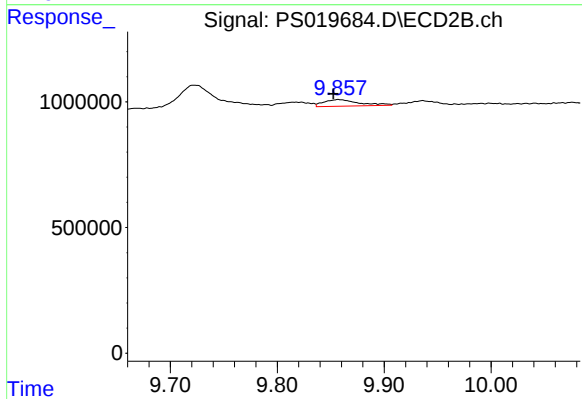

#14 DINOSEB


R.T.: 9.857 min
Delta R.T.: 0.004 min
Response: 601349
Conc: N.D.

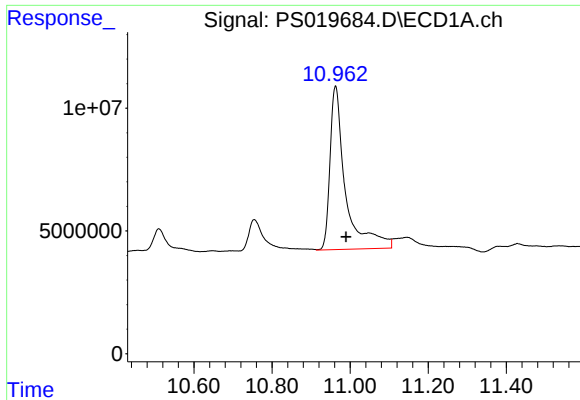

#15 Picloram

R.T.: 10.964 min
Delta R.T.: -0.025 min
Response: 184196054
Conc: 6.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

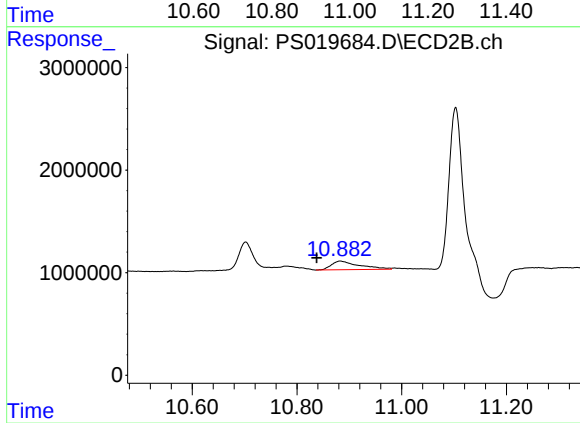

#15 Picloram

R.T.: 10.883 min
Delta R.T.: 0.045 min
Response: 3145810
Conc: N.D.