

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060922\
 Data File : PS019690.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2022 23:09
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 04:13:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.200	6.783	1062.1E6	434.7E6	442.710	560.948 #
Target Compounds							
1) T	Dalapon	2.994	0.000	540808	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.468f	5.912f	1654562	82311	<MDL	<MDL #
3) T	4-Nitroph...	6.993f	0.000	558379	0	<MDL	N.D. #
5) T	DICAMBA	0.000	7.010f	0	1909094	N.D.	<MDL
6) T	MCPD	0.000	7.010	0	1909094	N.D.	<MDL
7) T	MCPA	7.707	0.000	1477925	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.636f	0	2350718	N.D.	2.661
9) T	2,4-D	0.000	7.916f	0	658192	N.D.	<MDL
10) T	Pentachlo...	8.621	8.287	1443575	1391365	<MDL	<MDL #
11) T	2,4,5-TP ...	9.183	8.620	1927449	1050377	<MDL	<MDL #
12) T	2,4,5-T	9.435	9.060	9786933	702355	<MDL	<MDL #
13) T	2,4-DB	10.008	9.562	6427130	1078375	1.589	1.745
14) T	DINOSEB	0.000	9.859	0	517631	N.D.	<MDL
15) T	Picloram	10.964	10.887f	175.1E6	9572502	5.901	1.488 #
16) T	DCPA	11.427	10.782	3377613	2045330	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060922\
Data File : PS019690.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2022 23:09
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 04:13:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

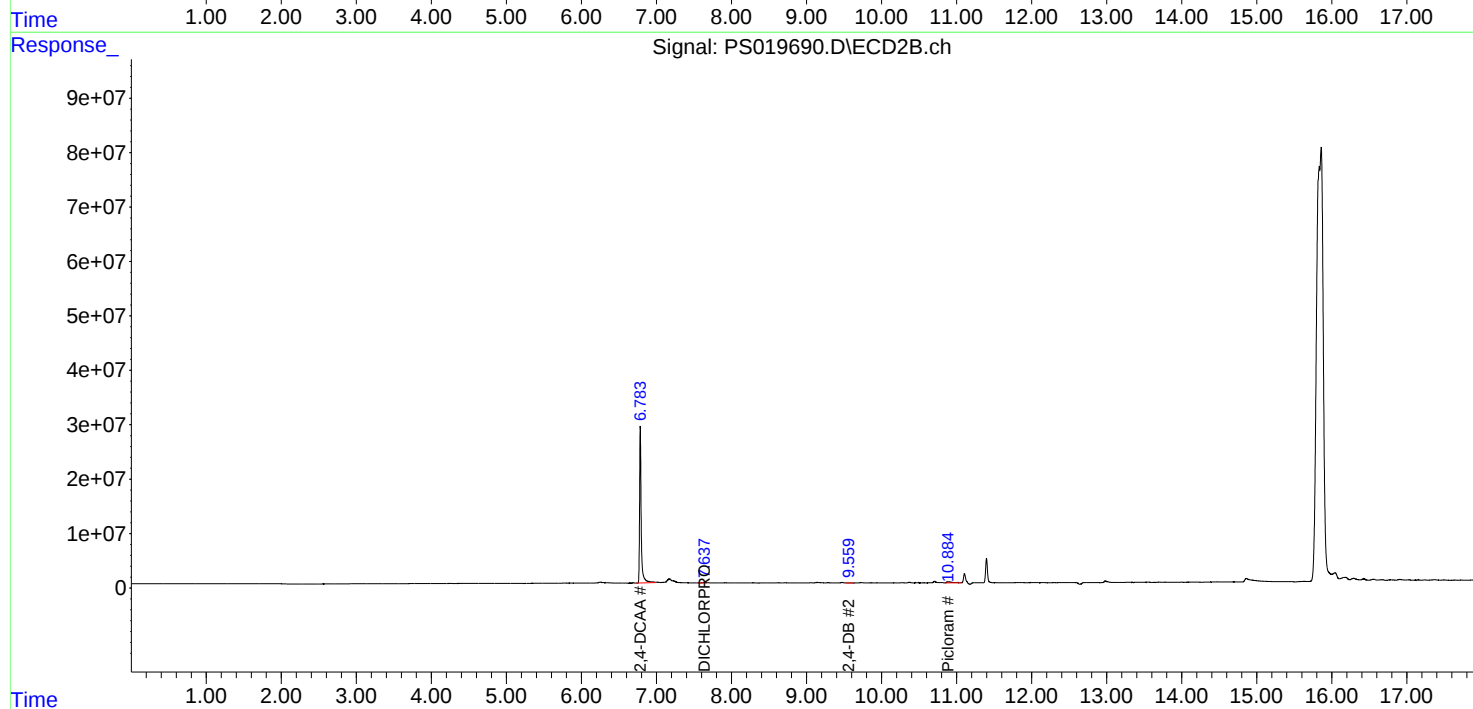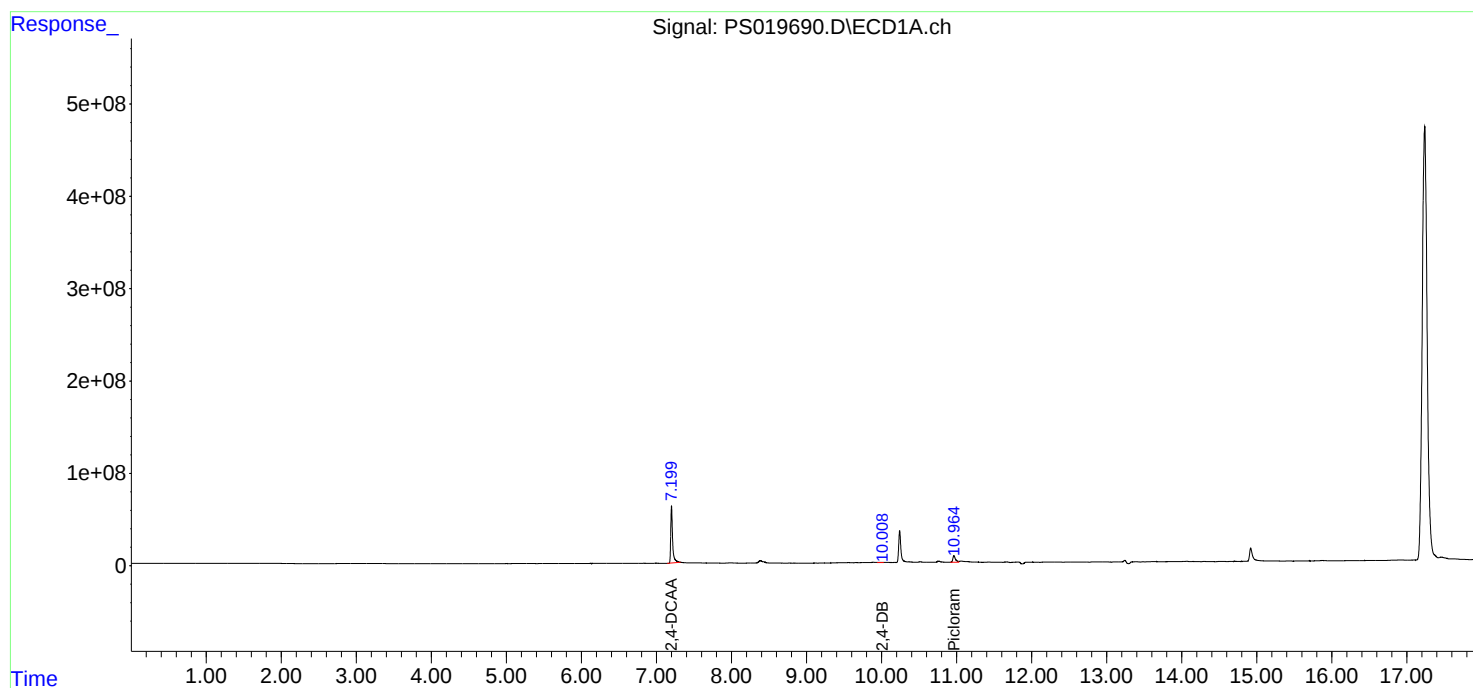


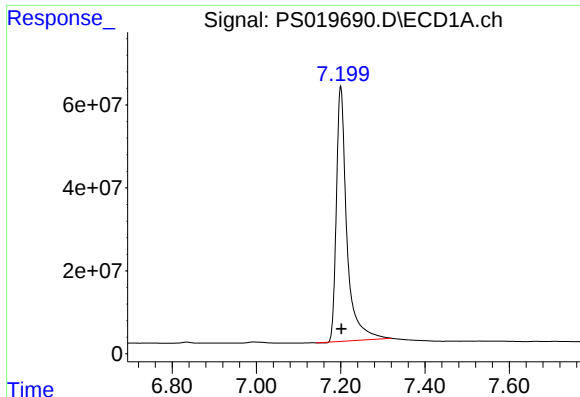

#4 2,4-DCAA


R.T.: 7.200 min
Delta R.T.: -0.002 min
Response: 1062134160
Conc: 442.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

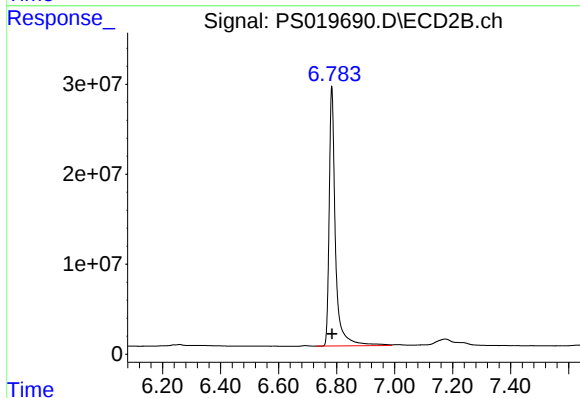


#4 2,4-DCAA

R.T.: 6.783 min
Delta R.T.: -0.001 min
Response: 434662307
Conc: 560.95 ng/ml

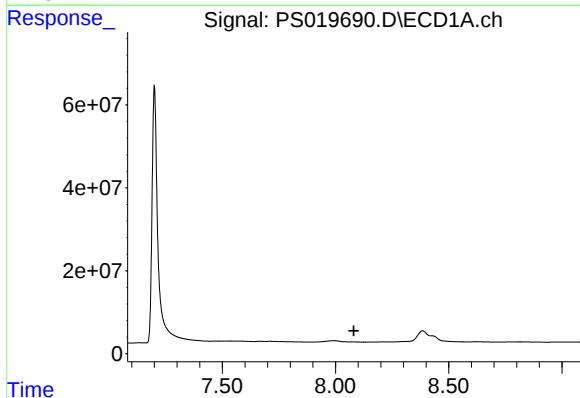


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.081 min
Response: 0
Conc: N.D.

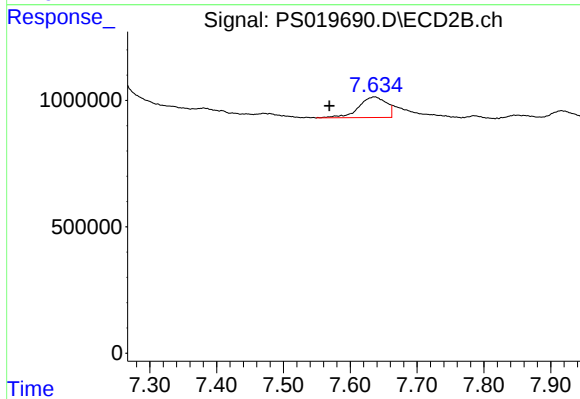

#8 DICHLORPROP


R.T.: 7.636 min
Delta R.T.: 0.067 min
Response: 2350718
Conc: 2.66 ng/ml

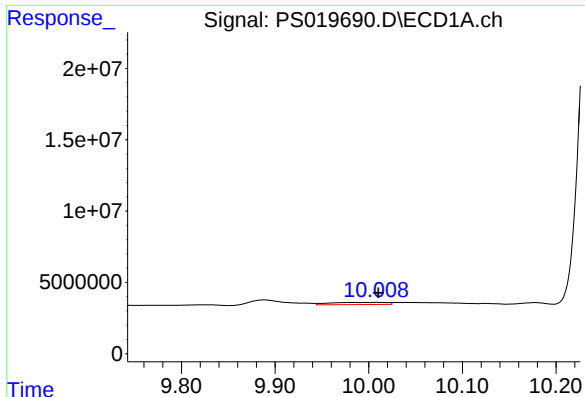

#13 2,4-DB


R.T.: 10.008 min
Delta R.T.: -0.003 min
Response: 6427130
Conc: 1.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

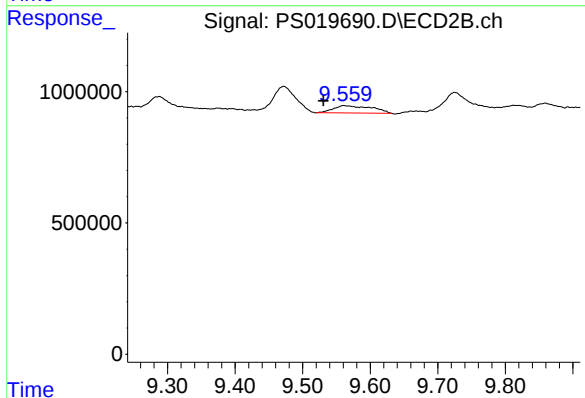


#13 2,4-DB

R.T.: 9.562 min
Delta R.T.: 0.031 min
Response: 1078375
Conc: 1.75 ng/ml

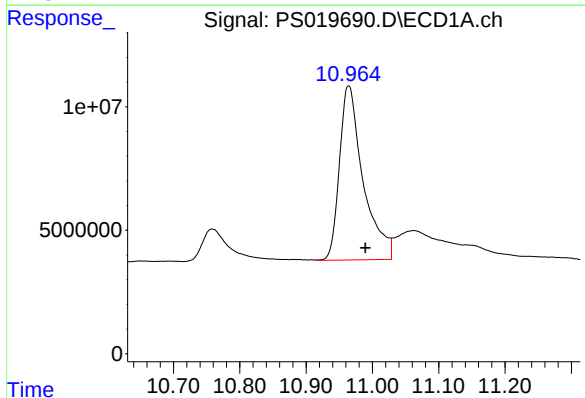

#15 Picloram

R.T.: 10.964 min
Delta R.T.: -0.025 min
Response: 175139880
Conc: 5.90 ng/ml

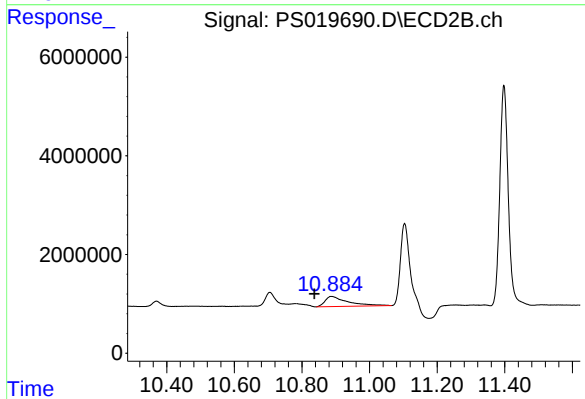

#15 Picloram

R.T.: 10.887 min
Delta R.T.: 0.050 min
Response: 9572502
Conc: 1.49 ng/ml