

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060922\
 Data File : PS019675.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2022 14:45
 Operator : AJ\MA
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 09:15:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.197	6.781	1824.3E6	620.1E6	760.397	800.285
Target Compounds							
1) T	Dalapon	3.013	2.526	3214.5E6	700.0E6	634.182	697.580
2) T	3,5-DICHL...	6.411	5.961	2266.6E6	905.7E6	717.127	755.550
3) T	4-Nitroph...	7.029	6.399	763.9E6	317.3E6	778.424	741.205
5) T	DICAMBA	7.387	6.945	6785.8E6	2604.9E6	714.467	762.007
6) T	MCPD	7.557	7.043	544.6E6	206.4E6	72.560	76.254
7) T	MCPA	7.705	7.255	767.0E6	286.1E6	70.992	74.455
8) T	DICHLORPROP	8.078	7.565	1796.6E6	666.1E6	701.619	754.057
9) T	2,4-D	8.308	7.856	2079.9E6	798.5E6	727.361	748.619
10) T	Pentachlo...	8.614	8.282	24569.2E6	8869.7E6	710.320	760.942
11) T	2,4,5-TP ...	9.164	8.642	11412.9E6	3832.2E6	726.890	762.296
12) T	2,4,5-T	9.449	9.020	13463.4E6	3590.4E6	715.389	763.391
13) T	2,4-DB	10.001	9.525	3043.2E6	475.4E6	752.154	769.251
14) T	DINOSEB	11.155	9.850	11725.3E6	2693.2E6	758.078	758.078
15) T	Picloram	10.980	10.832	21046.0E6	4398.7E6	709.161	683.848
16) T	DCPA	11.423	10.780	18488.8E6	4698.4E6	767.043	761.180



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060922\
Data File : PS019675.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2022 14:45
Operator : AJ\MA
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 09:15:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

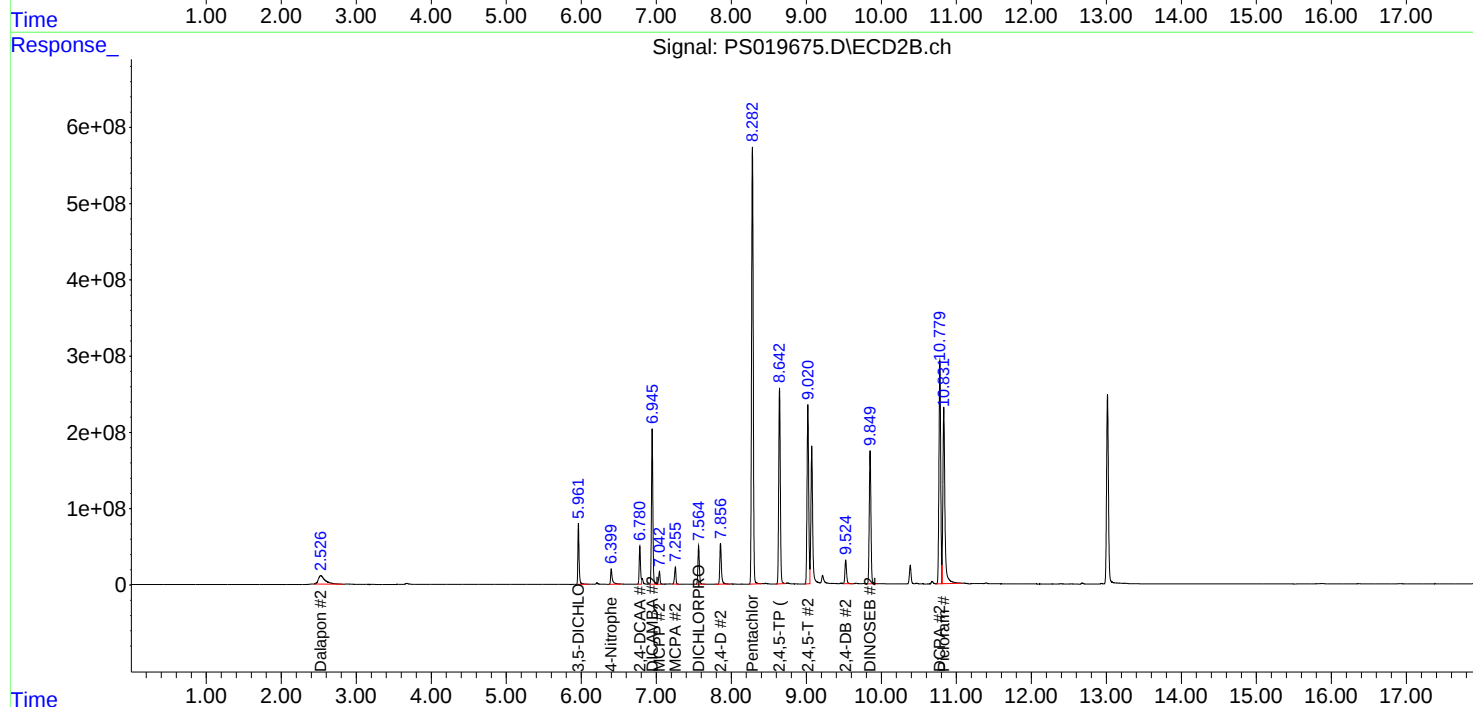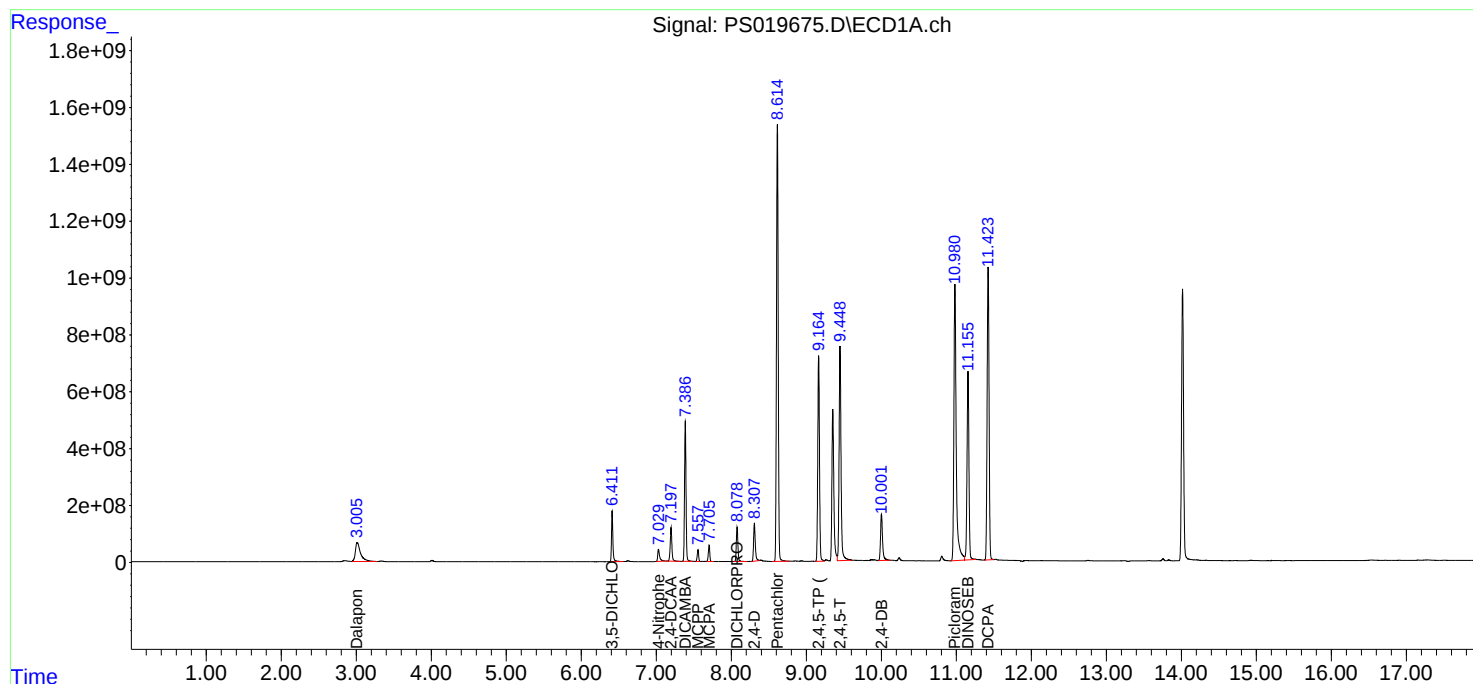


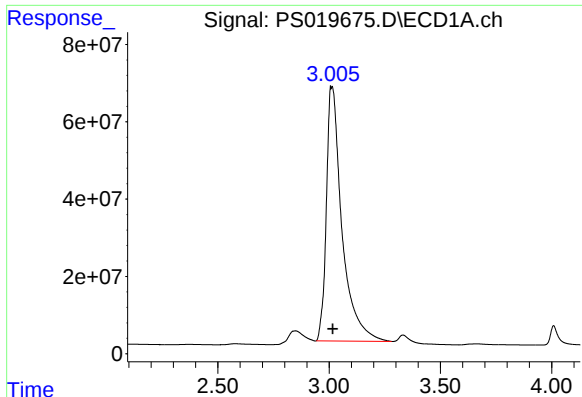

#1 Dalapon


R.T.: 3.013 min
Delta R.T.: -0.003 min
Response: 3214520362
Conc: 634.18 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

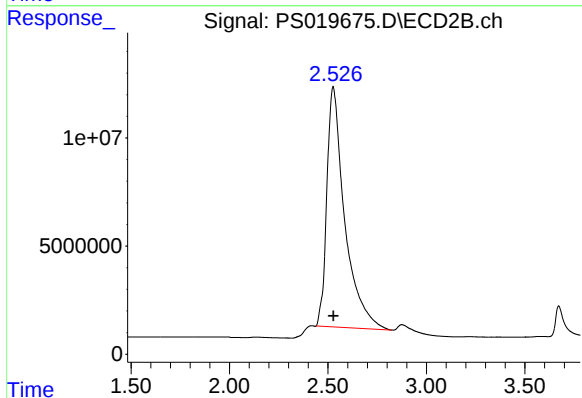


#1 Dalapon

R.T.: 2.526 min
Delta R.T.: -0.001 min
Response: 699981249
Conc: 697.58 ng/ml

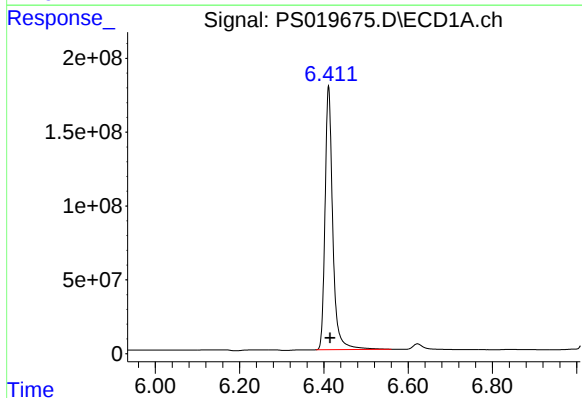


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.411 min
Delta R.T.: -0.003 min
Response: 2266576432
Conc: 717.13 ng/ml

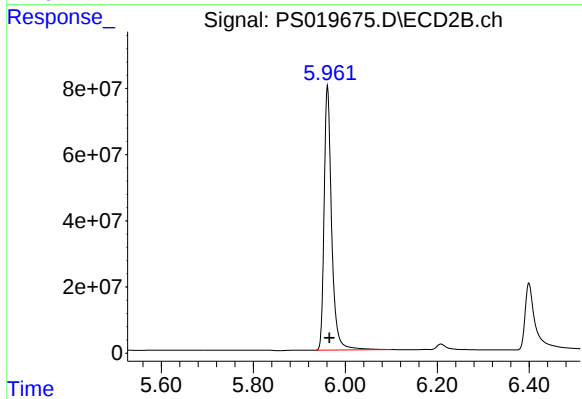

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.961 min
Delta R.T.: -0.004 min
Response: 905657973
Conc: 755.55 ng/ml

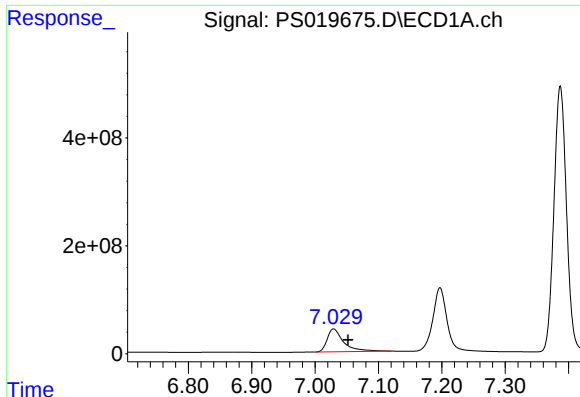

#3 4-Nitrophenol


R.T.: 7.029 min
Delta R.T.: -0.023 min
Response: 763881103
Conc: 778.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

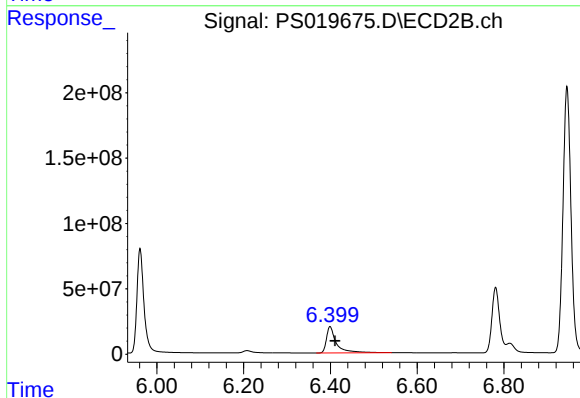


#3 4-Nitrophenol

R.T.: 6.399 min
Delta R.T.: -0.011 min
Response: 317262351
Conc: 741.20 ng/ml

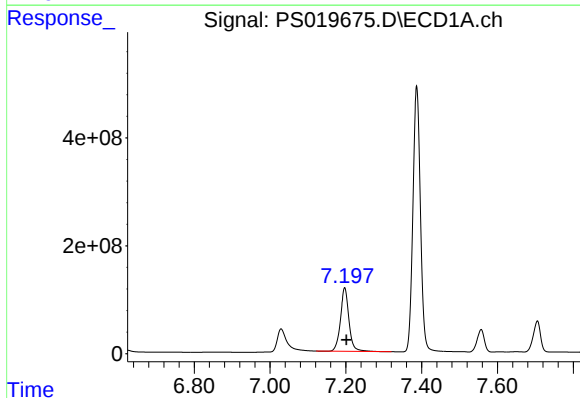


#4 2,4-DCAA

R.T.: 7.197 min
Delta R.T.: -0.005 min
Response: 1824319689
Conc: 760.40 ng/ml

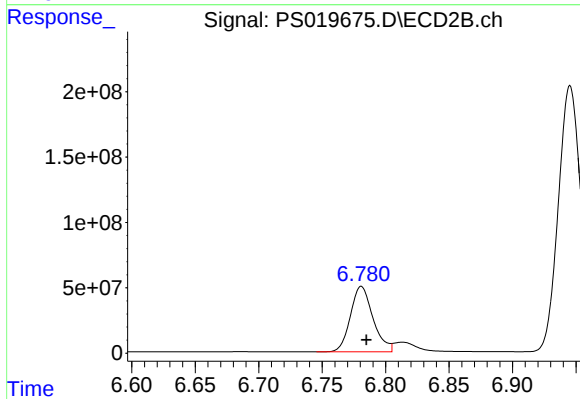

#4 2,4-DCAA


R.T.: 6.781 min
Delta R.T.: -0.004 min
Response: 620116840
Conc: 800.28 ng/ml

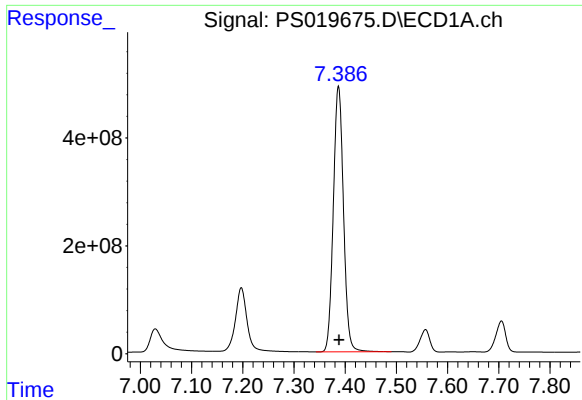

#5 DICAMBA


R.T.: 7.387 min
Delta R.T.: -0.002 min
Response: 6785832765
Conc: 714.47 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

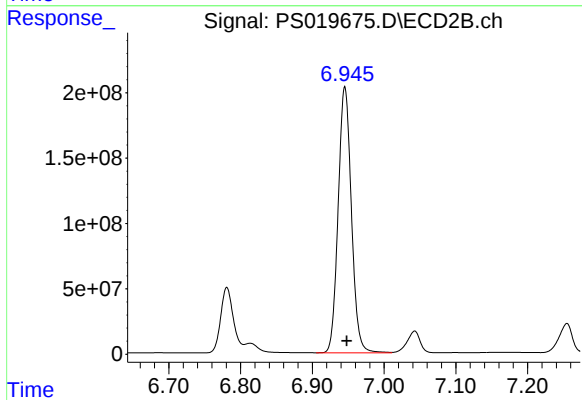


#5 DICAMBA

R.T.: 6.945 min
Delta R.T.: -0.002 min
Response: 2604879571
Conc: 762.01 ng/ml

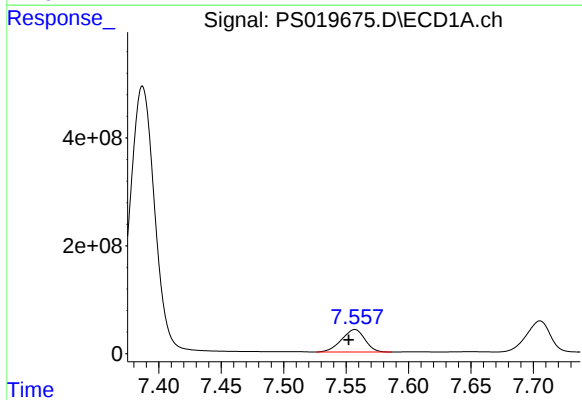


#6 MCP

R.T.: 7.557 min
Delta R.T.: 0.005 min
Response: 544603367
Conc: 72.56 ug/ml

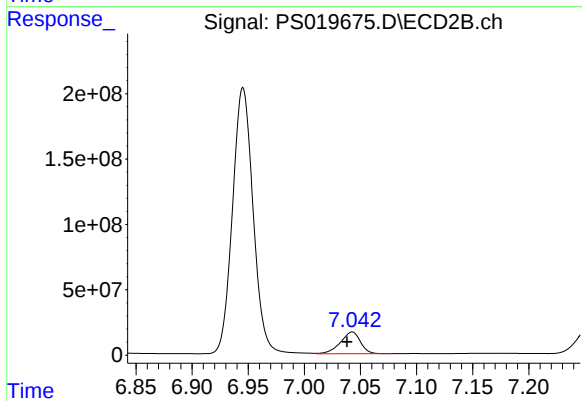

#6 MCP


R.T.: 7.043 min
Delta R.T.: 0.005 min
Response: 206420224
Conc: 76.25 ug/ml

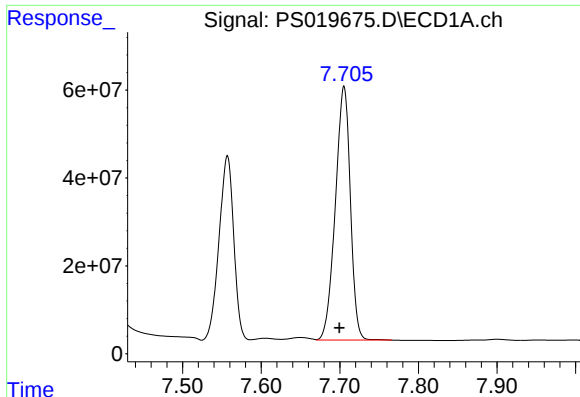

#7 MCPA


R.T.: 7.705 min
Delta R.T.: 0.006 min
Response: 766991820
Conc: 70.99 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

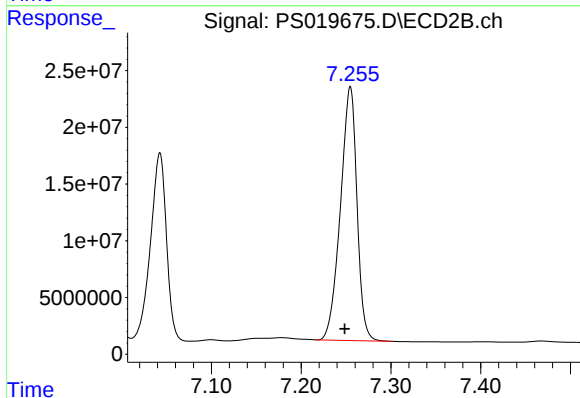


#7 MCPA

R.T.: 7.255 min
Delta R.T.: 0.006 min
Response: 286098050
Conc: 74.46 ug/ml

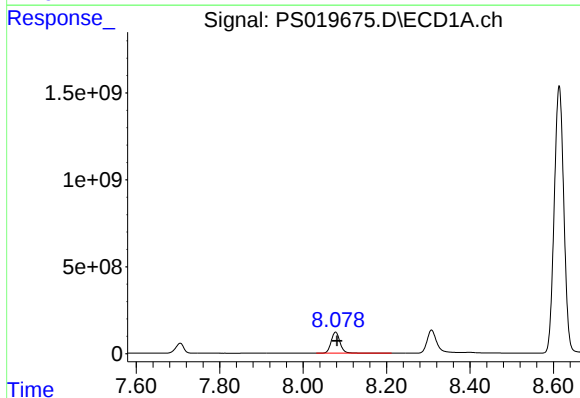


#8 DICHLORPROP

R.T.: 8.078 min
Delta R.T.: -0.003 min
Response: 1796574158
Conc: 701.62 ng/ml

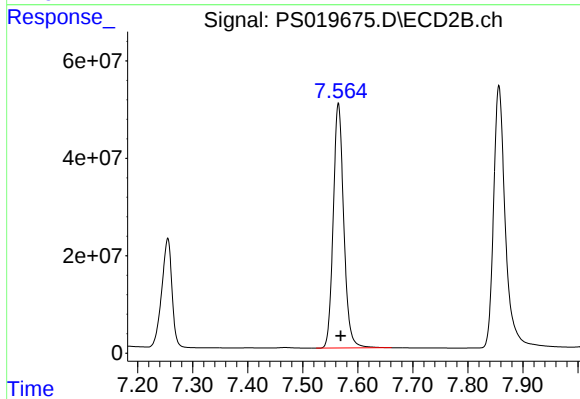

#8 DICHLORPROP


R.T.: 7.565 min
Delta R.T.: -0.004 min
Response: 666112568
Conc: 754.06 ng/ml

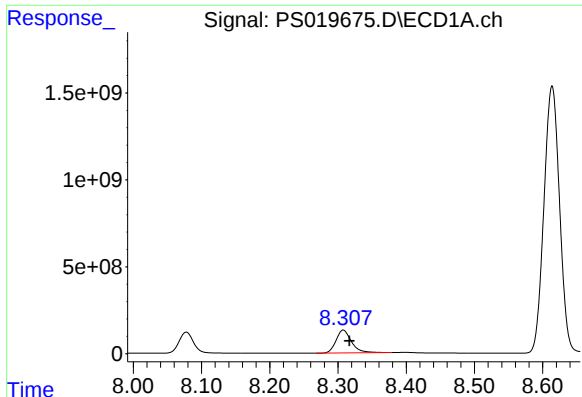

#9 2,4-D


R.T.: 8.308 min
Delta R.T.: -0.009 min
Response: 2079881671
Conc: 727.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

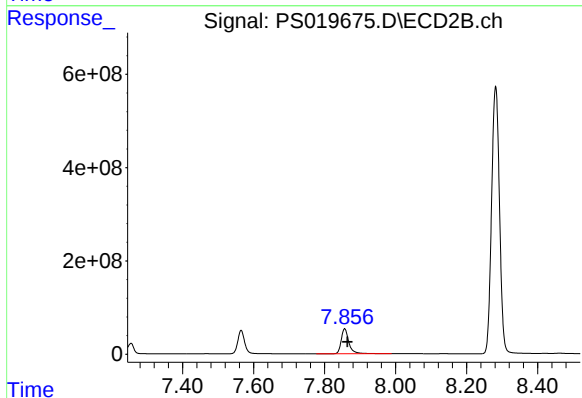


#9 2,4-D

R.T.: 7.856 min
Delta R.T.: -0.008 min
Response: 798497882
Conc: 748.62 ng/ml

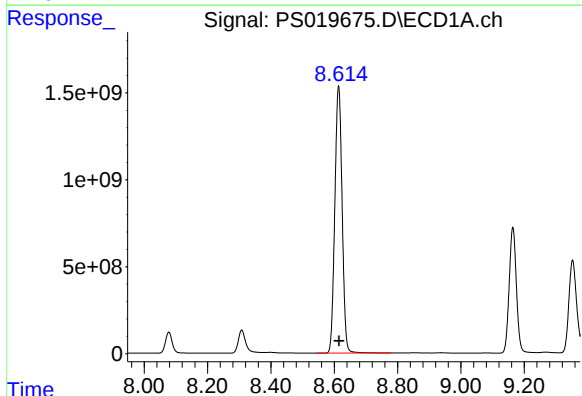


#10 Pentachlorophenol

R.T.: 8.614 min
Delta R.T.: -0.001 min
Response: 24569170161
Conc: 710.32 ng/ml

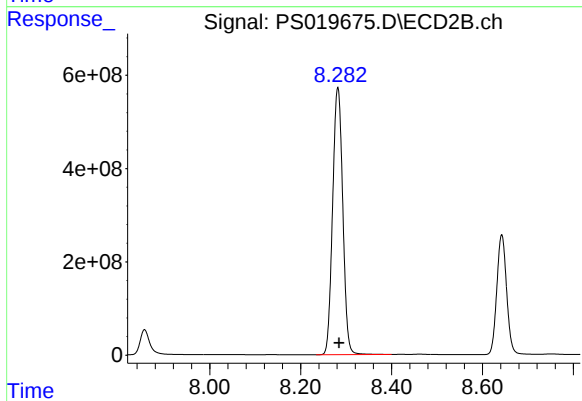

#10 Pentachlorophenol


R.T.: 8.282 min
Delta R.T.: -0.003 min
Response: 8869717321
Conc: 760.94 ng/ml

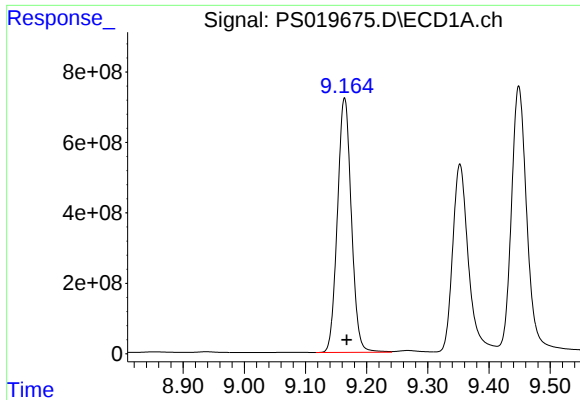

#11 2,4,5-TP (SILVEX)


R.T.: 9.164 min
Delta R.T.: -0.003 min
Response: 11412861890
Conc: 726.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

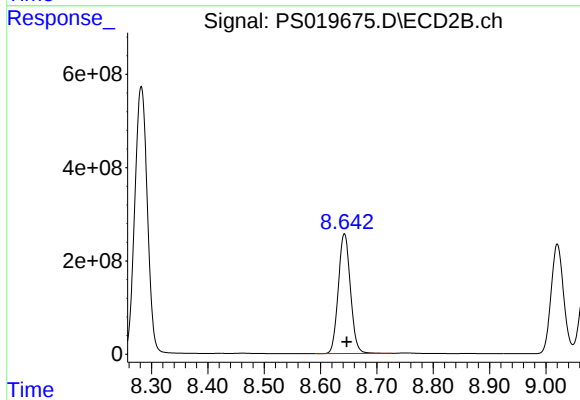


#11 2,4,5-TP (SILVEX)

R.T.: 8.642 min
Delta R.T.: -0.004 min
Response: 3832189249
Conc: 762.30 ng/ml

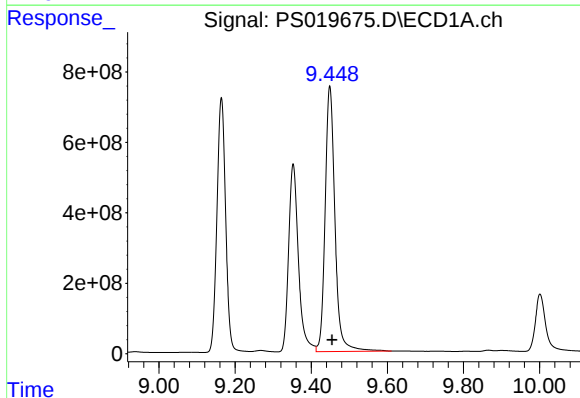


#12 2,4,5-T

R.T.: 9.449 min
Delta R.T.: -0.006 min
Response: 13463376414
Conc: 715.39 ng/ml

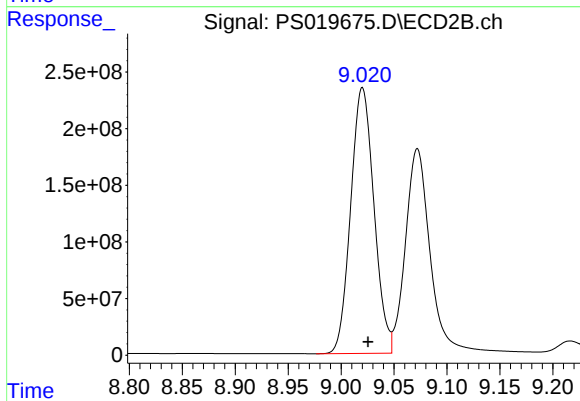

#12 2,4,5-T


R.T.: 9.020 min
Delta R.T.: -0.005 min
Response: 3590384844
Conc: 763.39 ng/ml

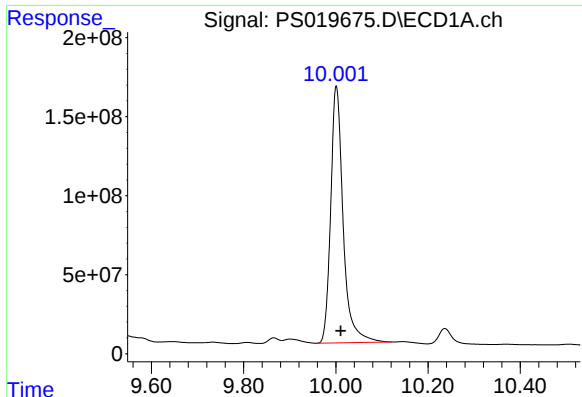

#13 2,4-DB


R.T.: 10.001 min
Delta R.T.: -0.009 min
Response: 3043229832
Conc: 752.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

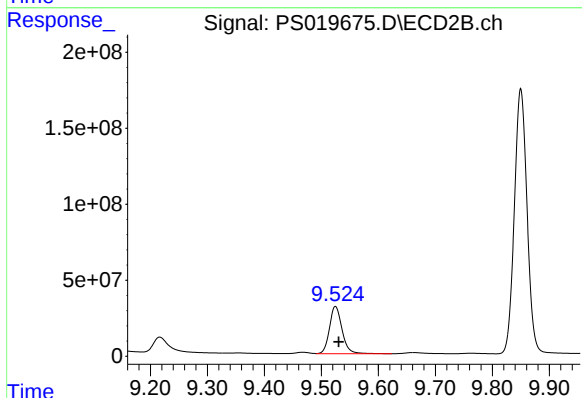


#13 2,4-DB

R.T.: 9.525 min
Delta R.T.: -0.006 min
Response: 475370011
Conc: 769.25 ng/ml

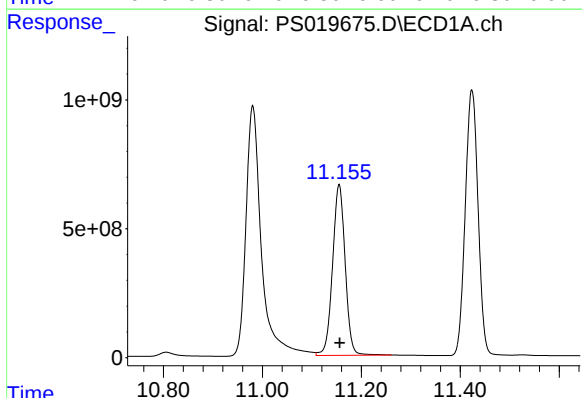


#14 DINOSEB

R.T.: 11.155 min
Delta R.T.: -0.001 min
Response: 11725312047
Conc: 758.08 ng/ml

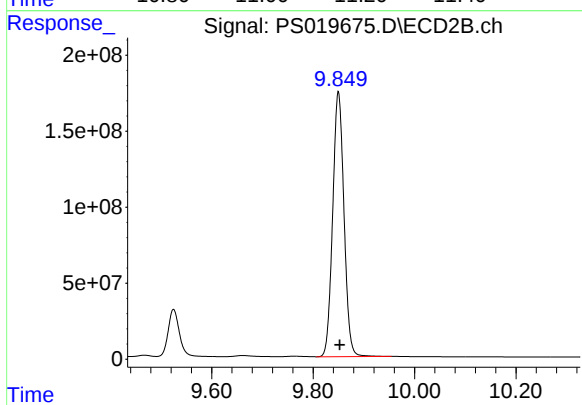

#14 DINOSEB


R.T.: 9.850 min
Delta R.T.: -0.003 min
Response: 2693163286
Conc: 758.08 ng/ml

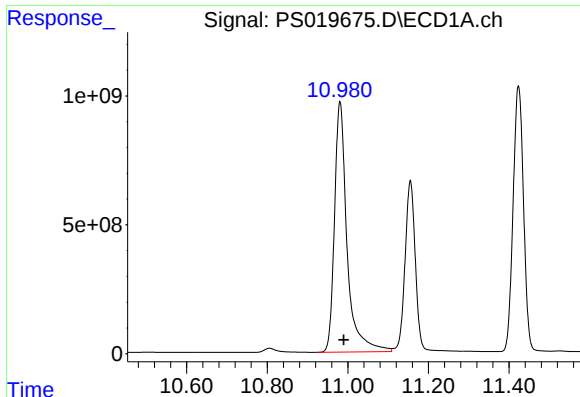

#15 Picloram


R.T.: 10.980 min
Delta R.T.: -0.009 min
Response: 21045952444
Conc: 709.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

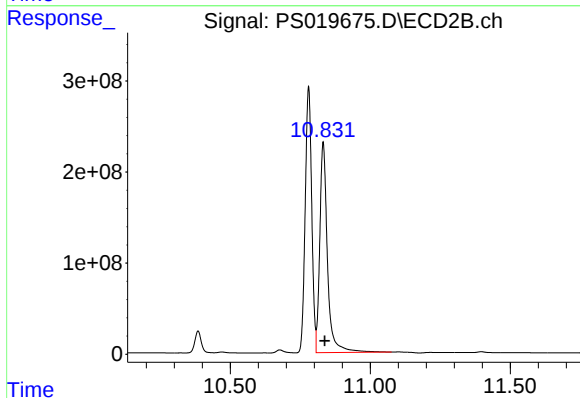


#15 Picloram

R.T.: 10.832 min
Delta R.T.: -0.006 min
Response: 4398686981
Conc: 683.85 ng/ml

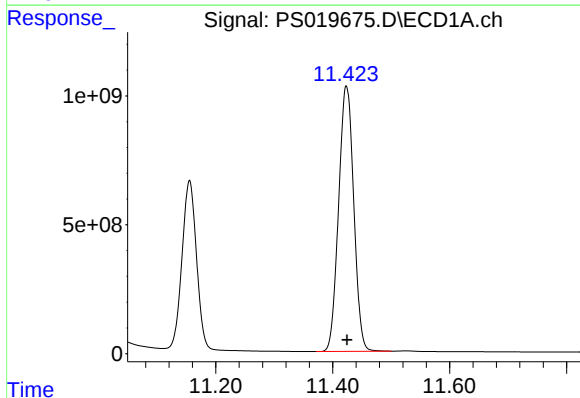

#16 DCPA

R.T.: 11.423 min
Delta R.T.: -0.001 min
Response: 18488822120
Conc: 767.04 ng/ml

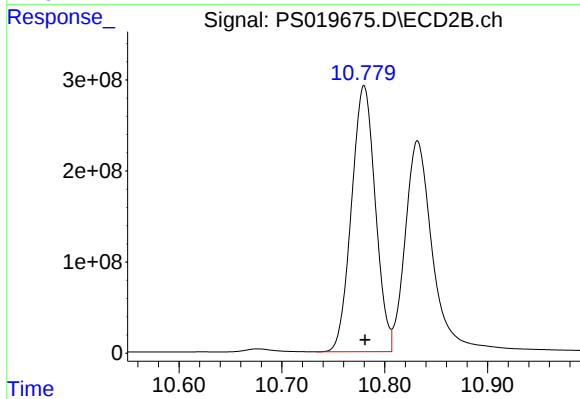

#16 DCPA

R.T.: 10.780 min
Delta R.T.: 0.000 min
Response: 4698371614
Conc: 761.18 ng/ml