

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060922\
 Data File : PS019688.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2022 22:21
 Operator : AJ\MA
 Sample : PB145449BSD
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB145449BSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 04:13:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.197	6.782	1260.1E6	415.1E6	525.225	535.638
Target Compounds							
1) T	Dalapon	3.013	2.526	2292.8E6	474.5E6	452.336	472.879
2) T	3,5-DICHL...	6.411	5.962	1548.5E6	613.5E6	489.929	511.812
3) T	4-Nitroph...	7.032	6.402	501.4E6	211.6E6	510.958	494.388
5) T	DICAMBA	7.386	6.945	4729.8E6	1792.0E6	497.987	524.219
6) T	MCPD	7.553	7.040	356.3E6	136.9E6	47.477	50.577
7) T	MCPA	7.701	7.251	512.8E6	191.4E6	47.467	49.824
8) T	DICHLORPROP	8.077	7.566	1242.0E6	452.0E6	485.045	511.671
9) T	2,4-D	8.309	7.858	1391.8E6	542.2E6	486.728	508.335
10) T	Pentachlo...	8.613	8.282	17799.3E6	6362.6E6	514.597	545.854
11) T	2,4,5-TP ...	9.164	8.643	7930.8E6	2666.2E6	505.114	530.351
12) T	2,4,5-T	9.450	9.021	9470.8E6	2466.6E6	503.242	524.445
13) T	2,4-DB	10.003	9.527	2019.1E6	314.4E6	499.025	508.726
14) T	DINOSEB	11.154	9.850	8335.3E6	1852.3E6	538.904	521.391
15) T	Picloram	10.983	10.834	15249.8E6	3124.9E6	513.855	485.823
16) T	DCPA	11.423	10.780	13280.4E6	3302.2E6	550.963	534.993



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060922\
Data File : PS019688.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2022 22:21
Operator : AJ\MA
Sample : PB145449BSD
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB145449BSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 04:13:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

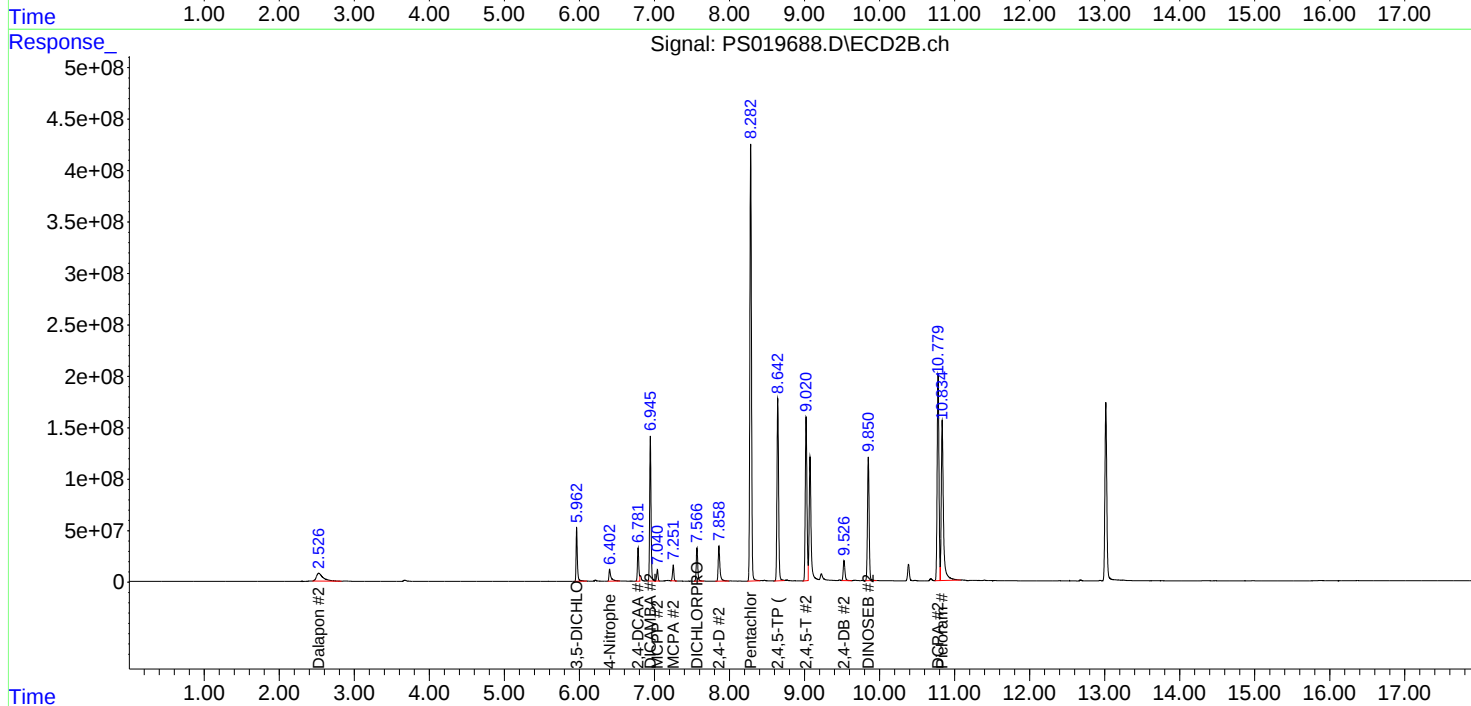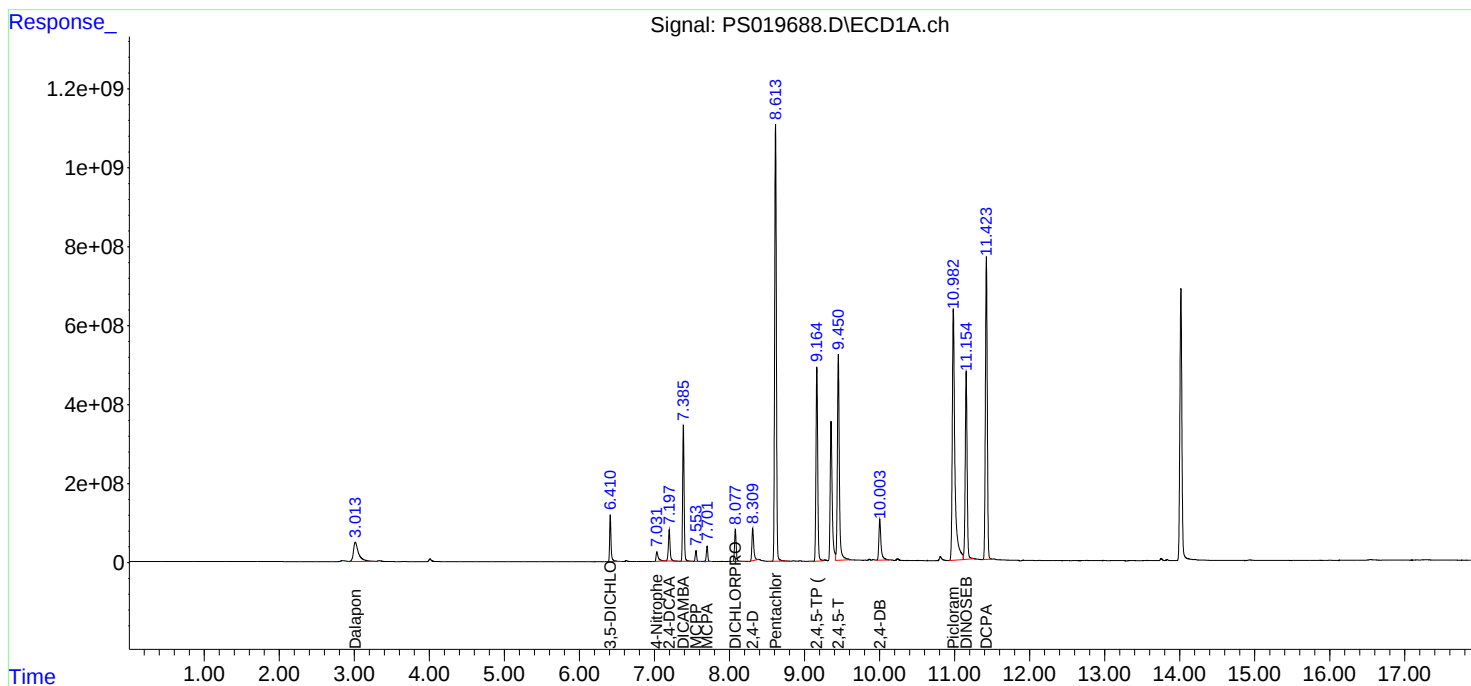


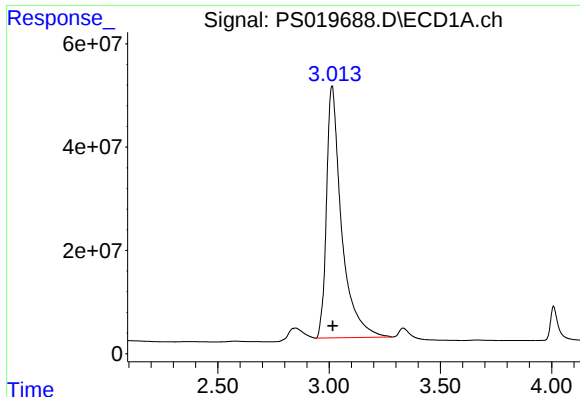

#1 Dalapon


R.T.: 3.013 min
Delta R.T.: -0.003 min
Response: 2292782685
Conc: 452.34 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB145449BSD

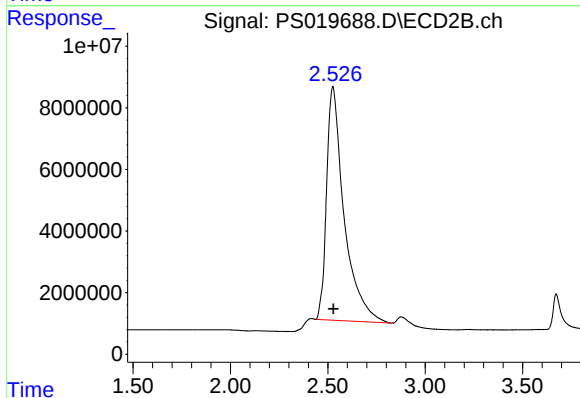


#1 Dalapon

R.T.: 2.526 min
Delta R.T.: -0.002 min
Response: 474506925
Conc: 472.88 ng/ml

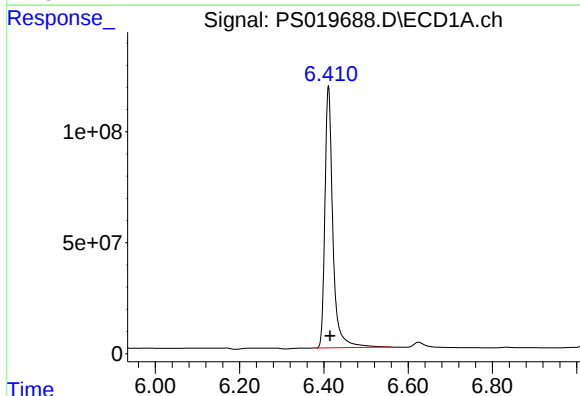


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.411 min
Delta R.T.: -0.004 min
Response: 1548487008
Conc: 489.93 ng/ml

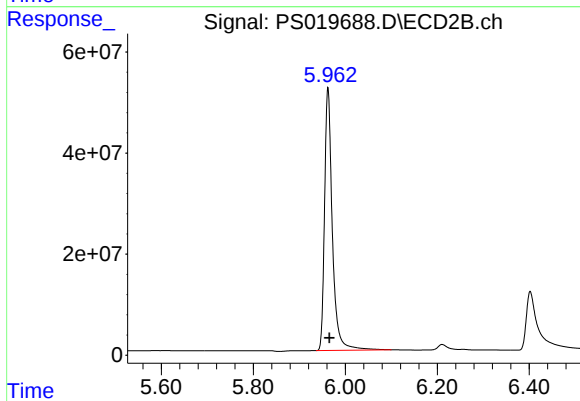

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.962 min
Delta R.T.: -0.003 min
Response: 613495199
Conc: 511.81 ng/ml

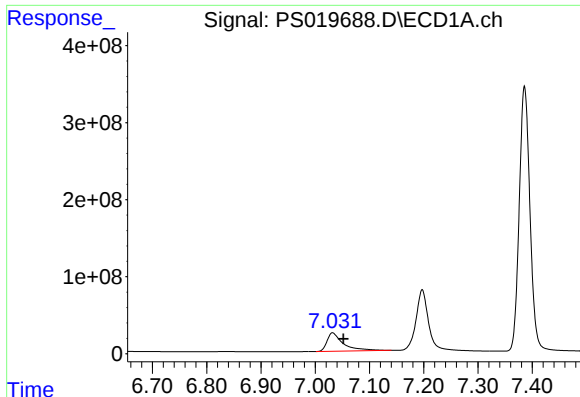

#3 4-Nitrophenol


R.T.: 7.032 min
Delta R.T.: -0.020 min
Response: 501411721
Conc: 510.96 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB145449BSD

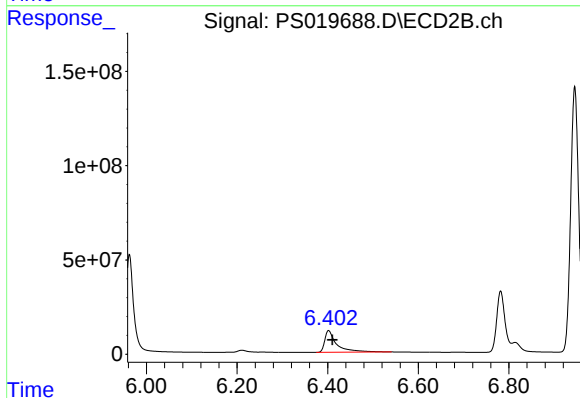


#3 4-Nitrophenol

R.T.: 6.402 min
Delta R.T.: -0.008 min
Response: 211615813
Conc: 494.39 ng/ml

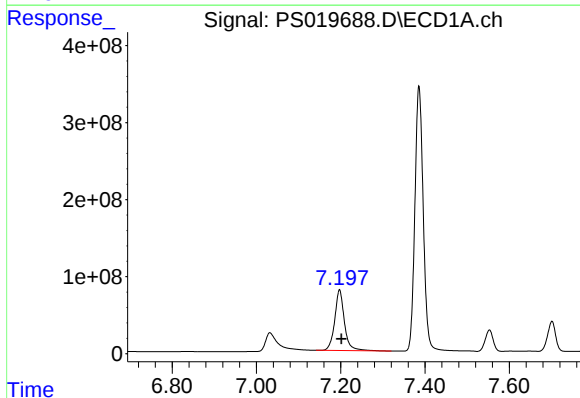


#4 2,4-DCAA

R.T.: 7.197 min
Delta R.T.: -0.005 min
Response: 1260102871
Conc: 525.23 ng/ml

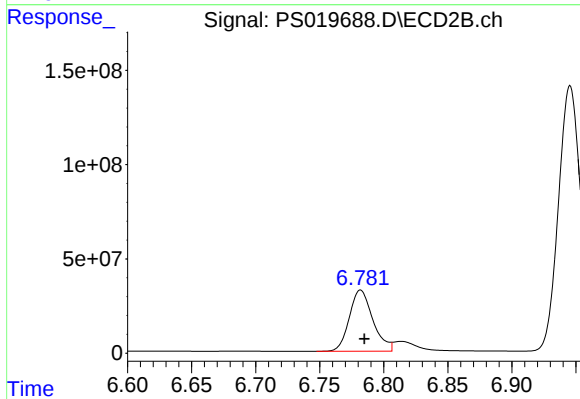

#4 2,4-DCAA


R.T.: 6.782 min
Delta R.T.: -0.003 min
Response: 415050398
Conc: 535.64 ng/ml

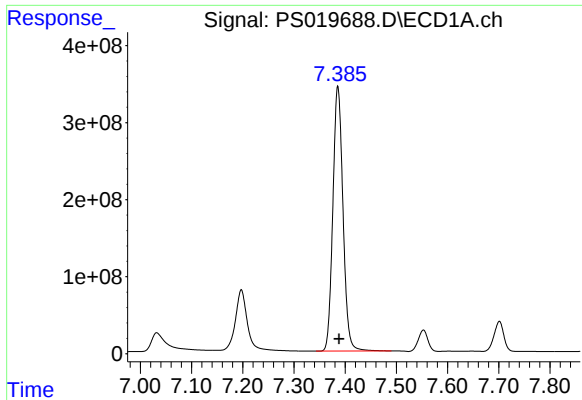

#5 DICAMBA


R.T.: 7.386 min
Delta R.T.: -0.003 min
Response: 4729757956
Conc: 497.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB145449BSD

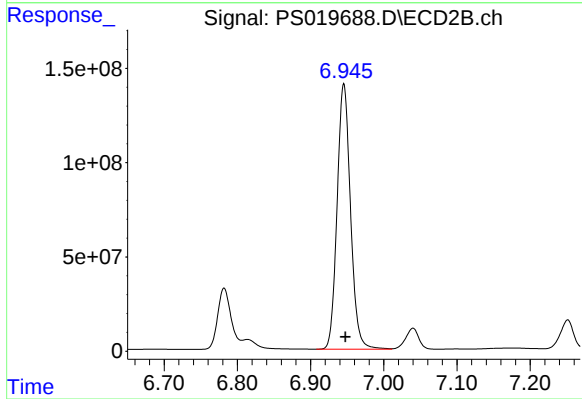


#5 DICAMBA

R.T.: 6.945 min
Delta R.T.: -0.002 min
Response: 1792014735
Conc: 524.22 ng/ml

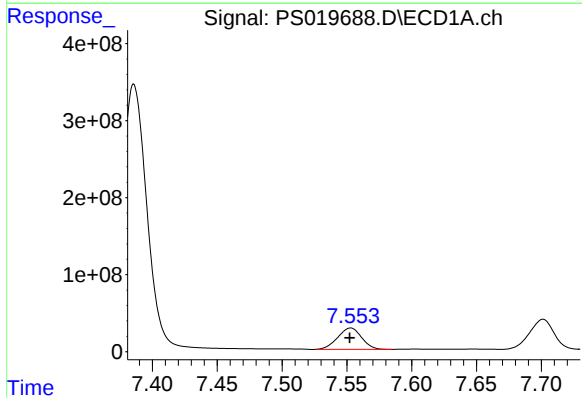


#6 MCP

R.T.: 7.553 min
Delta R.T.: 0.000 min
Response: 356339330
Conc: 47.48 ug/ml

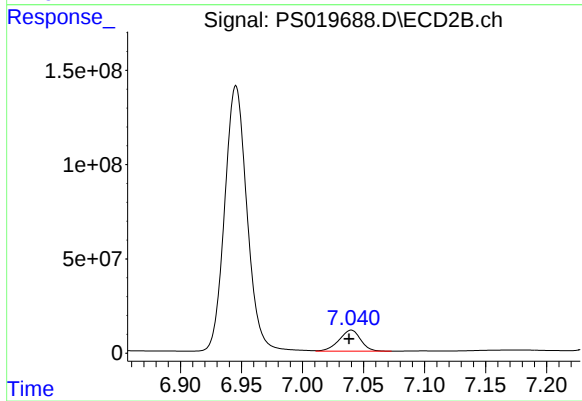

#6 MCP


R.T.: 7.040 min
Delta R.T.: 0.002 min
Response: 136912181
Conc: 50.58 ug/ml

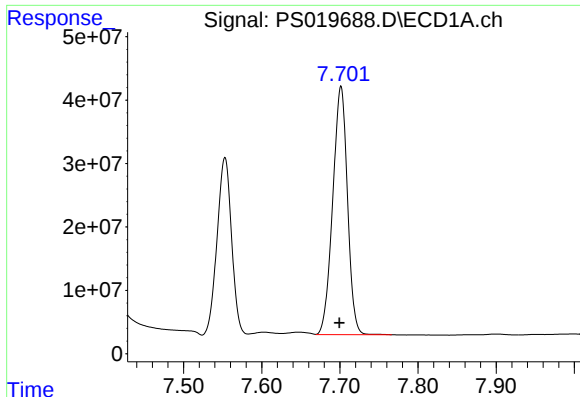

#7 MCPA


R.T.: 7.701 min
Delta R.T.: 0.002 min
Response: 512830106
Conc: 47.47 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB145449BSD

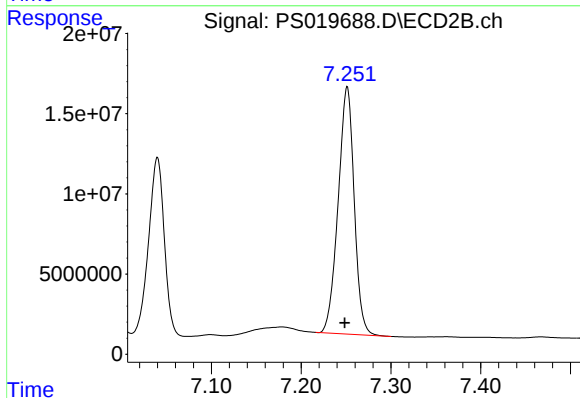


#7 MCPA

R.T.: 7.251 min
Delta R.T.: 0.003 min
Response: 191449561
Conc: 49.82 ug/ml

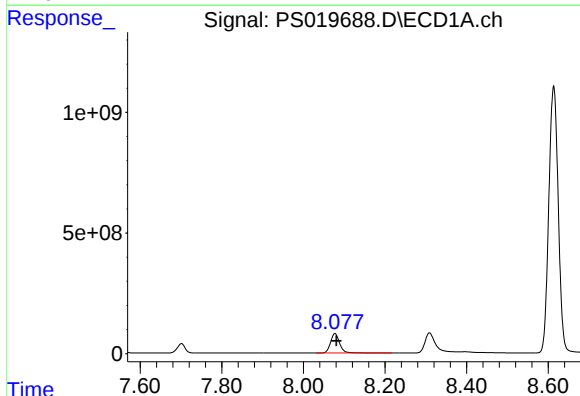


#8 DICHLORPROP

R.T.: 8.077 min
Delta R.T.: -0.004 min
Response: 1242011665
Conc: 485.05 ng/ml

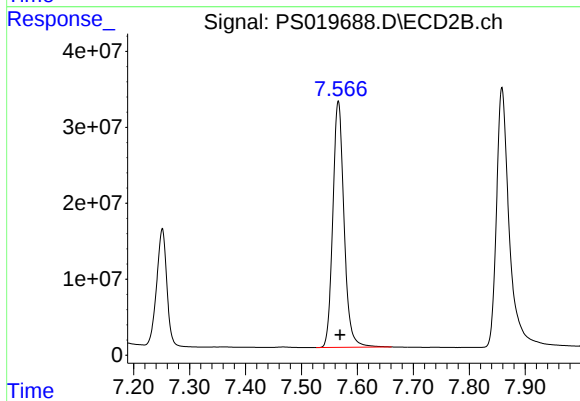

#8 DICHLORPROP


R.T.: 7.566 min
Delta R.T.: -0.003 min
Response: 451995888
Conc: 511.67 ng/ml

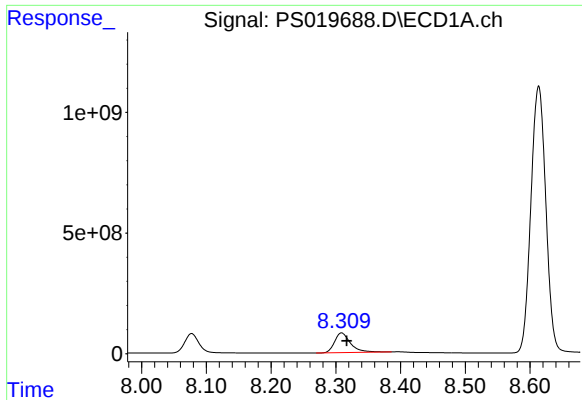

#9 2,4-D


R.T.: 8.309 min
Delta R.T.: -0.008 min
Response: 1391794444
Conc: 486.73 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB145449BSD

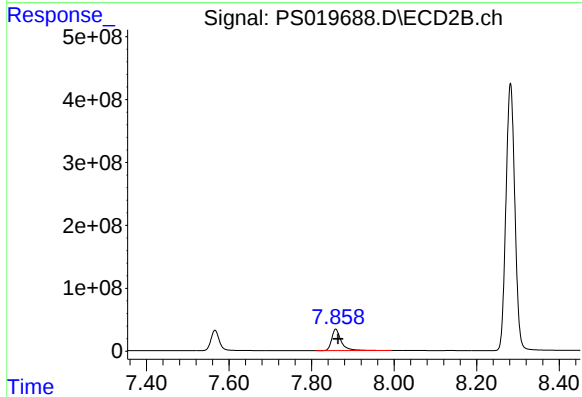


#9 2,4-D

R.T.: 7.858 min
Delta R.T.: -0.006 min
Response: 542204602
Conc: 508.34 ng/ml

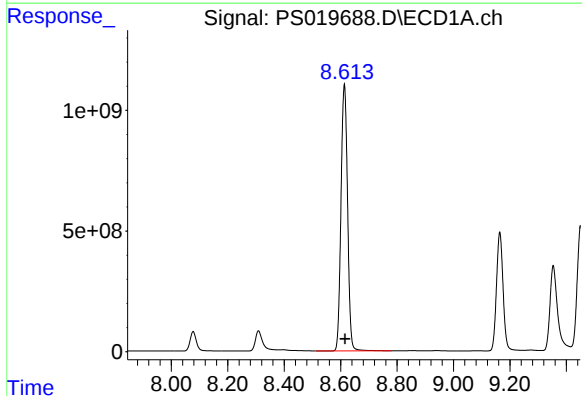


#10 Pentachlorophenol

R.T.: 8.613 min
Delta R.T.: -0.002 min
Response: 17799341925
Conc: 514.60 ng/ml

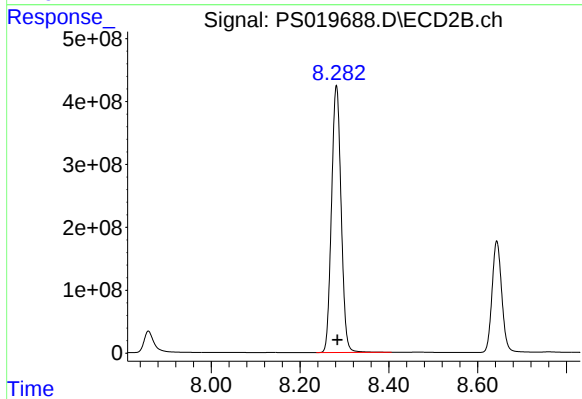

#10 Pentachlorophenol


R.T.: 8.282 min
Delta R.T.: -0.002 min
Response: 6362608319
Conc: 545.85 ng/ml

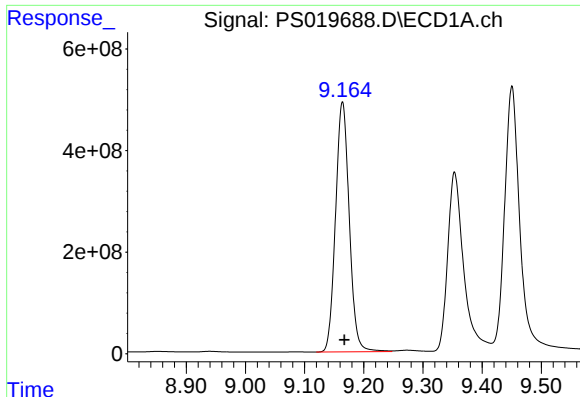

#11 2,4,5-TP (SILVEX)


R.T.: 9.164 min
Delta R.T.: -0.003 min
Response: 7930772939
Conc: 505.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB145449BSD

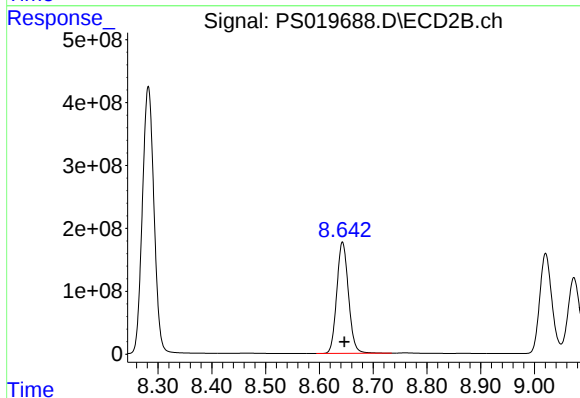


#11 2,4,5-TP (SILVEX)

R.T.: 8.643 min
Delta R.T.: -0.004 min
Response: 2666163790
Conc: 530.35 ng/ml

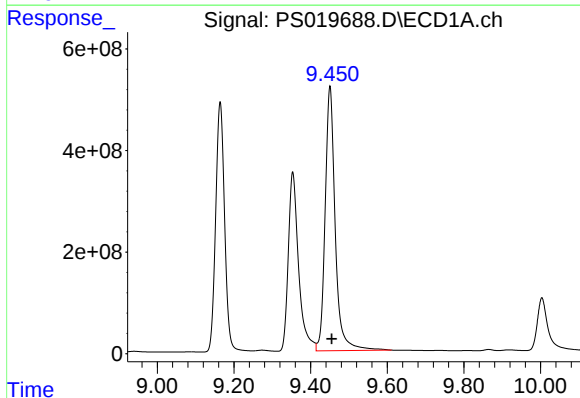


#12 2,4,5-T

R.T.: 9.450 min
Delta R.T.: -0.005 min
Response: 9470844785
Conc: 503.24 ng/ml

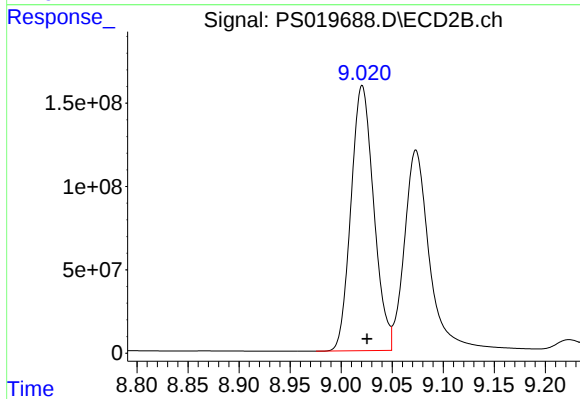

#12 2,4,5-T


R.T.: 9.021 min
Delta R.T.: -0.005 min
Response: 2466573260
Conc: 524.44 ng/ml

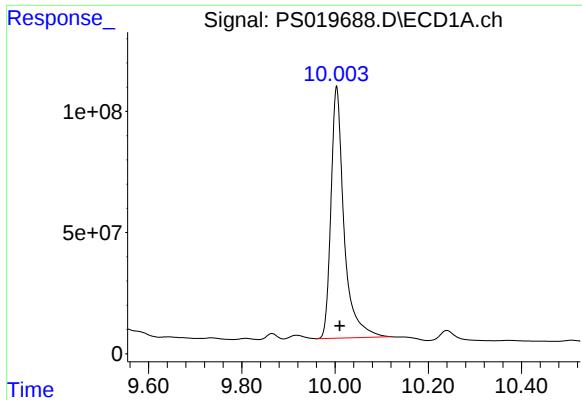

#13 2,4-DB


R.T.: 10.003 min
Delta R.T.: -0.007 min
Response: 2019065930
Conc: 499.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB145449BSD

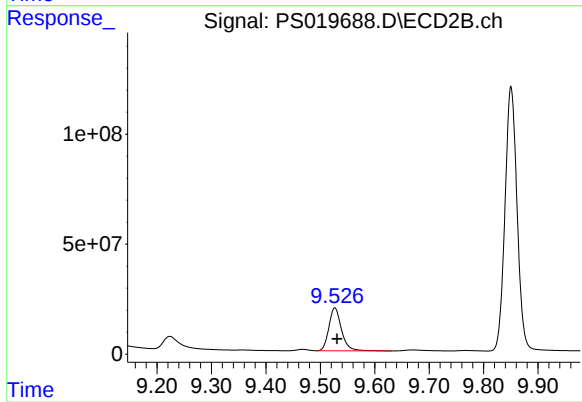


#13 2,4-DB

R.T.: 9.527 min
Delta R.T.: -0.004 min
Response: 314374931
Conc: 508.73 ng/ml

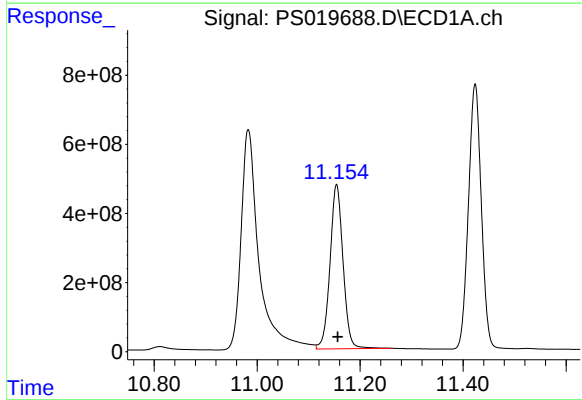


#14 DINOSEB

R.T.: 11.154 min
Delta R.T.: -0.002 min
Response: 8335313324
Conc: 538.90 ng/ml

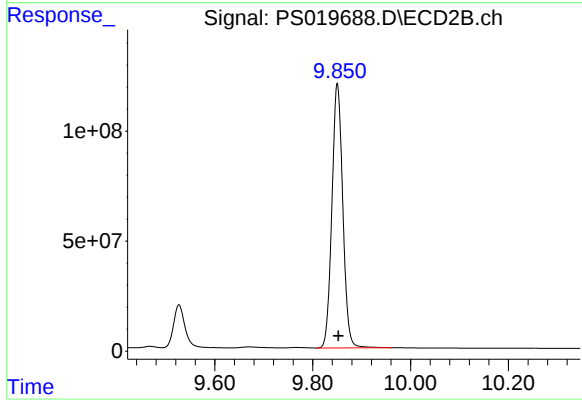

#14 DINOSEB


R.T.: 9.850 min
Delta R.T.: -0.002 min
Response: 1852303170
Conc: 521.39 ng/ml

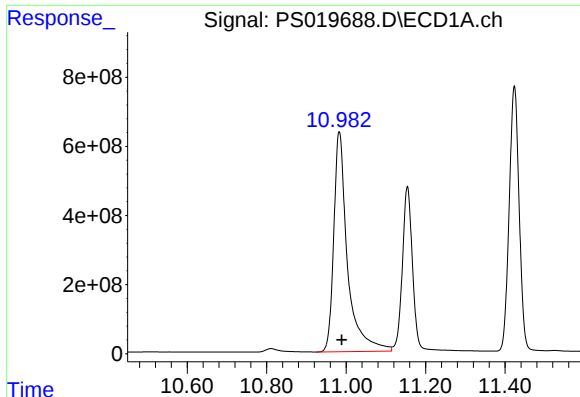

#15 Picloram


R.T.: 10.983 min
Delta R.T.: -0.007 min
Response: 15249802354
Conc: 513.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB145449BSD

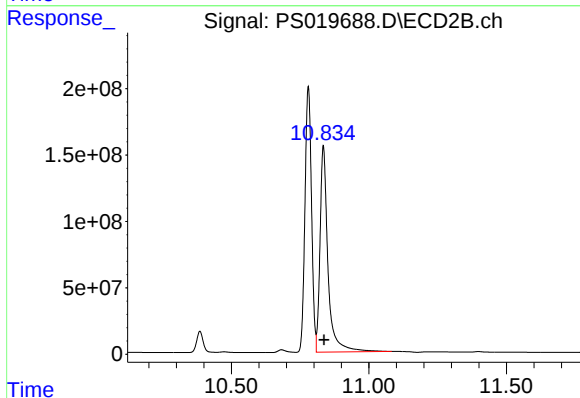


#15 Picloram

R.T.: 10.834 min
Delta R.T.: -0.003 min
Response: 3124937374
Conc: 485.82 ng/ml

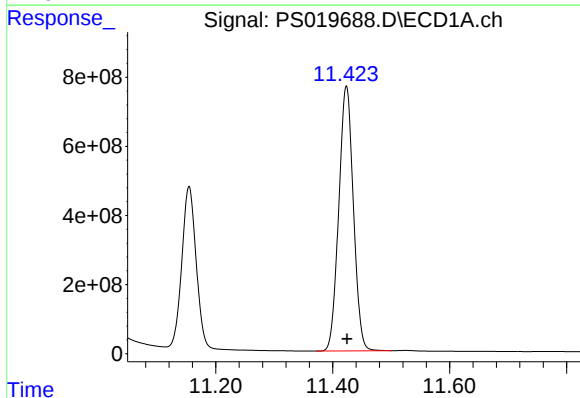

#16 DCPA

R.T.: 11.423 min
Delta R.T.: -0.001 min
Response: 13280415118
Conc: 550.96 ng/ml

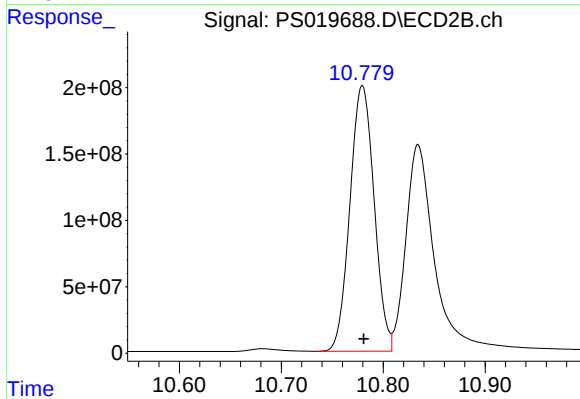

#16 DCPA

R.T.: 10.780 min
Delta R.T.: -0.001 min
Response: 3302237613
Conc: 534.99 ng/ml