

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060923\
 Data File : PS023258.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2023 09:06
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 21:12:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
3) T	4-Nitroph...	6.313	0.000	7800609	0	6.052	N.D. #
6) T	MCCP	6.753	0.000	323904	0	<MDL	N.D. #
7) T	MCPA	0.000	7.311	0	6395330	N.D.	2.380
8) T	DICHLORPROP	7.187f	7.660	9793071	839012	4.746	1.356 #
9) T	2,4-D	0.000	7.875f	0	1101833	N.D.	1.589
11) T	2,4,5-TP ...	8.186	0.000	5256025	0	<MDL	N.D. #
12) T	2,4,5-T	8.488	9.140f	1896632	1076850	<MDL	<MDL #
13) T	2,4-DB	8.939f	0.000	8164964	0	3.468	N.D. #
14) T	DINOSEB	10.116f	0.000	313785	0	<MDL	N.D. #
15) T	Picloram	9.894	10.897	27288789	8779328	1.572	1.924
16) T	DCPA	10.326	10.897	673061	8779328	<MDL	2.188 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060923\
Data File : PS023258.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2023 09:06
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 21:12:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

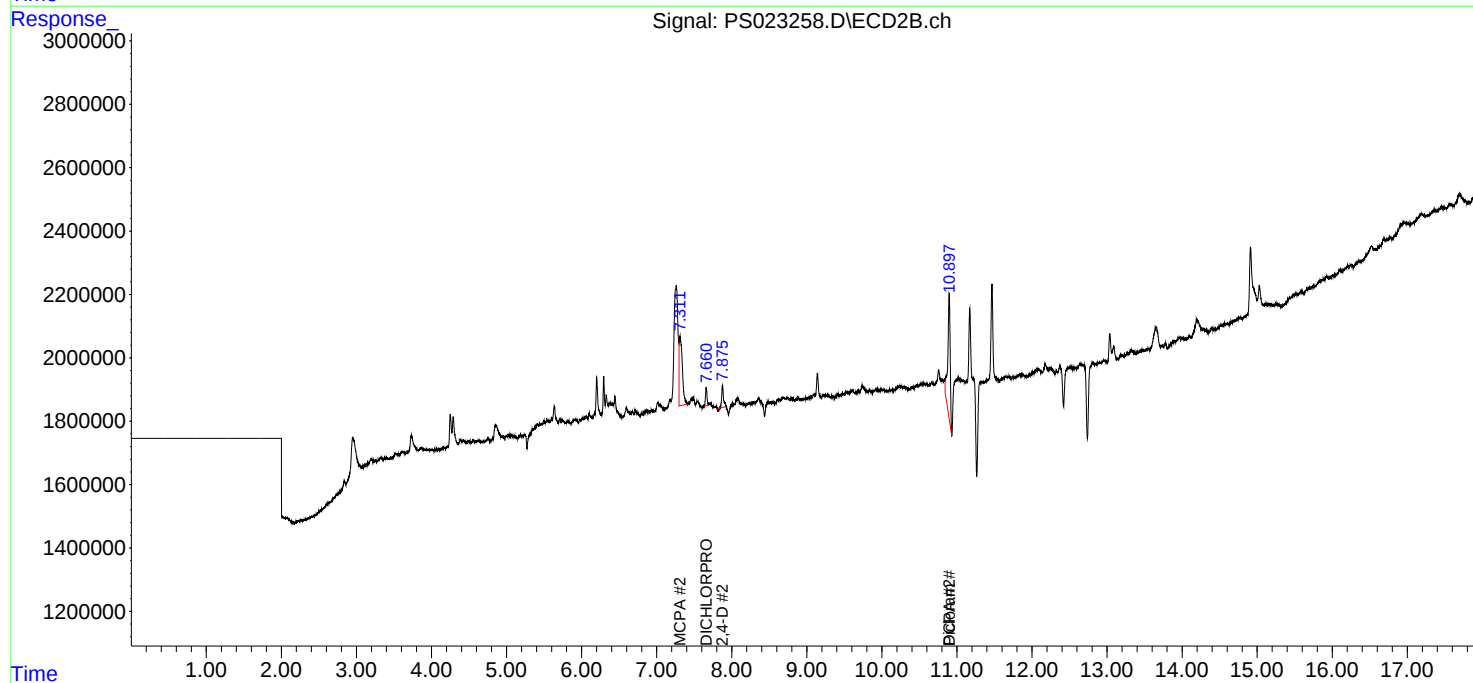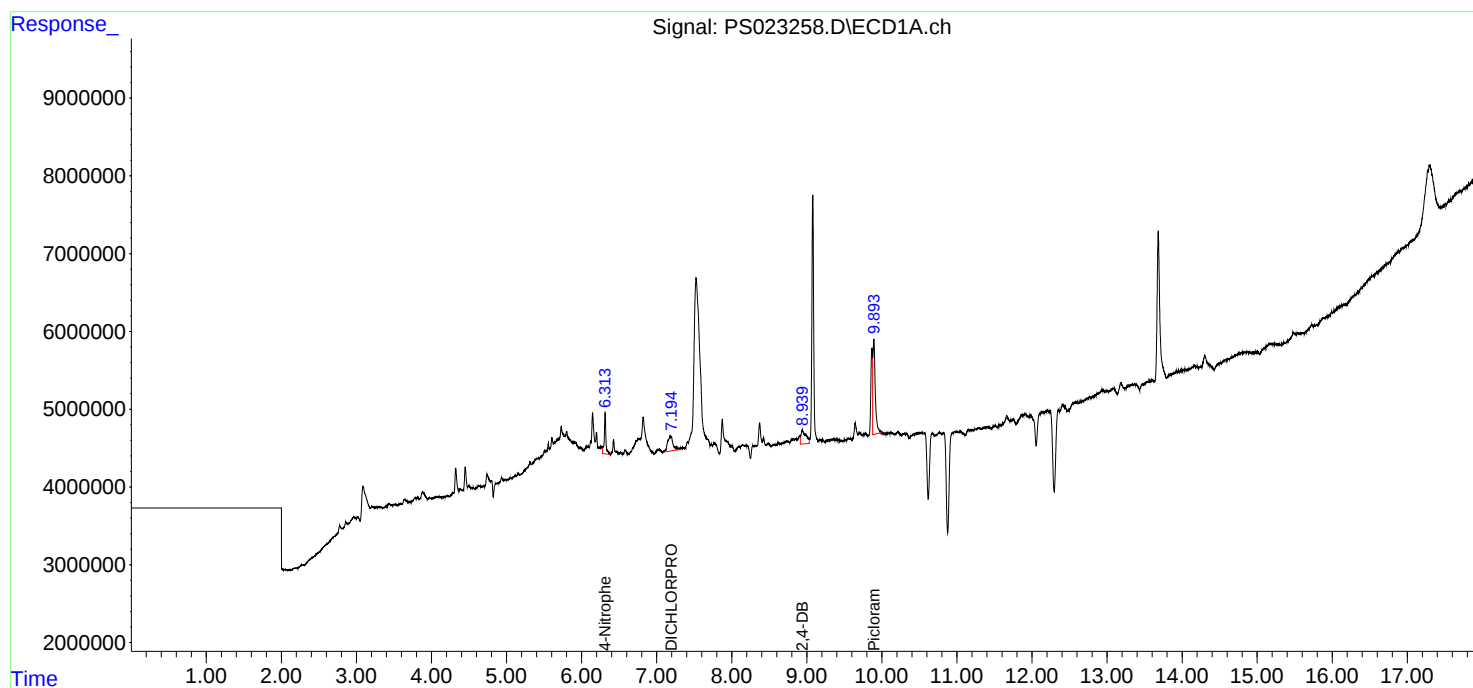


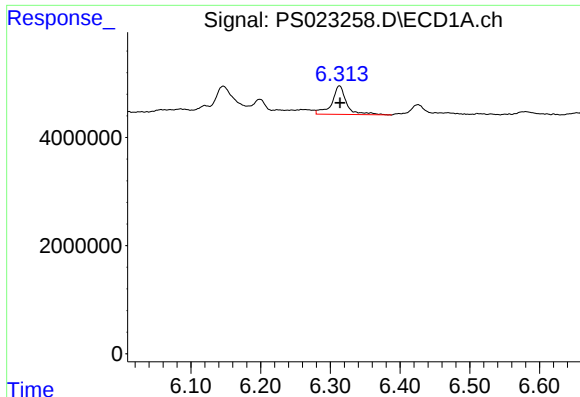

#3 4-Nitrophenol


R.T.: 6.313 min
Delta R.T.: 0.000 min
Response: 7800609
Conc: 6.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

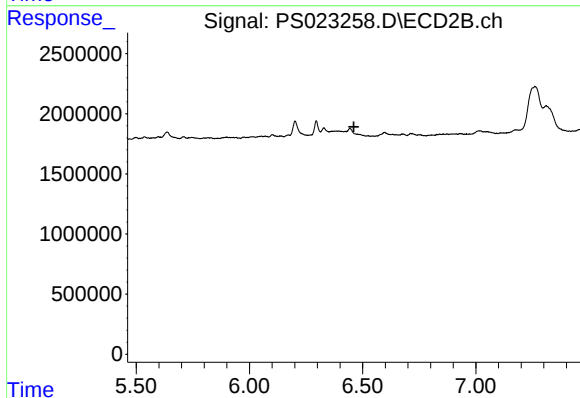


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

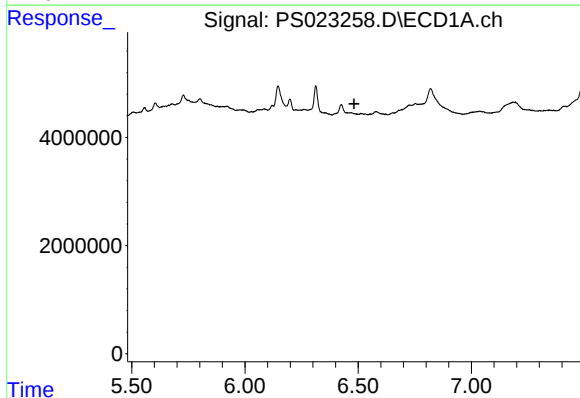


#4 2,4-DCAA

R.T.: 6.513 min
Delta R.T.: 0.031 min
Response: -14628
Conc: N.D.

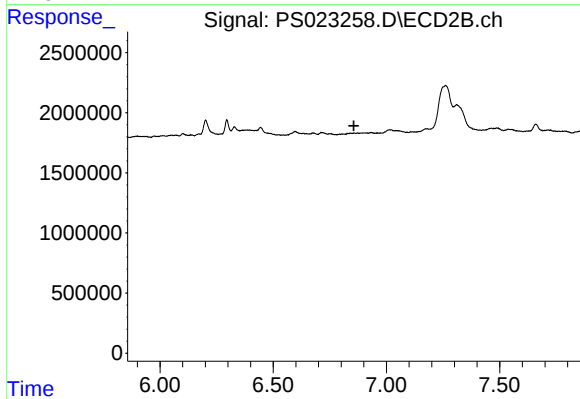

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.856 min
Response: 0
Conc: N.D.

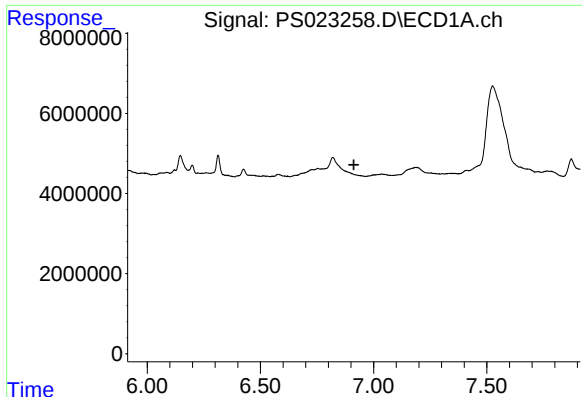

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.913 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

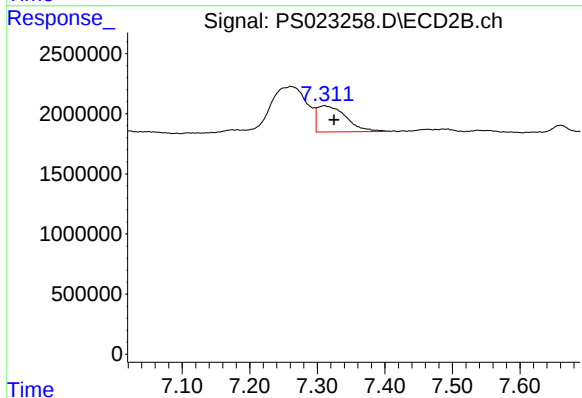


#7 MCPA

R.T.: 7.311 min
Delta R.T.: -0.014 min
Response: 6395330
Conc: 2.38 ug/ml

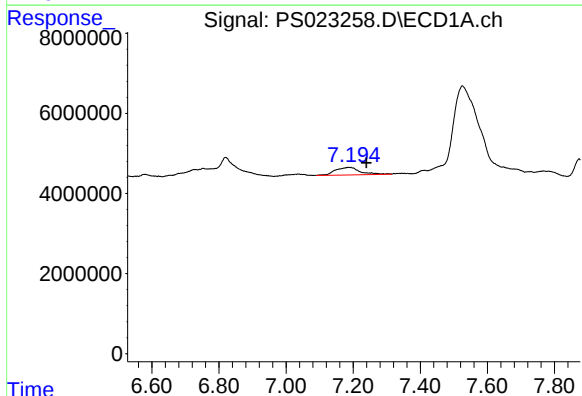


#8 DICHLORPROP

R.T.: 7.187 min
Delta R.T.: -0.053 min
Response: 9793071
Conc: 4.75 ng/ml

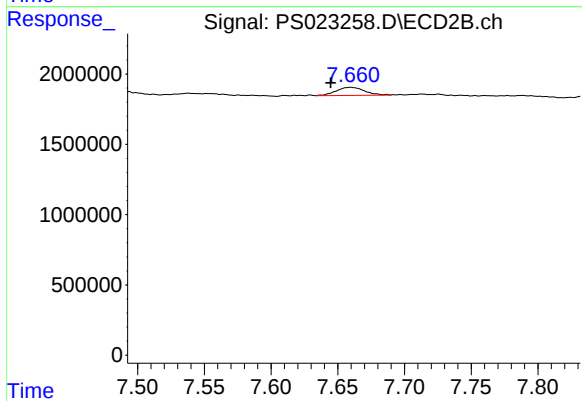

#8 DICHLORPROP


R.T.: 7.660 min
Delta R.T.: 0.015 min
Response: 839012
Conc: 1.36 ng/ml

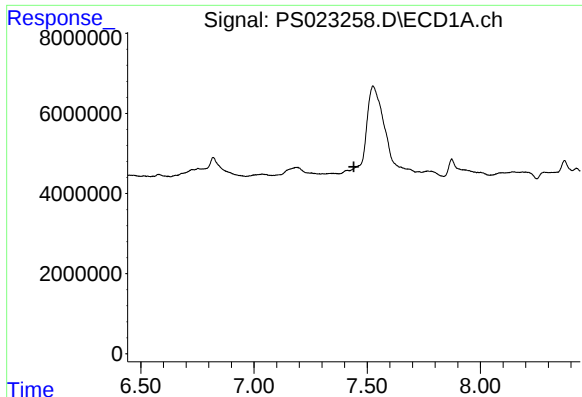

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.442 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

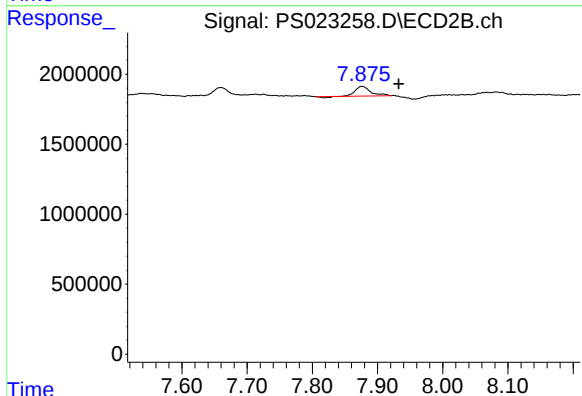


#9 2,4-D

R.T.: 7.875 min
Delta R.T.: -0.057 min
Response: 1101833
Conc: 1.59 ng/ml

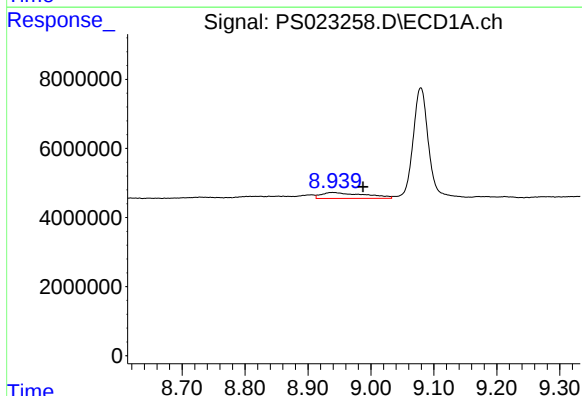


#13 2,4-DB

R.T.: 8.939 min
Delta R.T.: -0.048 min
Response: 8164964
Conc: 3.47 ng/ml

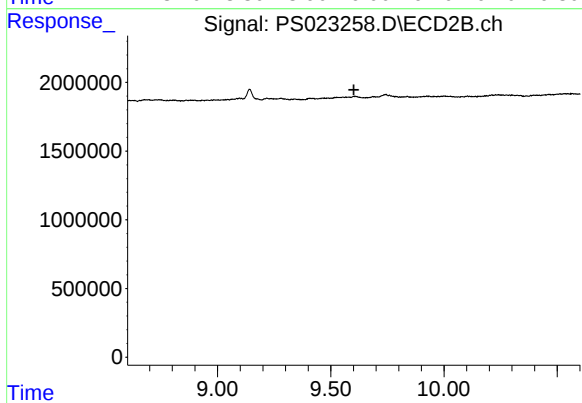

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.602 min
Response: 0
Conc: N.D.

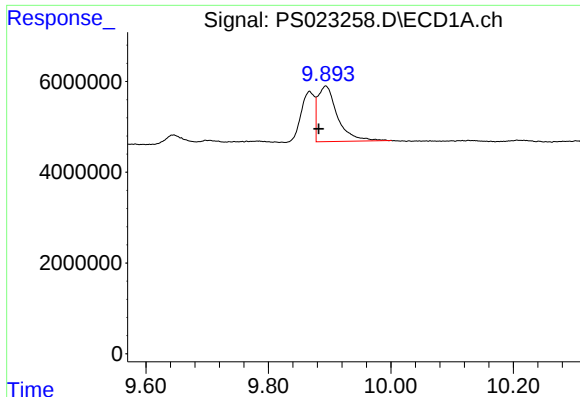

#15 Picloram


R.T.: 9.894 min
Delta R.T.: 0.011 min
Response: 27288789
Conc: 1.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

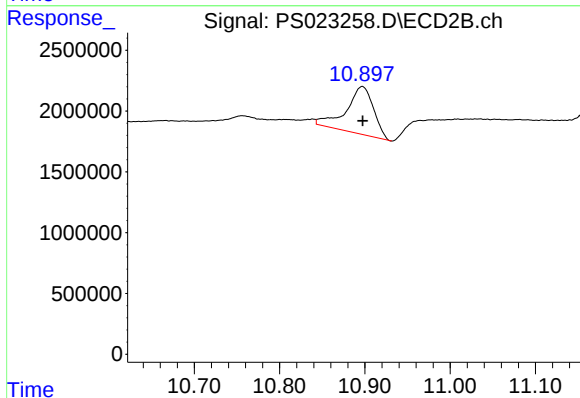


#15 Picloram

R.T.: 10.897 min
Delta R.T.: 0.000 min
Response: 8779328
Conc: 1.92 ng/ml

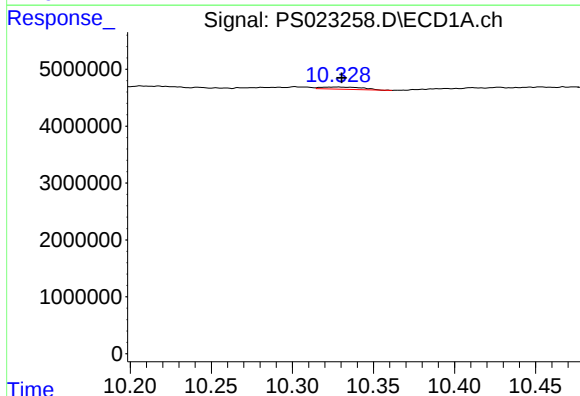

#16 DCPA

R.T.: 10.326 min
Delta R.T.: -0.004 min
Response: 673061
Conc: N.D.

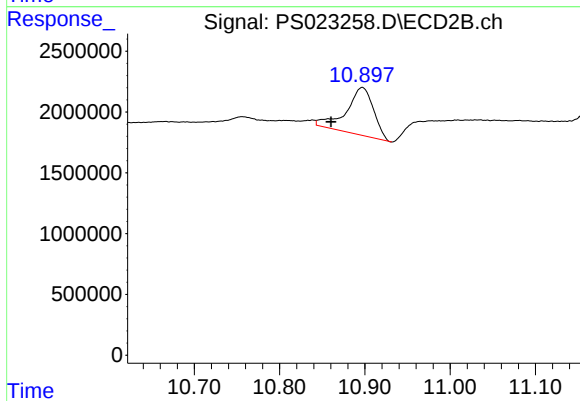

#16 DCPA

R.T.: 10.897 min
Delta R.T.: 0.036 min
Response: 8779328
Conc: 2.19 ng/ml