

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060923\
 Data File : PS023259.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2023 15:36
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 21:13:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.496	6.854	910.1E6	284.8E6	514.391	501.600
Target Compounds							
2) T	3,5-DICHL...	5.837	0.000	212899	0	<MDL	N.D. #
3) T	4-Nitroph...	6.330	0.000	6937105	0	5.382	N.D. #
5) T	DICAMBA	6.643	0.000	1168238	0	<MDL	N.D. #
6) T	MCP	6.738f	0.000	335700	0	<MDL	N.D. #
7) T	MCPA	6.945	7.257f	442267	2367323	<MDL	<MDL #
8) T	DICHLORPROP	7.260	0.000	7071473	0	3.427	N.D. #
9) T	2,4-D	7.450	0.000	49975320	0	20.454	N.D. #
10) T	Pentachlo...	7.693	0.000	2245076	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.208	0.000	865975	0	<MDL	N.D. #
12) T	2,4,5-T	8.447	9.140f	4715841	1337230	<MDL	<MDL #
13) T	2,4-DB	8.951	0.000	24680478	0	10.484	N.D. #
14) T	DINOSEB	10.039	0.000	464849	0	<MDL	N.D. #
15) T	Picloram	9.919	10.896	32329847	6296802	1.863	1.380 #
16) T	DCPA	10.306	10.861	754440	2771493	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060923\
Data File : PS023259.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2023 15:36
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 21:13:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

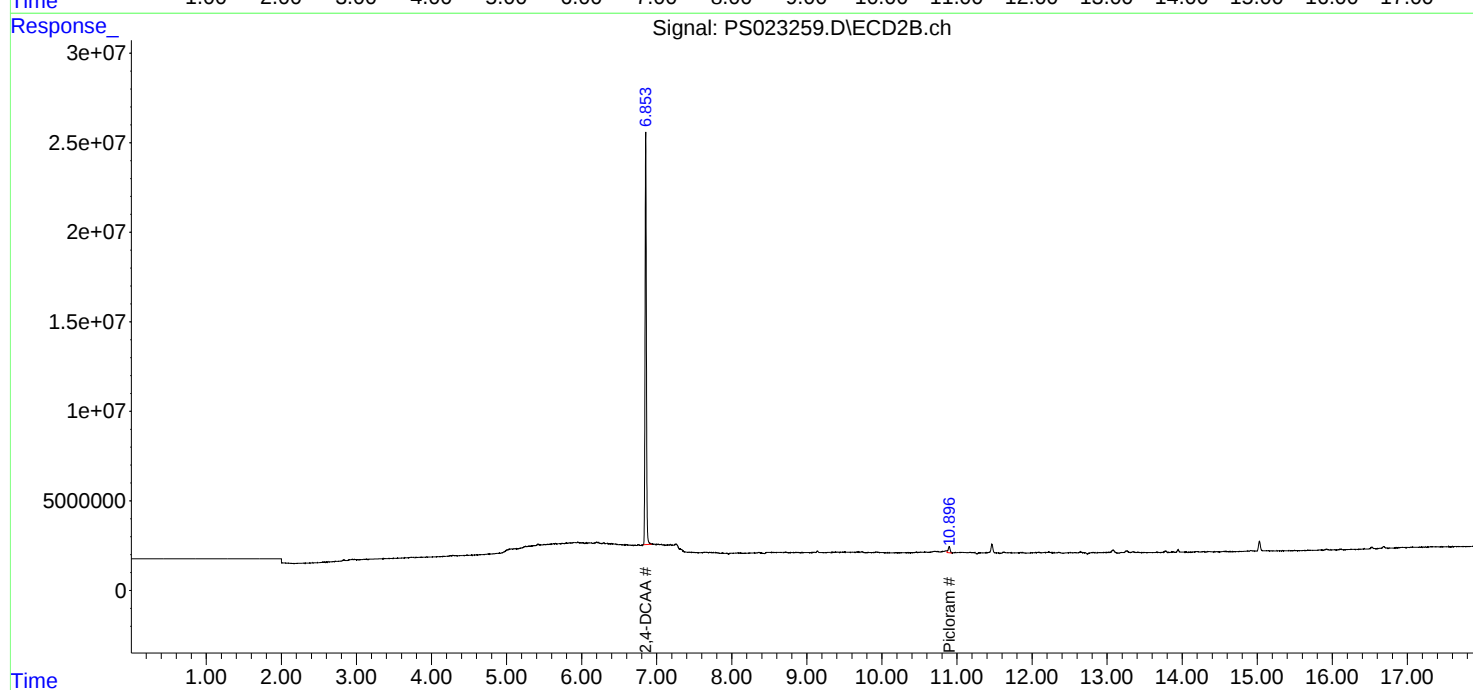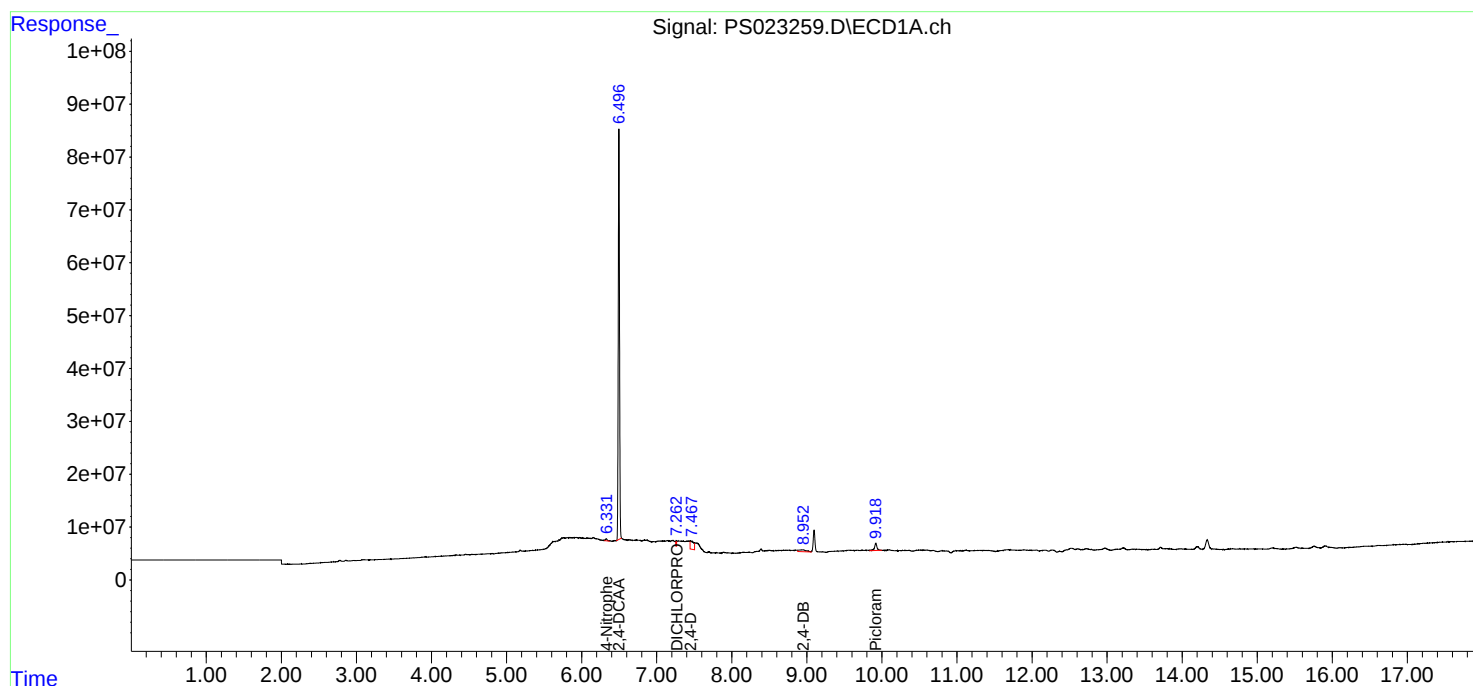


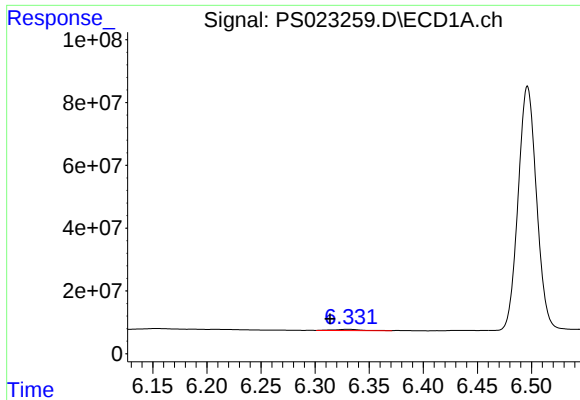

#3 4-Nitrophenol


R.T.: 6.330 min
Delta R.T.: 0.016 min
Response: 6937105
Conc: 5.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

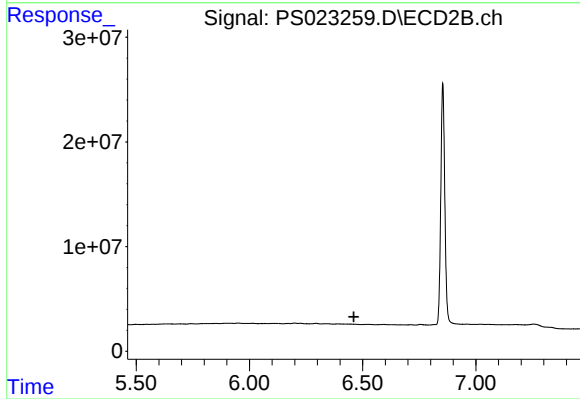


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

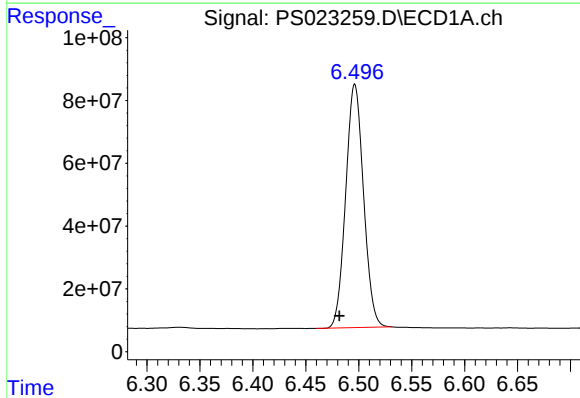


#4 2,4-DCAA

R.T.: 6.496 min
Delta R.T.: 0.015 min
Response: 910089287
Conc: 514.39 ng/ml

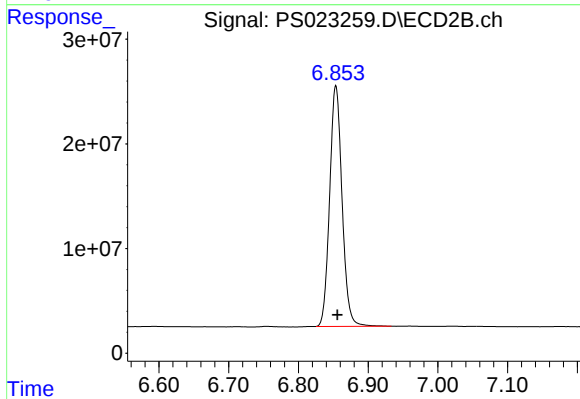

#4 2,4-DCAA


R.T.: 6.854 min
Delta R.T.: -0.002 min
Response: 284755843
Conc: 501.60 ng/ml

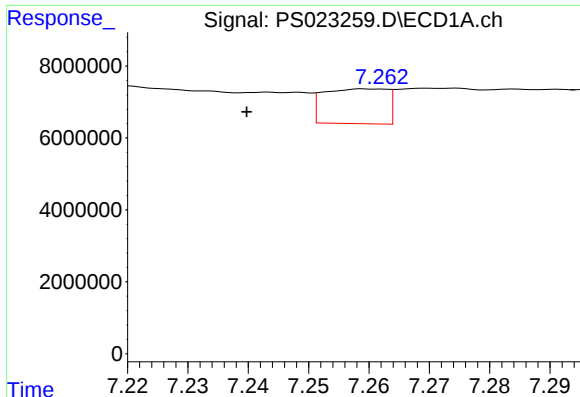

#8 DICHLORPROP


R.T.: 7.260 min
Delta R.T.: 0.020 min
Response: 7071473
Conc: 3.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

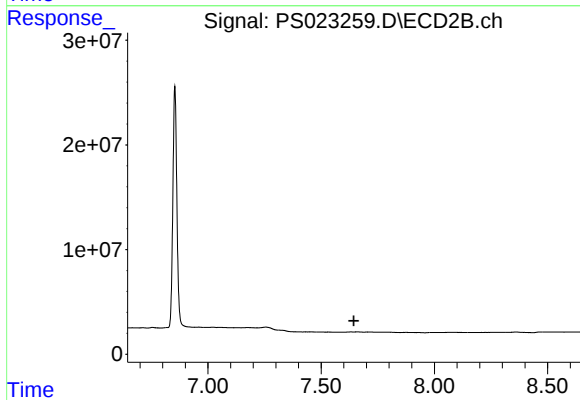


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.645 min
Response: 0
Conc: N.D.

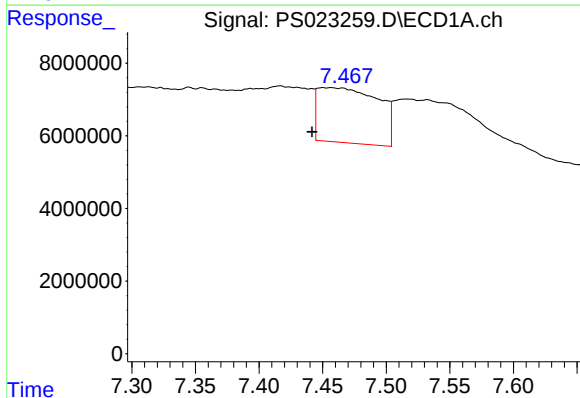


#9 2,4-D

R.T.: 7.450 min
Delta R.T.: 0.008 min
Response: 49975320
Conc: 20.45 ng/ml

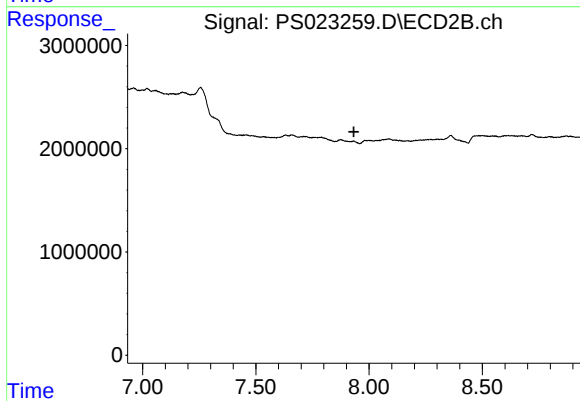

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.933 min
Response: 0
Conc: N.D.

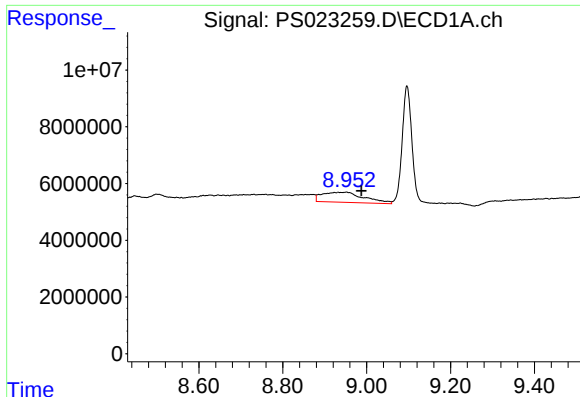

#13 2,4-DB


R.T.: 8.951 min
Delta R.T.: -0.036 min
Response: 24680478
Conc: 10.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

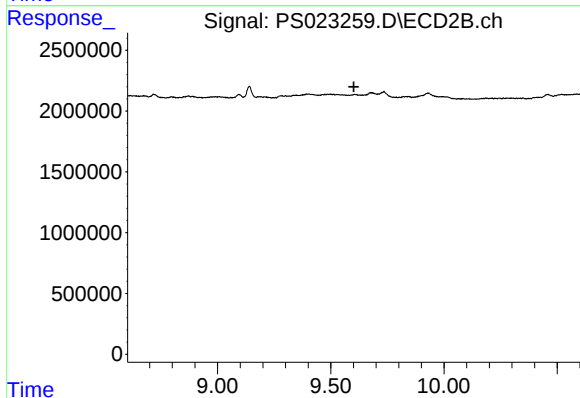


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.602 min
Response: 0
Conc: N.D.

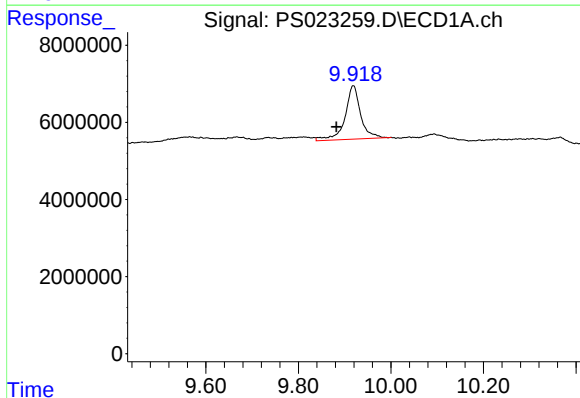

#15 Picloram

R.T.: 9.919 min
Delta R.T.: 0.036 min
Response: 32329847
Conc: 1.86 ng/ml

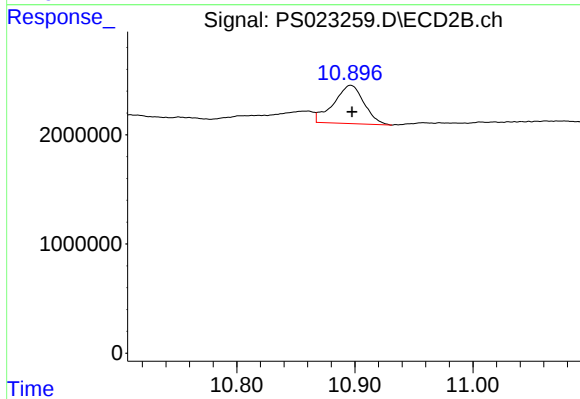

#15 Picloram

R.T.: 10.896 min
Delta R.T.: -0.001 min
Response: 6296802
Conc: 1.38 ng/ml