

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061020\
 Data File : PS010762.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2020 16:01
 Operator : DD\AJ
 Sample : L2886-03DL 2X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 GENDL

Manual Integrations
 APPROVED

Sohil
 6/11/2020 8:16:38 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 00:54:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.920	175.7E6	117.7E6	222.130m	215.787m
Target Compounds							
5) T	DICAMBA	7.421	7.089	84985003	82763738	27.027	36.770 #
9) T	2,4-D	8.344	8.009	1032.3E6	800.0E6	1309.560	1055.080
15) T	Picloram	11.022	11.001	484.0E6	426.3E6	94.800m	103.323

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061020\
Data File : PS010762.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2020 16:01
Operator : DD\AJ
Sample : L2886-03DL 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
GENDL


Manual Integrations
APPROVED

Sohil
6/11/2020 8:16:38 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 00:54:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

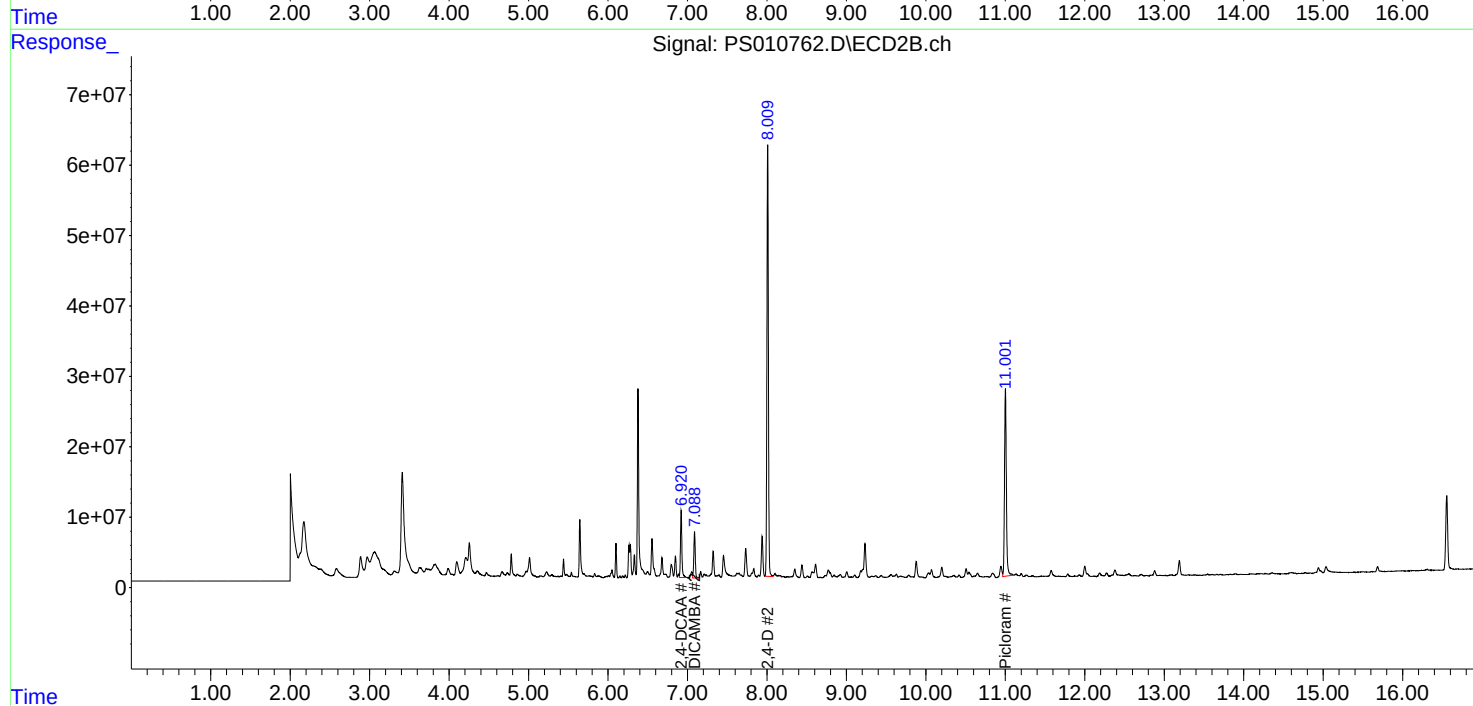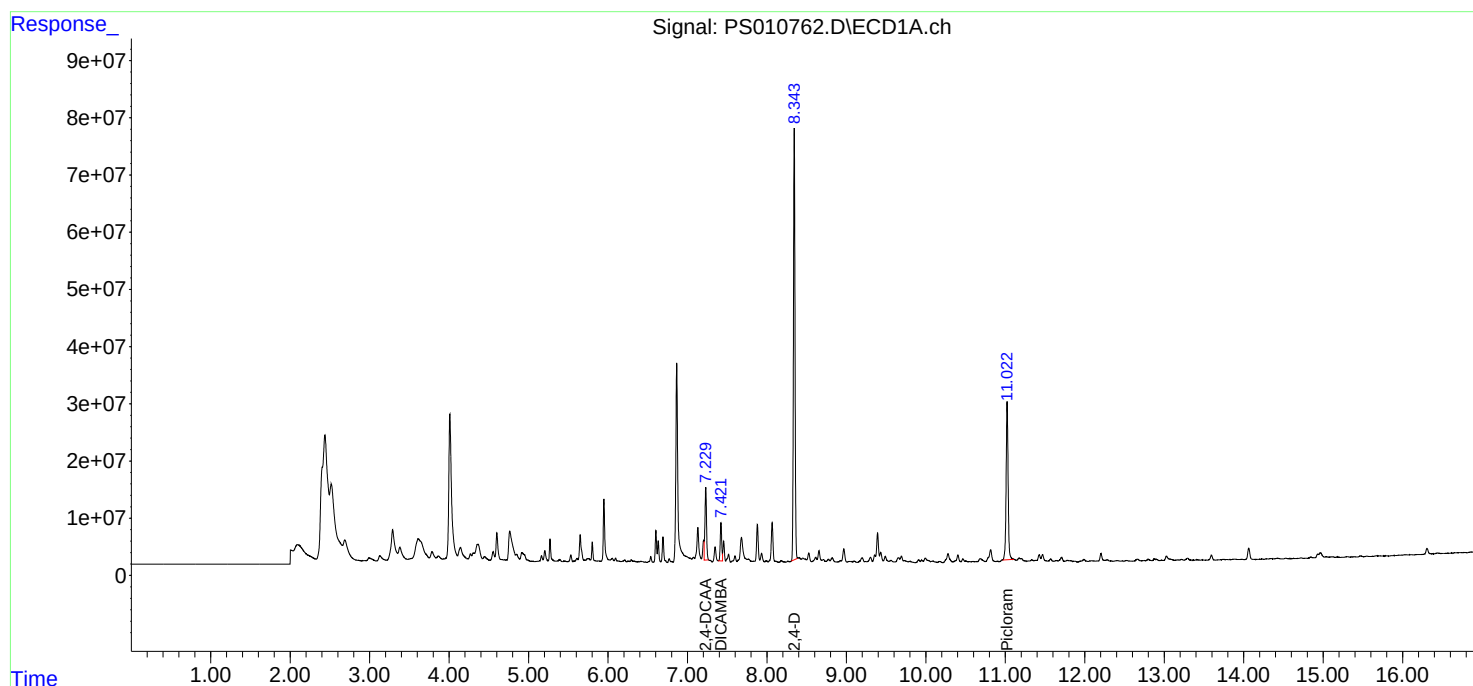

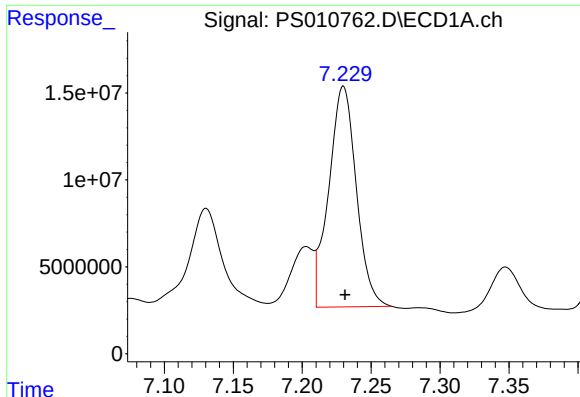


#4 2,4-DCAA

R.T.: 7.229 min
Delta R.T.: -0.002 min
Response: 175674053
Conc: 222.13 ng/ml m

Instrument :
ECD_S
ClientSampleId :
GENDL


Manual Integrations
APPROVED

Sohil
6/11/2020 8:16:38 AM

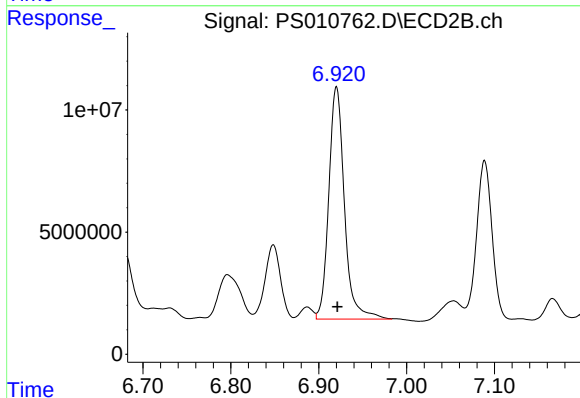


#4 2,4-DCAA

R.T.: 6.920 min
Delta R.T.: -0.002 min
Response: 117693736
Conc: 215.79 ng/ml m

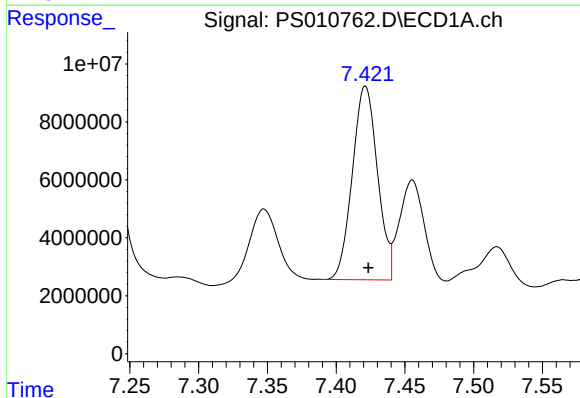


#5 DICAMBA

R.T.: 7.421 min
Delta R.T.: -0.002 min
Response: 84985003
Conc: 27.03 ng/ml

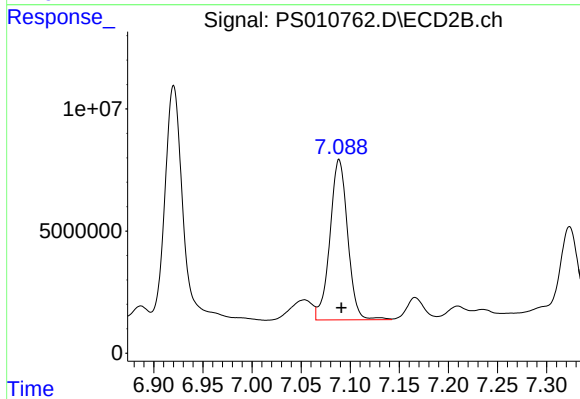

#5 DICAMBA

R.T.: 7.089 min
Delta R.T.: -0.002 min
Response: 82763738
Conc: 36.77 ng/ml

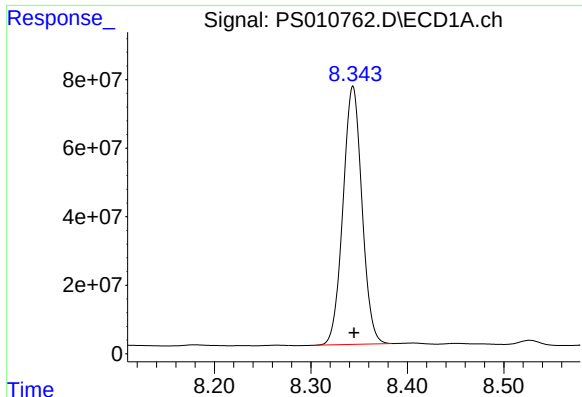


#9 2,4-D

R.T.: 8.344 min
Delta R.T.: -0.001 min
Response: 1032293245
Conc: 1309.56 ng/ml

Instrument :
ECD_S
ClientSampleId :
GENDL


Manual Integrations
APPROVED

Sohil
6/11/2020 8:16:38 AM

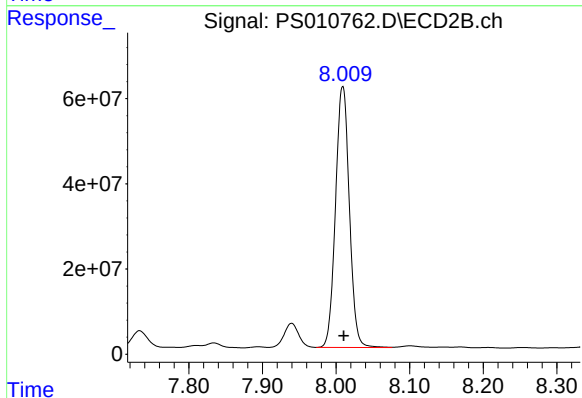


#9 2,4-D

R.T.: 8.009 min
Delta R.T.: -0.001 min
Response: 800020392
Conc: 1055.08 ng/ml

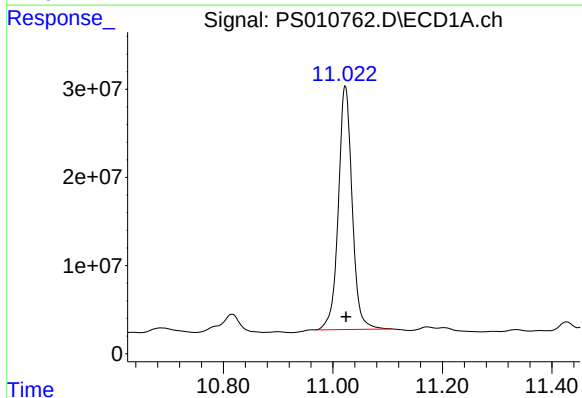

#15 Picloram

R.T.: 11.022 min
Delta R.T.: -0.002 min
Response: 483965338
Conc: 94.80 ng/ml m

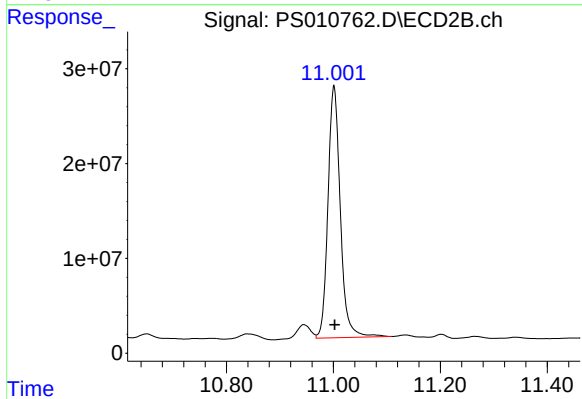

#15 Picloram

R.T.: 11.001 min
Delta R.T.: -0.001 min
Response: 426306058
Conc: 103.32 ng/ml