

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061021\
 Data File : PS015344.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2021 17:50
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 18:40:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.223	6.783	1286.1E6	278.5E6	510.270	519.746
Target Compounds							
3) T	4-Nitroph...	7.020	0.000	11296429	0	8.013	N.D. #
8) T	DICHLORPROP	0.000	7.590	0	3152041	N.D.	5.802
12) T	2,4,5-T	9.457	0.000	5934294	0	<MDL	N.D. #
15) T	Picloram	11.013	10.843	31778905	8292714	1.918	1.997
16) T	DCPA	0.000	10.843	0	8292714	N.D.	1.924



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061021\
Data File : PS015344.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2021 17:50
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 18:40:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

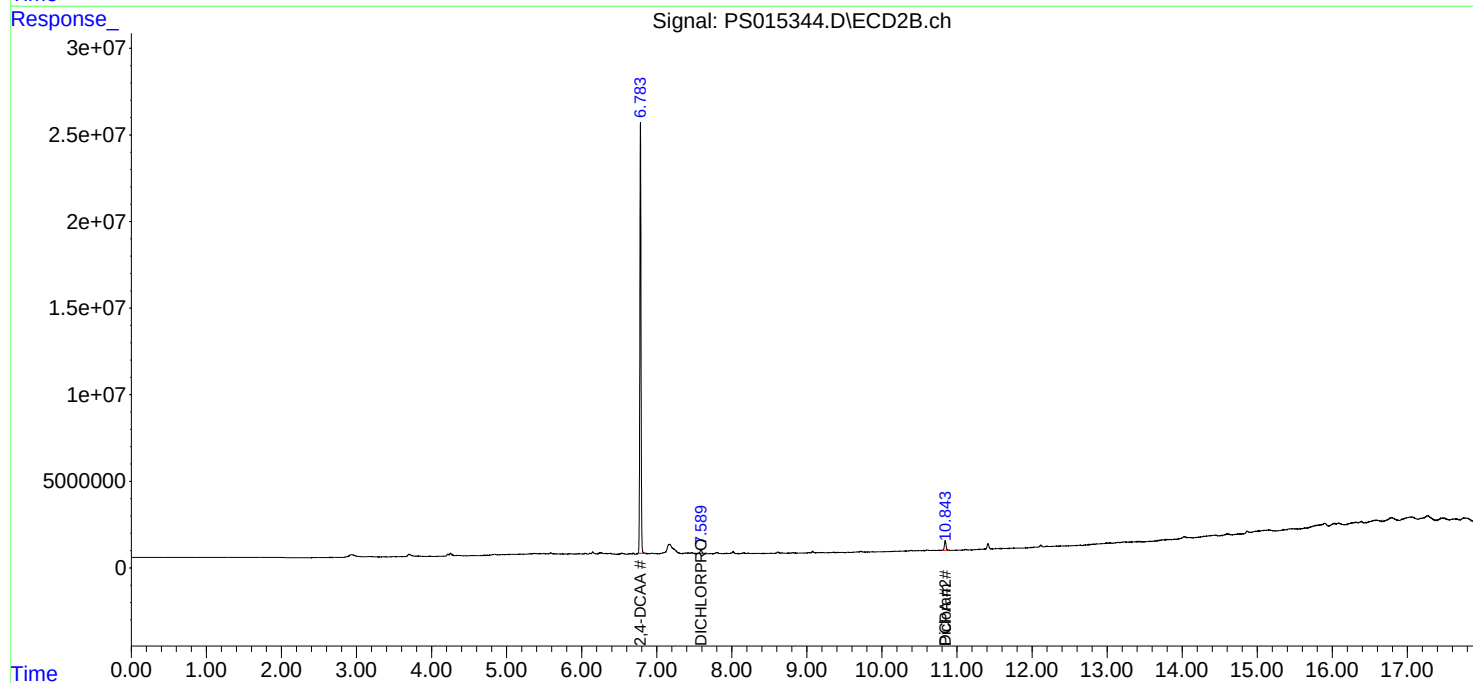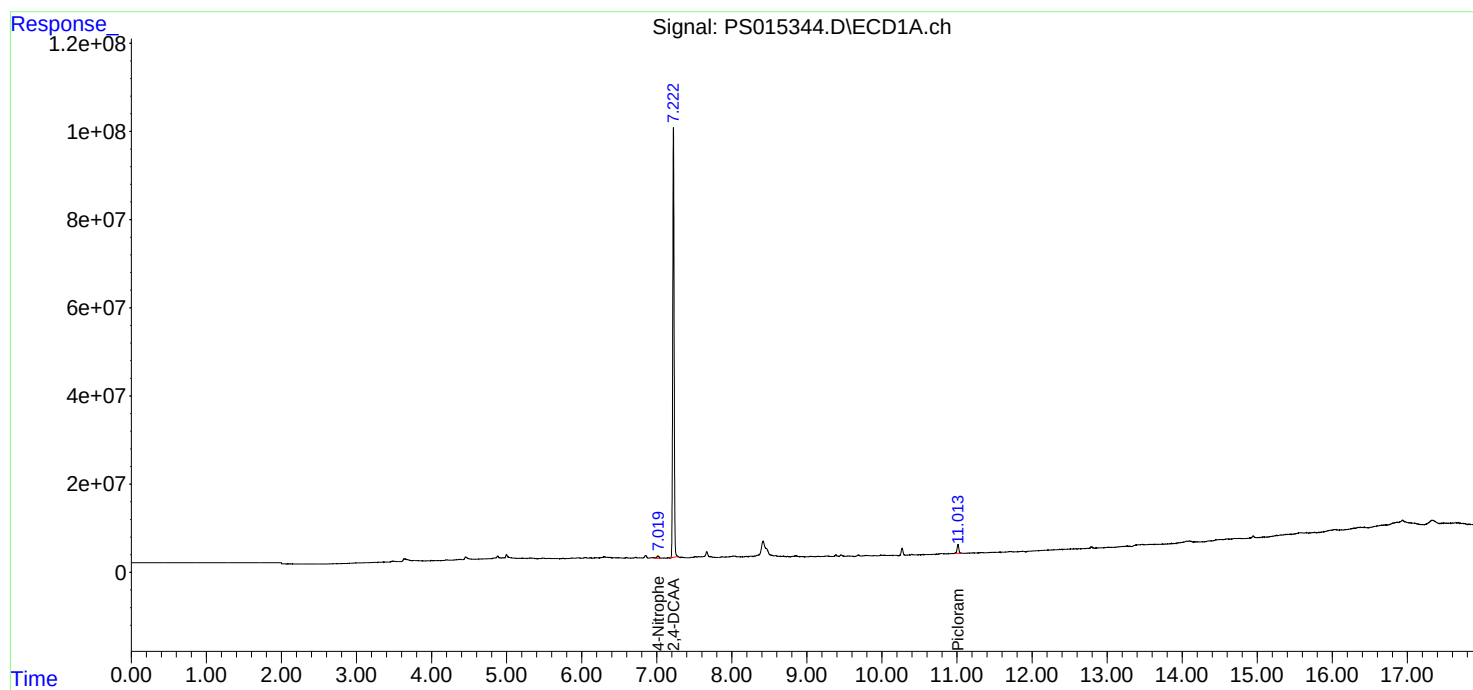


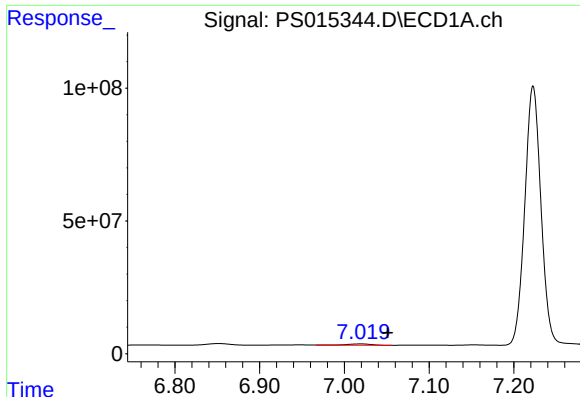

#3 4-Nitrophenol


R.T.: 7.020 min
Delta R.T.: -0.032 min
Response: 11296429
Conc: 8.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

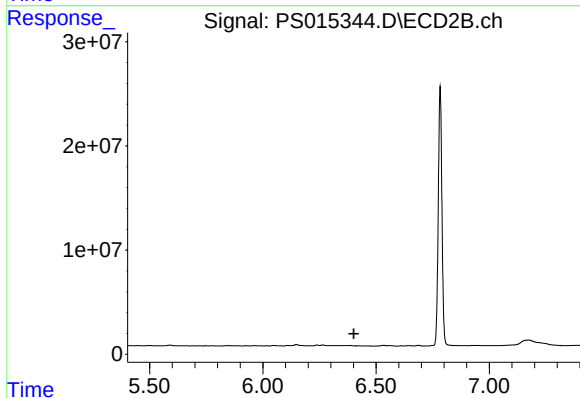


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.402 min
Response: 0
Conc: N.D.

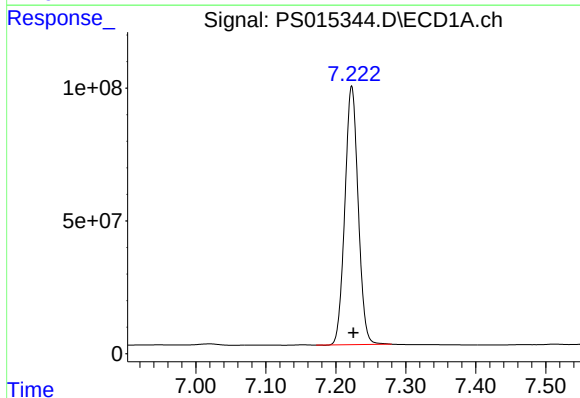


#4 2,4-DCAA

R.T.: 7.223 min
Delta R.T.: -0.002 min
Response: 1286072625
Conc: 510.27 ng/ml

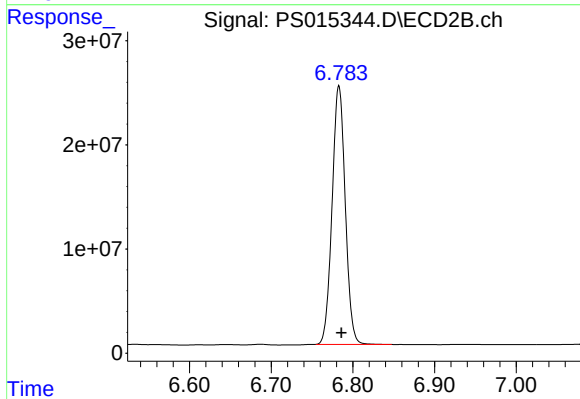

#4 2,4-DCAA


R.T.: 6.783 min
Delta R.T.: -0.003 min
Response: 278465075
Conc: 519.75 ng/ml

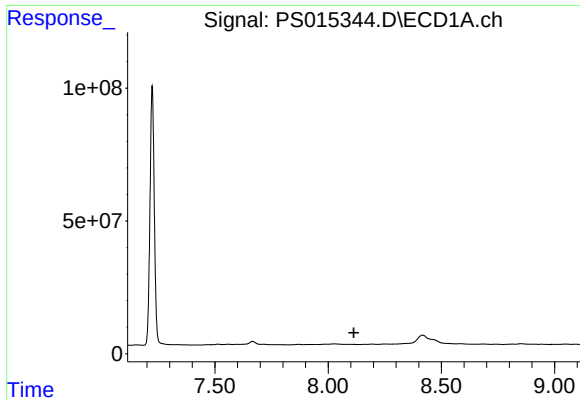

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.113 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

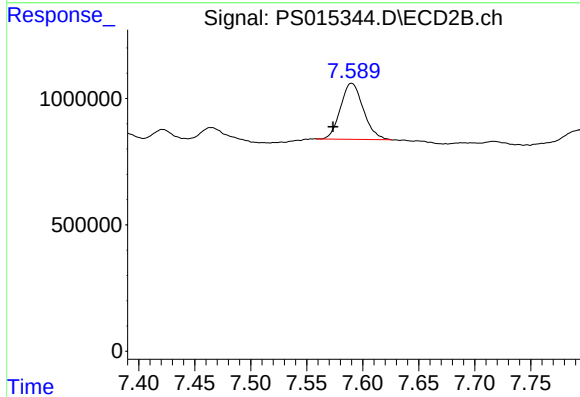


#8 DICHLORPROP

R.T.: 7.590 min
Delta R.T.: 0.016 min
Response: 3152041
Conc: 5.80 ng/ml

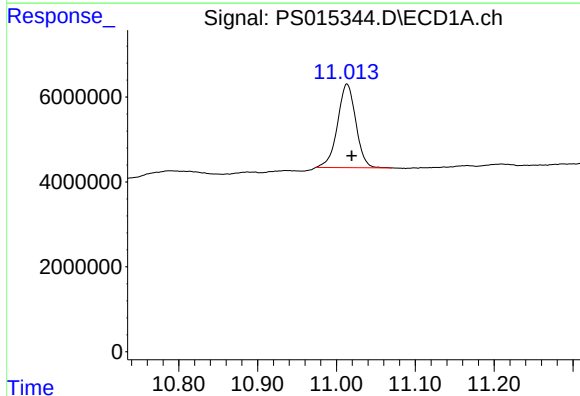


#15 Picloram

R.T.: 11.013 min
Delta R.T.: -0.006 min
Response: 31778905
Conc: 1.92 ng/ml

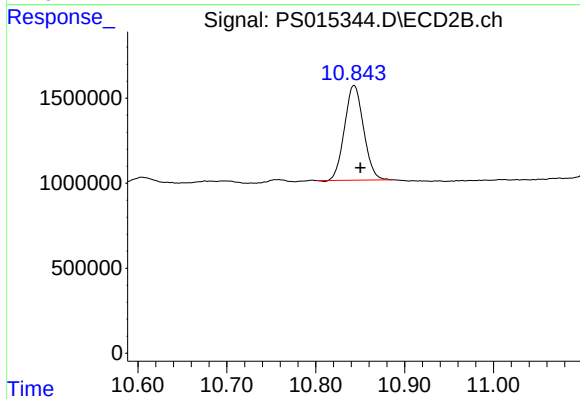

#15 Picloram


R.T.: 10.843 min
Delta R.T.: -0.007 min
Response: 8292714
Conc: 2.00 ng/ml

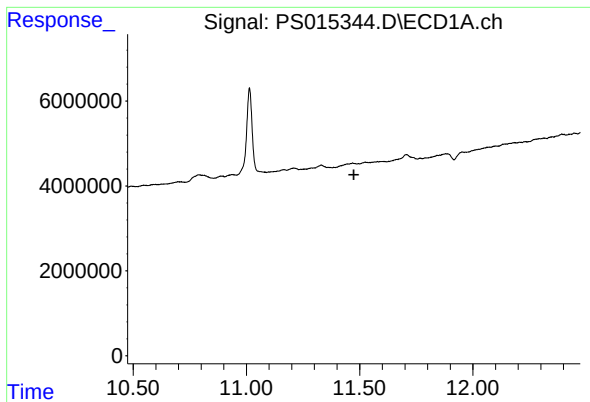

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.475 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

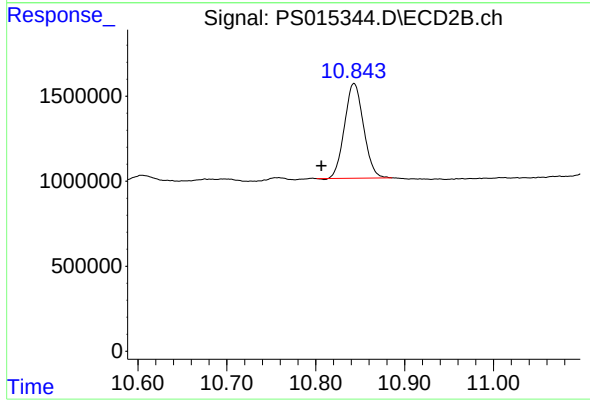

#16 DCPA

R.T.: 10.843 min
Delta R.T.: 0.037 min
Response: 8292714
Conc: 1.92 ng/ml