

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061021\
 Data File : PS015401.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2021 16:45
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 02:45:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.221	6.782	1396.6E6	288.7E6	554.131	538.849
Target Compounds							
3) T	4-Nitroph...	7.019	0.000	7335847	0	5.204	N.D. #
15) T	Picloram	11.012	10.842	31211325	8076406	1.884	1.945
16) T	DCPA	0.000	10.842	0	8076406	N.D.	1.873



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061021\
Data File : PS015401.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2021 16:45
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 02:45:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

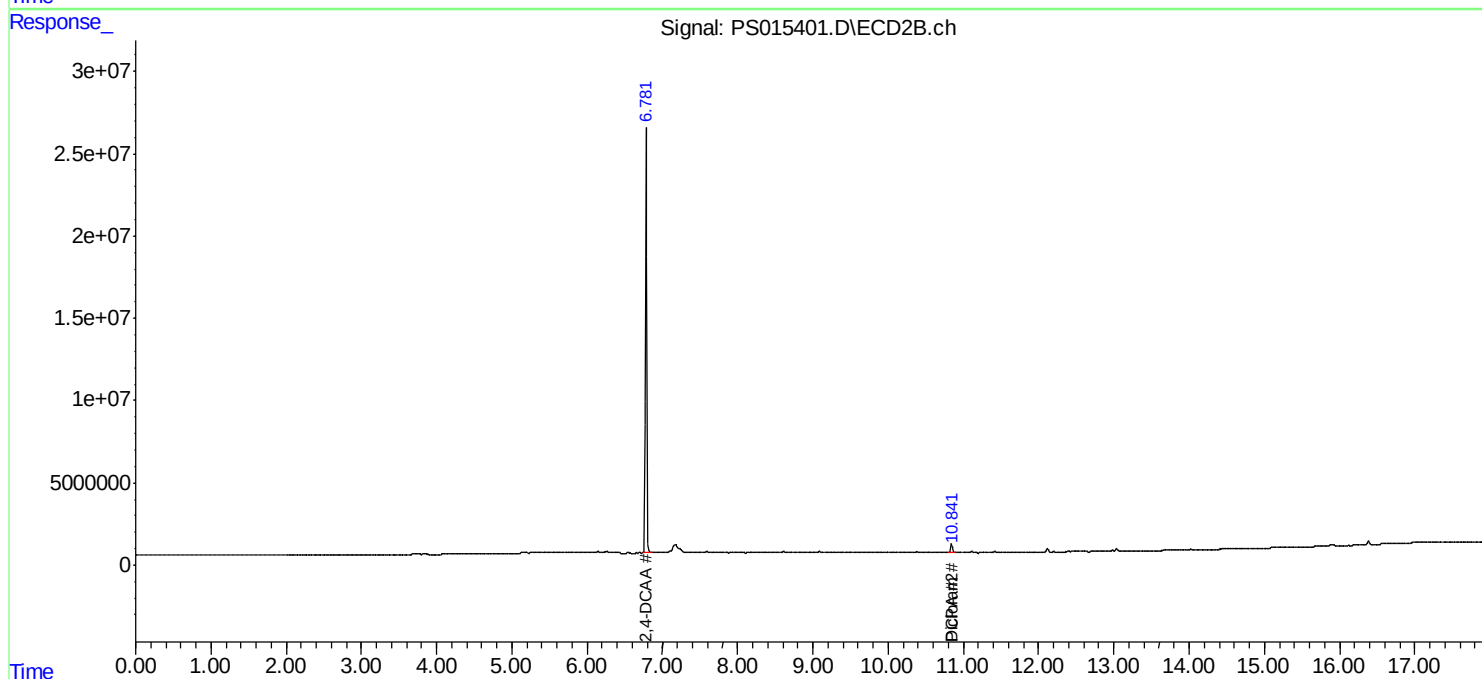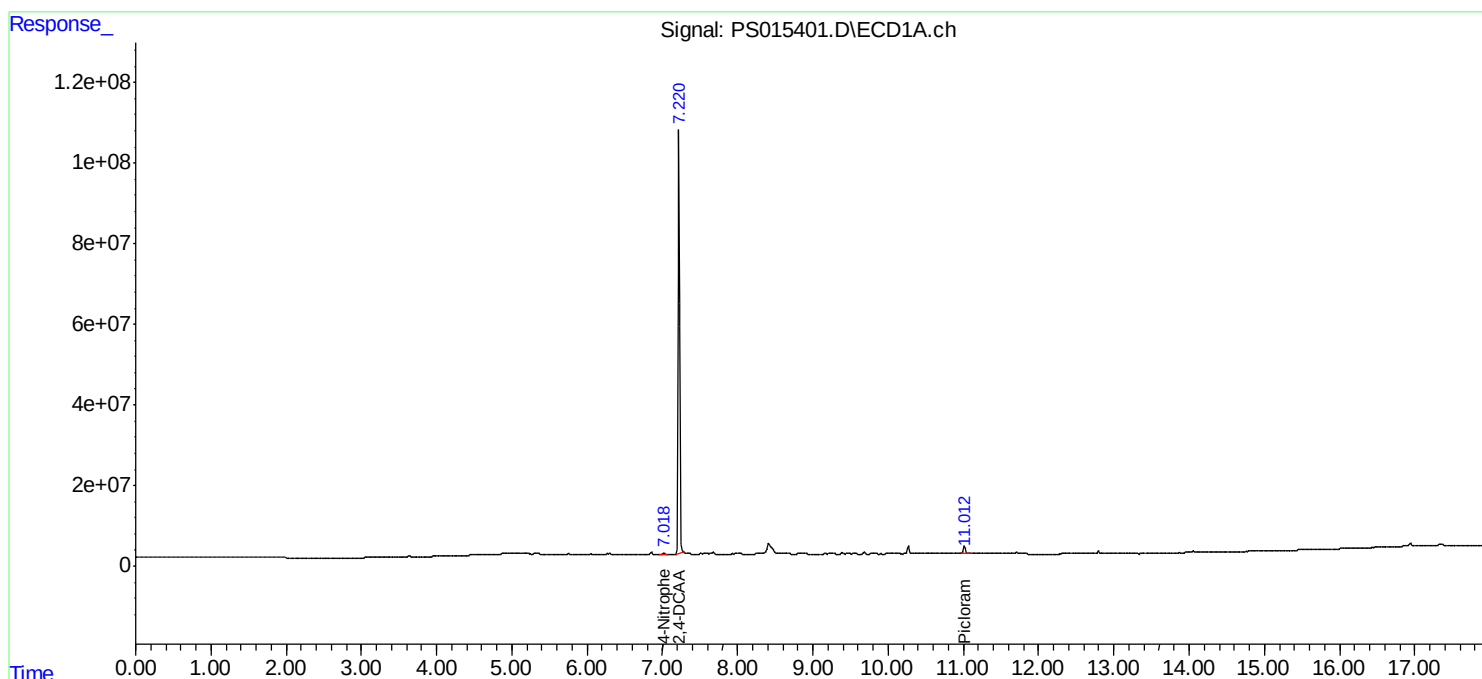


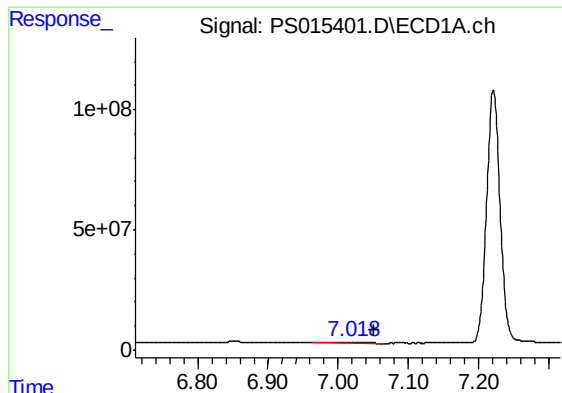

#3 4-Nitrophenol


R.T.: 7.019 min
Delta R.T.: -0.032 min
Response: 7335847
Conc: 5.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

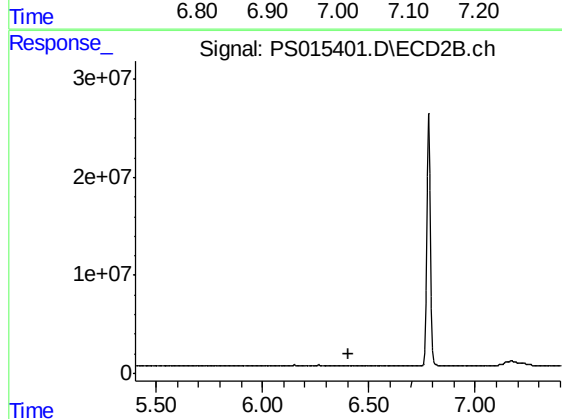


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

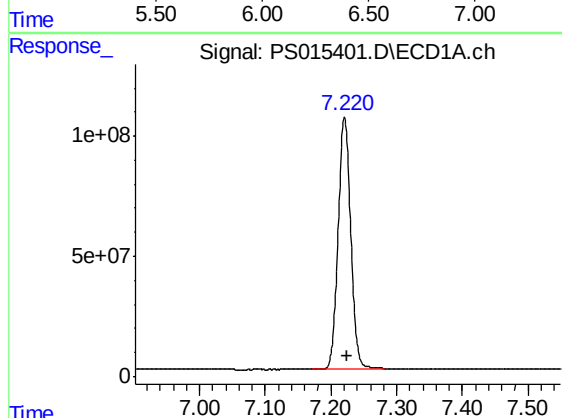


#4 2,4-DCAA

R.T.: 7.221 min
Delta R.T.: -0.005 min
Response: 1396617047
Conc: 554.13 ng/ml

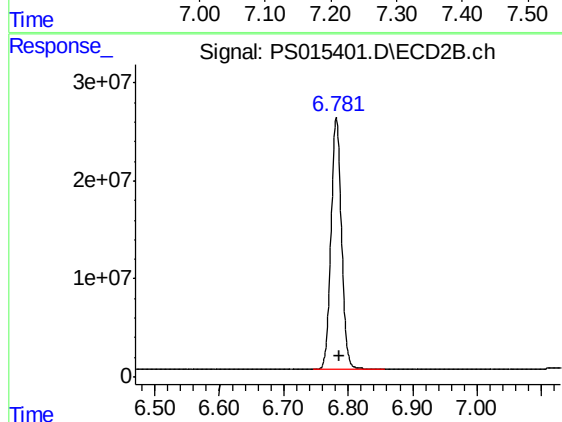

#4 2,4-DCAA


R.T.: 6.782 min
Delta R.T.: -0.004 min
Response: 288699732
Conc: 538.85 ng/ml

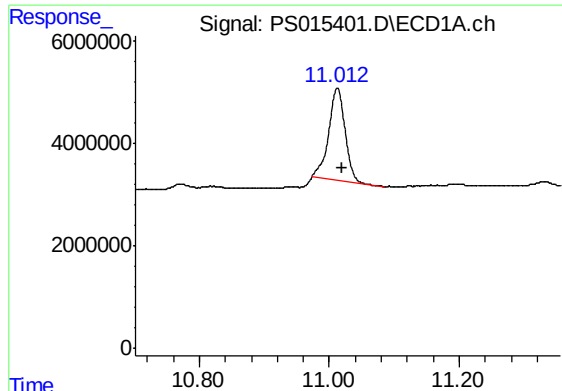

#15 Picloram


R.T.: 11.012 min
Delta R.T.: -0.007 min
Response: 31211325
Conc: 1.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

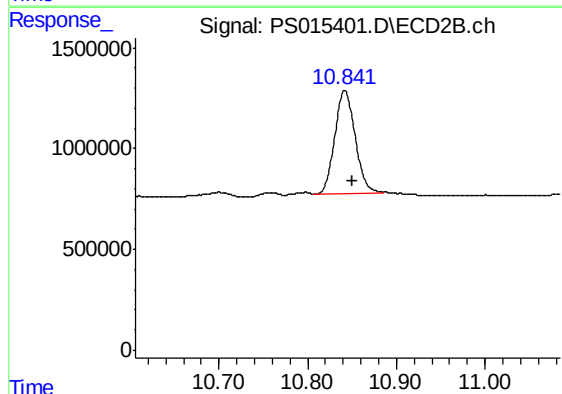


#15 Picloram

R.T.: 10.842 min
Delta R.T.: -0.008 min
Response: 8076406
Conc: 1.94 ng/ml

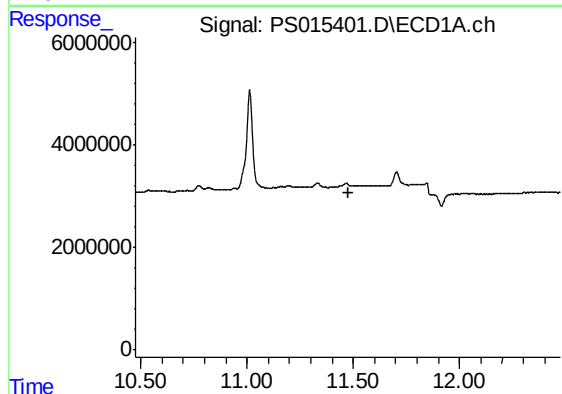

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.475 min
Response: 0
Conc: N.D.

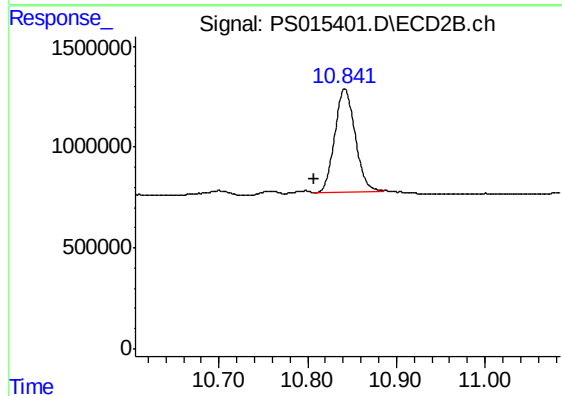

#16 DCPA

R.T.: 10.842 min
Delta R.T.: 0.035 min
Response: 8076406
Conc: 1.87 ng/ml