

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061025\
 Data File : PS030605.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2025 19:37
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 01:38:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060425.M
 Quant Title : 8080.M
 QLast Update : Wed Jun 04 13:21:22 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.359	7.769	1705.9E6	517.2E6	451.868	480.801
Target Compounds							
1) T	Dalapon	2.752f	2.664f	31685862	38351630	5.611	13.997 #
2) T	3,5-DICHL...	6.515	0.000	2085745	0	<MDL	N.D. #
3) T	4-Nitroph...	7.152	0.000	9180182	0	5.006	N.D. #
5) T	DICAMBA	7.544	7.974	3040827	14463853	<MDL	2.245 #
6) T	MCPD	7.794f	0.000	11469380	0	1.158	N.D. #
7) T	MCPA	7.911	0.000	988397	0	<MDL	N.D. #
8) T	DICHLORPROP	8.269	8.686	1701180	4293820	<MDL	2.893 #
10) T	Pentachlo...	8.804f	0.000	2866215	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.392	0.000	4558501	0	<MDL	N.D. #
12) T	2,4,5-T	9.687	10.367	2103230	2364943	<MDL	<MDL #
13) T	2,4-DB	10.288	10.974f	388836	7735176	<MDL	6.729 #
14) T	DINOSEB	11.484	11.314	1339898	1394068	<MDL	<MDL #
15) T	Picloram	11.291	12.423	6905802	9658695	<MDL	<MDL #
16) T	DCPA	11.777	12.364	4038673	2859290	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061025\
Data File : PS030605.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2025 19:37
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 01:38:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060425.M
Quant Title : 8080.M
QLast Update : Wed Jun 04 13:21:22 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

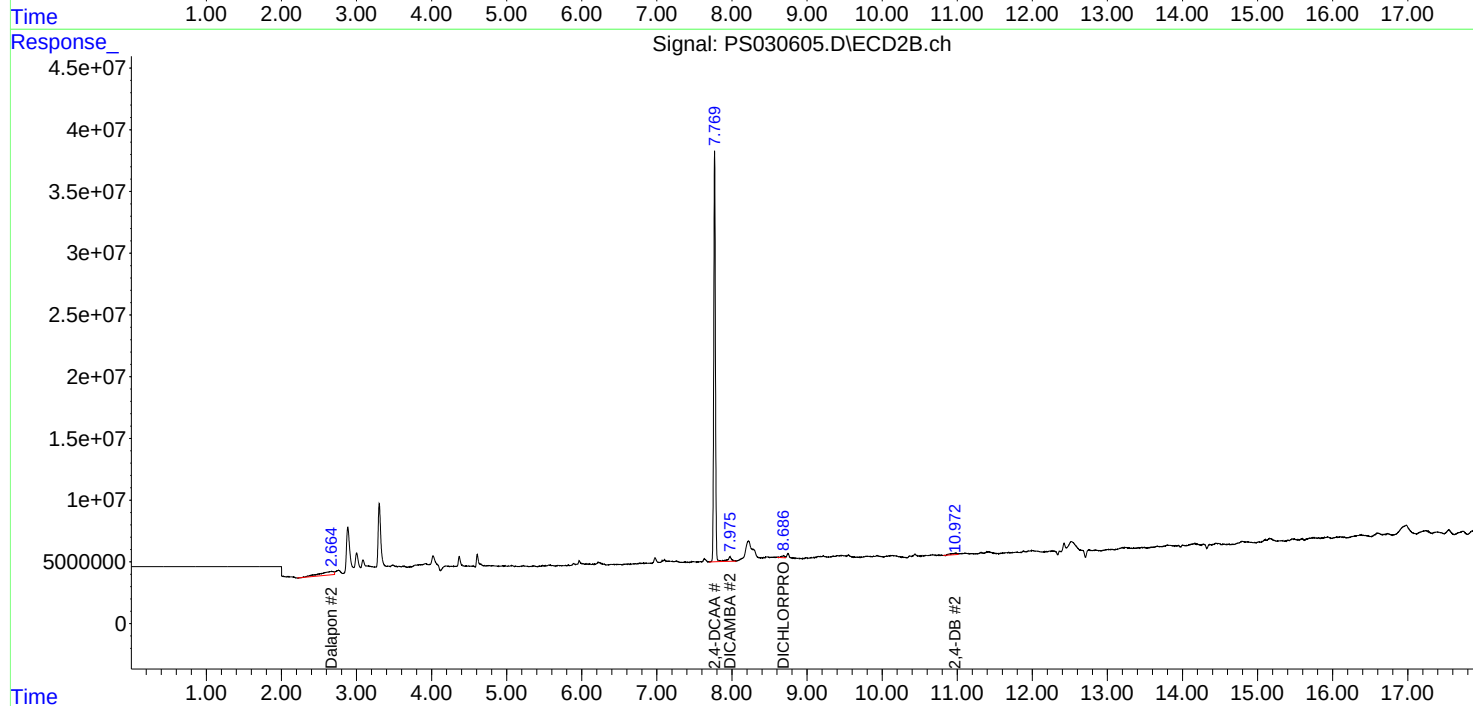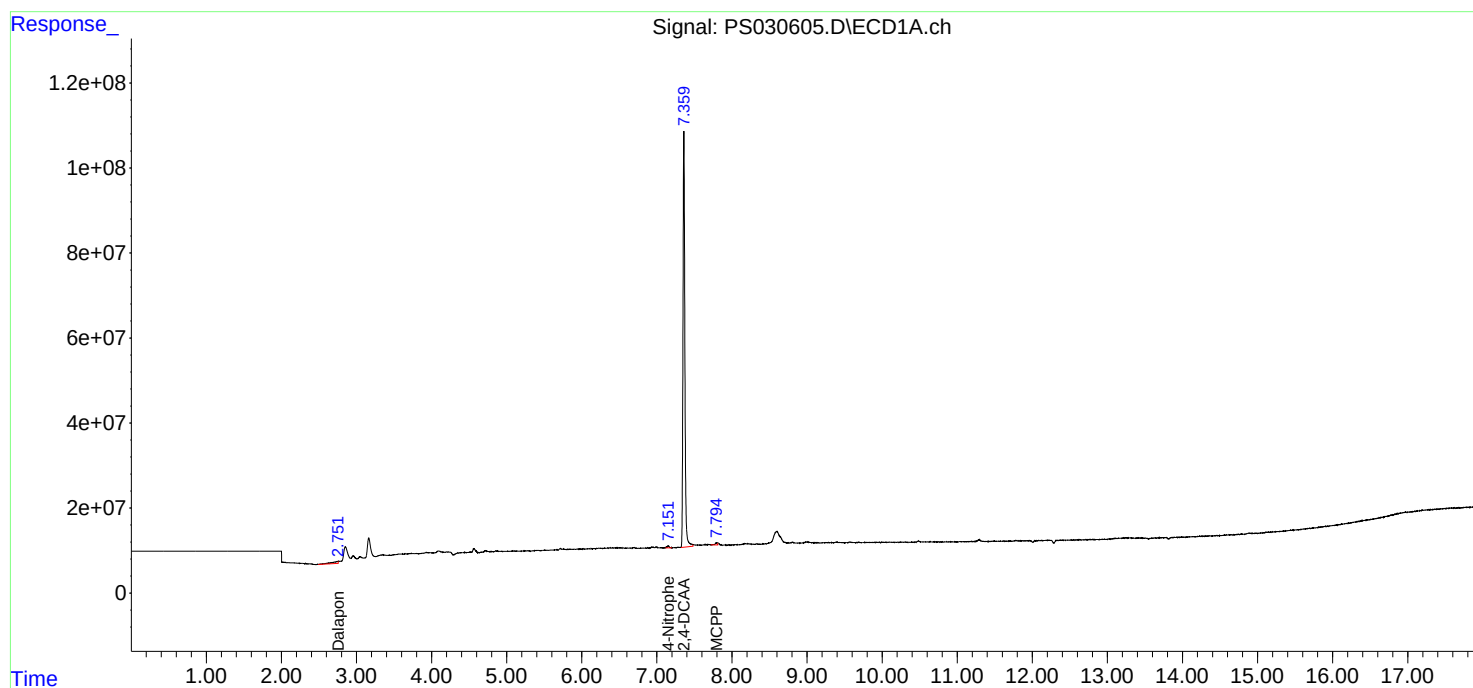


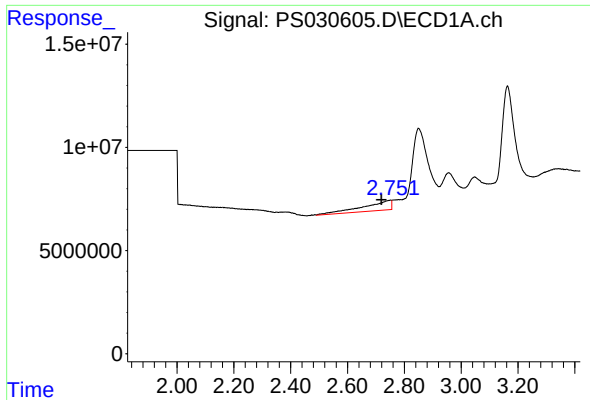

#1 Dalapon


R.T.: 2.752 min
Delta R.T.: 0.032 min
Response: 31685862
Conc: 5.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

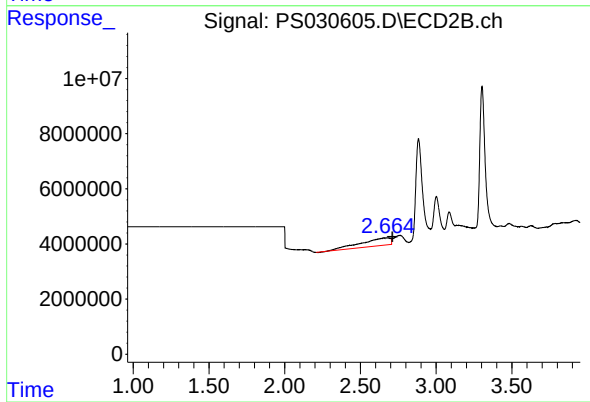


#1 Dalapon

R.T.: 2.664 min
Delta R.T.: -0.046 min
Response: 38351630
Conc: 14.00 ng/ml

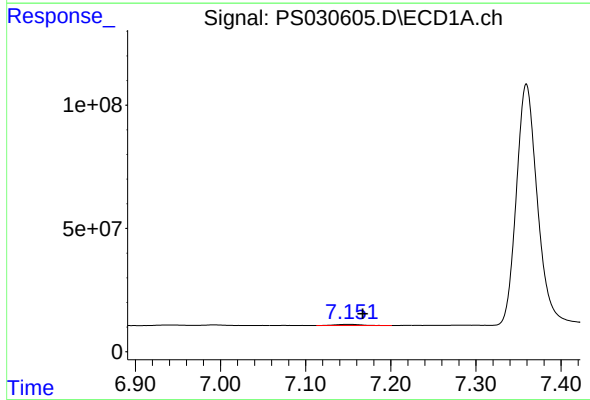


#3 4-Nitrophenol

R.T.: 7.152 min
Delta R.T.: -0.015 min
Response: 9180182
Conc: 5.01 ng/ml

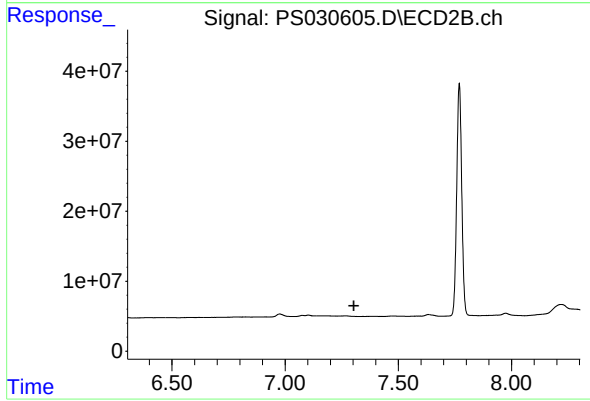

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.304 min
Response: 0
Conc: N.D.

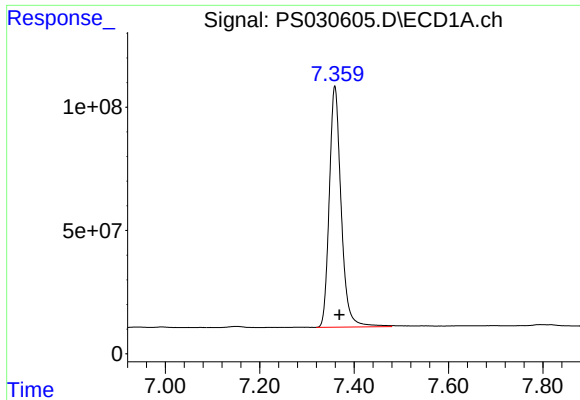

#4 2,4-DCAA


R.T.: 7.359 min
Delta R.T.: -0.010 min
Response: 1705869137
Conc: 451.87 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

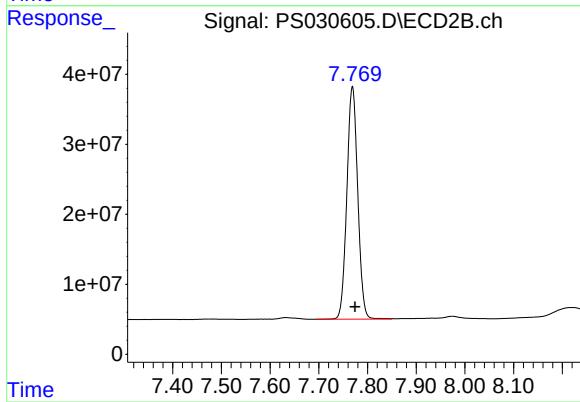


#4 2,4-DCAA

R.T.: 7.769 min
Delta R.T.: -0.005 min
Response: 517154089
Conc: 480.80 ng/ml

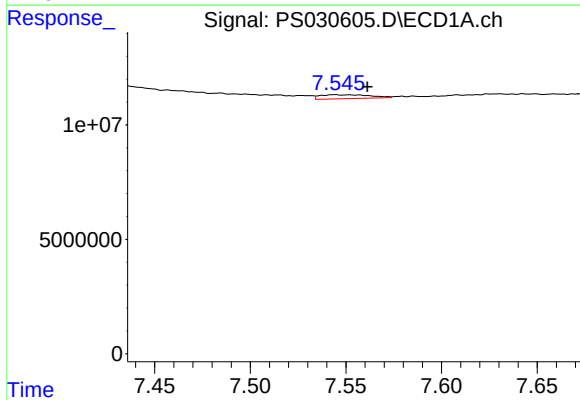


#5 DICAMBA

R.T.: 7.544 min
Delta R.T.: -0.017 min
Response: 3040827
Conc: N.D.

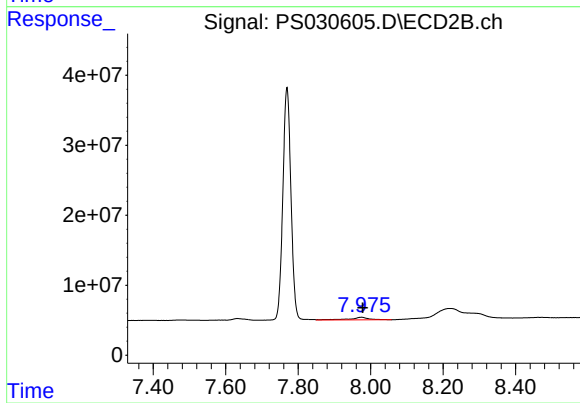

#5 DICAMBA


R.T.: 7.974 min
Delta R.T.: -0.005 min
Response: 14463853
Conc: 2.25 ng/ml

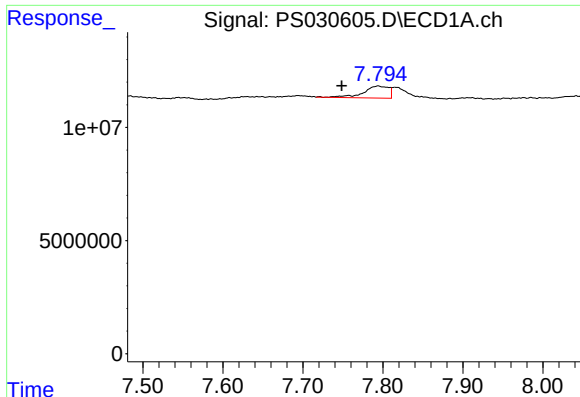

#6 MCP


R.T.: 7.794 min
Delta R.T.: 0.045 min
Response: 11469380
Conc: 1.16 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

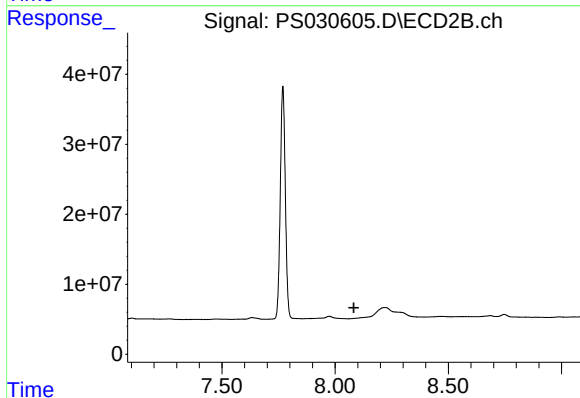


#6 MCP

R.T.: 0.000 min
Exp R.T. : 8.083 min
Response: 0
Conc: N.D.

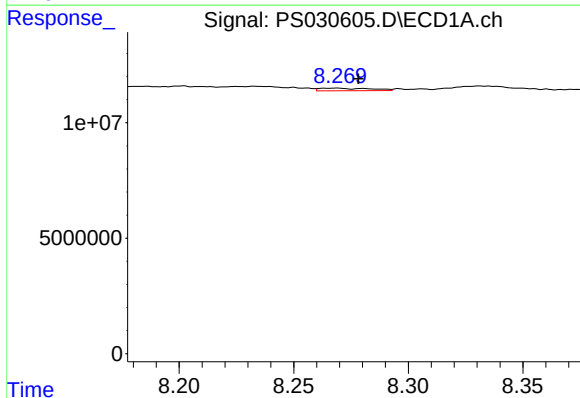


#8 DICHLORPROP

R.T.: 8.269 min
Delta R.T.: -0.009 min
Response: 1701180
Conc: N.D.

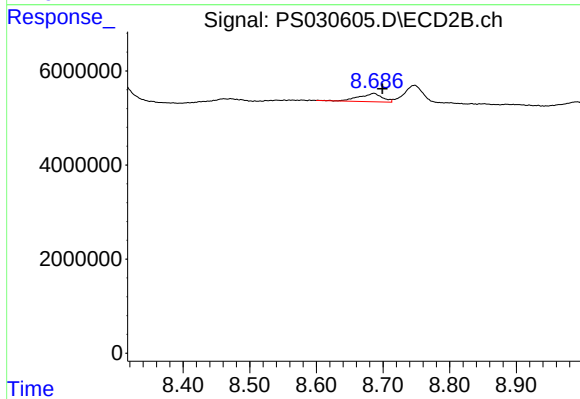

#8 DICHLORPROP


R.T.: 8.686 min
Delta R.T.: -0.013 min
Response: 4293820
Conc: 2.89 ng/ml

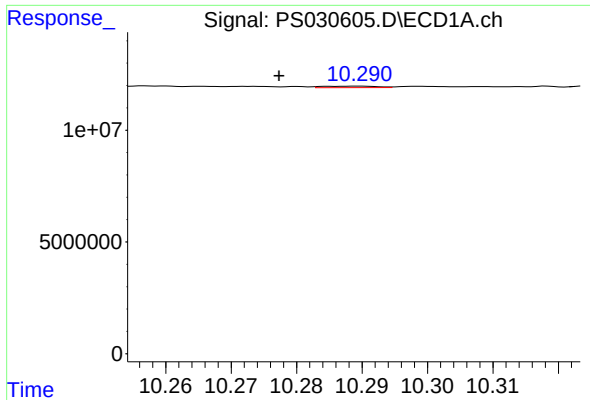

#13 2,4-DB

R.T.: 10.288 min
Delta R.T.: 0.011 min
Response: 388836
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

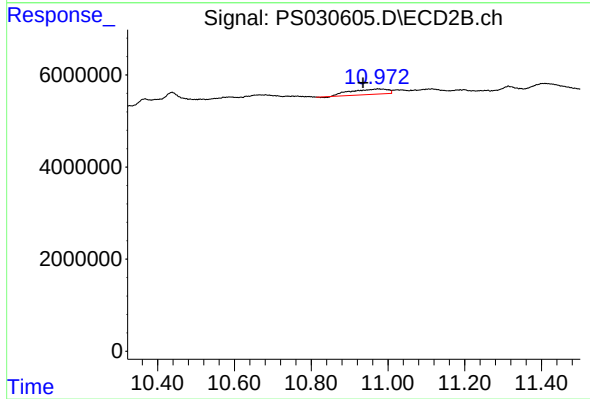

#13 2,4-DB

R.T.: 10.974 min
Delta R.T.: 0.039 min
Response: 7735176
Conc: 6.73 ng/ml