

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061119\
 Data File : PS005000.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2019 20:47
 Operator : SM\AJ
 Sample : PB120505TB
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 01:18:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.575	5.288	729.7E6	509.0E6	520.535	527.509
Target Compounds							
2) T	3,5-DICHL...	0.000	4.607	0	245.5E6	N.D.	199.270
3) T	4-Nitroph...	5.379	0.000	32218288	0	51.673	N.D. #
5) T	DICAMBA	0.000	5.395	0	13369610	N.D.	3.619
6) T	MCP	5.930	0.000	10250086	0	2.462	N.D. #
7) T	MCPA	6.068	5.681	16852587	25910752	2.910	6.333 #
9) T	2,4-D	6.662	0.000	63052736	0	46.094	N.D. #
10) T	Pentachlo...	6.862	6.631	17743611	19598934	1.010	1.595 #
11) T	2,4,5-TP ...	0.000	6.944	0	96778434	N.D.	18.809
13) T	2,4-DB	8.232	0.000	25423234	0	26.319	N.D. #
14) T	DINOSEB	0.000	8.153	0	44081045	N.D.	11.467



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061119\
Data File : PS005000.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2019 20:47
Operator : SM\AJ
Sample : PB120505TB
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 01:18:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

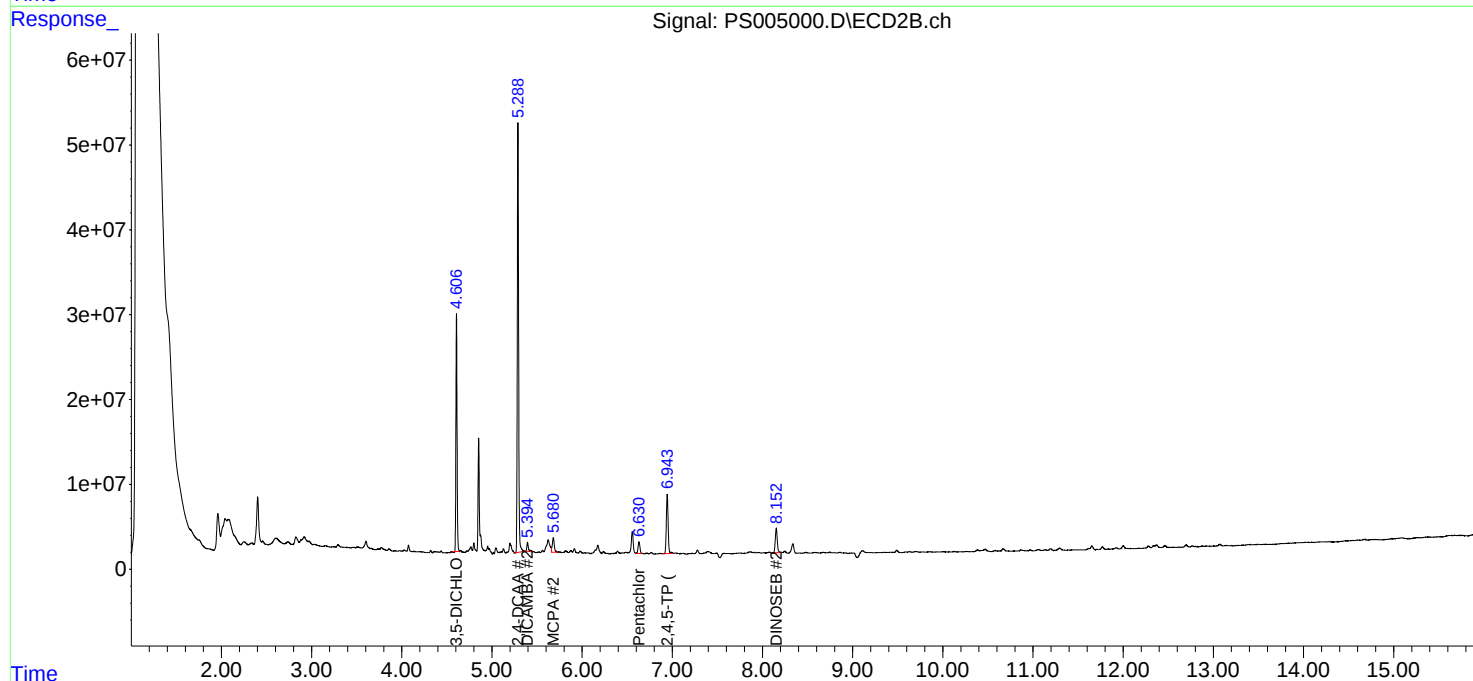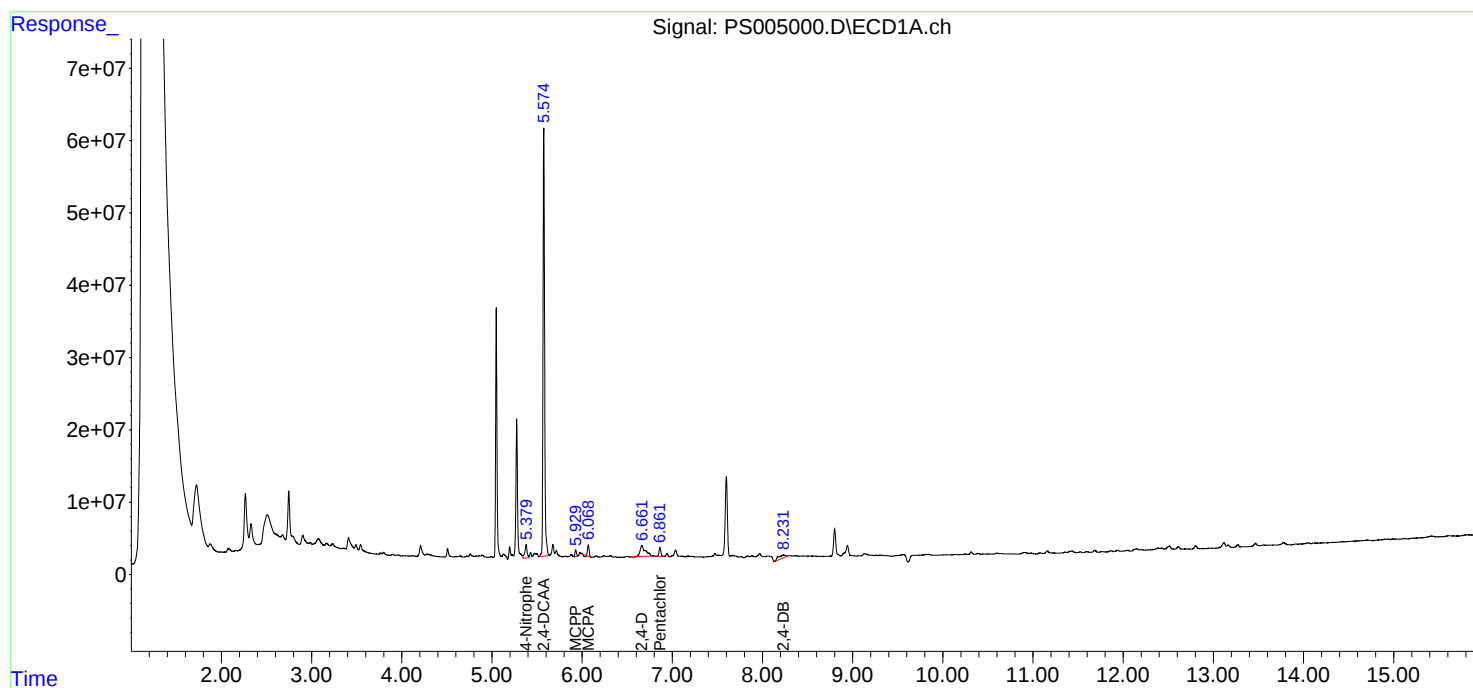


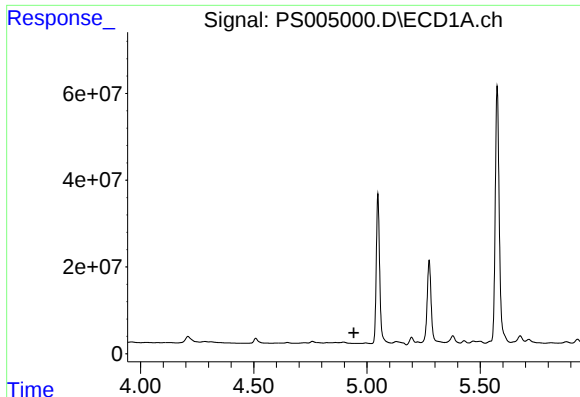

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

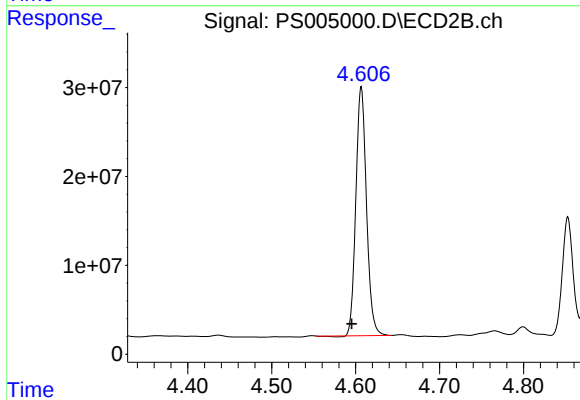


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.607 min
Delta R.T.: 0.011 min
Response: 245525879
Conc: 199.27 ng/ml

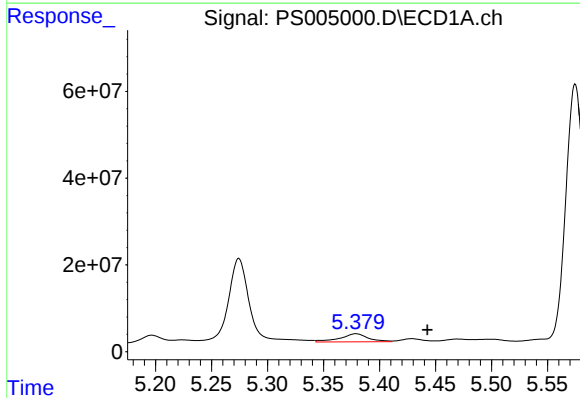


#3 4-Nitrophenol

R.T.: 5.379 min
Delta R.T.: -0.064 min
Response: 32218288
Conc: 51.67 ng/ml

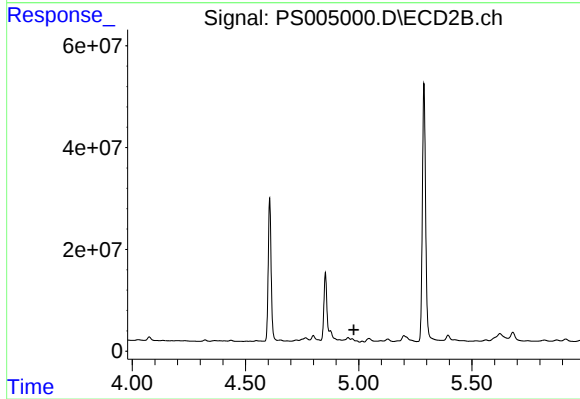

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

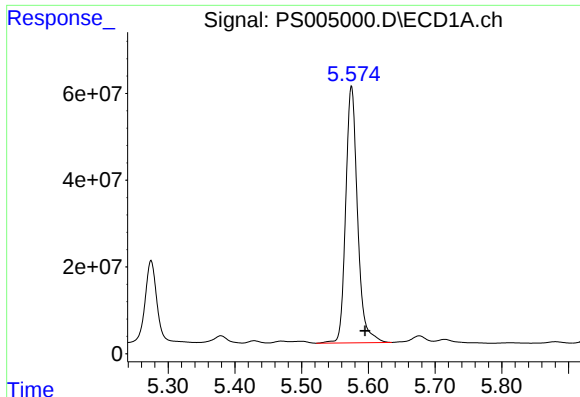

#4 2,4-DCAA


R.T.: 5.575 min
Delta R.T.: -0.020 min
Response: 729662462
Conc: 520.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

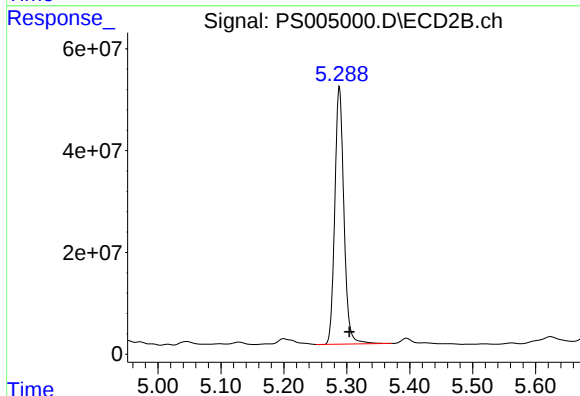


#4 2,4-DCAA

R.T.: 5.288 min
Delta R.T.: -0.016 min
Response: 508959967
Conc: 527.51 ng/ml

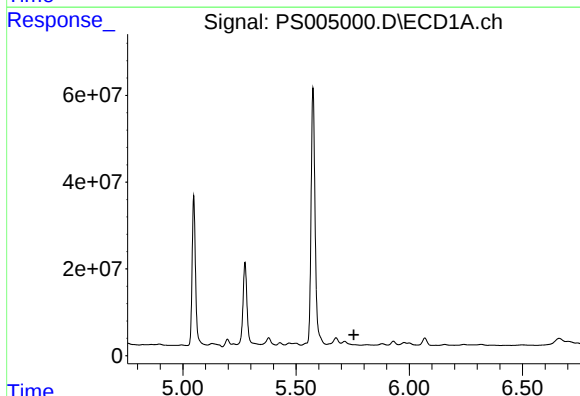


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.755 min
Response: 0
Conc: N.D.

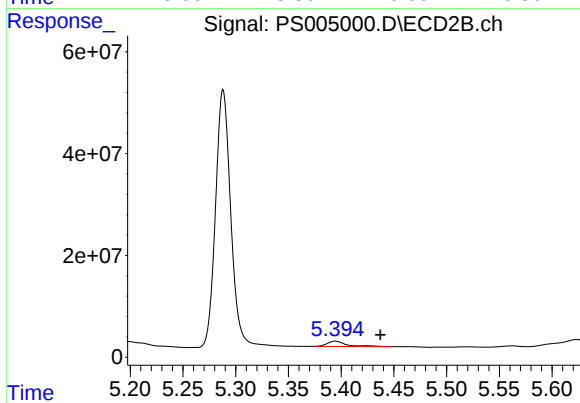

#5 DICAMBA


R.T.: 5.395 min
Delta R.T.: -0.043 min
Response: 13369610
Conc: 3.62 ng/ml

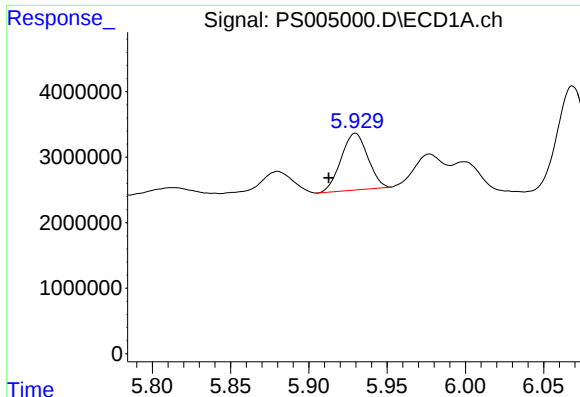

#6 MCPP


R.T.: 5.930 min
Delta R.T.: 0.017 min
Response: 10250086
Conc: 2.46 ug/ml

Instrument :
ECD_S
ClientSampleId :

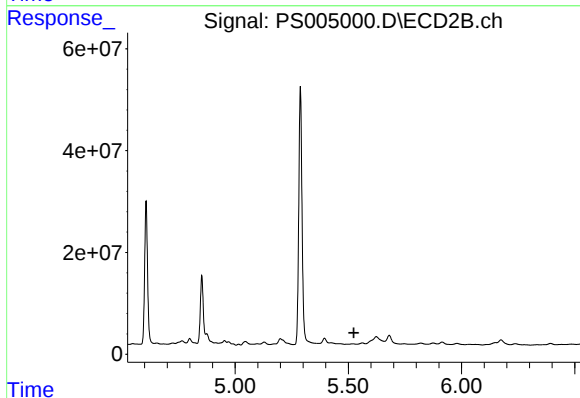


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

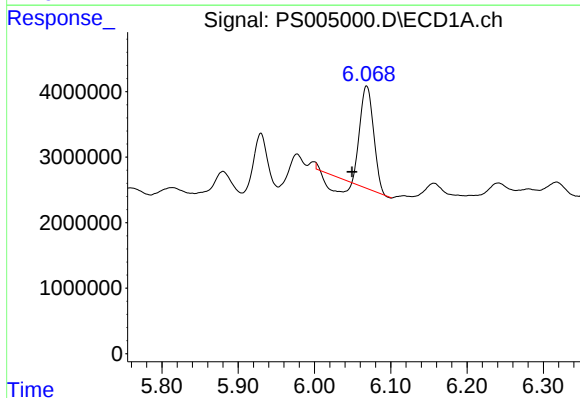


#7 MCPA

R.T.: 6.068 min
Delta R.T.: 0.019 min
Response: 16852587
Conc: 2.91 ug/ml

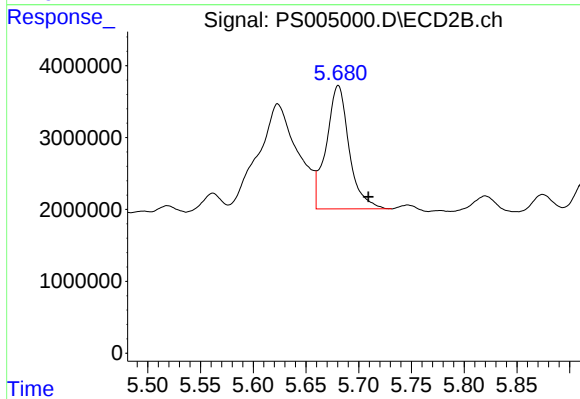

#7 MCPA


R.T.: 5.681 min
Delta R.T.: -0.029 min
Response: 25910752
Conc: 6.33 ug/ml

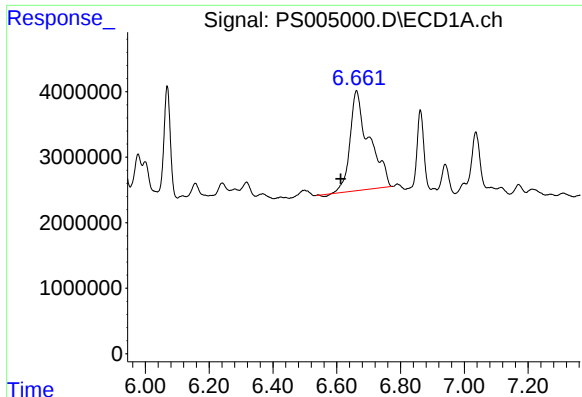

#9 2,4-D


R.T.: 6.662 min
Delta R.T.: 0.050 min
Response: 63052736
Conc: 46.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

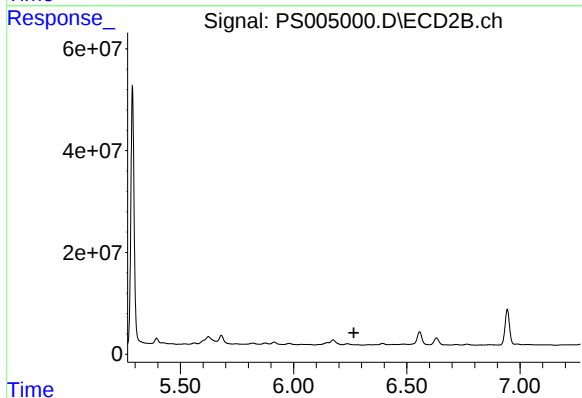


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

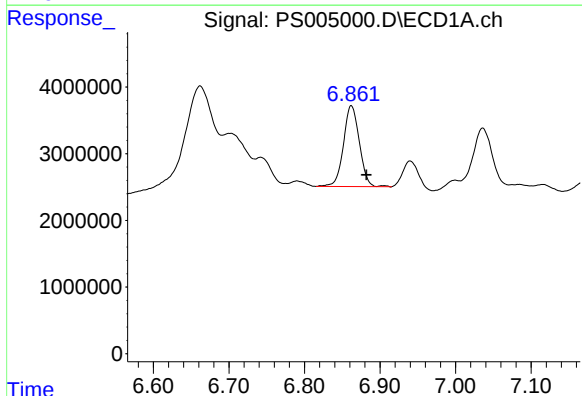


#10 Pentachlorophenol

R.T.: 6.862 min
Delta R.T.: -0.020 min
Response: 17743611
Conc: 1.01 ng/ml

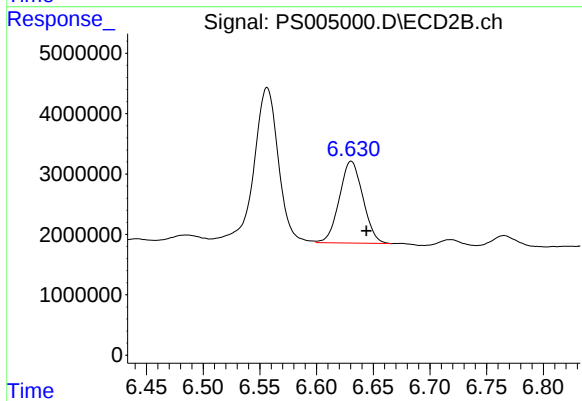

#10 Pentachlorophenol


R.T.: 6.631 min
Delta R.T.: -0.013 min
Response: 19598934
Conc: 1.60 ng/ml

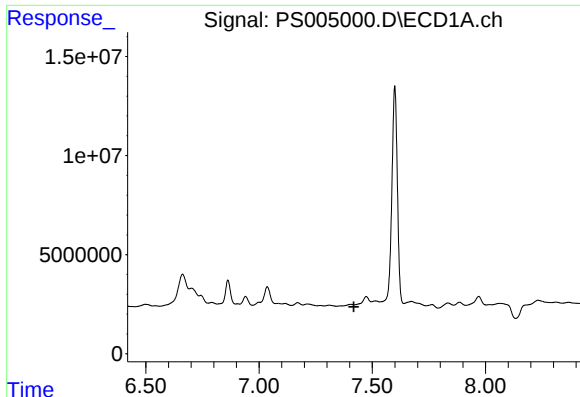

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

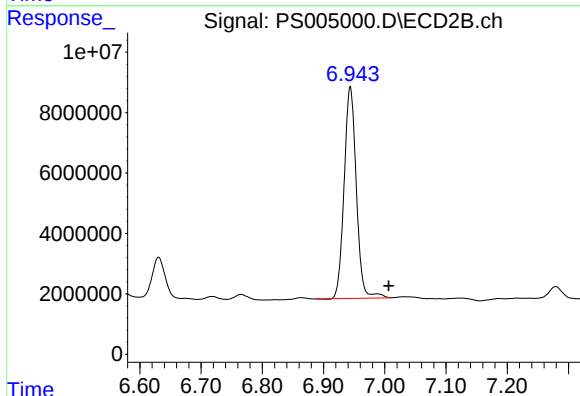


#11 2,4,5-TP (SILVEX)

R.T.: 6.944 min
Delta R.T.: -0.063 min
Response: 96778434
Conc: 18.81 ng/ml

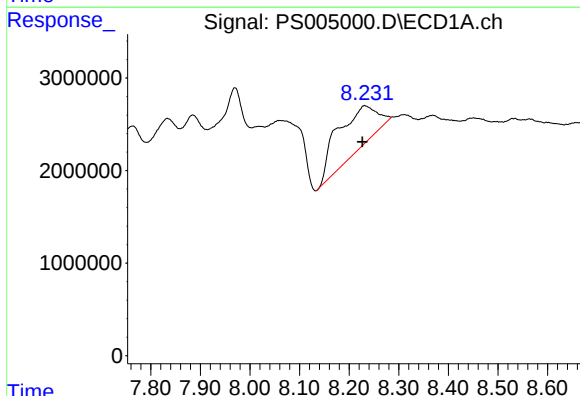


#13 2,4-DB

R.T.: 8.232 min
Delta R.T.: 0.005 min
Response: 25423234
Conc: 26.32 ng/ml

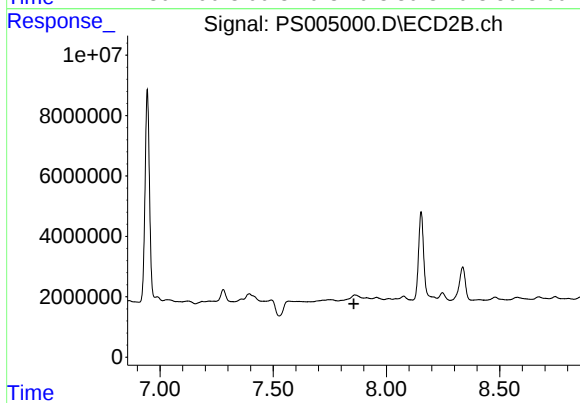

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 7.856 min
Response: 0
Conc: N.D.

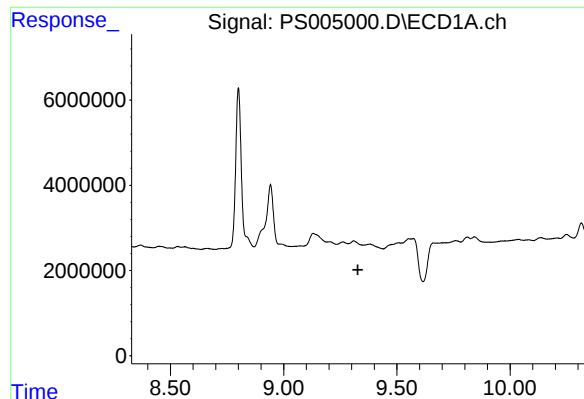

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

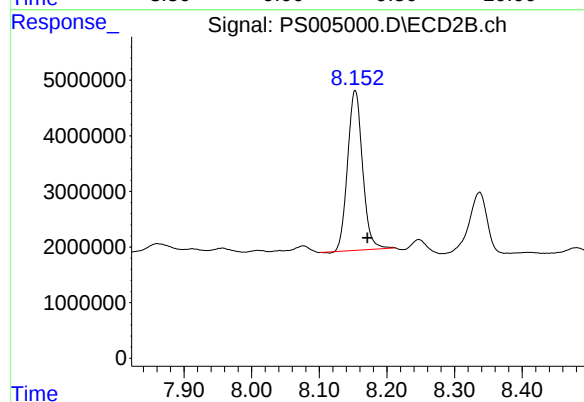

#14 DINOSEB

R.T.: 8.153 min
Delta R.T.: -0.018 min
Response: 44081045
Conc: 11.47 ng/ml