

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061119\
 Data File : PS005002.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2019 21:31
 Operator : SM\AJ
 Sample : K3163-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 01:19:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.609	5.323	442.0E6	289.9E6	315.353	300.457
Target Compounds							
1) T	Dalapon	2.112	0.000	21551618	0	13.001	N.D. #
2) T	3,5-DICHL...	0.000	4.641	0	250.1E6	N.D.	202.958
5) T	DICAMBA	5.710	5.428	23728093	16626003	4.469	4.501
6) T	MCPD	5.964	0.000	8665389	0	2.082	N.D. #
7) T	MCPA	6.041	5.659	81560317	17922629	14.081	4.380 #
9) T	2,4-D	0.000	6.206	0	29965091	N.D.	27.723
10) T	Pentachlo...	0.000	6.591	0	28484707	N.D.	2.319
11) T	2,4,5-TP ...	0.000	6.978	0	168.7E6	N.D.	32.789
12) T	2,4,5-T	7.635	0.000	286.4E6	0	38.458	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061119\
Data File : PS005002.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2019 21:31
Operator : SM\AJ
Sample : K3163-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 01:19:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

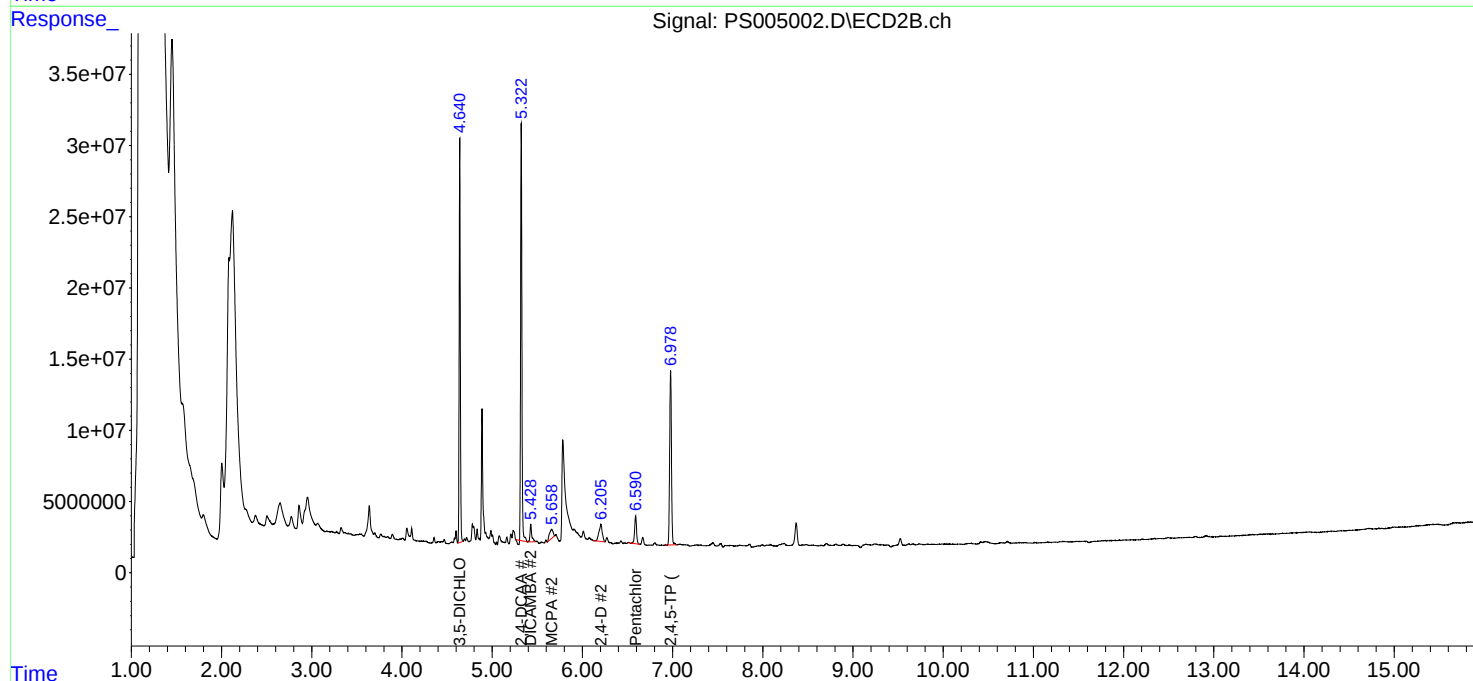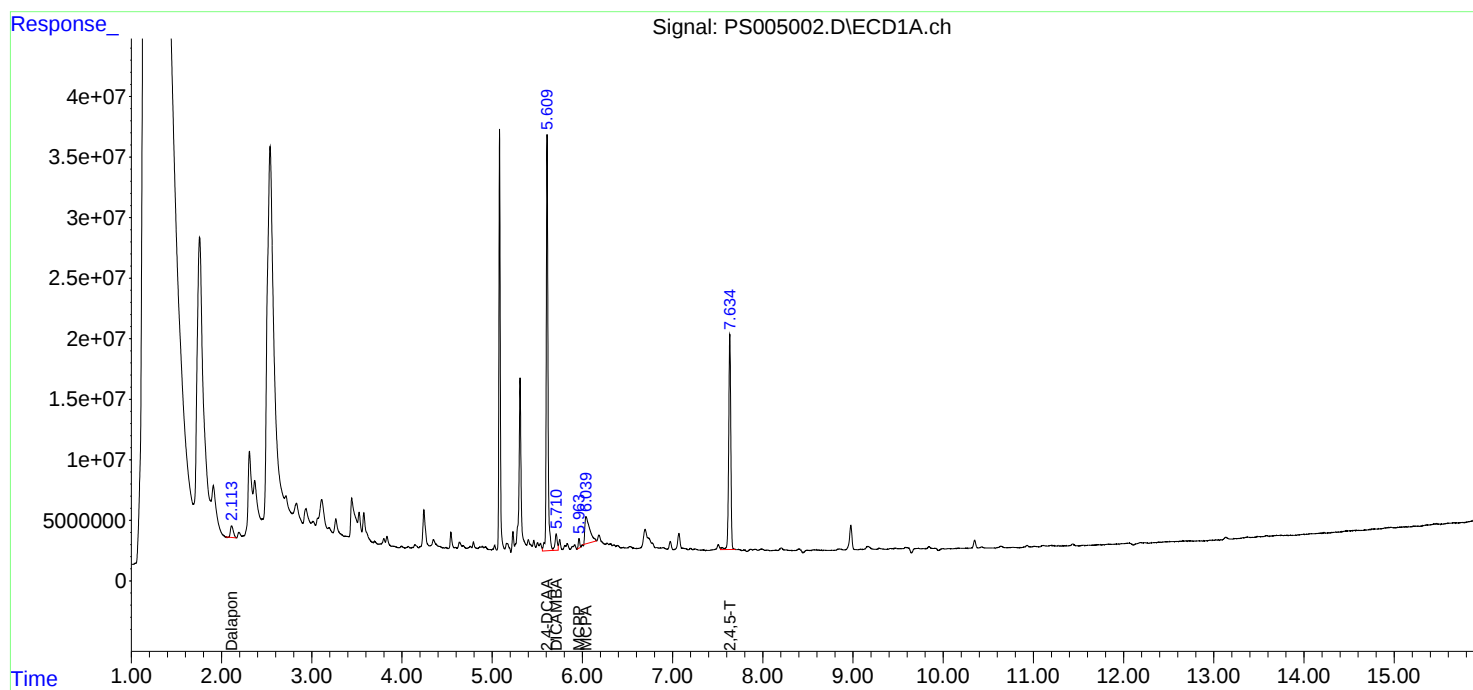


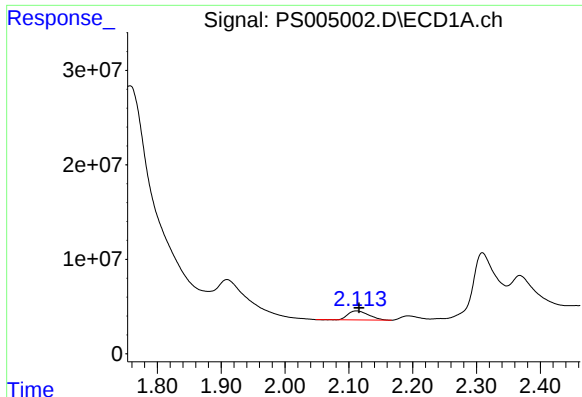

#1 Dalapon


R.T.: 2.112 min
Delta R.T.: -0.004 min
Response: 21551618
Conc: 13.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

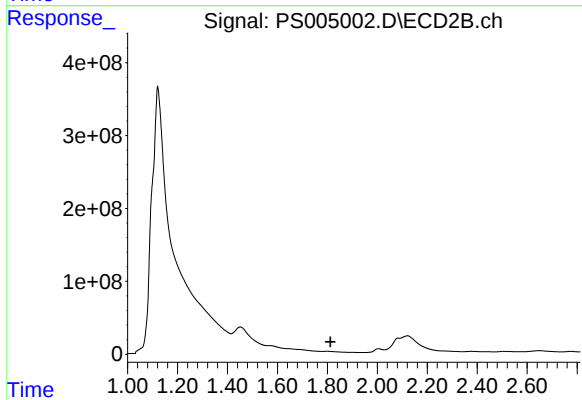


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.813 min
Response: 0
Conc: N.D.

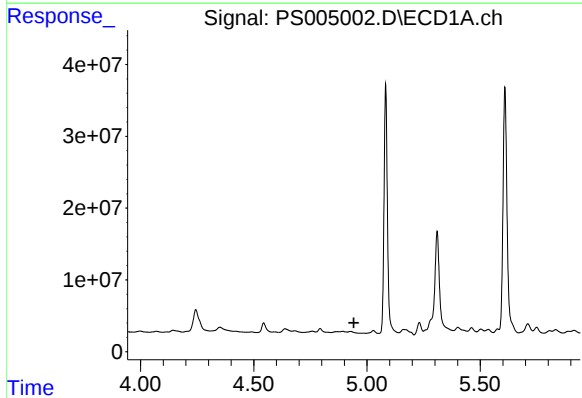


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

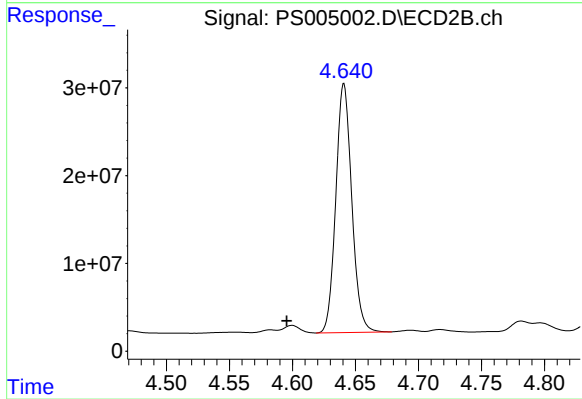

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.641 min
Delta R.T.: 0.045 min
Response: 250070024
Conc: 202.96 ng/ml

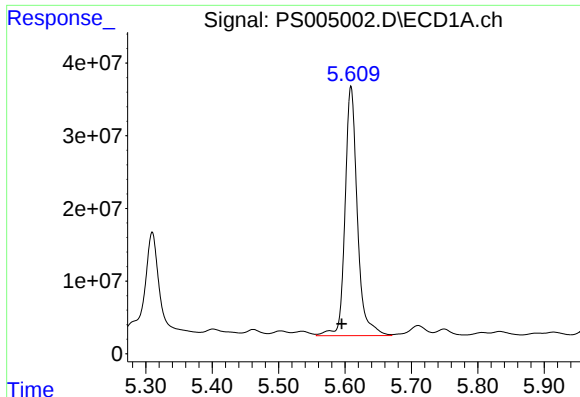

#4 2,4-DCAA


R.T.: 5.609 min
Delta R.T.: 0.014 min
Response: 442048496
Conc: 315.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

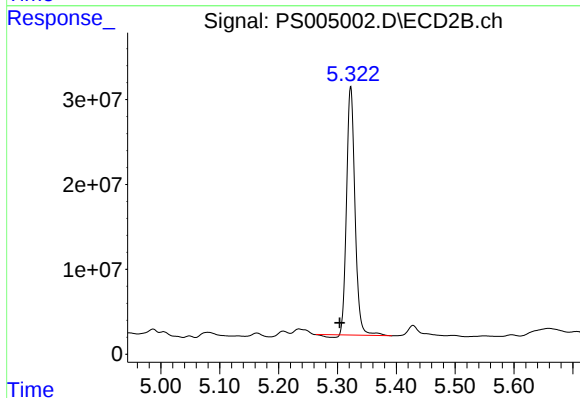


#4 2,4-DCAA

R.T.: 5.323 min
Delta R.T.: 0.019 min
Response: 289891859
Conc: 300.46 ng/ml

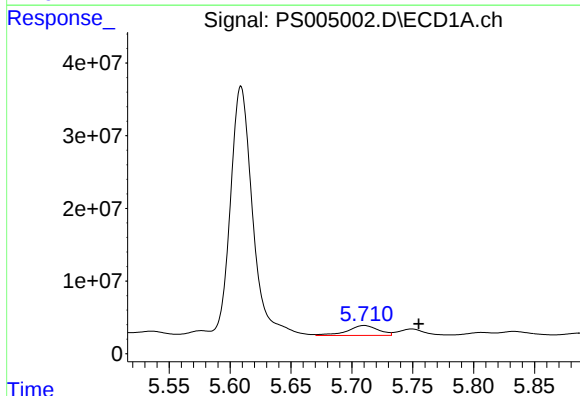


#5 DICAMBA

R.T.: 5.710 min
Delta R.T.: -0.045 min
Response: 23728093
Conc: 4.47 ng/ml

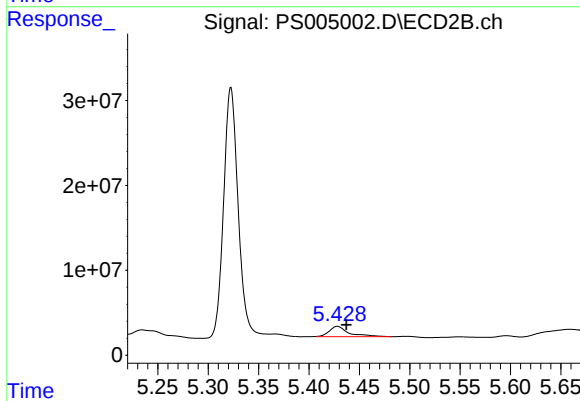

#5 DICAMBA


R.T.: 5.428 min
Delta R.T.: -0.009 min
Response: 16626003
Conc: 4.50 ng/ml

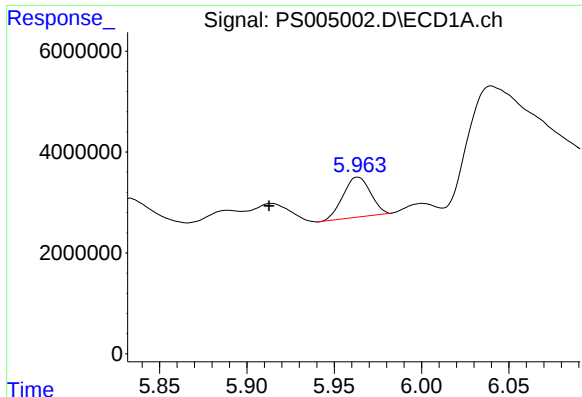

#6 MCPP


R.T.: 5.964 min
Delta R.T.: 0.051 min
Response: 8665389
Conc: 2.08 ug/ml

Instrument :
ECD_S
ClientSampleId :

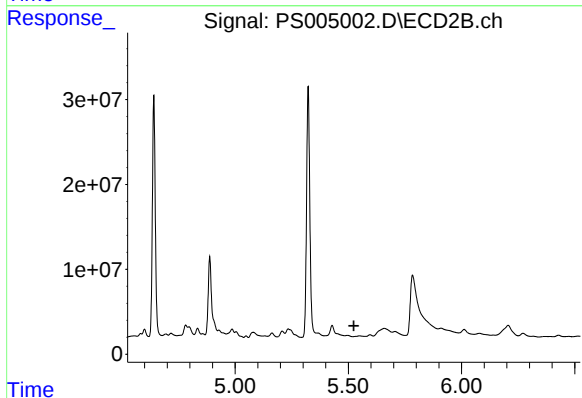


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

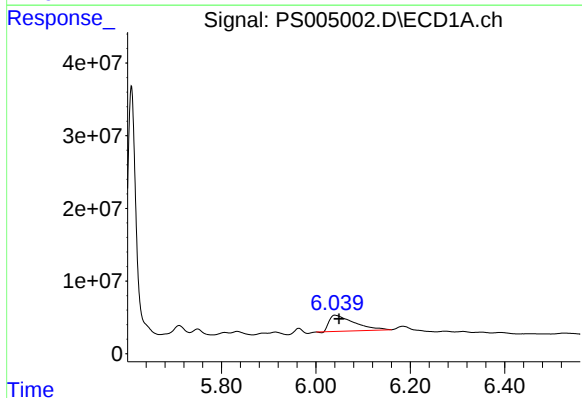


#7 MCPA

R.T.: 6.041 min
Delta R.T.: -0.008 min
Response: 81560317
Conc: 14.08 ug/ml

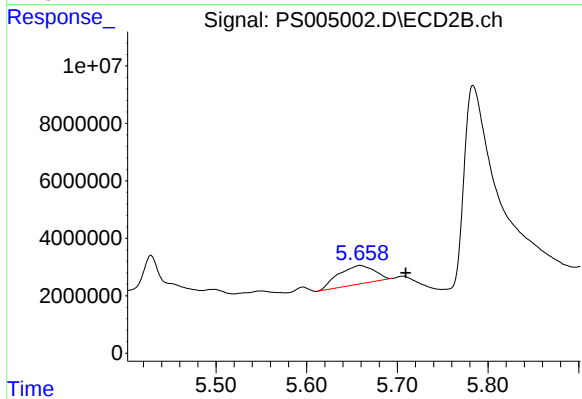

#7 MCPA


R.T.: 5.659 min
Delta R.T.: -0.050 min
Response: 17922629
Conc: 4.38 ug/ml

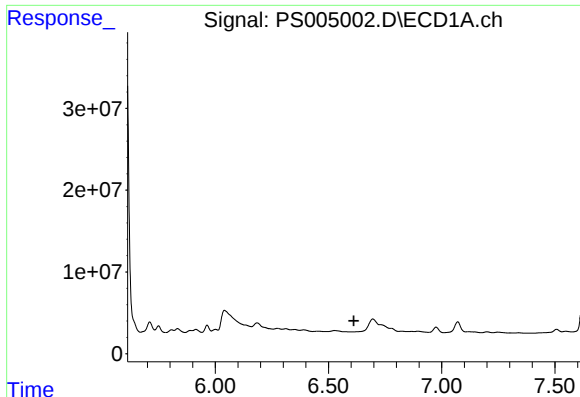

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.612 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

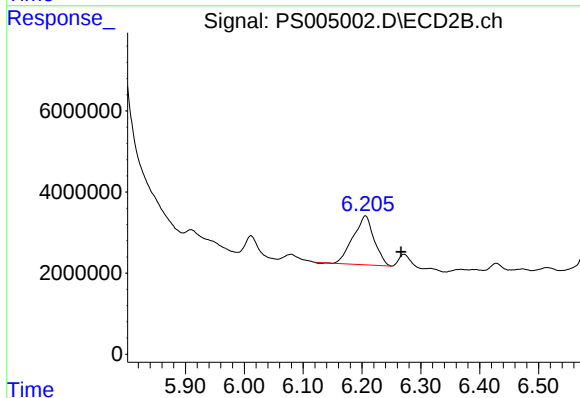


#9 2,4-D

R.T.: 6.206 min
Delta R.T.: -0.061 min
Response: 29965091
Conc: 27.72 ng/ml

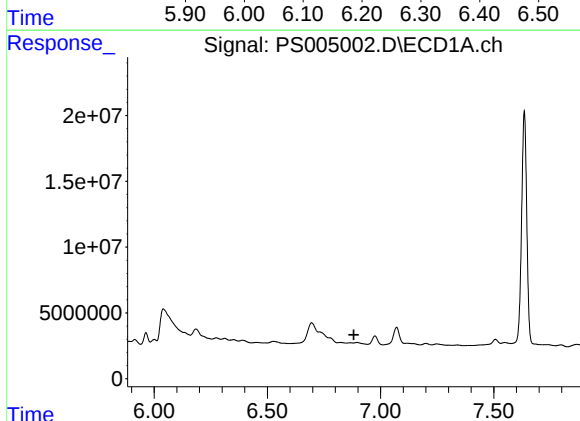


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.882 min
Response: 0
Conc: N.D.

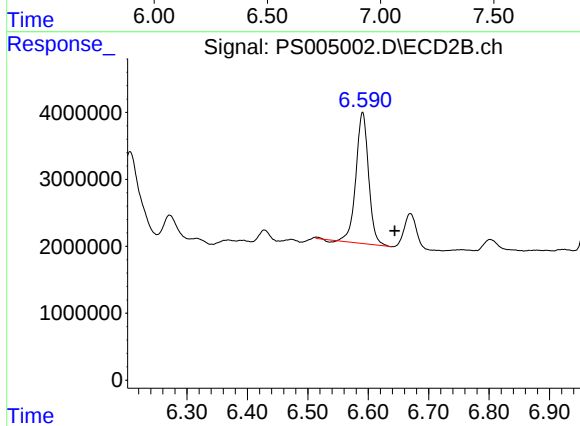

#10 Pentachlorophenol


R.T.: 6.591 min
Delta R.T.: -0.053 min
Response: 28484707
Conc: 2.32 ng/ml

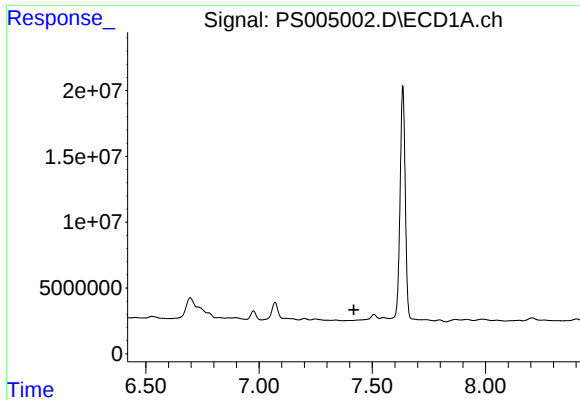

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

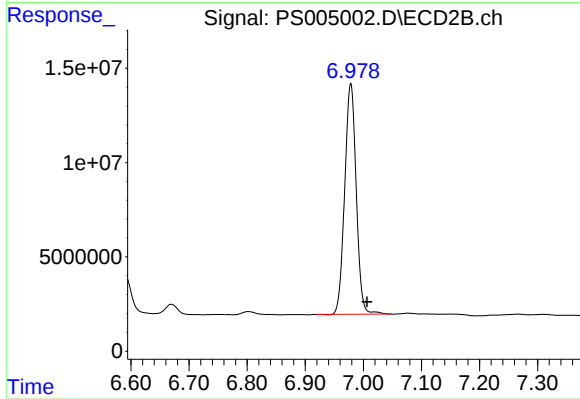


#11 2,4,5-TP (SILVEX)

R.T.: 6.978 min
Delta R.T.: -0.028 min
Response: 168708338
Conc: 32.79 ng/ml

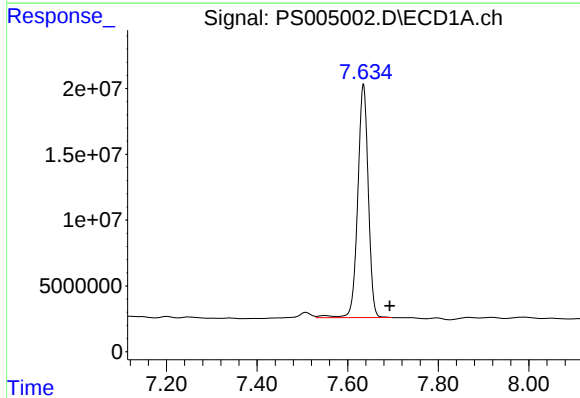

#12 2,4,5-T

R.T.: 7.635 min
Delta R.T.: -0.059 min
Response: 286413417
Conc: 38.46 ng/ml

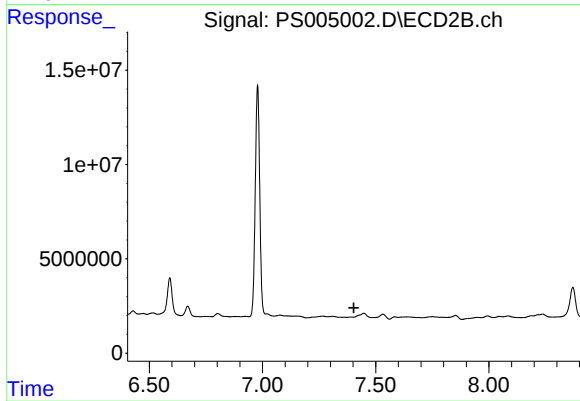

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.404 min
Response: 0
Conc: N.D.