

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061119\
 Data File : PS005003.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2019 21:53
 Operator : SM\AJ
 Sample : K3262-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 STOCK-PILE-1

Manual Integrations
 APPROVED

Ankita
 6/12/2019 2:28:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 01:19:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	5.590	5.302	422.0E6	282.6E6	301.022	292.905m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061119\
Data File : PS005003.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2019 21:53
Operator : SM\AJ
Sample : K3262-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
STOCK-PILE-1


Manual Integrations
APPROVED

Ankita
6/12/2019 2:28:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 01:19:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

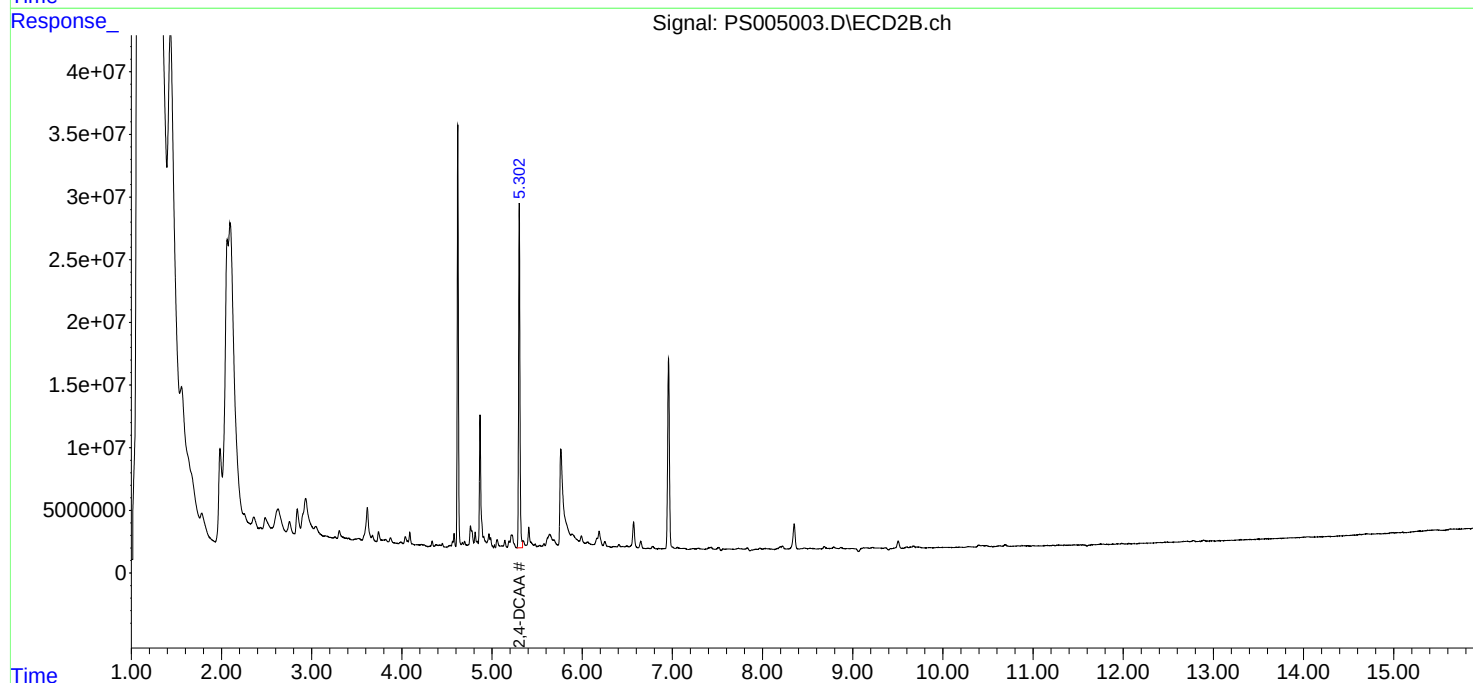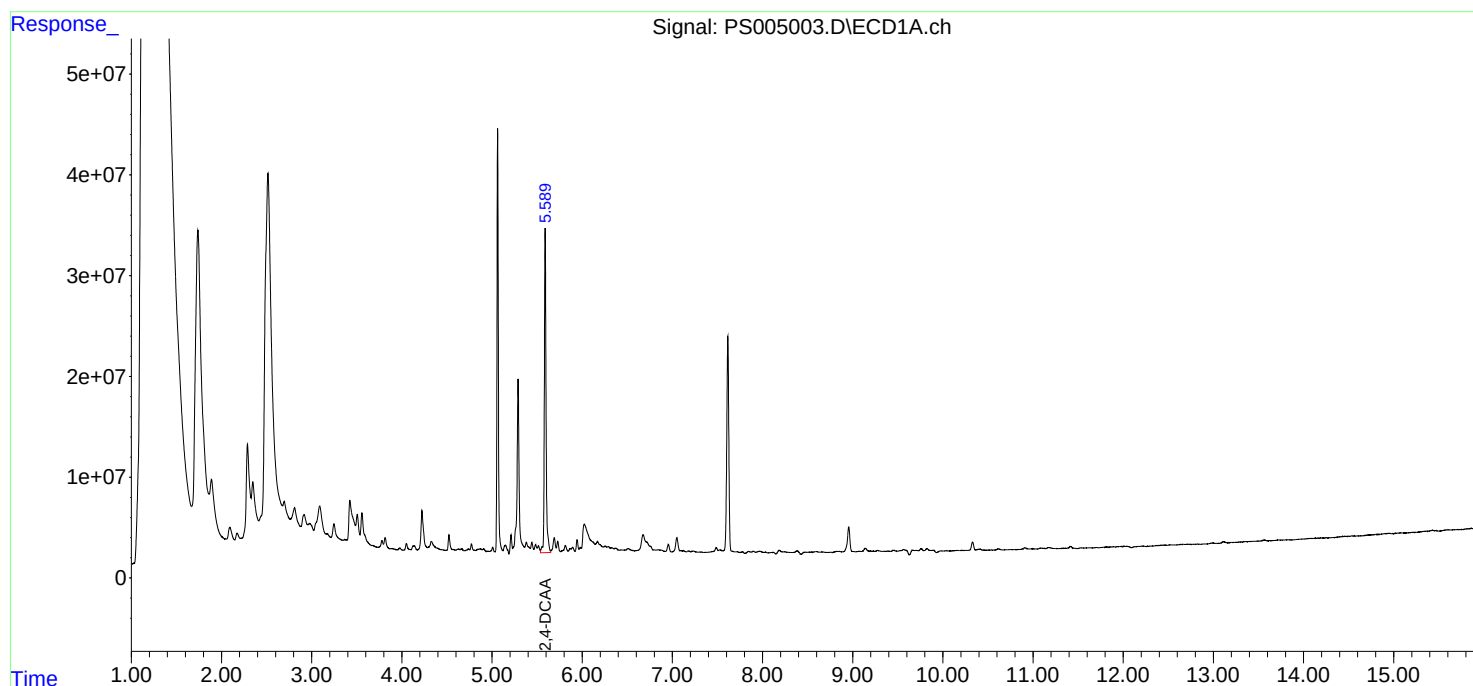

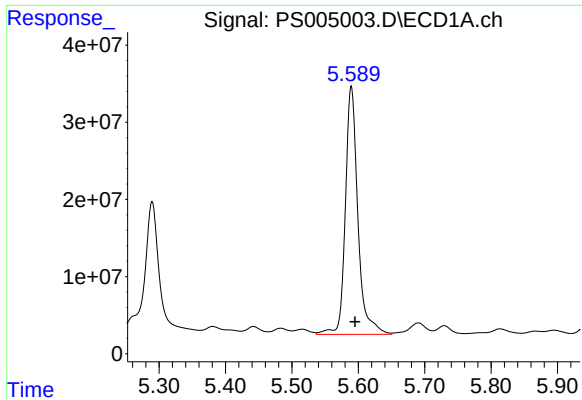


#4 2,4-DCAA

R.T.: 5.590 min
Delta R.T.: -0.006 min
Response: 421959617
Conc: 301.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
STOCK-PILE-1

Manual Integrations
APPROVED

Ankita
6/12/2019 2:28:24 PM

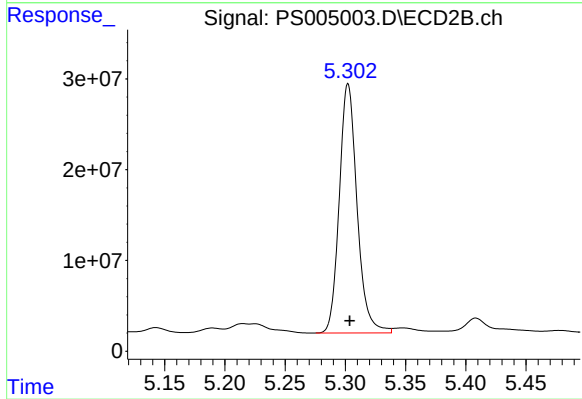

#4 2,4-DCAA

R.T.: 5.302 min
Delta R.T.: -0.002 min
Response: 282605255
Conc: 292.90 ng/ml m