

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061120\
 Data File : PS010776.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2020 18:41
 Operator : DD\AJ
 Sample : PB129494BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 01:53:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.920	425.7E6	311.9E6	538.255	571.772
Target Compounds							
1) T	Dalapon	2.994	2.583	28086497	92165664	28.567	125.885 #
2) T	3,5-DICHL...	0.000	6.100	0	28425278	N.D.	34.680
3) T	4-Nitroph...	7.005	0.000	7306068	0	19.707	N.D. #
7) T	MCPA	7.777	7.385	48358304	39442284	13.833	14.513
8) T	DICHLORPROP	0.000	7.740	0	8211260	N.D.	14.240
10) T	Pentachlo...	8.710	0.000	8544020	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.844	0	7362955	N.D.	2.452
12) T	2,4,5-T	9.431	0.000	26212589	0	6.445	N.D. #
14) T	DINOSEB	11.169	10.032	18034934	9590966	5.582	4.458
15) T	Picloram	10.995	0.000	38343873	0	7.511	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061120\
Data File : PS010776.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2020 18:41
Operator : DD\AJ
Sample : PB129494BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 01:53:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

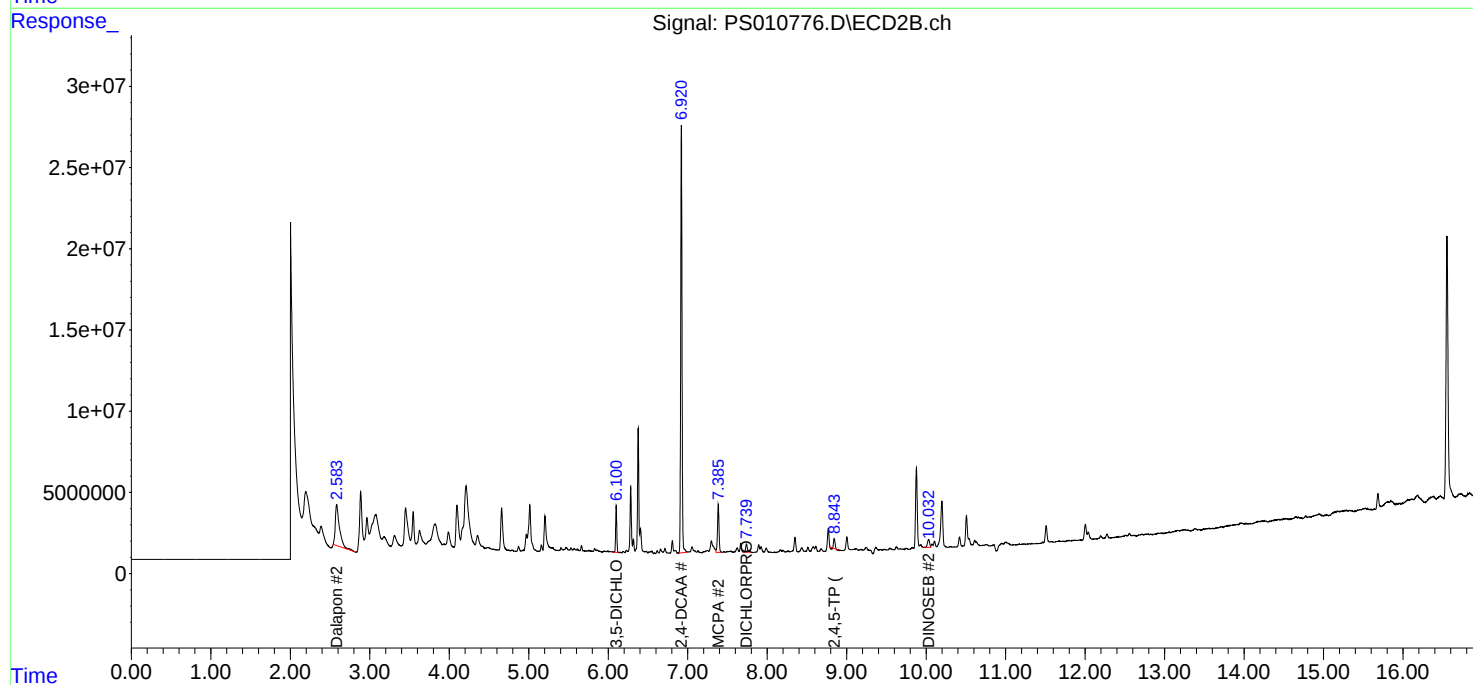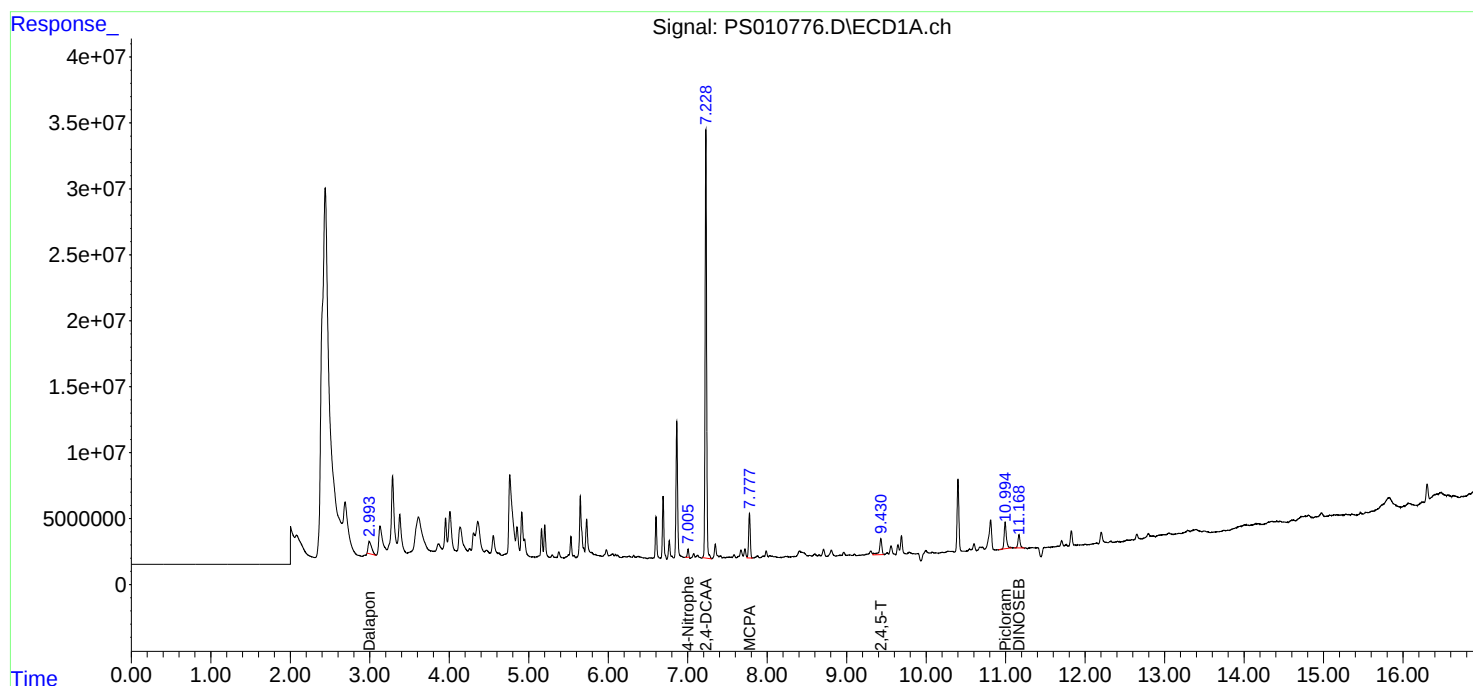


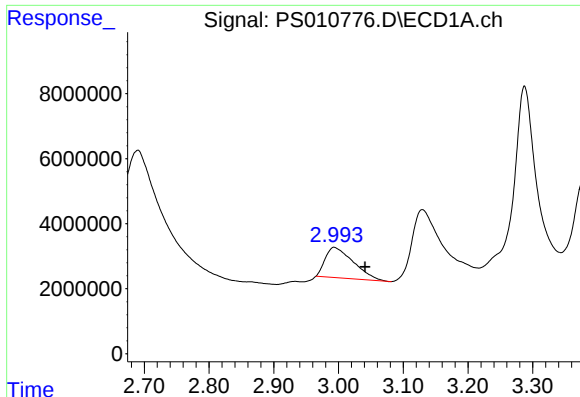

#1 Dalapon


R.T.: 2.994 min
Delta R.T.: -0.047 min
Response: 28086497
Conc: 28.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

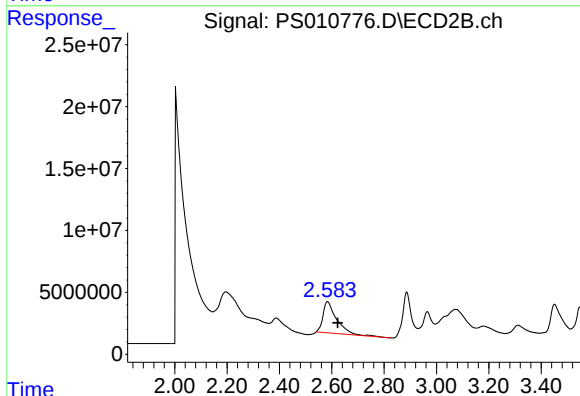


#1 Dalapon

R.T.: 2.583 min
Delta R.T.: -0.040 min
Response: 92165664
Conc: 125.88 ng/ml

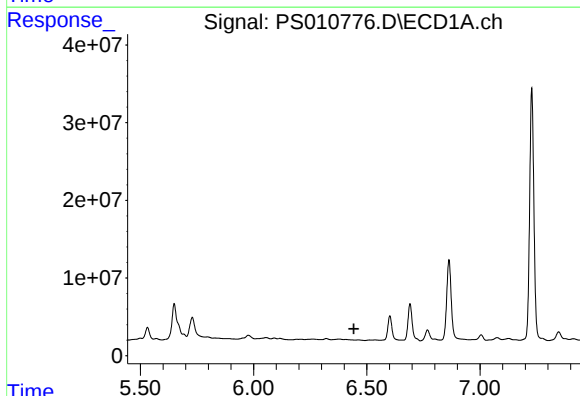


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

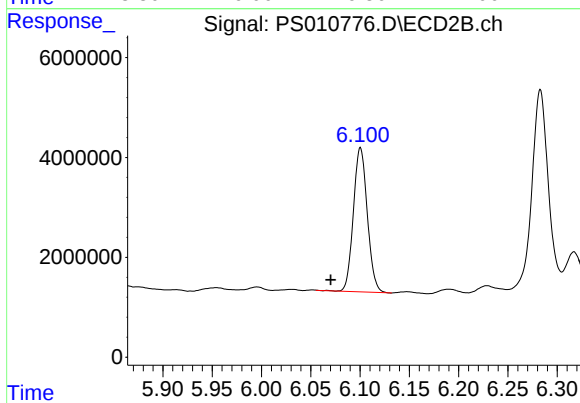

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 28425278
Conc: 34.68 ng/ml

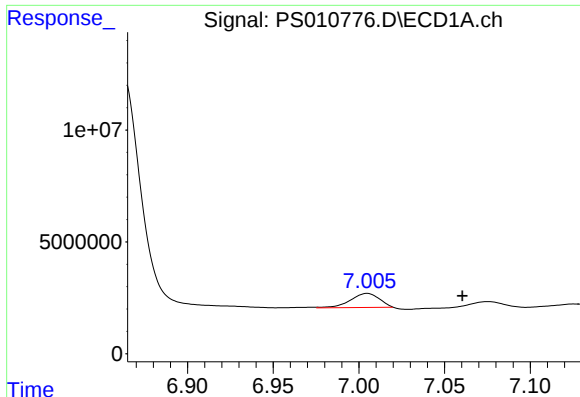

#3 4-Nitrophenol


R.T.: 7.005 min
Delta R.T.: -0.056 min
Response: 7306068
Conc: 19.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

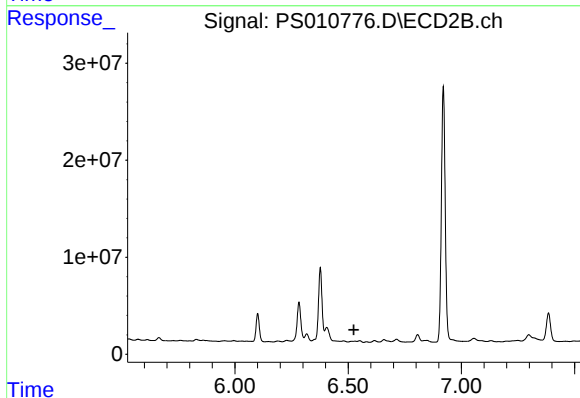


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.525 min
Response: 0
Conc: N.D.

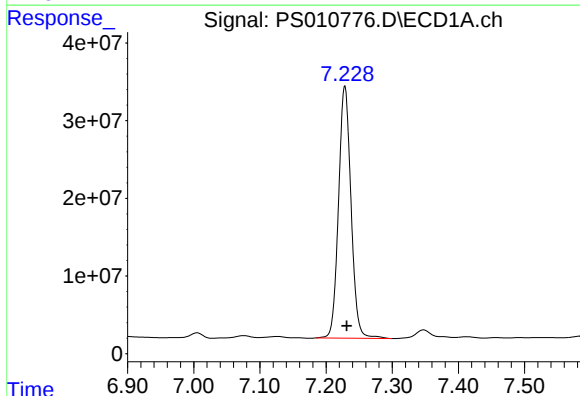


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: -0.003 min
Response: 425685394
Conc: 538.26 ng/ml

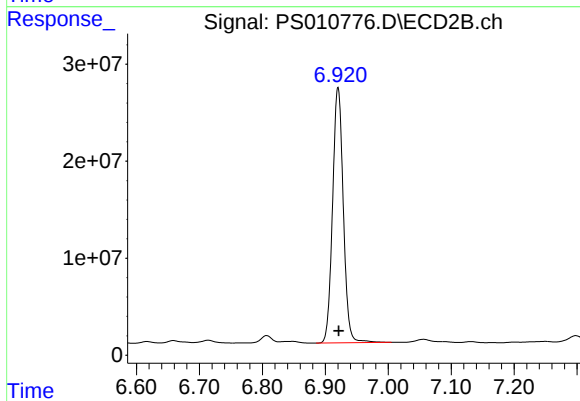

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: -0.001 min
Response: 311853406
Conc: 571.77 ng/ml

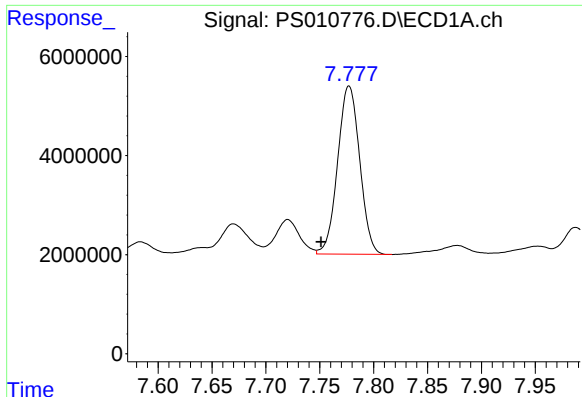

#7 MCPA


R.T.: 7.777 min
Delta R.T.: 0.026 min
Response: 48358304
Conc: 13.83 ug/ml

Instrument :
ECD_S
ClientSampleId :

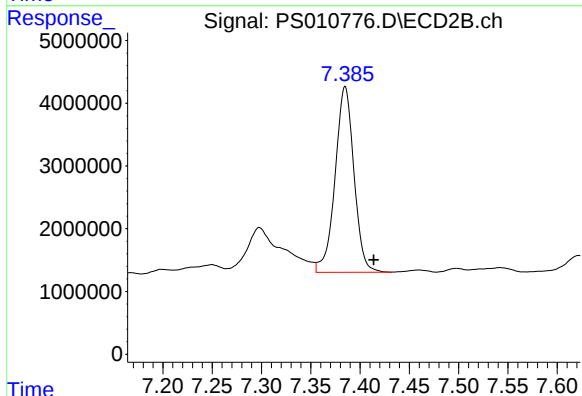


#7 MCPA

R.T.: 7.385 min
Delta R.T.: -0.029 min
Response: 39442284
Conc: 14.51 ug/ml

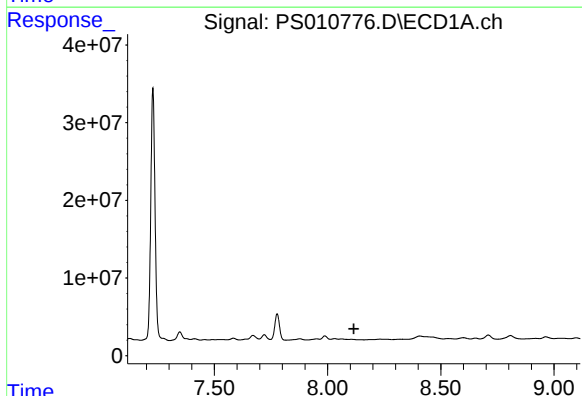


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.116 min
Response: 0
Conc: N.D.

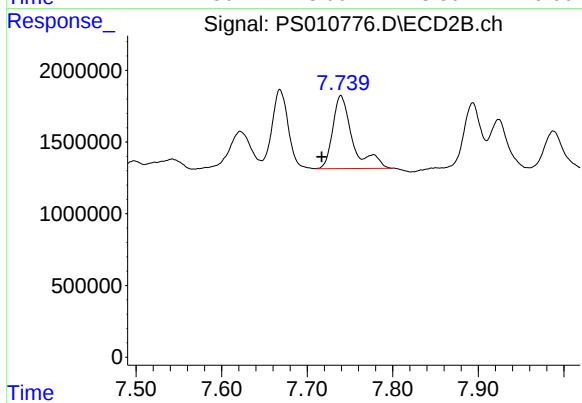

#8 DICHLORPROP


R.T.: 7.740 min
Delta R.T.: 0.022 min
Response: 8211260
Conc: 14.24 ng/ml

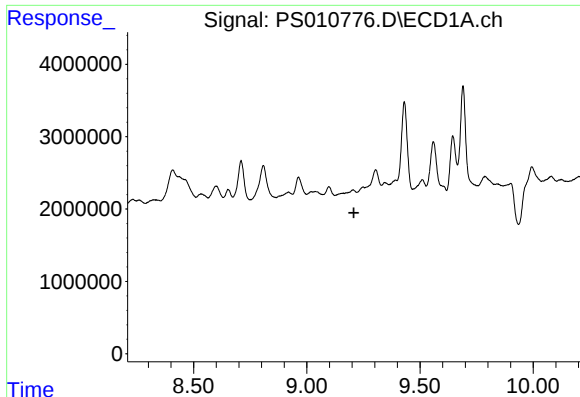

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.208 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

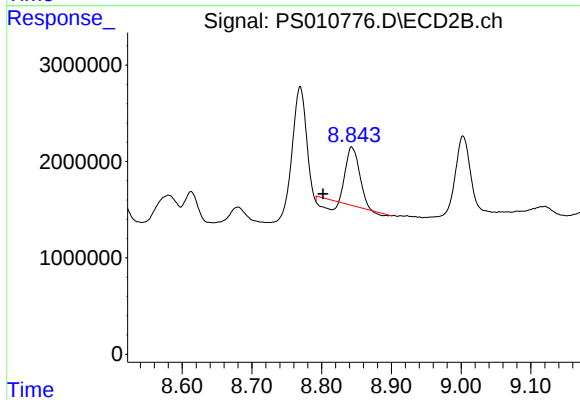


#11 2,4,5-TP (SILVEX)

R.T.: 8.844 min
Delta R.T.: 0.042 min
Response: 7362955
Conc: 2.45 ng/ml

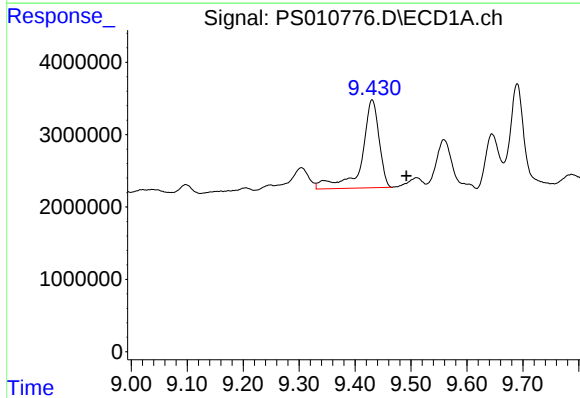


#12 2,4,5-T

R.T.: 9.431 min
Delta R.T.: -0.061 min
Response: 26212589
Conc: 6.45 ng/ml

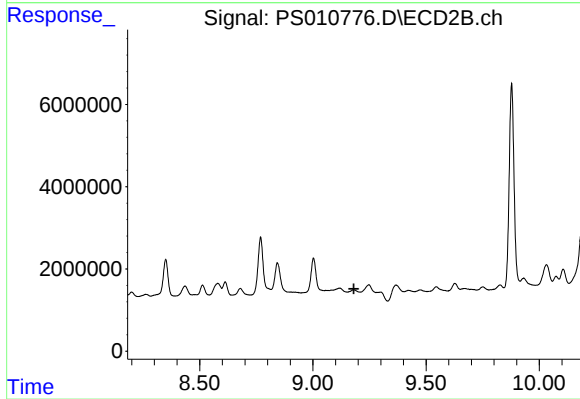

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.181 min
Response: 0
Conc: N.D.

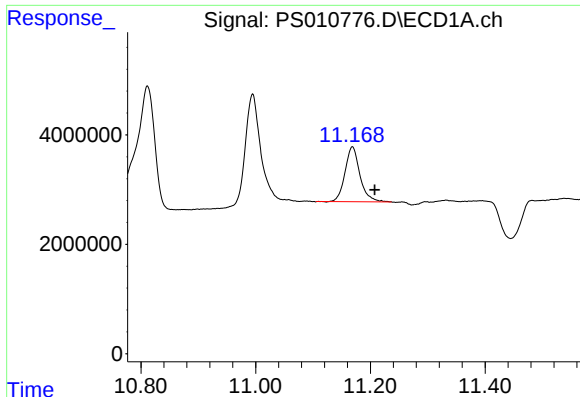

#14 DINOSEB


R.T.: 11.169 min
Delta R.T.: -0.039 min
Response: 18034934
Conc: 5.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

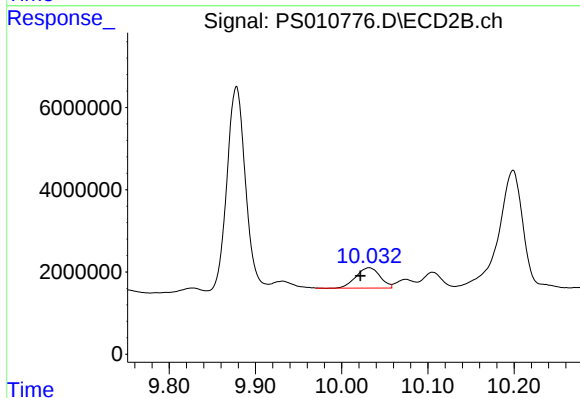


#14 DINOSEB

R.T.: 10.032 min
Delta R.T.: 0.010 min
Response: 9590966
Conc: 4.46 ng/ml

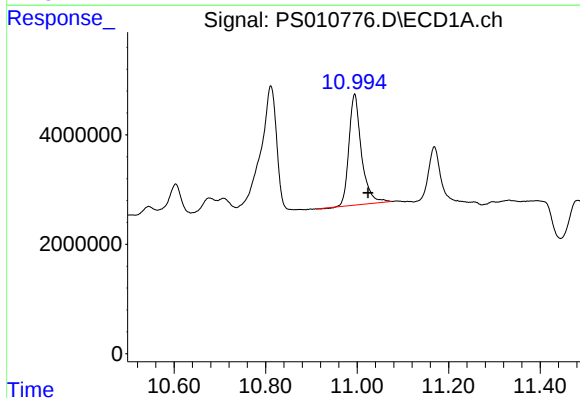

#15 Picloram

R.T.: 10.995 min
Delta R.T.: -0.030 min
Response: 38343873
Conc: 7.51 ng/ml

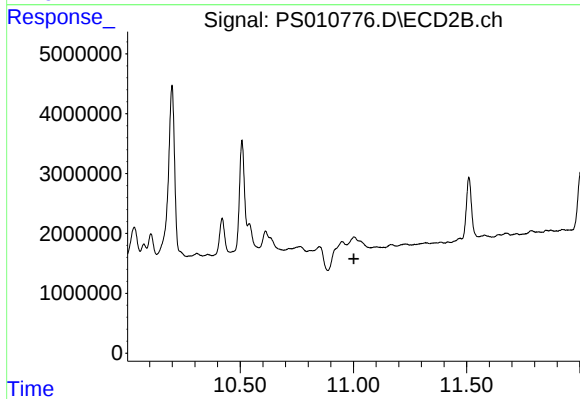

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.