

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061120\
 Data File : PS010785.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2020 22:08
 Operator : DD\AJ
 Sample : L2819-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 01:56:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.920	252.6E6	180.0E6	319.386	330.047
Target Compounds							
1) T	Dalapon	2.994	2.585	34715613	117.3E6	35.309	160.270 #
2) T	3,5-DICHL...	0.000	6.100	0	118.7E6	N.D.	144.851
3) T	4-Nitroph...	6.998	6.552	7763957	7223075	20.942	21.805
5) T	DICAMBA	7.408	7.054	7215192	13741366	2.295	6.105 #
7) T	MCPA	7.682	7.455	148.1E6	94472748	42.376	34.761
8) T	DICHLORPROP	8.060	7.738	7824945	16602819	10.324	28.793 #
10) T	Pentachlo...	8.710	0.000	10186513	0	<MDL	N.D. #
12) T	2,4,5-T	9.428	0.000	60803991	0	14.951	N.D. #
14) T	DINOSEB	11.167	10.066	18752308	77501336	5.804	36.023 #
15) T	Picloram	10.994	0.000	111.2E6	0	21.788	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061120\
Data File : PS010785.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2020 22:08
Operator : DD\AJ
Sample : L2819-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 01:56:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

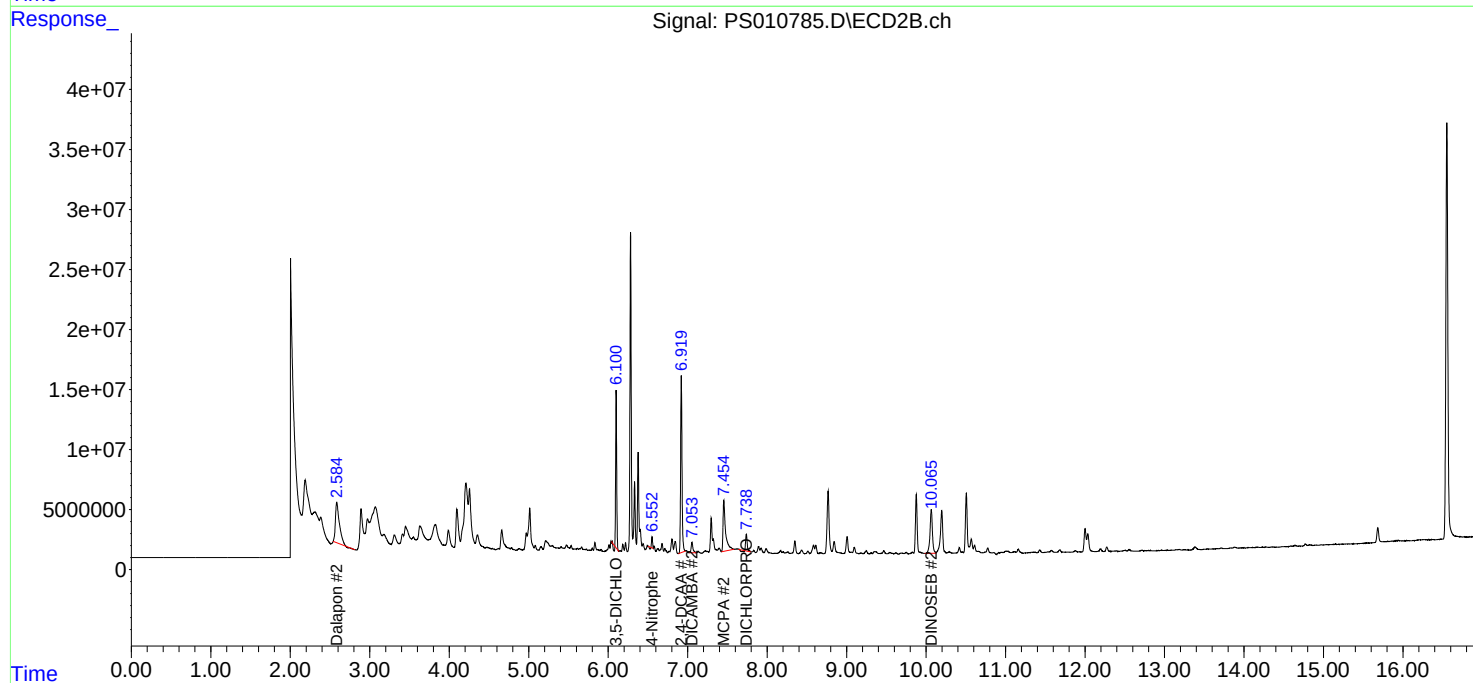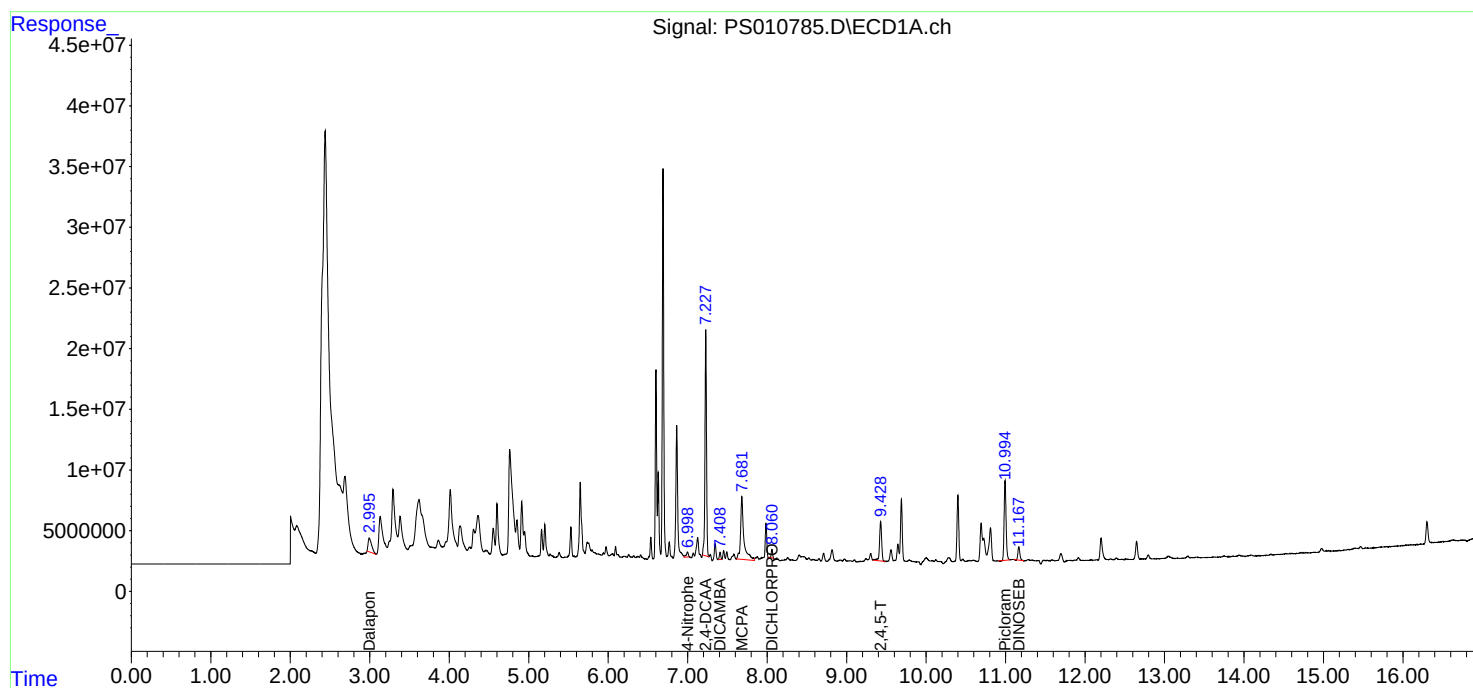


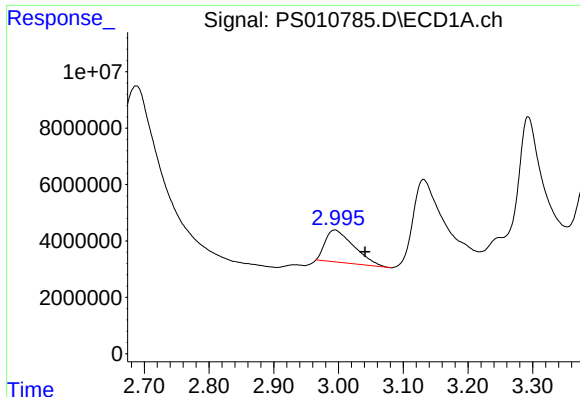

#1 Dalapon


R.T.: 2.994 min
Delta R.T.: -0.047 min
Response: 34715613
Conc: 35.31 ng/ml

Instrument :
ECD_S
ClientSampleId :

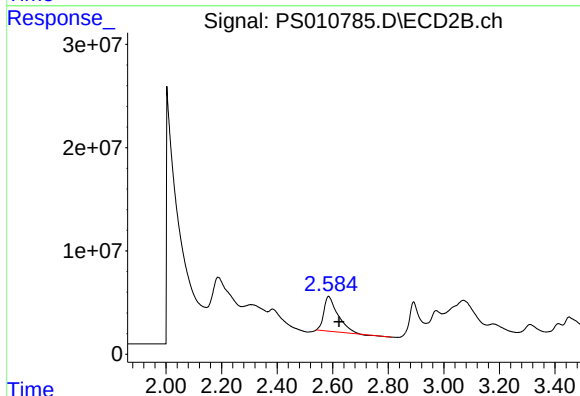


#1 Dalapon

R.T.: 2.585 min
Delta R.T.: -0.038 min
Response: 117340649
Conc: 160.27 ng/ml

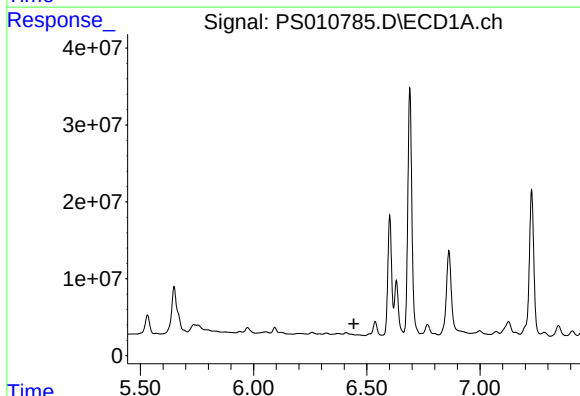


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

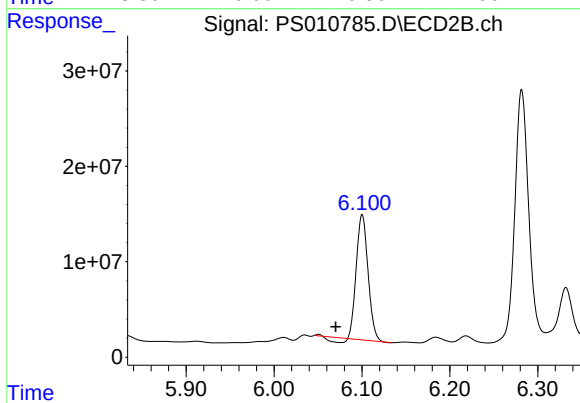

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 118726371
Conc: 144.85 ng/ml

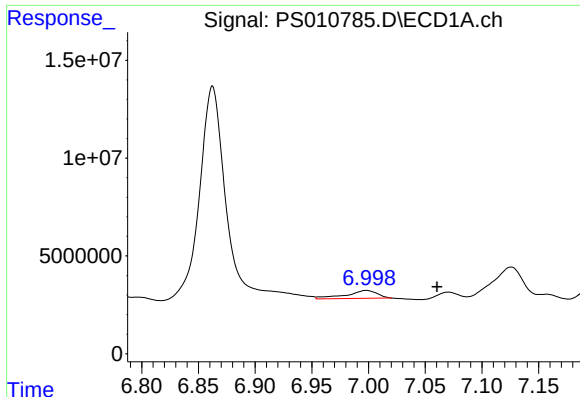

#3 4-Nitrophenol


R.T.: 6.998 min
Delta R.T.: -0.062 min
Response: 7763957
Conc: 20.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

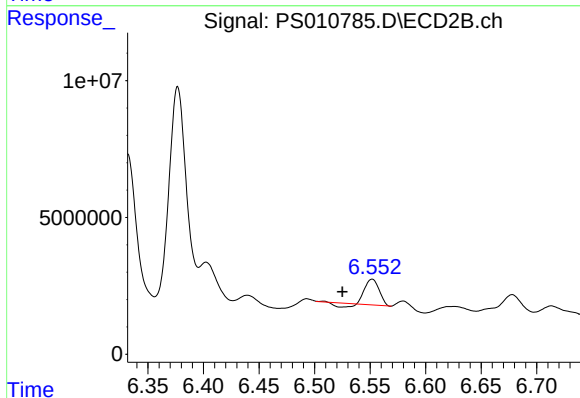


#3 4-Nitrophenol

R.T.: 6.552 min
Delta R.T.: 0.027 min
Response: 7223075
Conc: 21.80 ng/ml

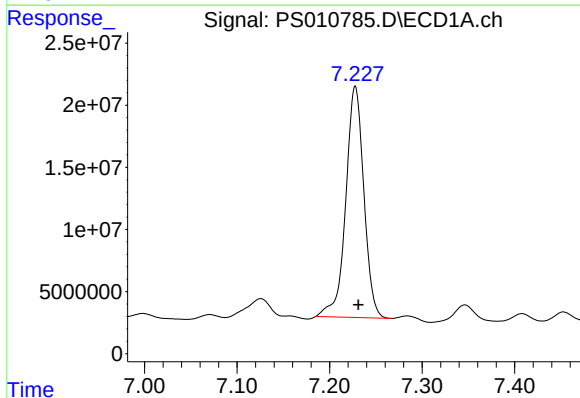


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: -0.003 min
Response: 252589988
Conc: 319.39 ng/ml

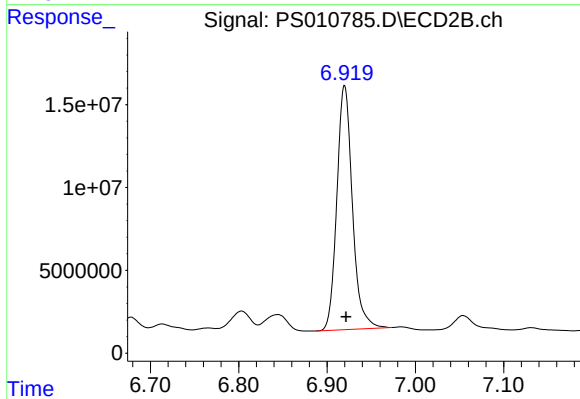

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: -0.001 min
Response: 180013071
Conc: 330.05 ng/ml

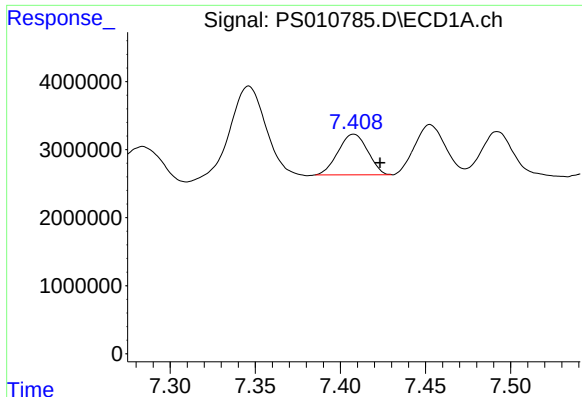

#5 DICAMBA


R.T.: 7.408 min
Delta R.T.: -0.016 min
Response: 7215192
Conc: 2.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

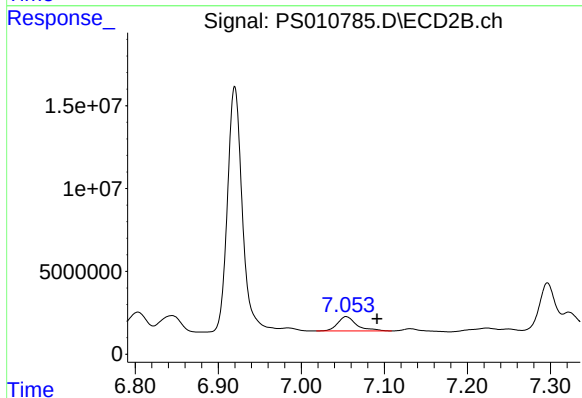


#5 DICAMBA

R.T.: 7.054 min
Delta R.T.: -0.037 min
Response: 13741366
Conc: 6.11 ng/ml

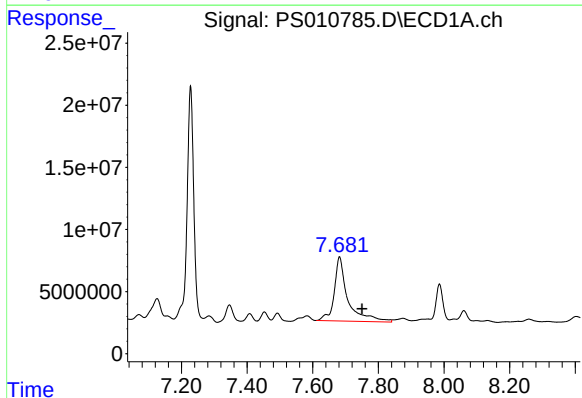


#7 MCPA

R.T.: 7.682 min
Delta R.T.: -0.069 min
Response: 148147106
Conc: 42.38 ug/ml

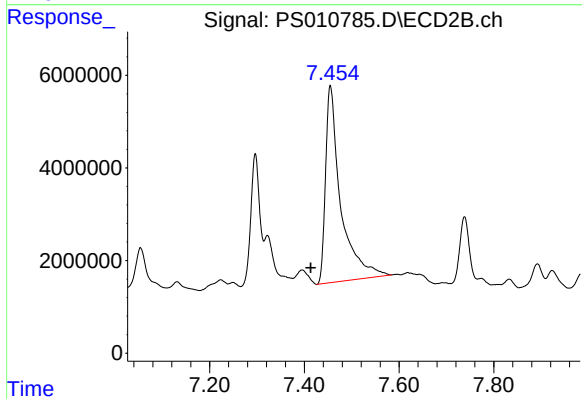

#7 MCPA


R.T.: 7.455 min
Delta R.T.: 0.041 min
Response: 94472748
Conc: 34.76 ug/ml

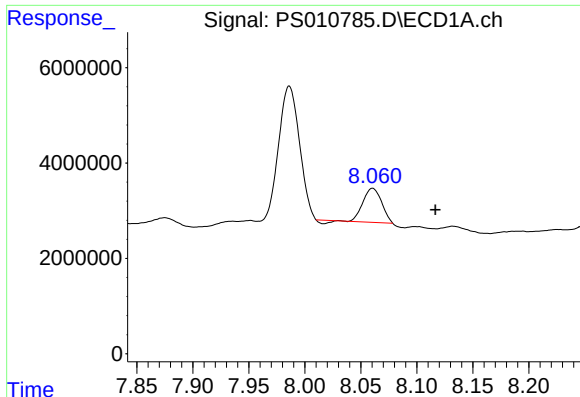

#8 DICHLORPROP


R.T.: 8.060 min
Delta R.T.: -0.056 min
Response: 7824945
Conc: 10.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

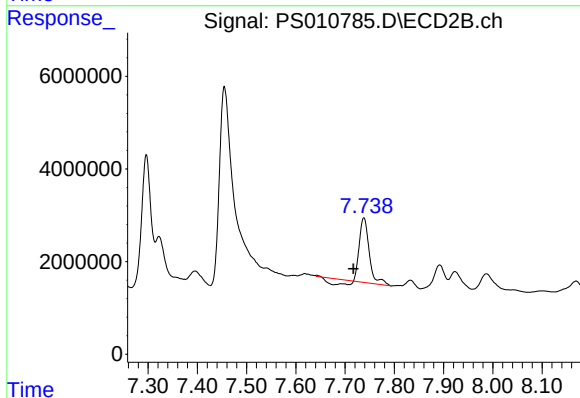


#8 DICHLORPROP

R.T.: 7.738 min
Delta R.T.: 0.021 min
Response: 16602819
Conc: 28.79 ng/ml

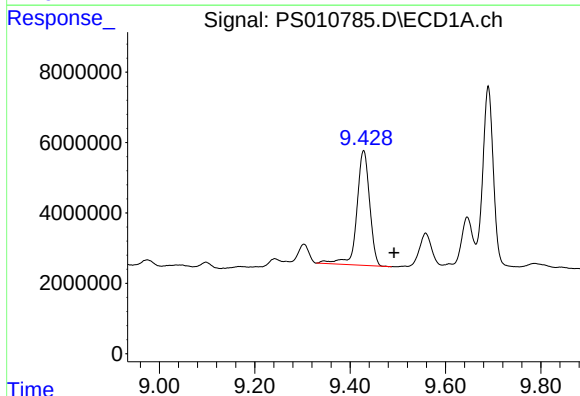


#12 2,4,5-T

R.T.: 9.428 min
Delta R.T.: -0.064 min
Response: 60803991
Conc: 14.95 ng/ml

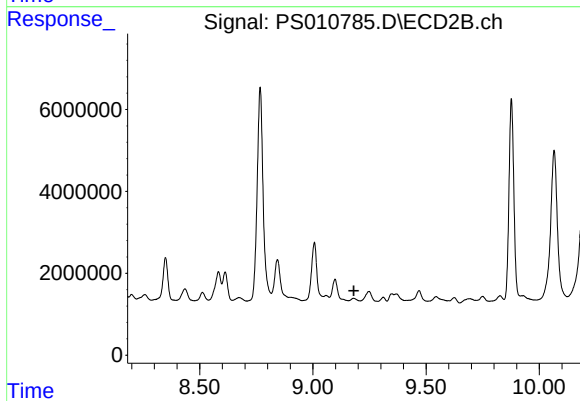

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.181 min
Response: 0
Conc: N.D.

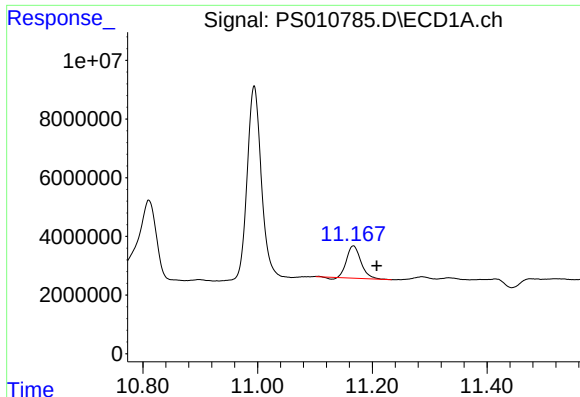

#14 DINOSEB


R.T.: 11.167 min
Delta R.T.: -0.040 min
Response: 18752308
Conc: 5.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

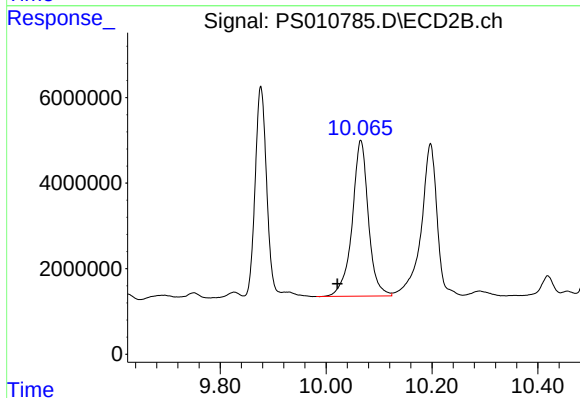


#14 DINOSEB

R.T.: 10.066 min
Delta R.T.: 0.044 min
Response: 77501336
Conc: 36.02 ng/ml

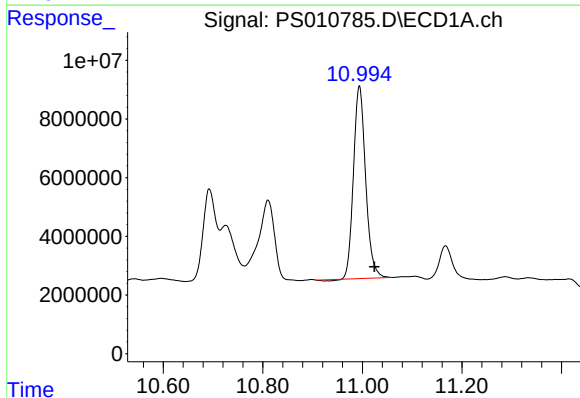

#15 Picloram

R.T.: 10.994 min
Delta R.T.: -0.030 min
Response: 111228856
Conc: 21.79 ng/ml

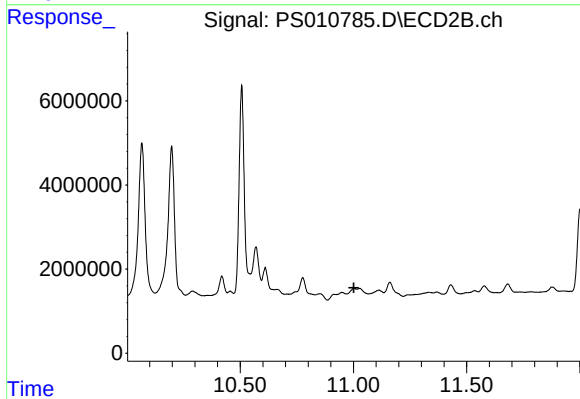

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.