

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061120\
 Data File : PS010787.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2020 22:54
 Operator : DD\AJ
 Sample : L2970-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 01:56:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.920	262.6E6	187.1E6	332.022	343.122
Target Compounds							
1) T	Dalapon	2.994	2.584	31600254	111.6E6	32.140	152.406 #
2) T	3,5-DICHL...	0.000	6.101	0	118.4E6	N.D.	144.473
3) T	4-Nitroph...	7.116	0.000	13392529	0	36.125	N.D. #
5) T	DICAMBA	7.408	7.054	7046066	14393172	2.241	6.395 #
7) T	MCPA	7.682	7.456	162.0E6	111.1E6	46.330	40.887
8) T	DICHLORPROP	0.000	7.739	0	20597135	N.D.	35.720
10) T	Pentachlo...	8.710	0.000	12223257	0	1.146	N.D. #
12) T	2,4,5-T	9.428	0.000	62595073	0	15.391	N.D. #
14) T	DINOSEB	11.167	10.065	21120341	67148746	6.537	31.211 #
15) T	Picloram	10.993	0.000	115.4E6	0	22.610	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061120\
Data File : PS010787.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2020 22:54
Operator : DD\AJ
Sample : L2970-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 01:56:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

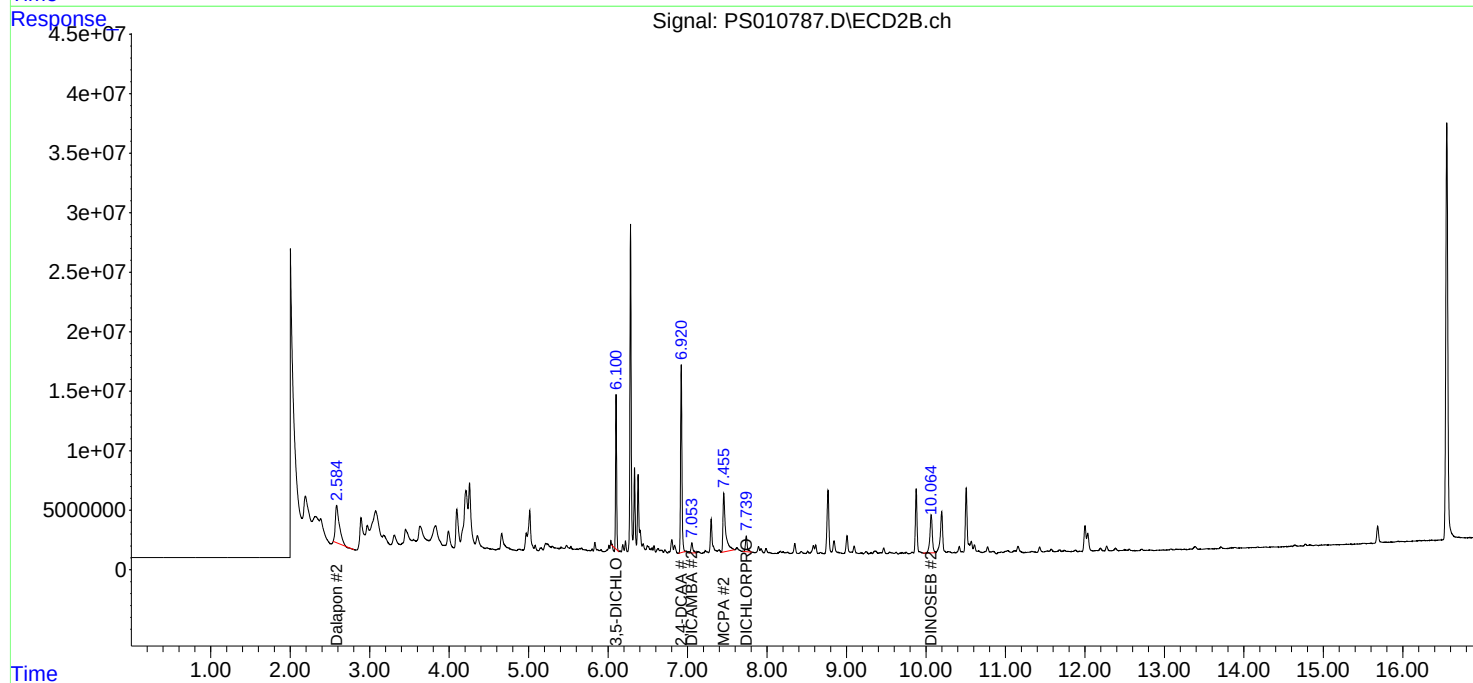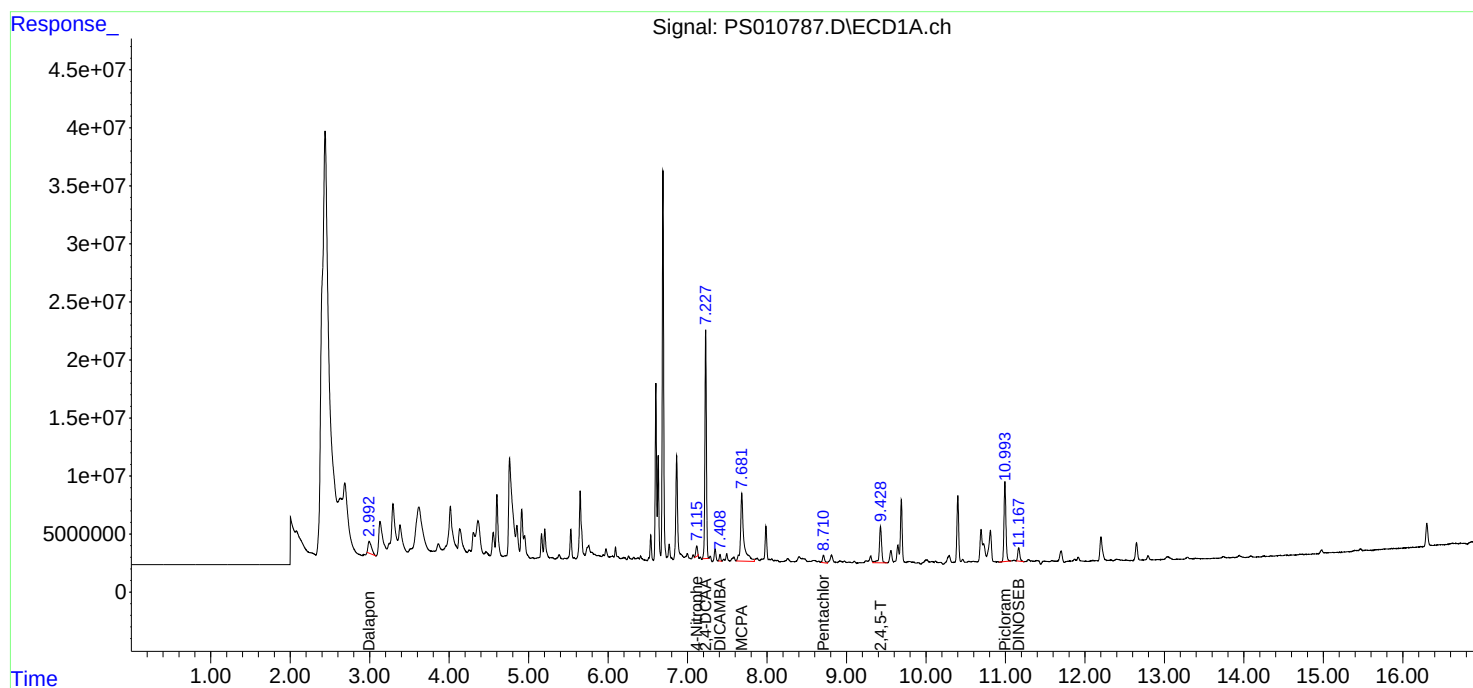


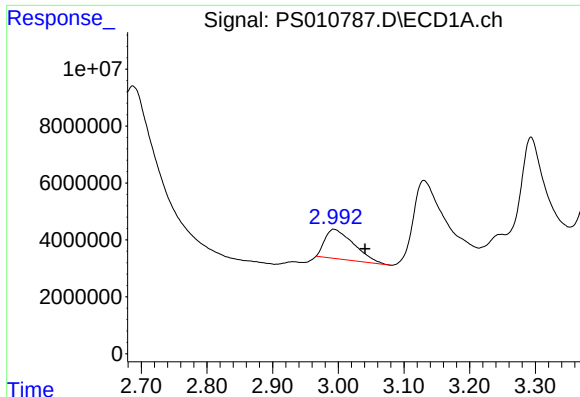

#1 Dalapon


R.T.: 2.994 min
Delta R.T.: -0.047 min
Response: 31600254
Conc: 32.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

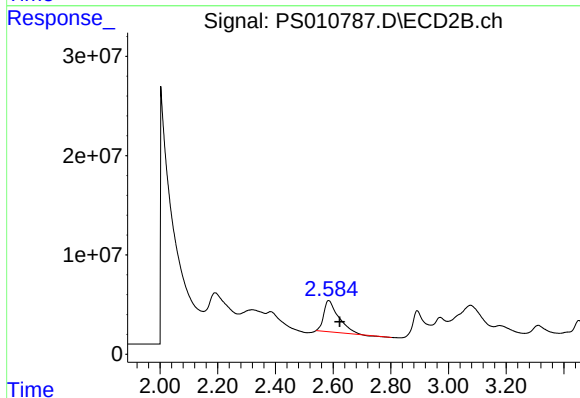


#1 Dalapon

R.T.: 2.584 min
Delta R.T.: -0.039 min
Response: 111583374
Conc: 152.41 ng/ml

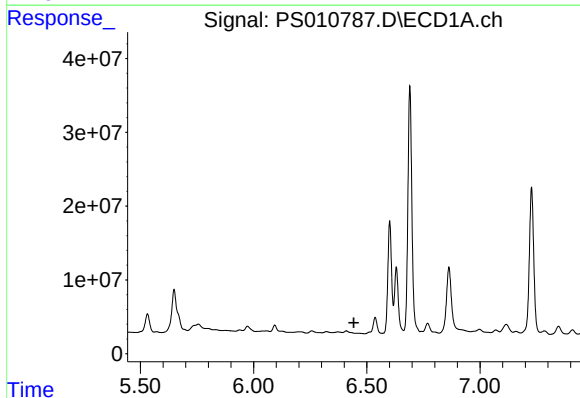


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

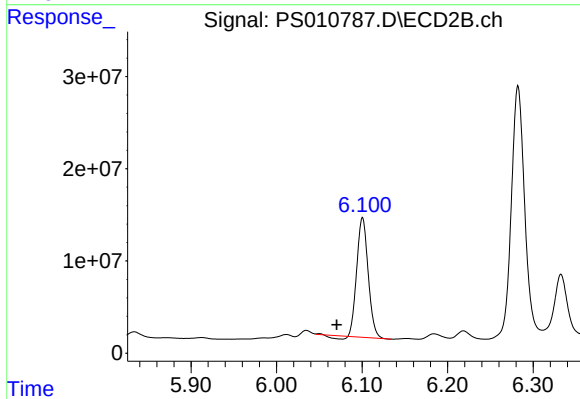

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.101 min
Delta R.T.: 0.030 min
Response: 118416768
Conc: 144.47 ng/ml

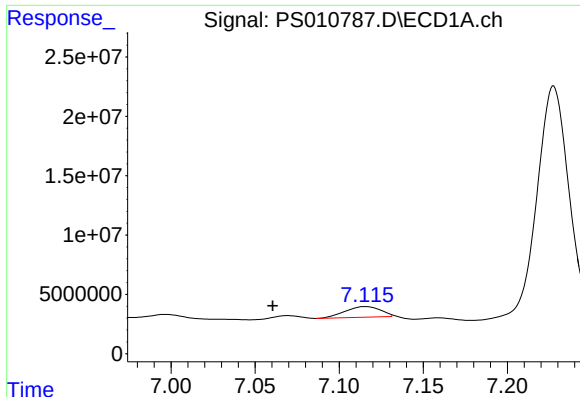

#3 4-Nitrophenol


R.T.: 7.116 min
Delta R.T.: 0.055 min
Response: 13392529
Conc: 36.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

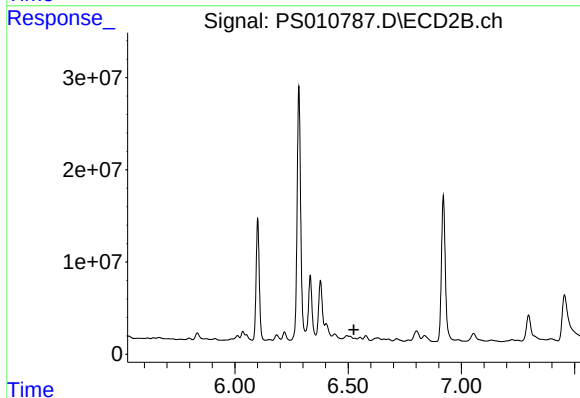


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.525 min
Response: 0
Conc: N.D.

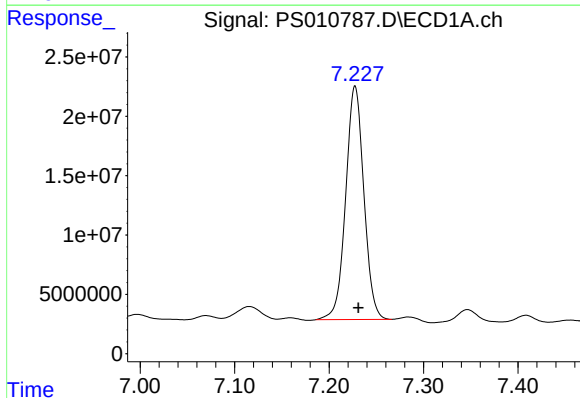


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: -0.004 min
Response: 262583445
Conc: 332.02 ng/ml

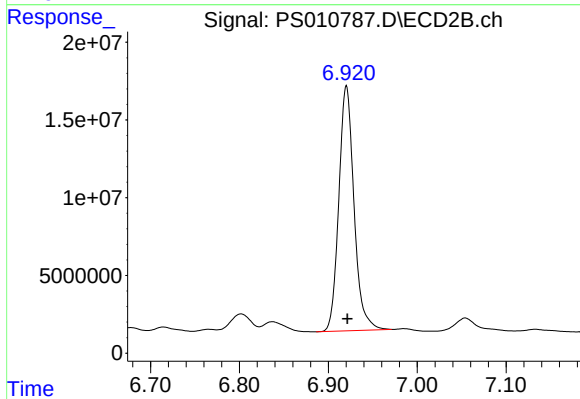

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: -0.001 min
Response: 187144007
Conc: 343.12 ng/ml

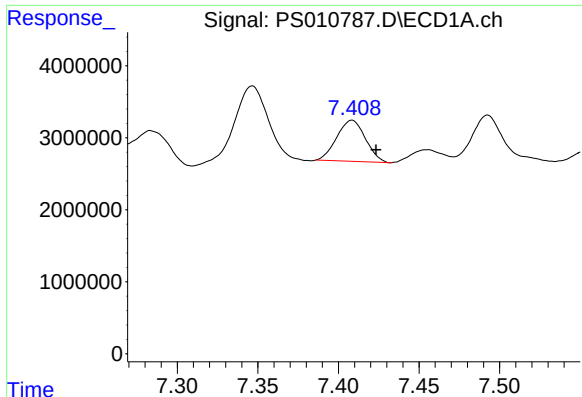

#5 DICAMBA


R.T.: 7.408 min
Delta R.T.: -0.015 min
Response: 7046066
Conc: 2.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

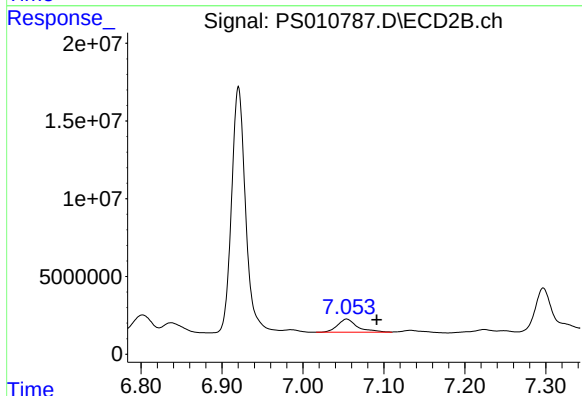


#5 DICAMBA

R.T.: 7.054 min
Delta R.T.: -0.037 min
Response: 14393172
Conc: 6.39 ng/ml

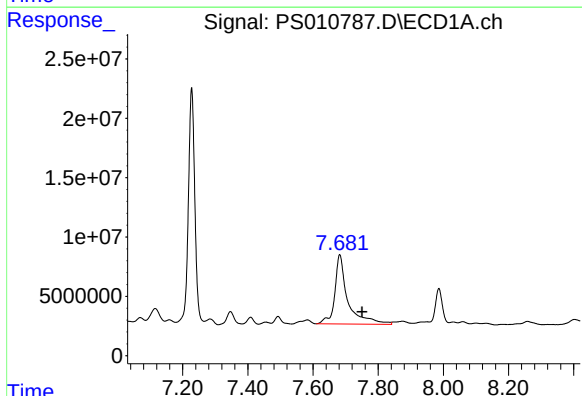


#7 MCPA

R.T.: 7.682 min
Delta R.T.: -0.069 min
Response: 161969062
Conc: 46.33 ug/ml

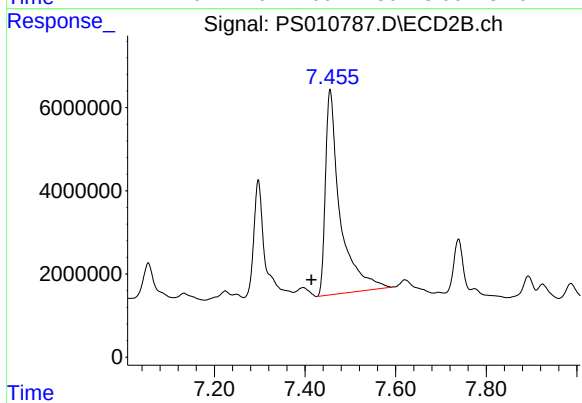

#7 MCPA


R.T.: 7.456 min
Delta R.T.: 0.042 min
Response: 111121262
Conc: 40.89 ug/ml

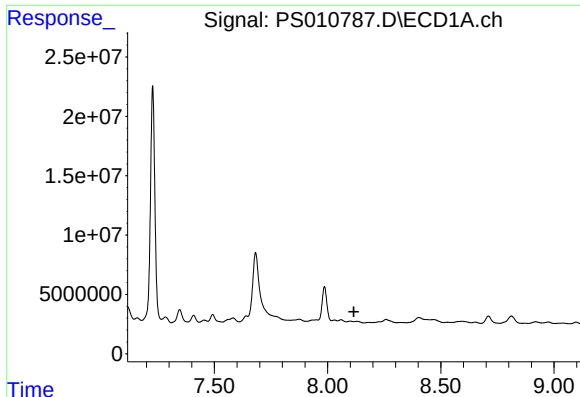

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.116 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

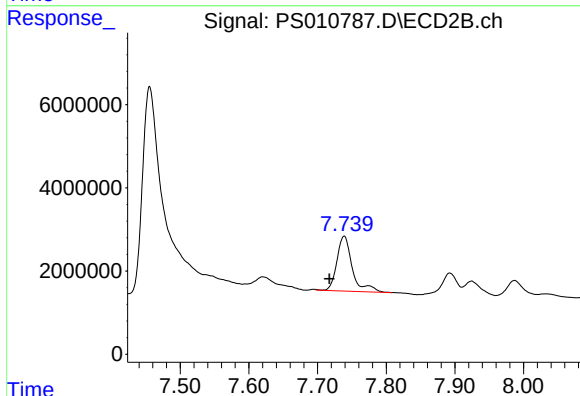


#8 DICHLORPROP

R.T.: 7.739 min
Delta R.T.: 0.021 min
Response: 20597135
Conc: 35.72 ng/ml

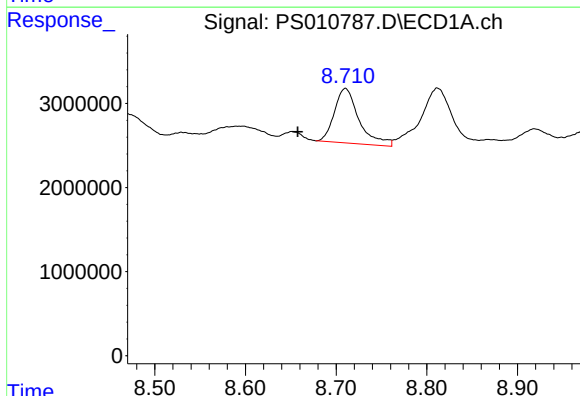


#10 Pentachlorophenol

R.T.: 8.710 min
Delta R.T.: 0.052 min
Response: 12223257
Conc: 1.15 ng/ml

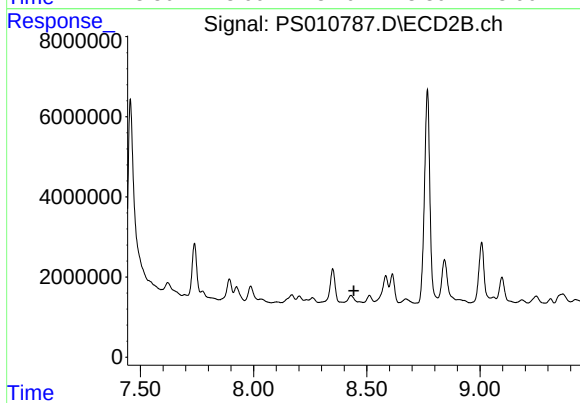

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.443 min
Response: 0
Conc: N.D.

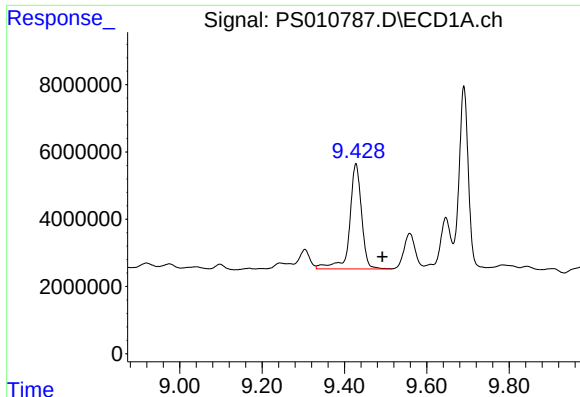

#12 2,4,5-T


R.T.: 9.428 min
Delta R.T.: -0.064 min
Response: 62595073
Conc: 15.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

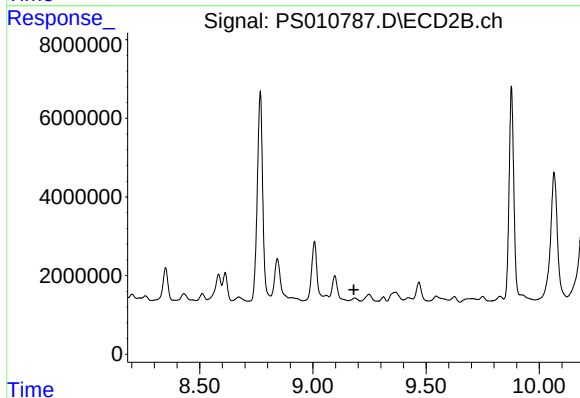


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.181 min
Response: 0
Conc: N.D.

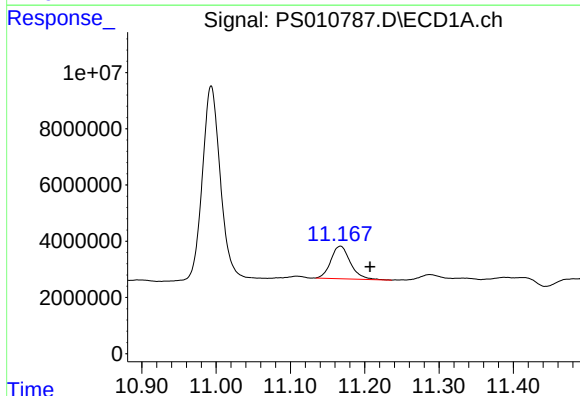


#14 DINOSEB

R.T.: 11.167 min
Delta R.T.: -0.040 min
Response: 21120341
Conc: 6.54 ng/ml

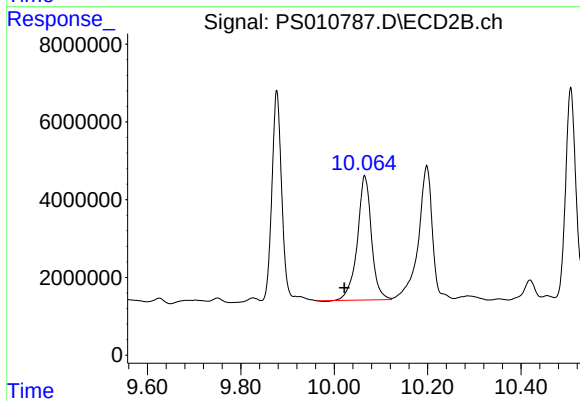

#14 DINOSEB


R.T.: 10.065 min
Delta R.T.: 0.044 min
Response: 67148746
Conc: 31.21 ng/ml

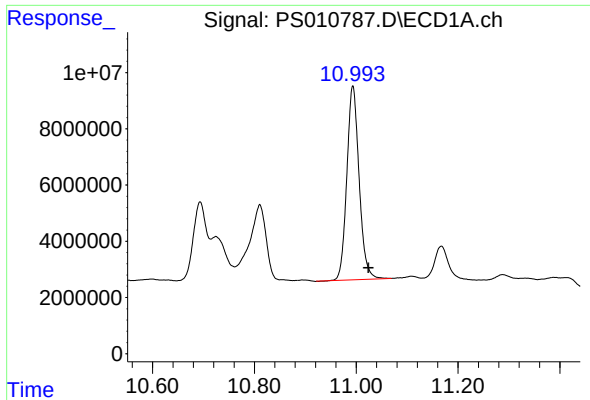

#15 Picloram

R.T.: 10.993 min
Delta R.T.: -0.031 min
Response: 115428694
Conc: 22.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

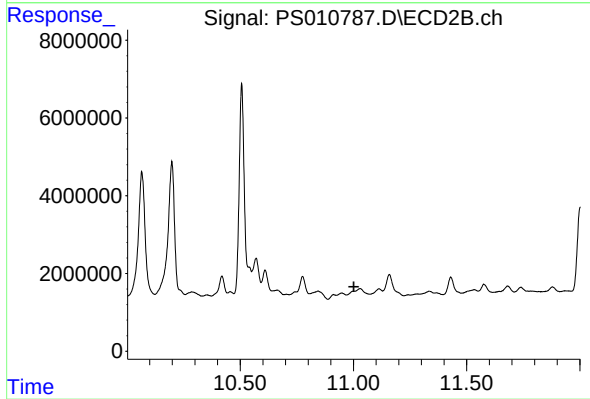

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.