

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061120\
 Data File : PS010790.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2020 00:03
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 01:57:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.920	392.8E6	287.1E6	496.716	526.440
Target Compounds							
9) T	2,4-D	8.359	0.000	1477814	0	1.875	N.D. #
15) T	Picloram	11.030	10.982	8741085	261.9E6	1.712	63.464 #
16) T	DCPA	0.000	10.982	0	261.9E6	N.D.	70.614



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061120\
Data File : PS010790.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2020 00:03
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 01:57:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

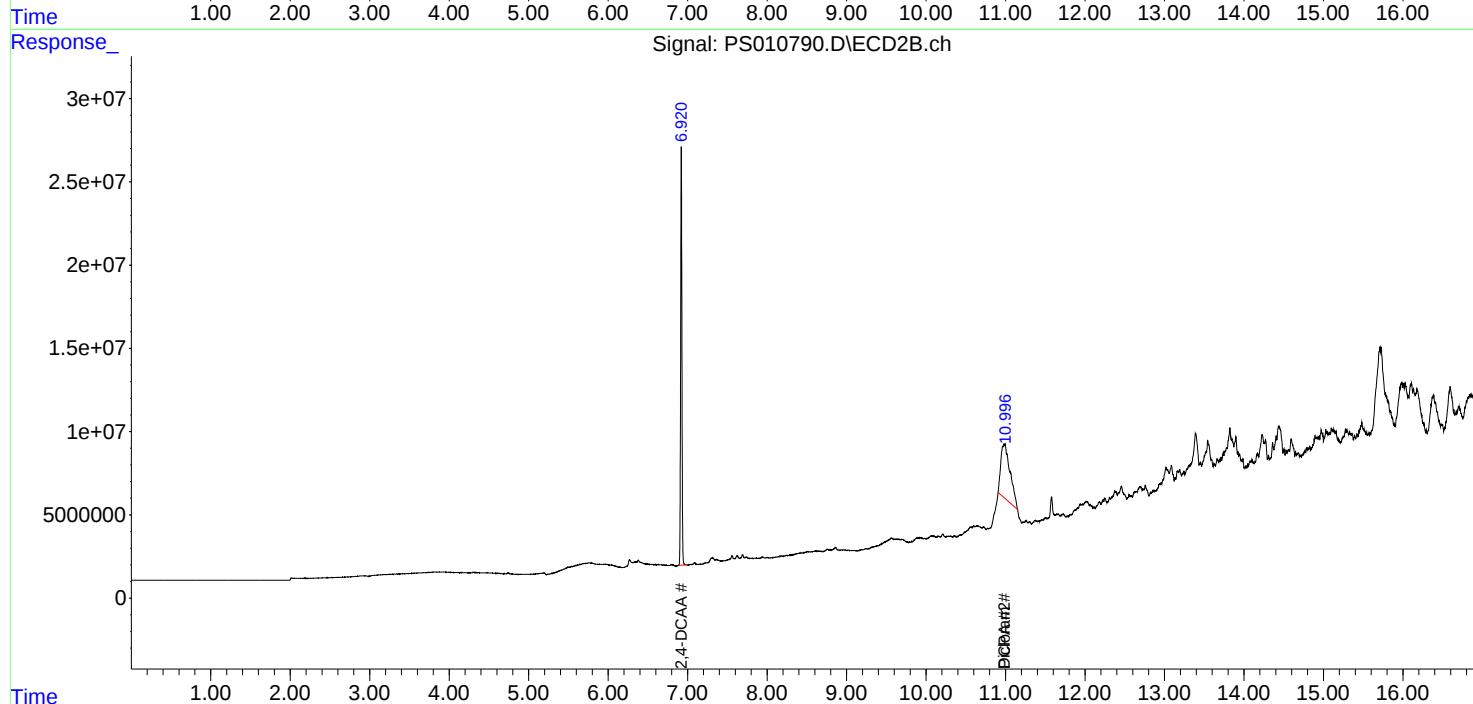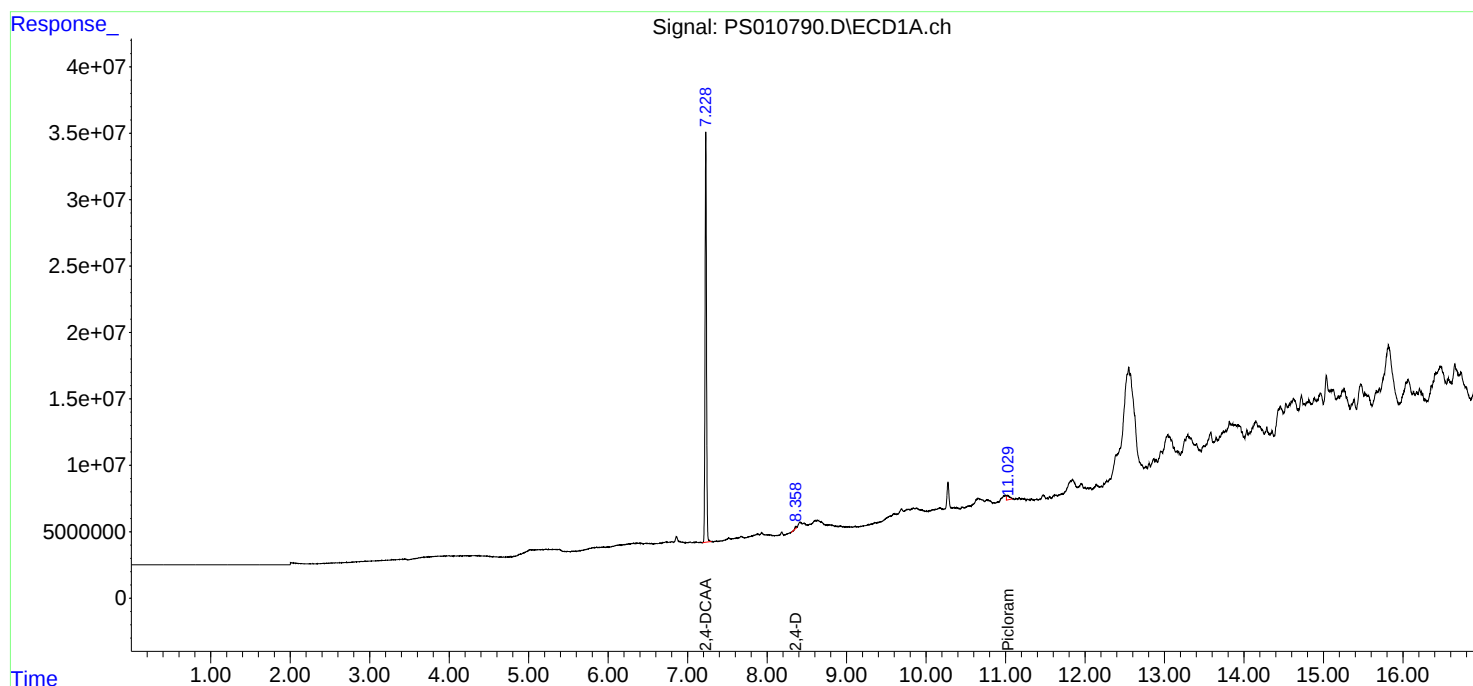


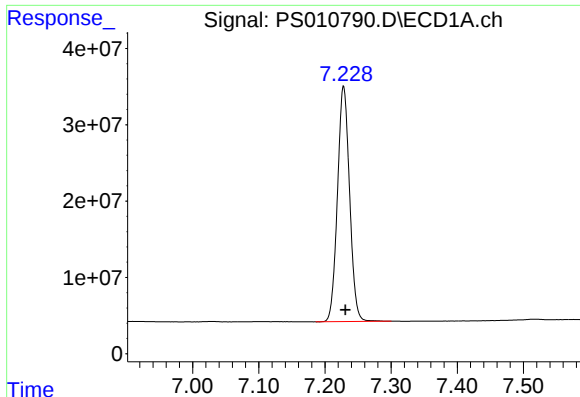

#4 2,4-DCAA


R.T.: 7.228 min
Delta R.T.: -0.003 min
Response: 392833435
Conc: 496.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

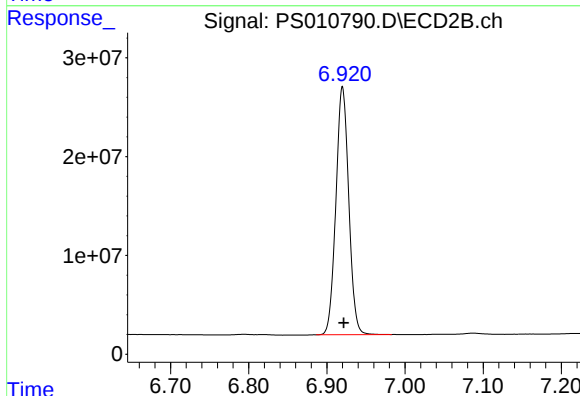


#4 2,4-DCAA

R.T.: 6.920 min
Delta R.T.: -0.001 min
Response: 287128556
Conc: 526.44 ng/ml

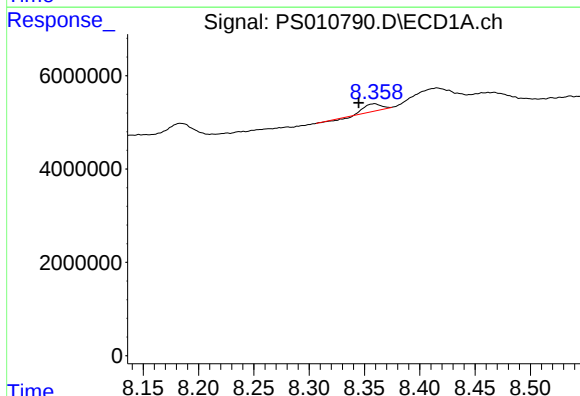


#9 2,4-D

R.T.: 8.359 min
Delta R.T.: 0.014 min
Response: 1477814
Conc: 1.87 ng/ml

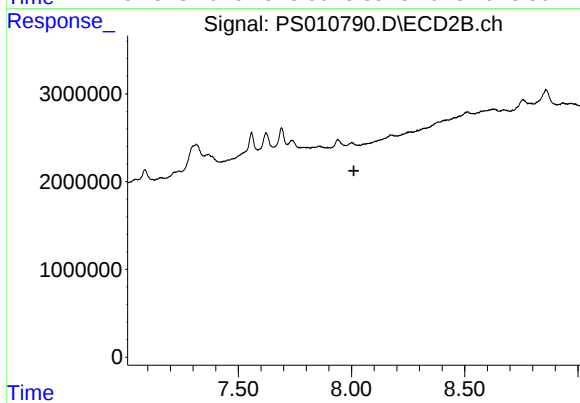

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.010 min
Response: 0
Conc: N.D.

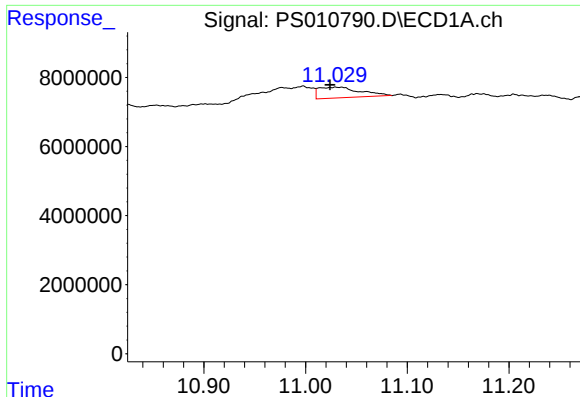

#15 Picloram


R.T.: 11.030 min
Delta R.T.: 0.006 min
Response: 8741085
Conc: 1.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

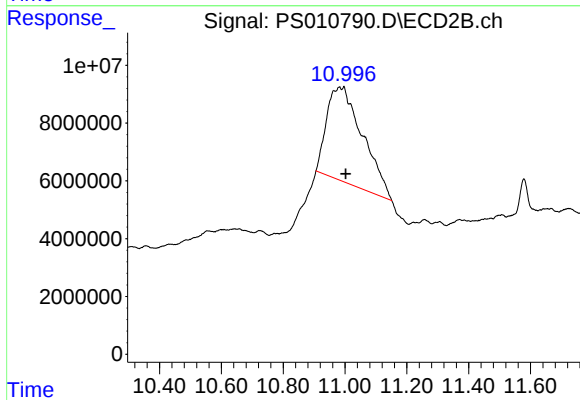


#15 Picloram

R.T.: 10.982 min
Delta R.T.: -0.021 min
Response: 261850462
Conc: 63.46 ng/ml

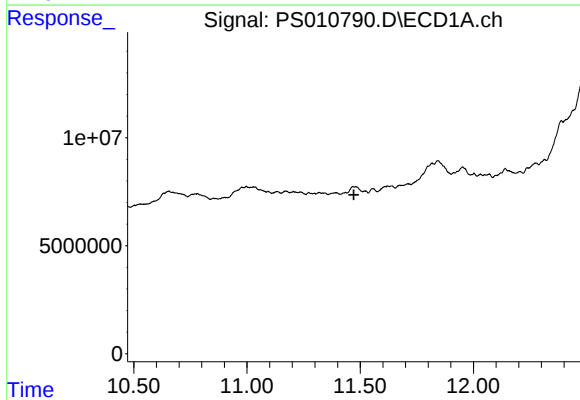

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.472 min
Response: 0
Conc: N.D.

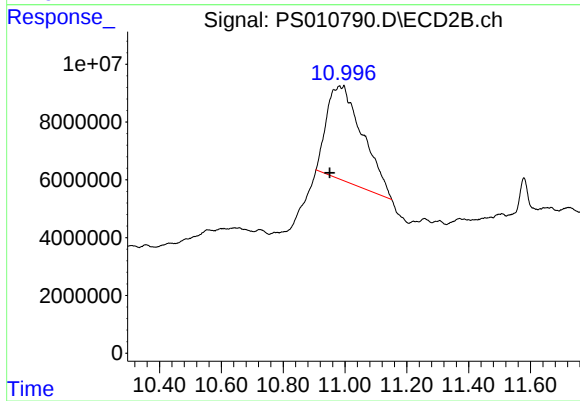

#16 DCPA

R.T.: 10.982 min
Delta R.T.: 0.030 min
Response: 261850462
Conc: 70.61 ng/ml