

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061121\
 Data File : PS015416.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2021 22:47
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 04:34:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
Target Compounds							
2) T	3,5-DICHL...	6.470	0.000	9556443	0	2.771	N.D. #
3) T	4-Nitroph...	7.010f	0.000	5042844	0	3.577	N.D. #
8) T	DICHLORPROP	0.000	7.589	0	4938442	N.D.	9.090
9) T	2,4-D	8.338	0.000	7985483	0	3.134	N.D. #
10) T	Pentachlo...	8.651	0.000	6363069	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.205	0.000	2554987	0	<MDL	N.D. #
12) T	2,4,5-T	9.484	9.077f	6880683	17517064	<MDL	6.051 #
13) T	2,4-DB	10.026	0.000	10421566	0	4.092	N.D. #
15) T	Picloram	11.014	10.841	220.3E6	91651737	13.296	22.069 #
16) T	DCPA	11.466	10.841	5001484	91651737	<MDL	21.260 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061121\
Data File : PS015416.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2021 22:47
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 04:34:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

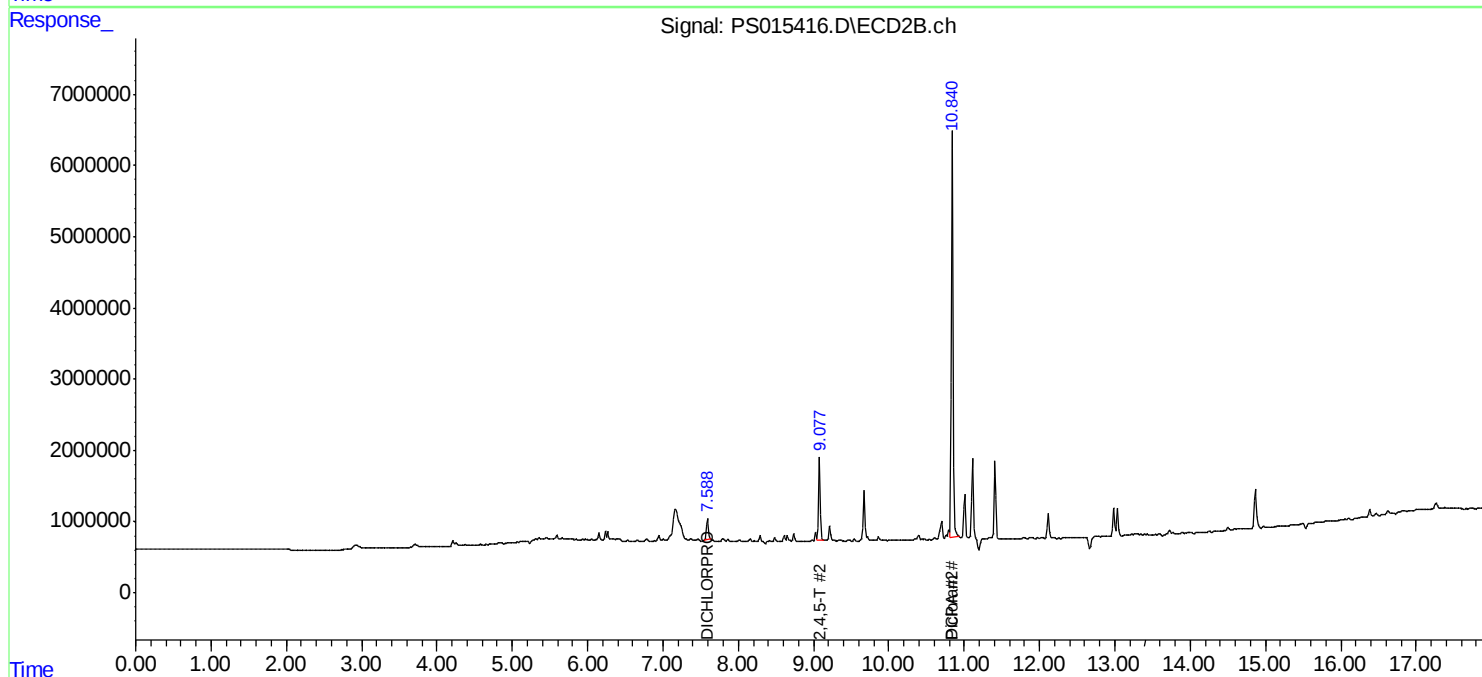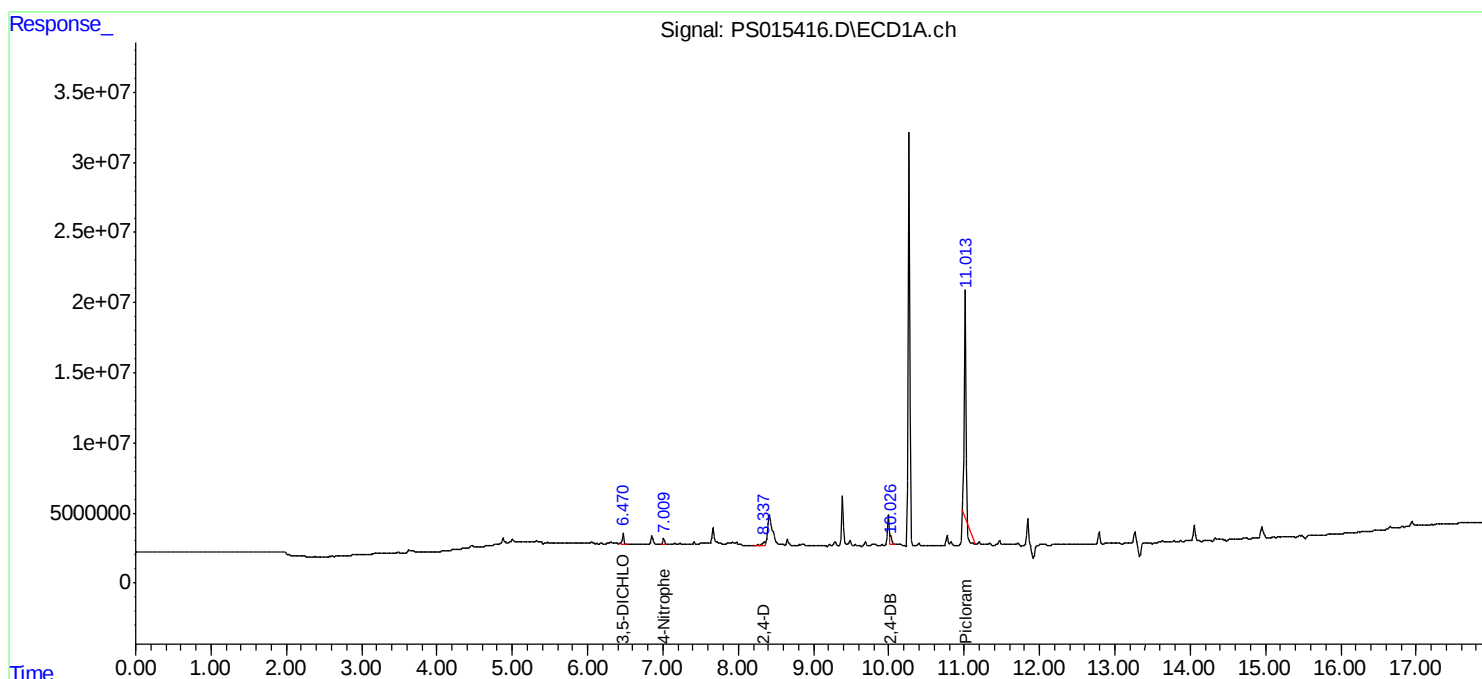


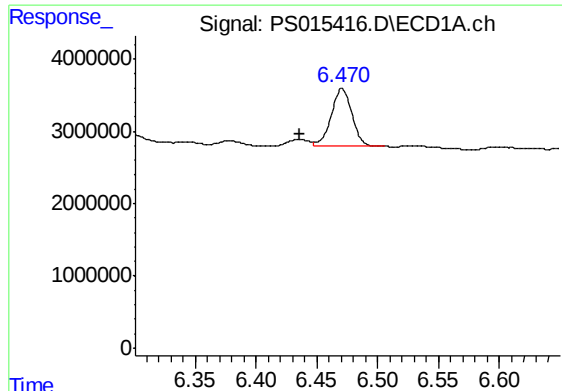

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.470 min
Delta R.T.: 0.034 min
Response: 9556443
Conc: 2.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

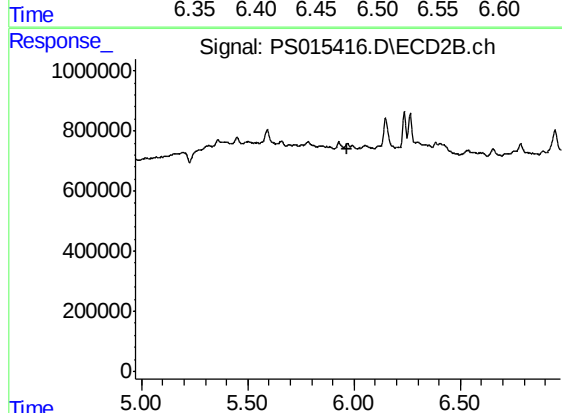


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.971 min
Response: 0
Conc: N.D.

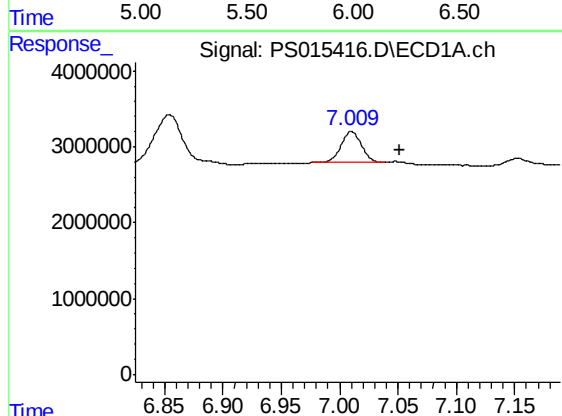


#3 4-Nitrophenol

R.T.: 7.010 min
Delta R.T.: -0.041 min
Response: 5042844
Conc: 3.58 ng/ml

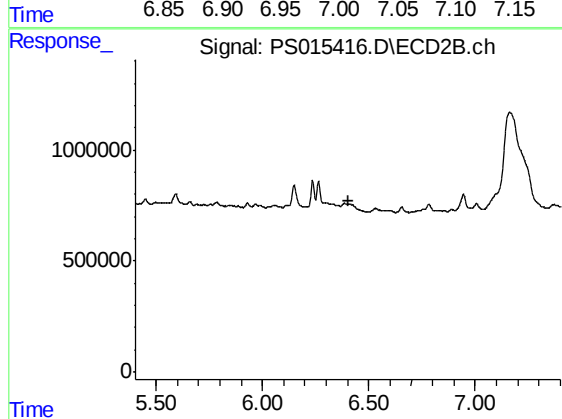

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

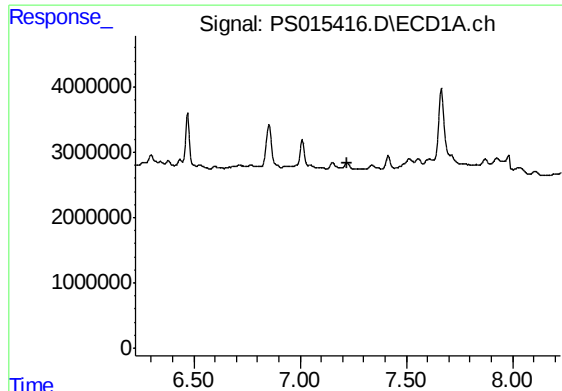

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.225 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

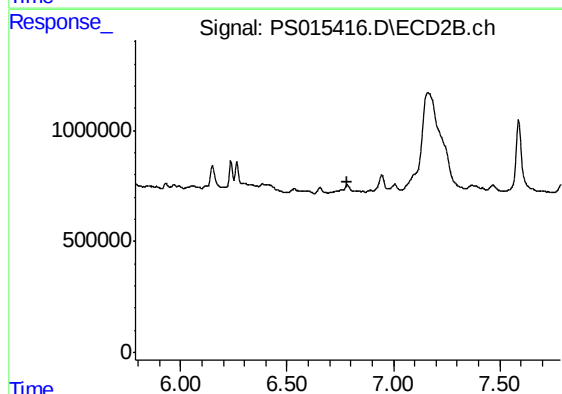


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.786 min
Response: 0
Conc: N.D.

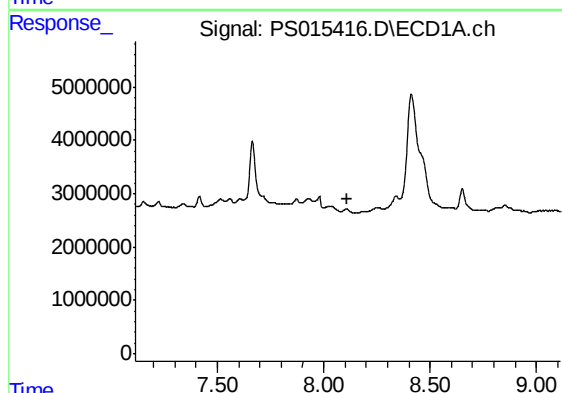


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.113 min
Response: 0
Conc: N.D.

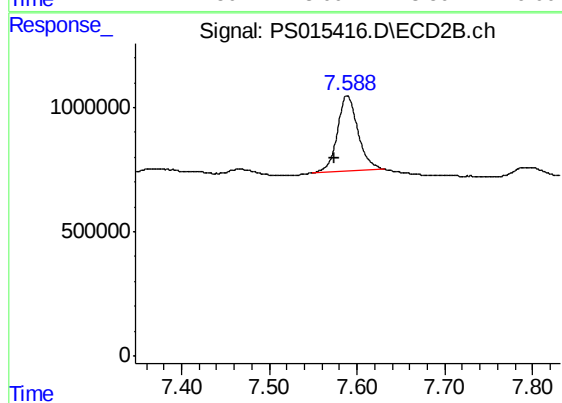

#8 DICHLORPROP


R.T.: 7.589 min
Delta R.T.: 0.015 min
Response: 4938442
Conc: 9.09 ng/ml

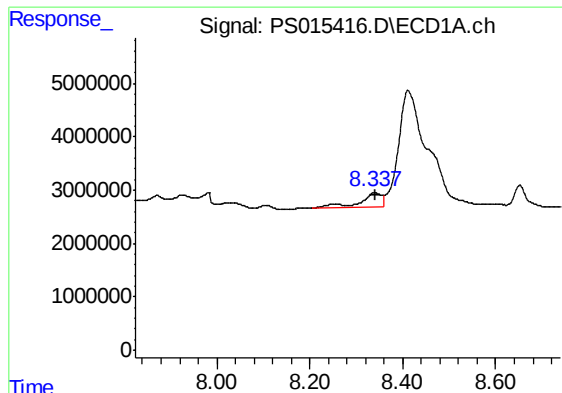

#9 2,4-D


R.T.: 8.338 min
Delta R.T.: -0.003 min
Response: 7985483
Conc: 3.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

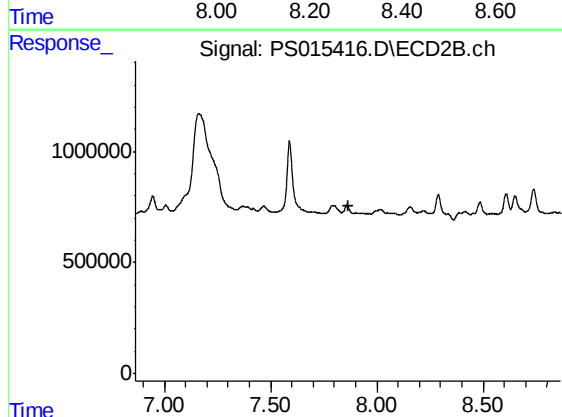


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.864 min
Response: 0
Conc: N.D.

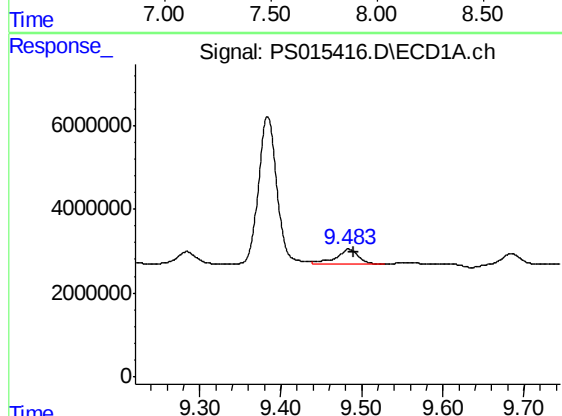


#12 2,4,5-T

R.T.: 9.484 min
Delta R.T.: -0.006 min
Response: 6880683
Conc: N.D.

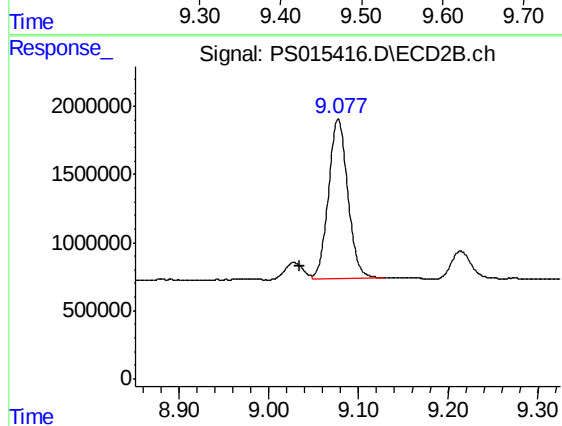

#12 2,4,5-T


R.T.: 9.077 min
Delta R.T.: 0.043 min
Response: 17517064
Conc: 6.05 ng/ml

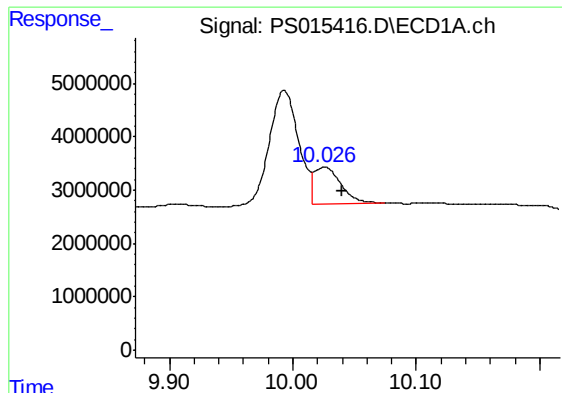

#13 2,4-DB


R.T.: 10.026 min
Delta R.T.: -0.014 min
Response: 10421566
Conc: 4.09 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

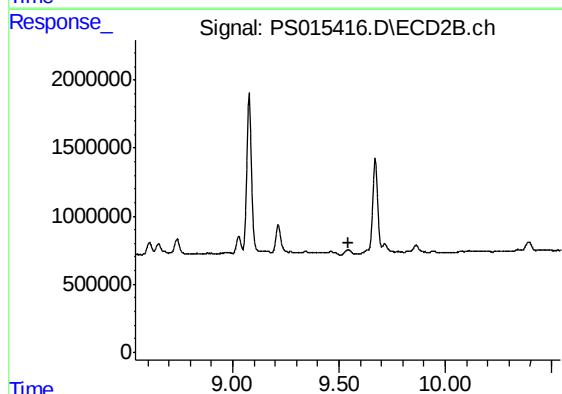


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.542 min
Response: 0
Conc: N.D.

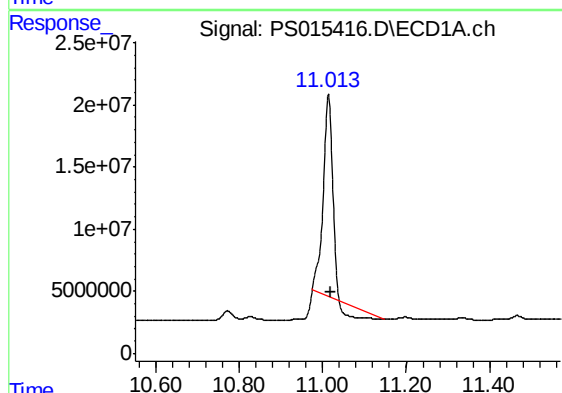


#15 Picloram

R.T.: 11.014 min
Delta R.T.: -0.006 min
Response: 220264582
Conc: 13.30 ng/ml

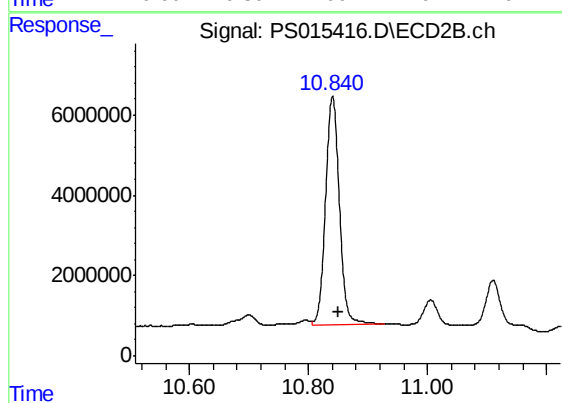

#15 Picloram


R.T.: 10.841 min
Delta R.T.: -0.010 min
Response: 91651737
Conc: 22.07 ng/ml

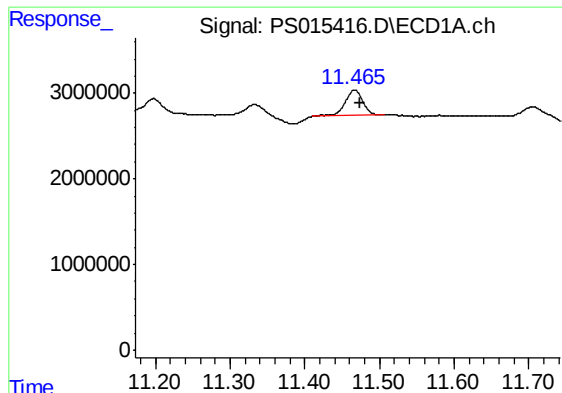

#16 DCPA

R.T.: 11.466 min
Delta R.T.: -0.009 min
Response: 5001484
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

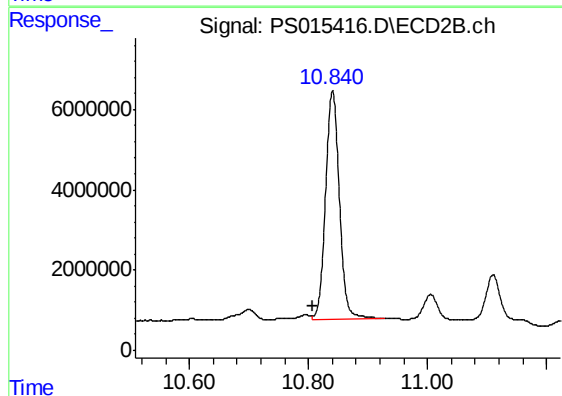

#16 DCPA

R.T.: 10.841 min
Delta R.T.: 0.034 min
Response: 91651737
Conc: 21.26 ng/ml