

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061121\
 Data File : PS015417.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2021 23:12
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 04:34:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.221	6.782	1241.4E6	291.3E6	492.547	543.614
Target Compounds							
3) T	4-Nitroph...	7.017	0.000	7086831	0	5.027	N.D. #
12) T	2,4,5-T	0.000	9.078f	0	6334703	N.D.	2.188
13) T	2,4-DB	10.028	0.000	3912831	0	1.537	N.D. #
15) T	Picloram	11.015	10.841	129.9E6	43160598	7.843	10.393 #
16) T	DCPA	0.000	10.841	0	43160598	N.D.	10.012



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061121\
Data File : PS015417.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2021 23:12
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 04:34:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

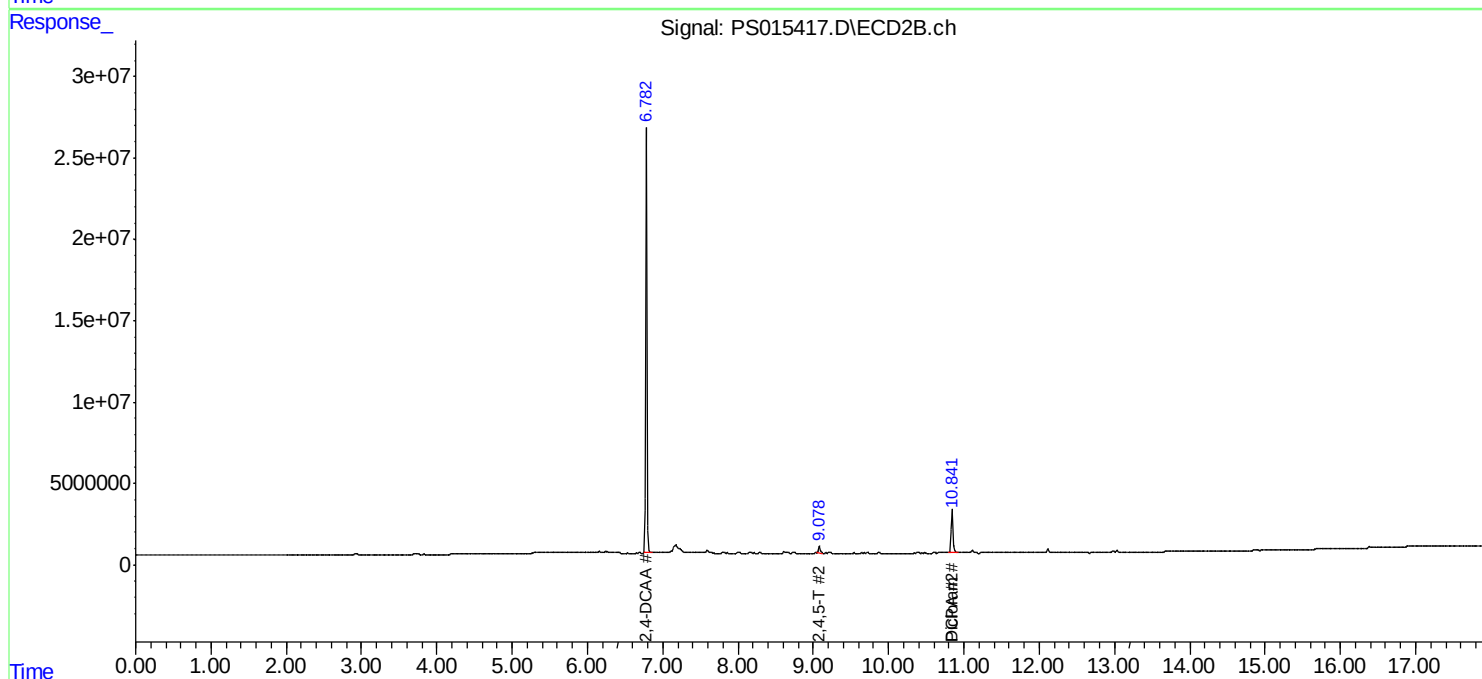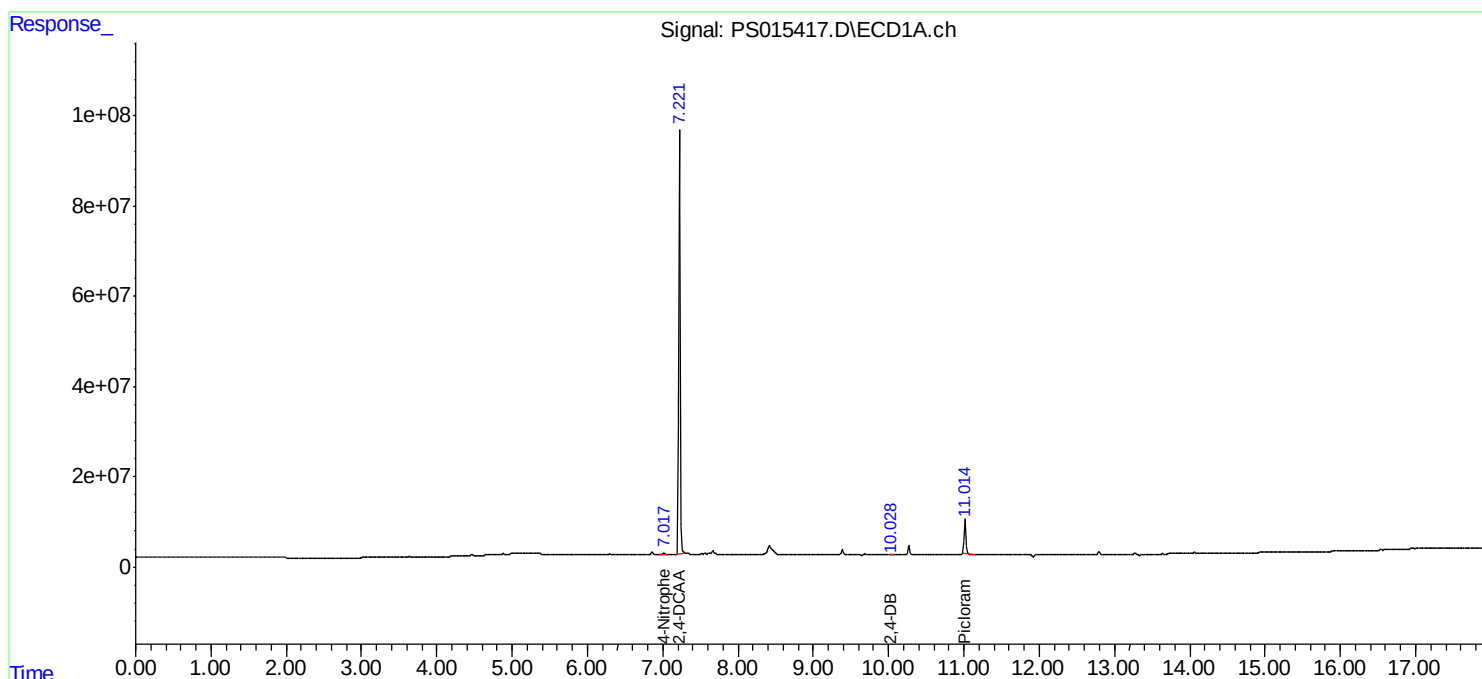


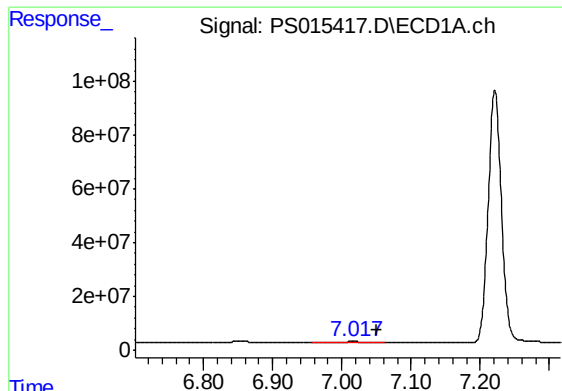

#3 4-Nitrophenol


R.T.: 7.017 min
Delta R.T.: -0.034 min
Response: 7086831
Conc: 5.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

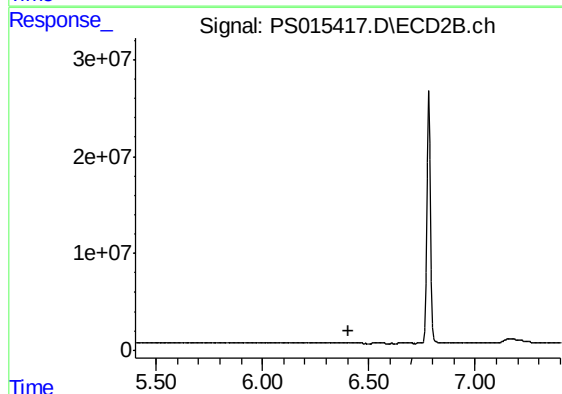


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

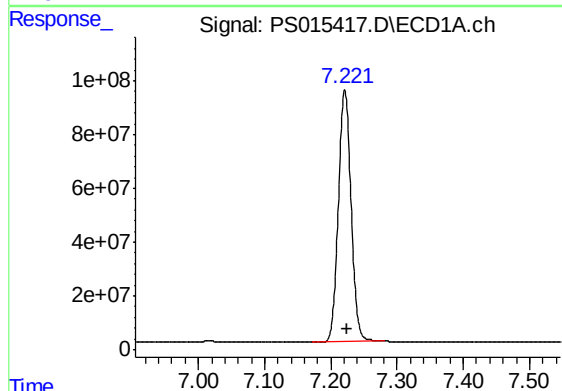


#4 2,4-DCAA

R.T.: 7.221 min
Delta R.T.: -0.004 min
Response: 1241402704
Conc: 492.55 ng/ml

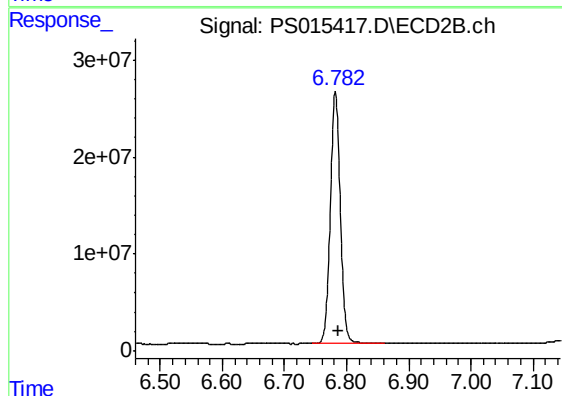

#4 2,4-DCAA


R.T.: 6.782 min
Delta R.T.: -0.004 min
Response: 291252763
Conc: 543.61 ng/ml

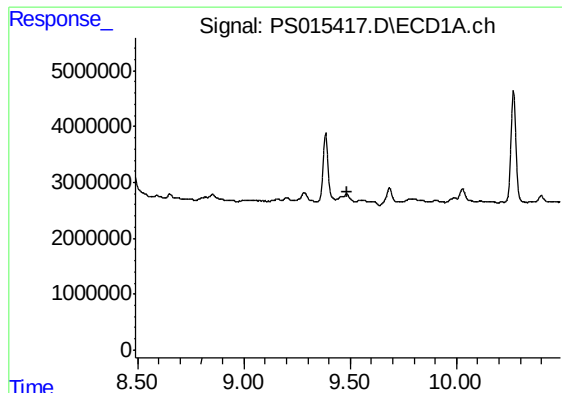

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

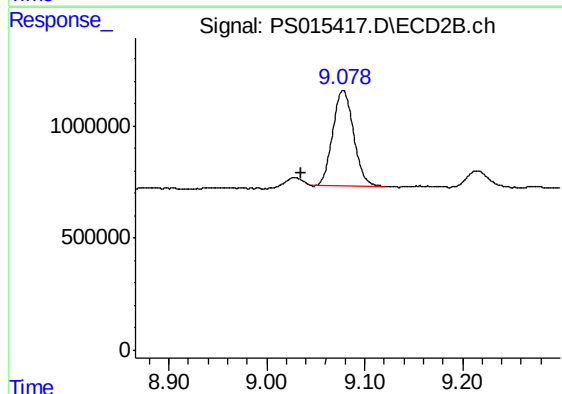


#12 2,4,5-T

R.T.: 9.078 min
Delta R.T.: 0.043 min
Response: 6334703
Conc: 2.19 ng/ml

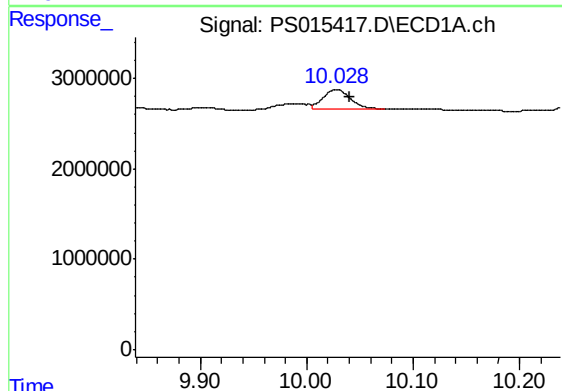


#13 2,4-DB

R.T.: 10.028 min
Delta R.T.: -0.012 min
Response: 3912831
Conc: 1.54 ng/ml

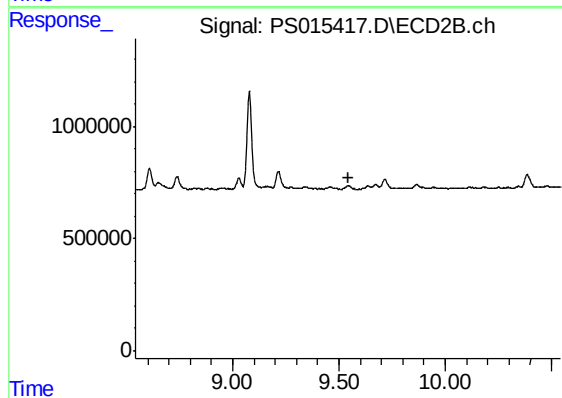

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.542 min
Response: 0
Conc: N.D.

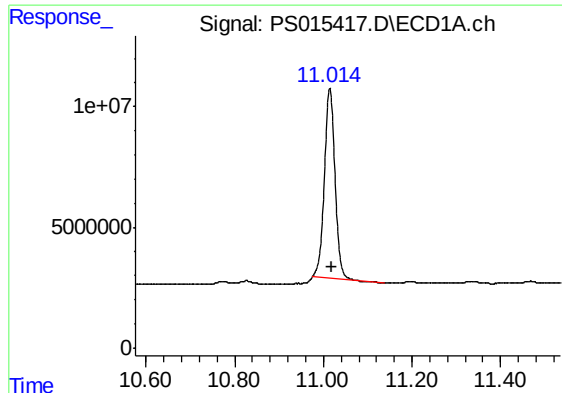

#15 Picloram


R.T.: 11.015 min
Delta R.T.: -0.005 min
Response: 129929217
Conc: 7.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

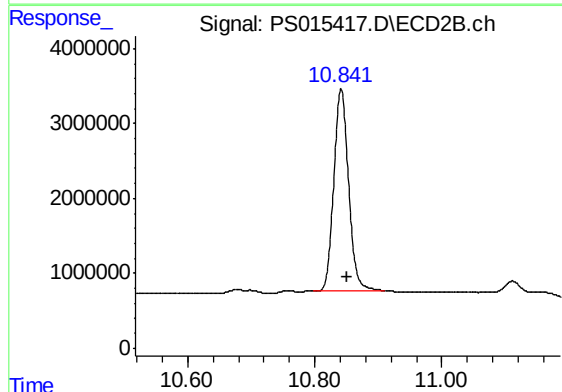


#15 Picloram

R.T.: 10.841 min
Delta R.T.: -0.009 min
Response: 43160598
Conc: 10.39 ng/ml

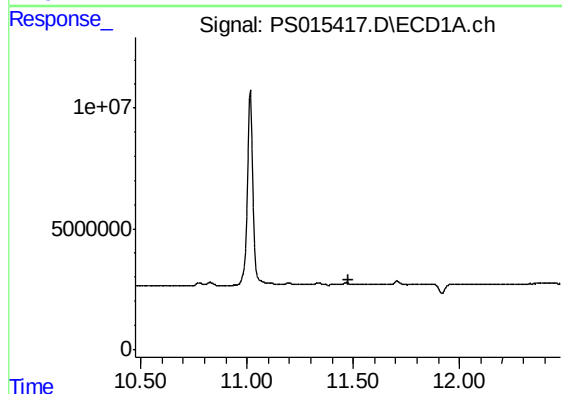

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.475 min
Response: 0
Conc: N.D.

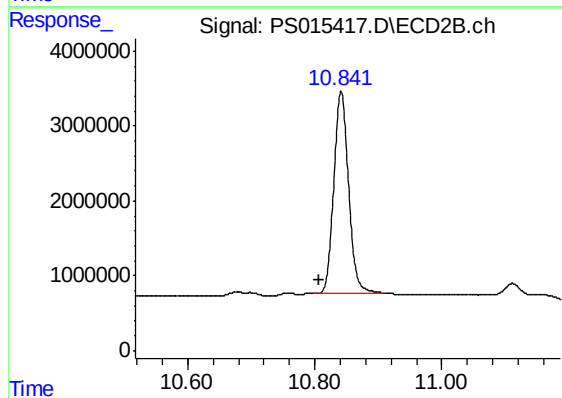

#16 DCPA

R.T.: 10.841 min
Delta R.T.: 0.035 min
Response: 43160598
Conc: 10.01 ng/ml