

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061121\
 Data File : PS015429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2021 08:51
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 02:15:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.230	6.781	1022.6E6	293.9E6	405.745	548.474	#
Target Compounds								
3) T	4-Nitroph...	7.025	0.000	4312799	0	3.059	N.D.	#
5) T	DICAMBA	7.422	0.000	2901797	0	<MDL	N.D.	#
7) T	MCPA	7.675f	0.000	9655597	0	<MDL	N.D.	#
10) T	Pentachlo...	8.658	0.000	8069139	0	<MDL	N.D.	#
11) T	2,4,5-TP ...	9.208	0.000	5128693	0	<MDL	N.D.	#
12) T	2,4,5-T	9.493	9.077f	6341368	4140900	<MDL	1.430	#
15) T	Picloram	11.022	10.842	25009636	7312068	1.510	1.761	
16) T	DCPA	11.472	10.842	6041714	7312068	<MDL	1.696	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061121\
Data File : PS015429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2021 08:51
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 02:15:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

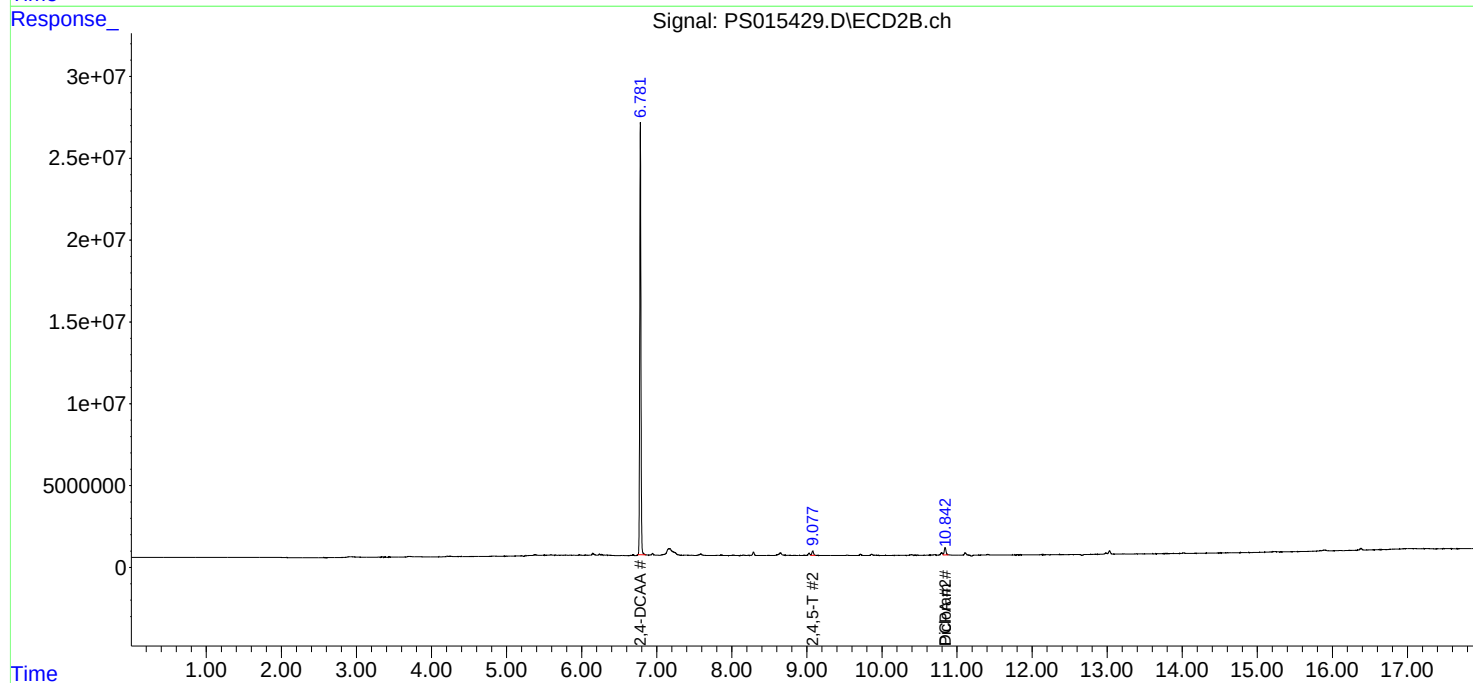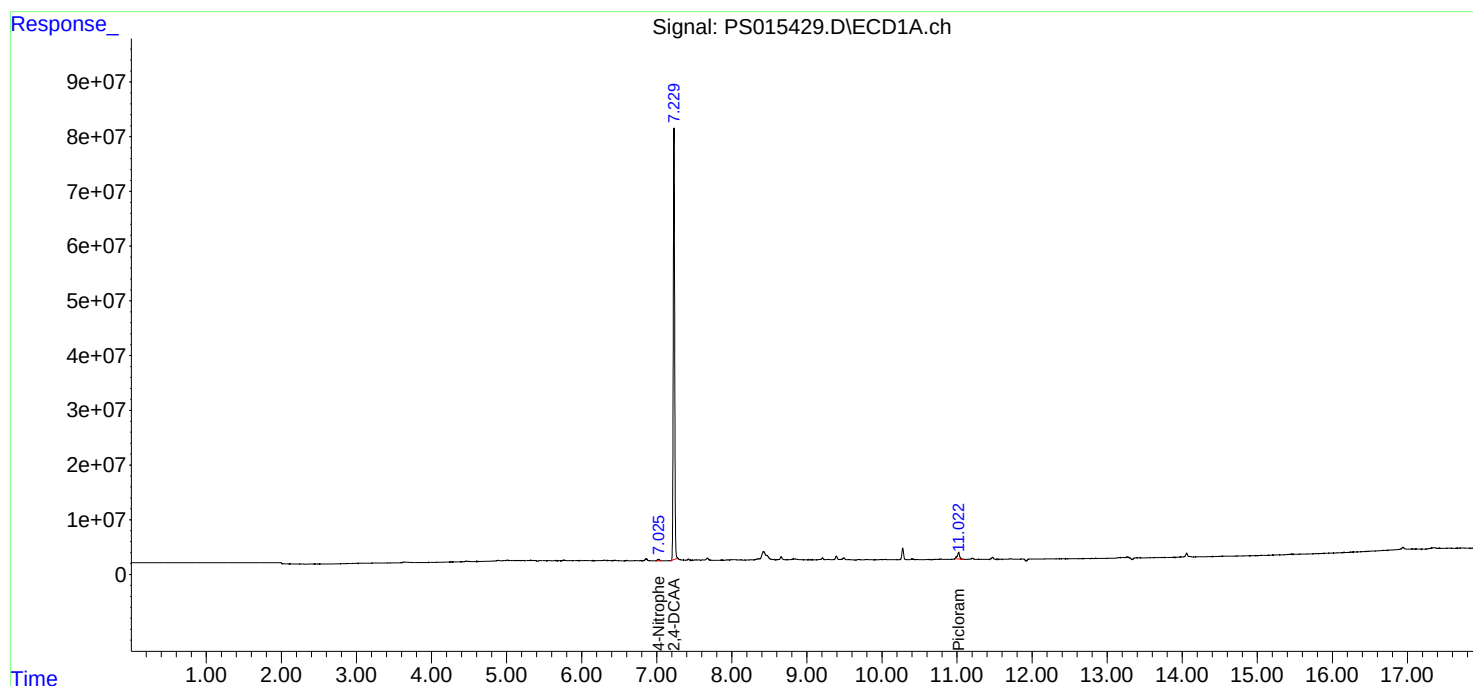


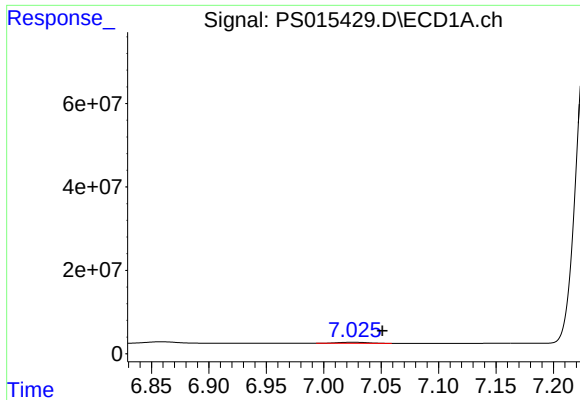

#3 4-Nitrophenol


R.T.: 7.025 min
Delta R.T.: -0.026 min
Response: 4312799
Conc: 3.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

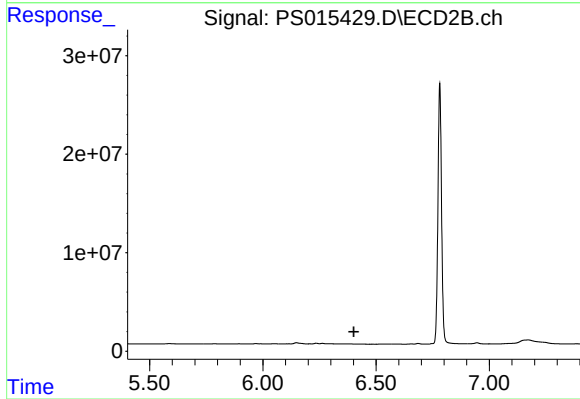


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

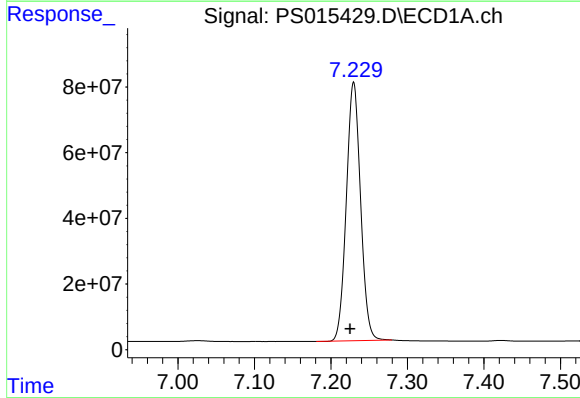


#4 2,4-DCAA

R.T.: 7.230 min
Delta R.T.: 0.005 min
Response: 1022629081
Conc: 405.74 ng/ml

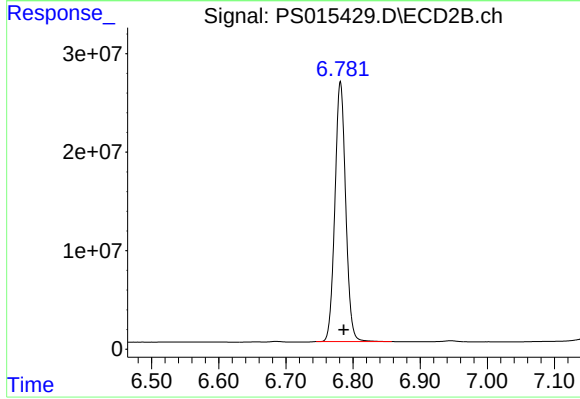

#4 2,4-DCAA


R.T.: 6.781 min
Delta R.T.: -0.005 min
Response: 293856717
Conc: 548.47 ng/ml

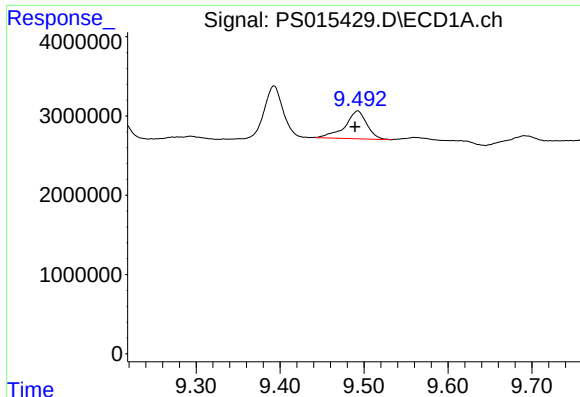

#12 2,4,5-T


R.T.: 9.493 min
Delta R.T.: 0.003 min
Response: 6341368
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

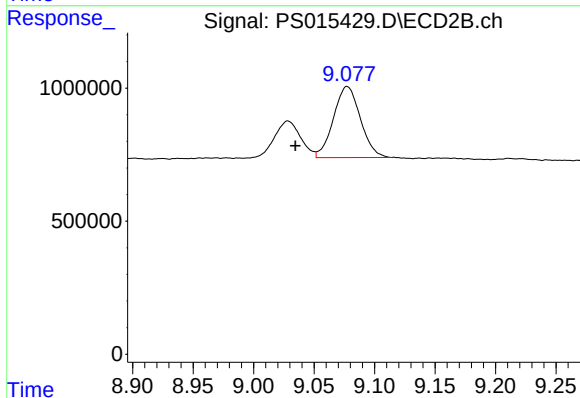


#12 2,4,5-T

R.T.: 9.077 min
Delta R.T.: 0.043 min
Response: 4140900
Conc: 1.43 ng/ml

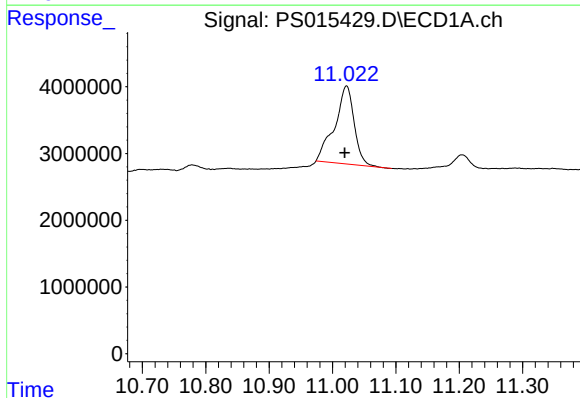


#15 Picloram

R.T.: 11.022 min
Delta R.T.: 0.003 min
Response: 25009636
Conc: 1.51 ng/ml

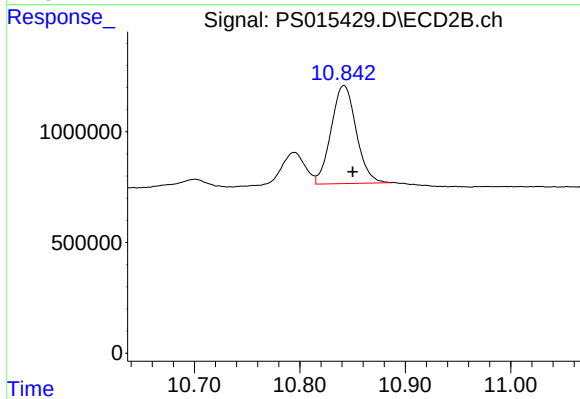

#15 Picloram


R.T.: 10.842 min
Delta R.T.: -0.008 min
Response: 7312068
Conc: 1.76 ng/ml

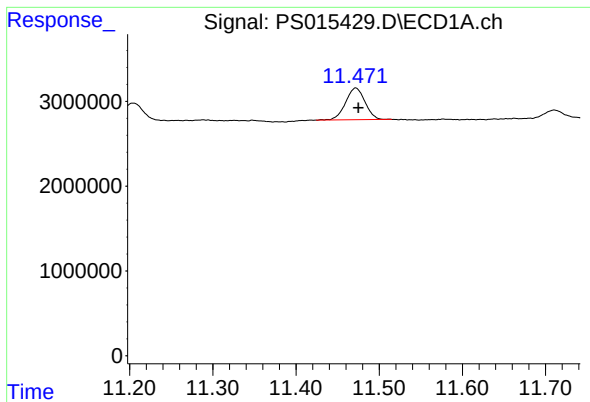

#16 DCPA

R.T.: 11.472 min
Delta R.T.: -0.003 min
Response: 6041714
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

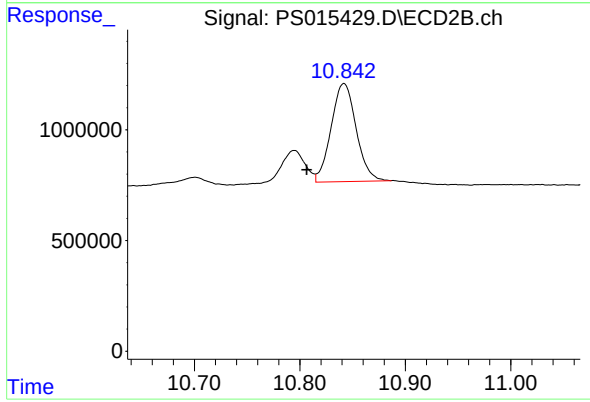

#16 DCPA

R.T.: 10.842 min
Delta R.T.: 0.035 min
Response: 7312068
Conc: 1.70 ng/ml