

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061121\
 Data File : PS015441.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2021 14:07
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 02:19:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.230	6.782	1180.9E6	293.8E6	468.558	548.394
Target Compounds							
3) T	4-Nitroph...	7.024	0.000	5893583	0	4.181	N.D. #
5) T	DICAMBA	7.422	0.000	3912524	0	<MDL	N.D. #
7) T	MCPA	7.674f	0.000	13574904	0	1.353	N.D. #
9) T	2,4-D	8.347	0.000	6470004	0	2.539	N.D. #
10) T	Pentachlo...	8.657	0.000	9784293	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.208	0.000	6237030	0	<MDL	N.D. #
12) T	2,4,5-T	9.493	9.078f	8690535	4707724	<MDL	1.626 #
14) T	DINOSEB	11.204	0.000	5631459	0	<MDL	N.D. #
15) T	Picloram	11.022	10.842	33271483	7866472	2.008	1.894
16) T	DCPA	11.471	10.842	8599063	7866472	<MDL	1.825 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061121\
Data File : PS015441.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2021 14:07
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 02:19:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

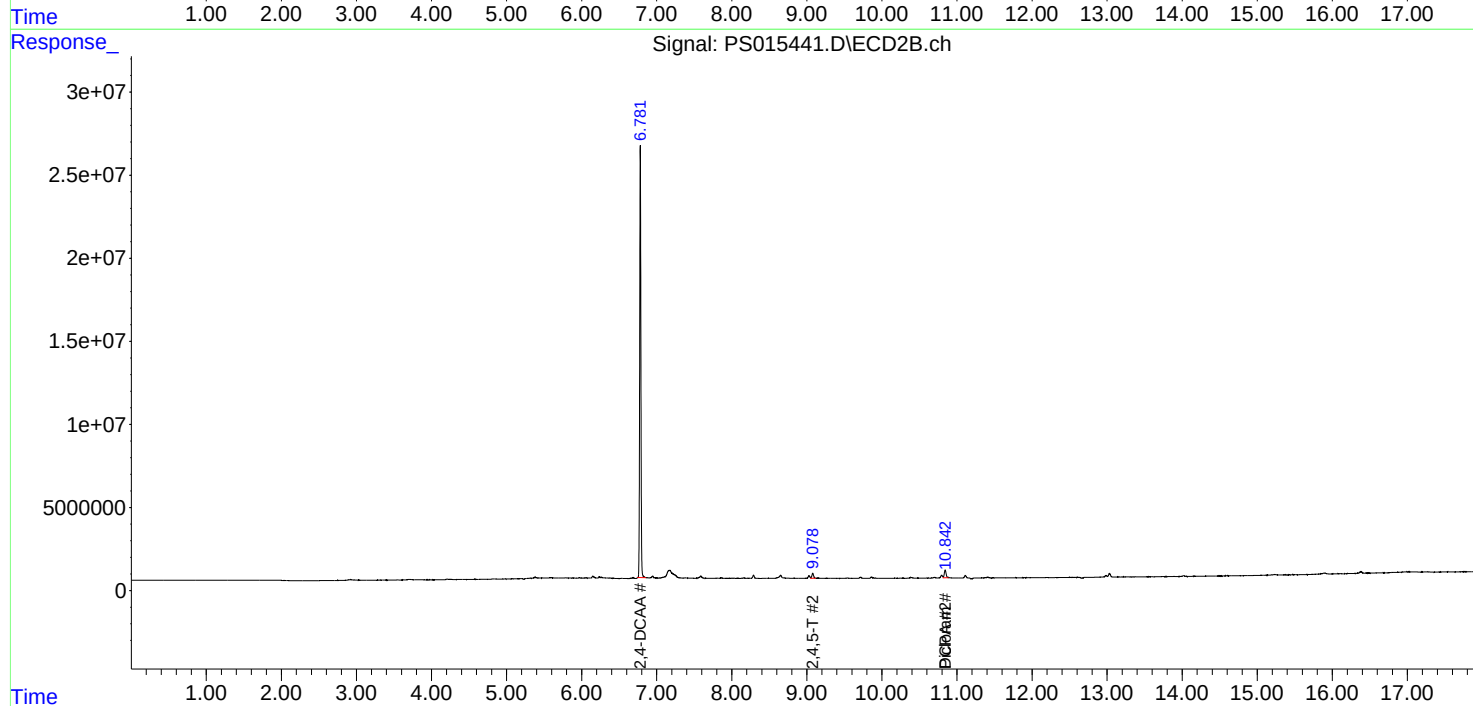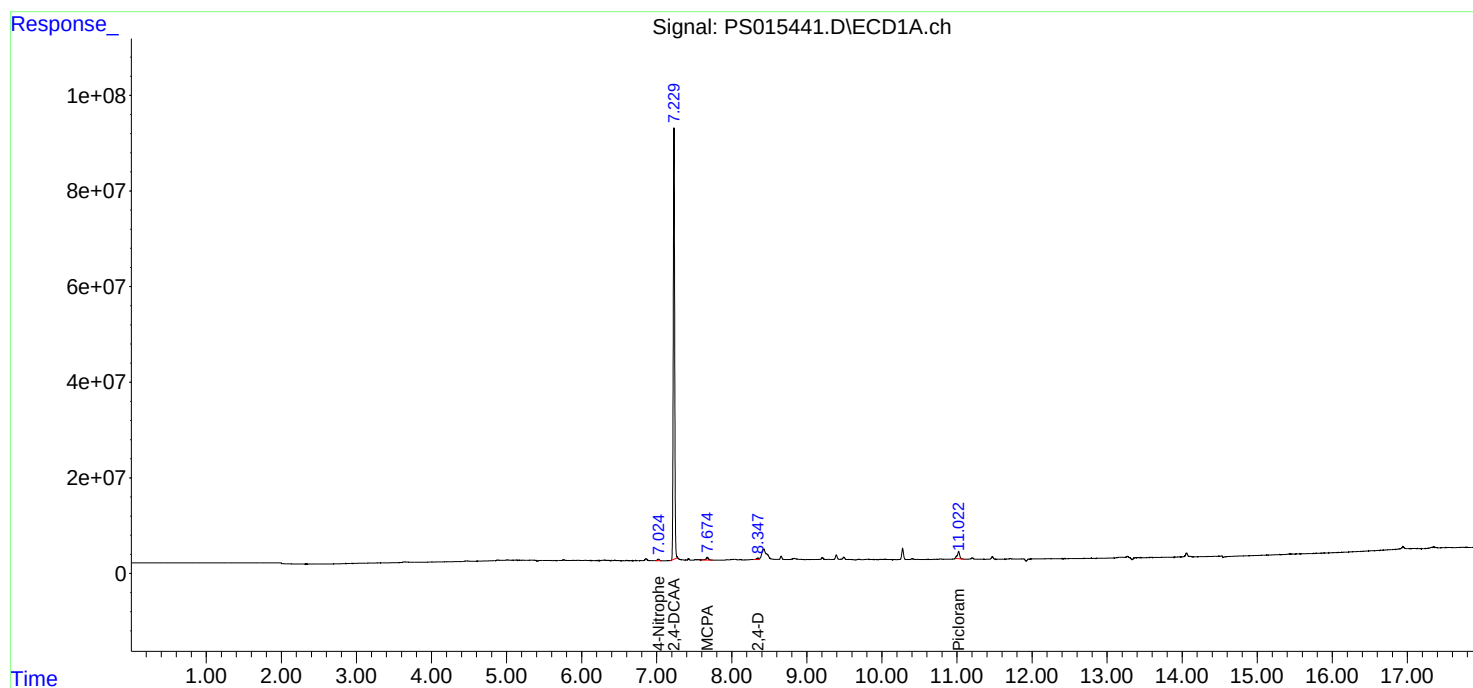


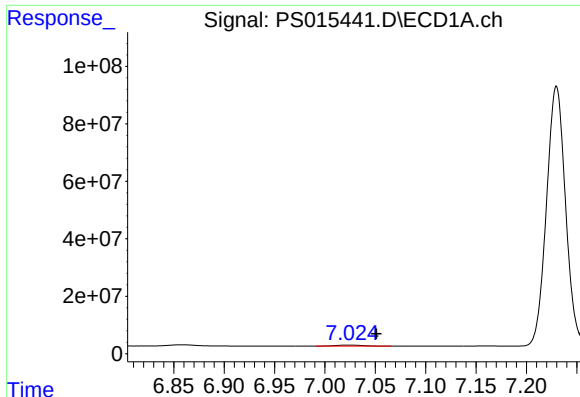

#3 4-Nitrophenol


R.T.: 7.024 min
Delta R.T.: -0.027 min
Response: 5893583
Conc: 4.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

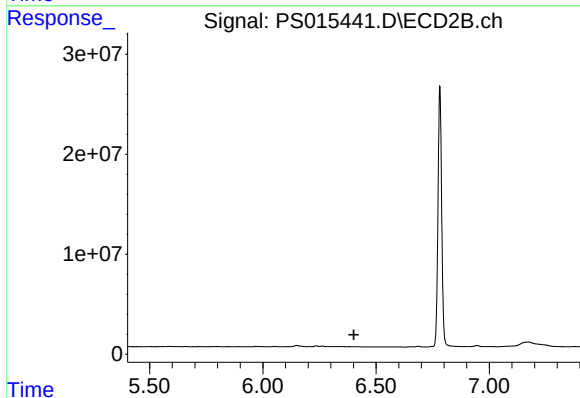


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

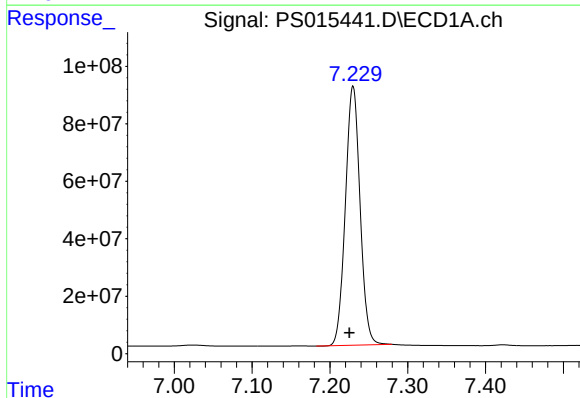


#4 2,4-DCAA

R.T.: 7.230 min
Delta R.T.: 0.005 min
Response: 1180942506
Conc: 468.56 ng/ml

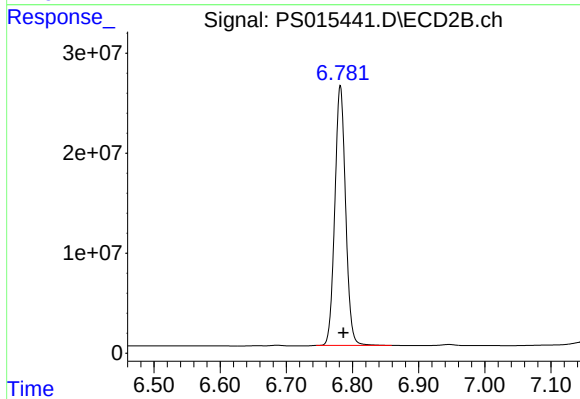

#4 2,4-DCAA


R.T.: 6.782 min
Delta R.T.: -0.005 min
Response: 293813866
Conc: 548.39 ng/ml

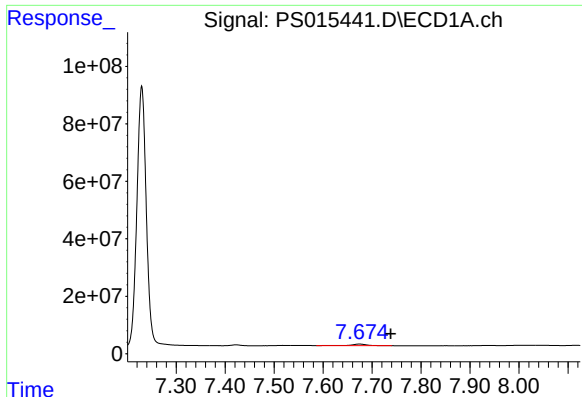

#7 MCPA


R.T.: 7.674 min
Delta R.T.: -0.064 min
Response: 13574904
Conc: 1.35 ug/ml

Instrument :
ECD_S
ClientSampleId :

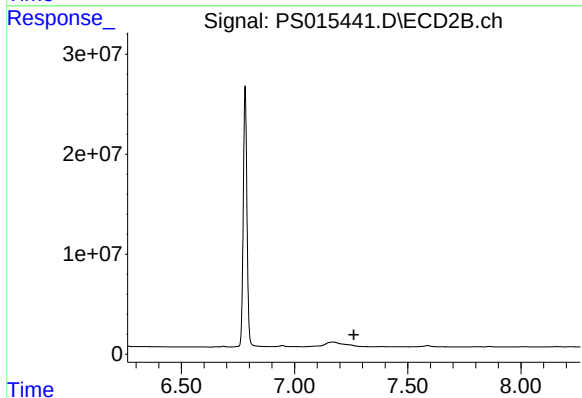


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.262 min
Response: 0
Conc: N.D.

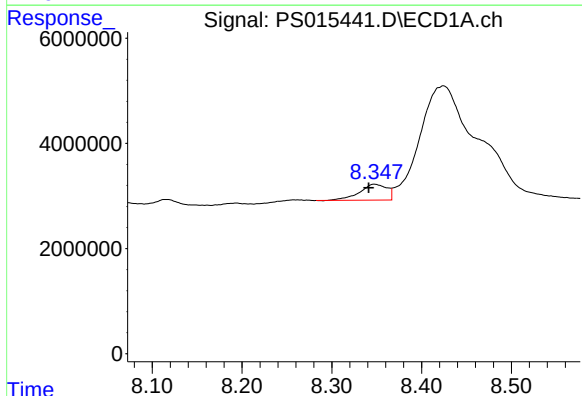


#9 2,4-D

R.T.: 8.347 min
Delta R.T.: 0.006 min
Response: 6470004
Conc: 2.54 ng/ml

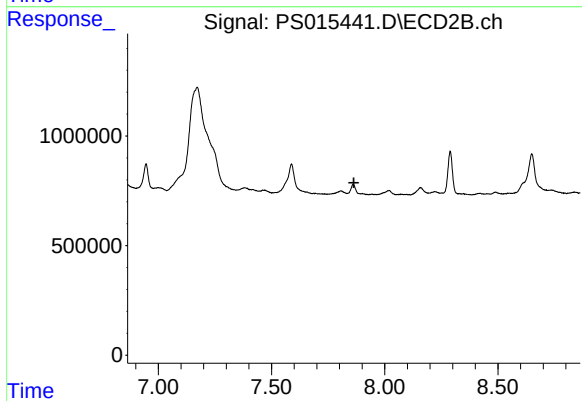

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.864 min
Response: 0
Conc: N.D.

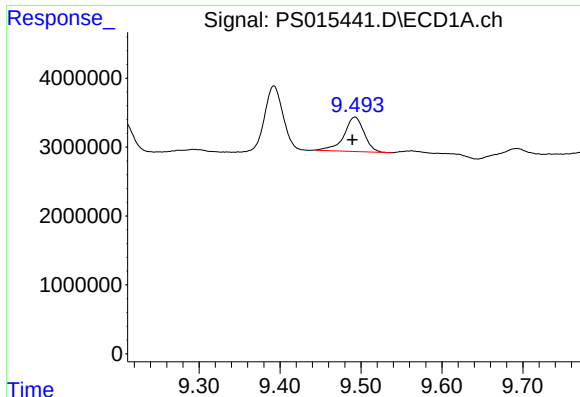

#12 2,4,5-T


R.T.: 9.493 min
Delta R.T.: 0.003 min
Response: 8690535
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

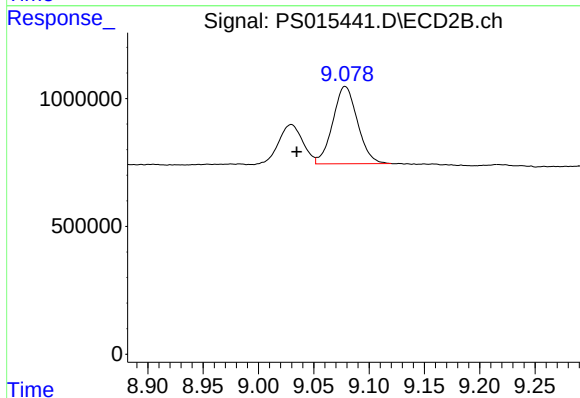


#12 2,4,5-T

R.T.: 9.078 min
Delta R.T.: 0.044 min
Response: 4707724
Conc: 1.63 ng/ml

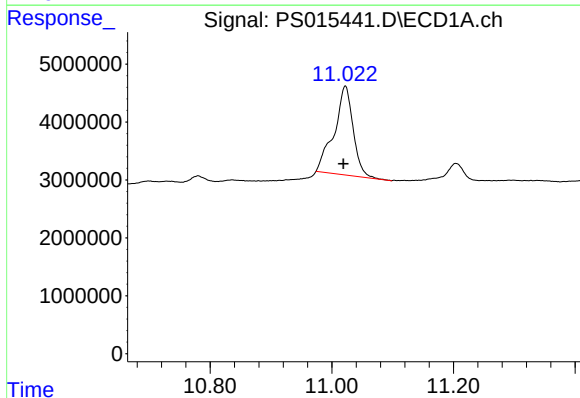


#15 Picloram

R.T.: 11.022 min
Delta R.T.: 0.003 min
Response: 33271483
Conc: 2.01 ng/ml

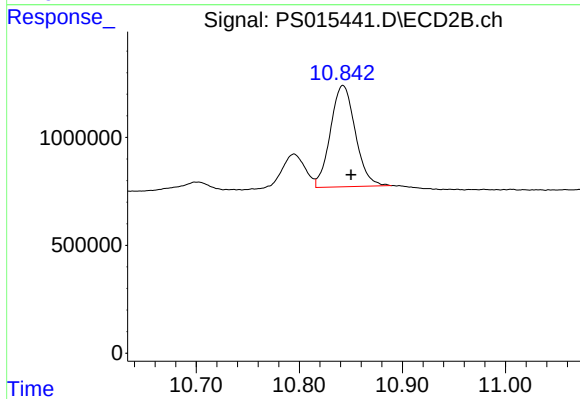

#15 Picloram


R.T.: 10.842 min
Delta R.T.: -0.008 min
Response: 7866472
Conc: 1.89 ng/ml

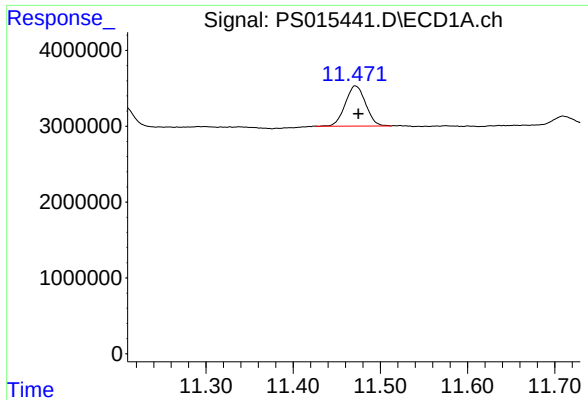

#16 DCPA

R.T.: 11.471 min
Delta R.T.: -0.004 min
Response: 8599063
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

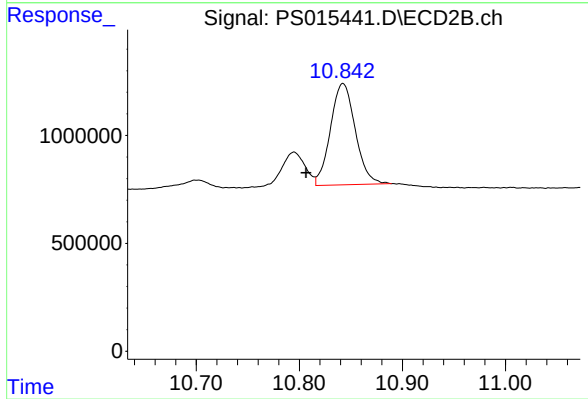

#16 DCPA

R.T.: 10.842 min
Delta R.T.: 0.036 min
Response: 7866472
Conc: 1.82 ng/ml