

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061121\
 Data File : PS0CCC1.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2021 18:33
 Operator : DD\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 141 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 02:36:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.781	1988.4E6	408.3E6	788.912	762.083
Target Compounds							
1) T	Dalapon	3.044	2.520	1976.5E6	428.7E6	752.003	655.117
2) T	3,5-DICHL...	6.440	5.968	2501.5E6	571.5E6	725.418	707.390
3) T	4-Nitroph...	7.055	6.399	975.1E6	221.3E6	691.694	695.380
5) T	DICAMBA	7.422	6.947	7377.8E6	1621.4E6	774.025	732.680
6) T	MCPD	7.593	7.044	583.6E6	131.9E6	81.093	74.645
7) T	MCPA	7.741	7.257	793.7E6	190.7E6	79.083	73.391
8) T	DICHLORPROP	8.116	7.567	1768.5E6	396.5E6	767.890	729.863
9) T	2,4-D	8.343	7.858	1940.5E6	462.3E6	761.554	717.843
10) T	Pentachlo...	8.657	8.289	25108.3E6	5377.6E6	775.647	730.532
11) T	2,4,5-TP ...	9.207	8.650	9886.5E6	2147.3E6	796.589	739.955
12) T	2,4,5-T	9.490	9.027	9630.0E6	2148.4E6	801.774	742.097
13) T	2,4-DB	10.039	9.533	2103.6E6	286.3E6	826.072	742.142
14) T	DINOSEB	11.204	9.862	7099.8E6	1522.9E6	888.629	833.937
15) T	Picloram	11.019	10.839	12968.4E6	3074.9E6	782.793	740.412
16) T	DCPA	11.471	10.795	14270.8E6	3296.1E6	846.323	764.571



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061121\
Data File : PS0CCC1.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2021 18:33
Operator : DD\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 141 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 02:36:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

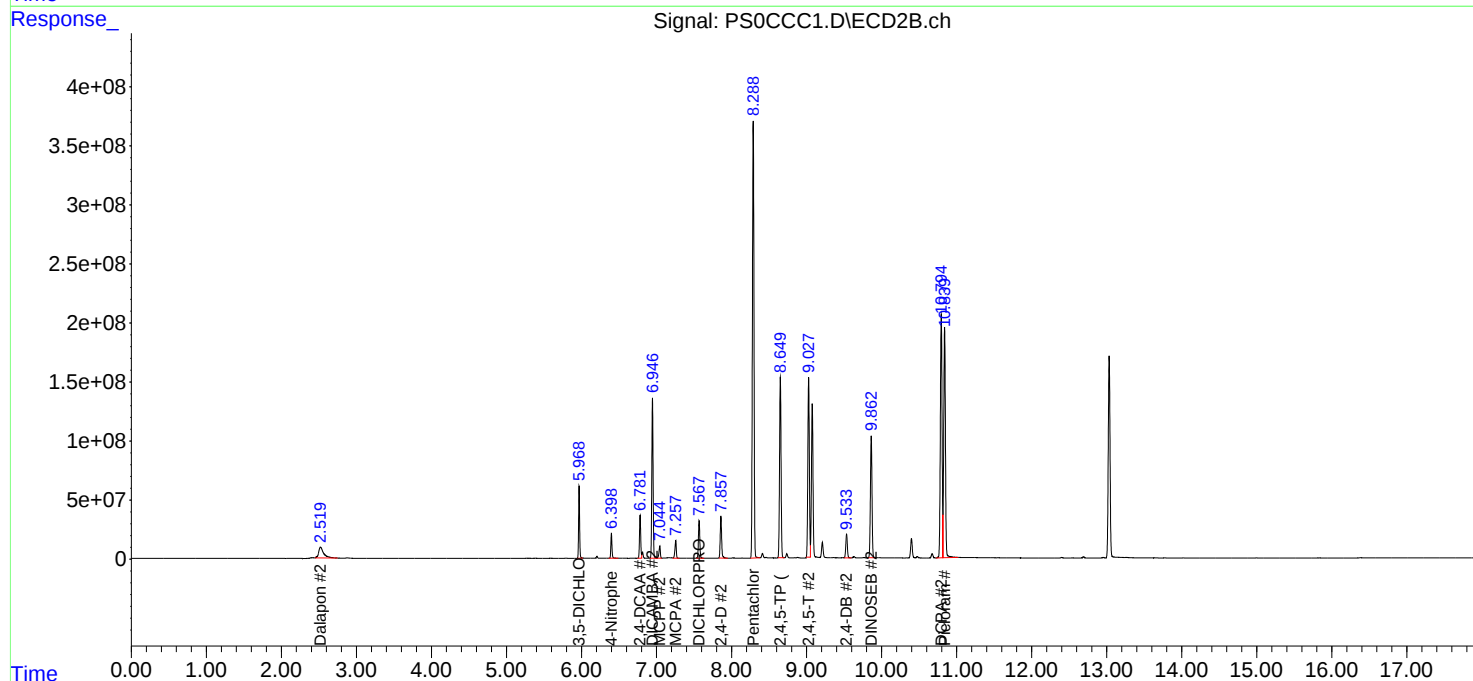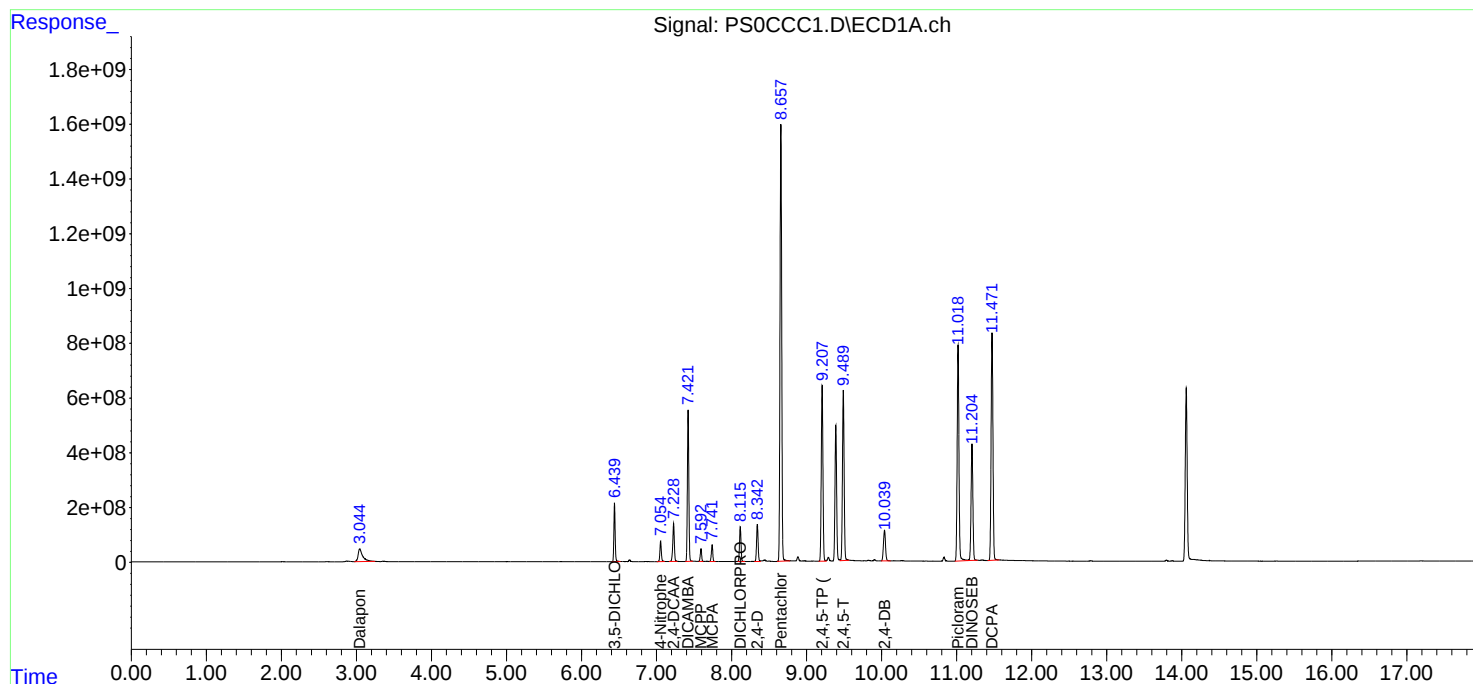


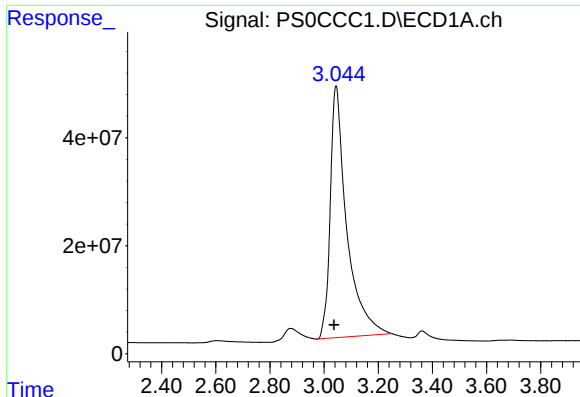

#1 Dalapon


R.T.: 3.044 min
Delta R.T.: 0.007 min
Response: 1976548720
Conc: 752.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

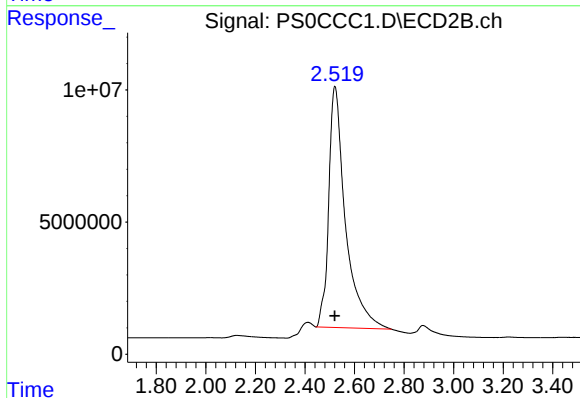


#1 Dalapon

R.T.: 2.520 min
Delta R.T.: 0.000 min
Response: 428742839
Conc: 655.12 ng/ml

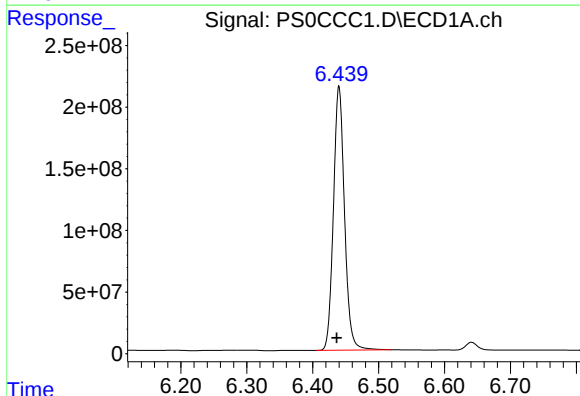


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.440 min
Delta R.T.: 0.003 min
Response: 2501540994
Conc: 725.42 ng/ml

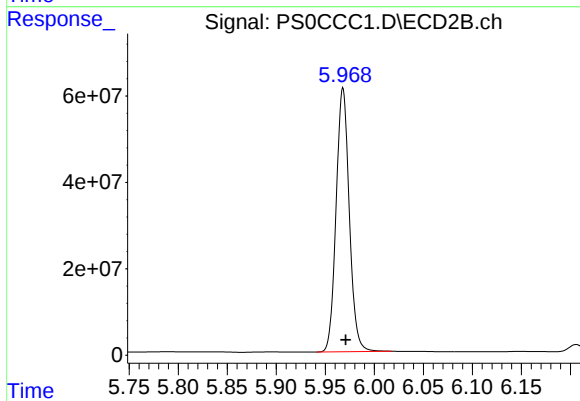

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.968 min
Delta R.T.: -0.003 min
Response: 571460893
Conc: 707.39 ng/ml

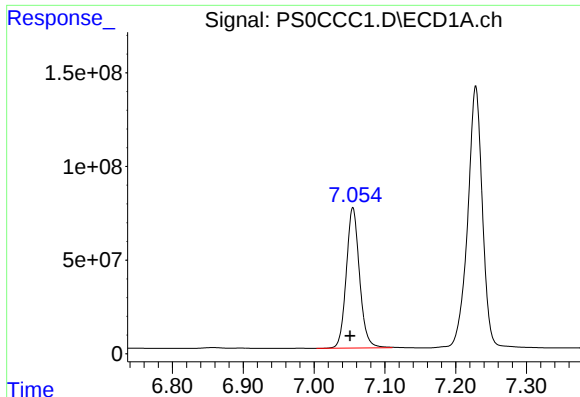

#3 4-Nitrophenol


R.T.: 7.055 min
Delta R.T.: 0.004 min
Response: 975078814
Conc: 691.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

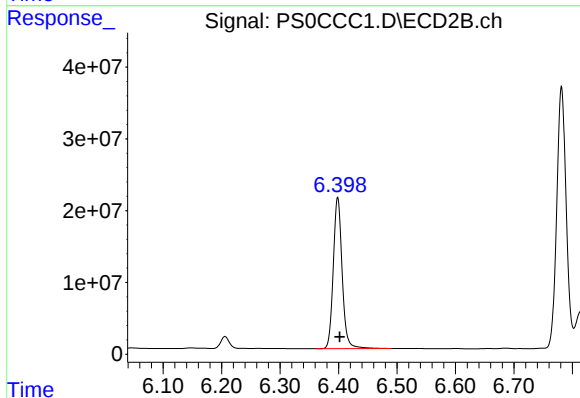


#3 4-Nitrophenol

R.T.: 6.399 min
Delta R.T.: -0.004 min
Response: 221251967
Conc: 695.38 ng/ml

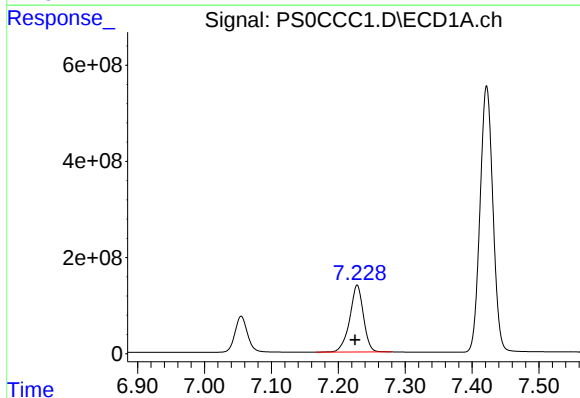


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: 0.003 min
Response: 1988354409
Conc: 788.91 ng/ml

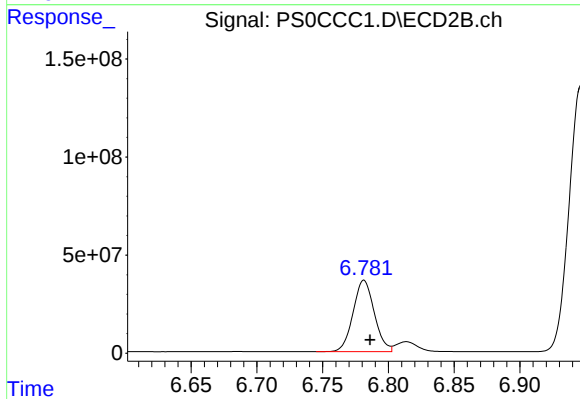

#4 2,4-DCAA


R.T.: 6.781 min
Delta R.T.: -0.005 min
Response: 408302160
Conc: 762.08 ng/ml

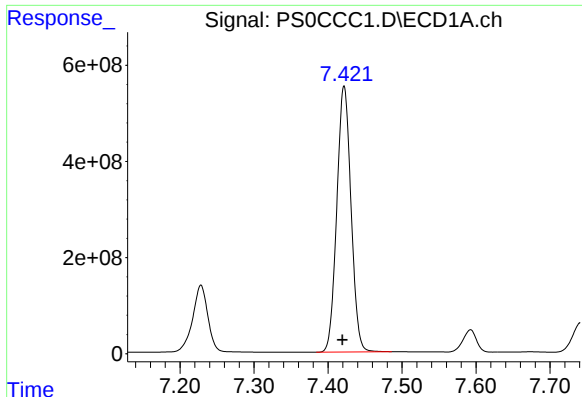

#5 DICAMBA


R.T.: 7.422 min
Delta R.T.: 0.002 min
Response: 7377812245
Conc: 774.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

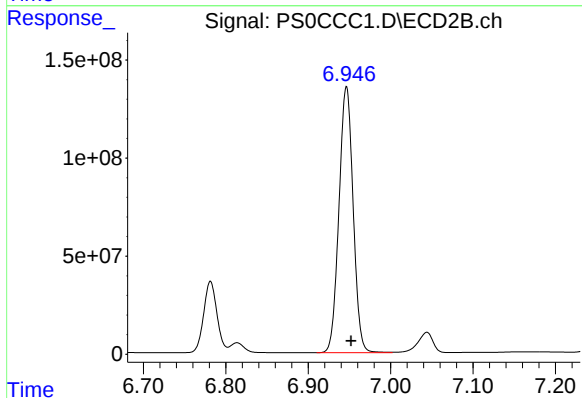


#5 DICAMBA

R.T.: 6.947 min
Delta R.T.: -0.005 min
Response: 1621375035
Conc: 732.68 ng/ml

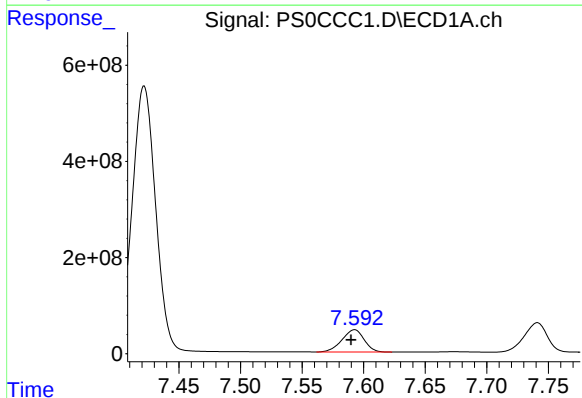


#6 MCP

R.T.: 7.593 min
Delta R.T.: 0.003 min
Response: 583568286
Conc: 81.09 ug/ml

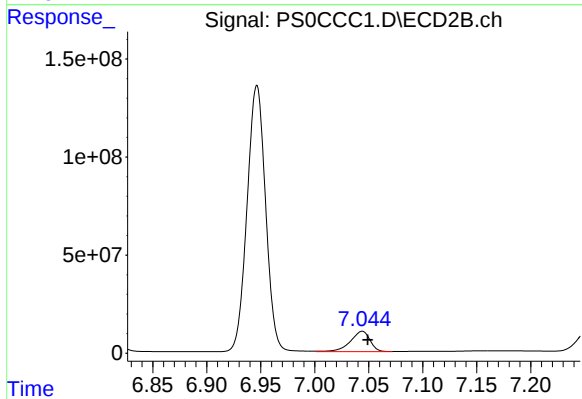

#6 MCP


R.T.: 7.044 min
Delta R.T.: -0.005 min
Response: 131905163
Conc: 74.64 ug/ml

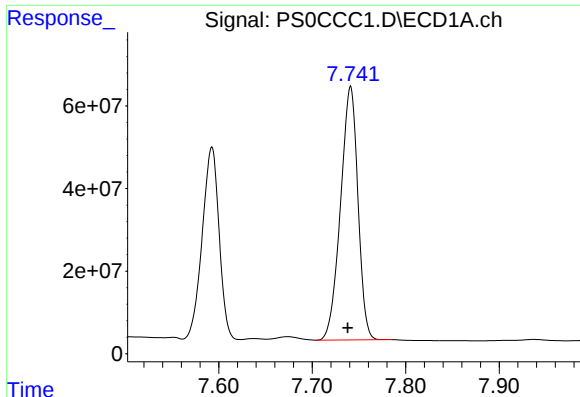

#7 MCPA


R.T.: 7.741 min
Delta R.T.: 0.003 min
Response: 793708907
Conc: 79.08 ug/ml

Instrument :
ECD_S
ClientSampleId :

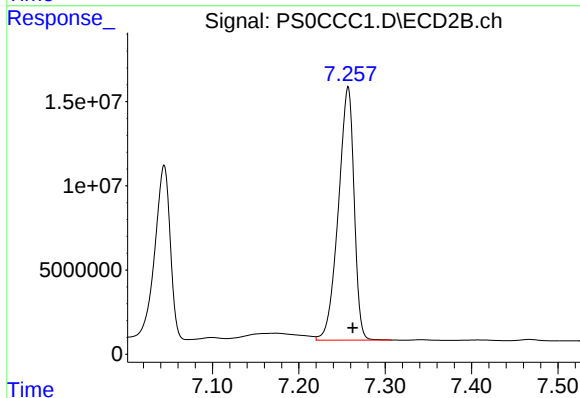


#7 MCPA

R.T.: 7.257 min
Delta R.T.: -0.005 min
Response: 190725131
Conc: 73.39 ug/ml

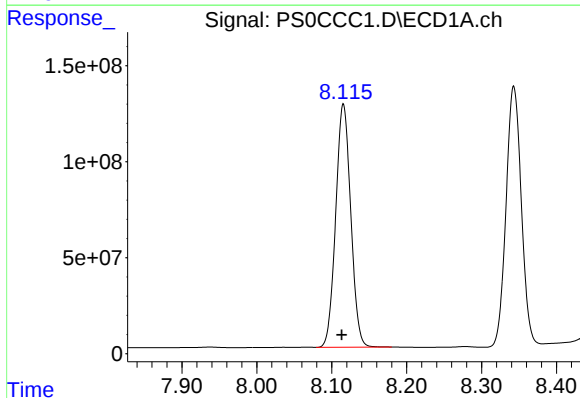


#8 DICHLORPROP

R.T.: 8.116 min
Delta R.T.: 0.002 min
Response: 1768530029
Conc: 767.89 ng/ml

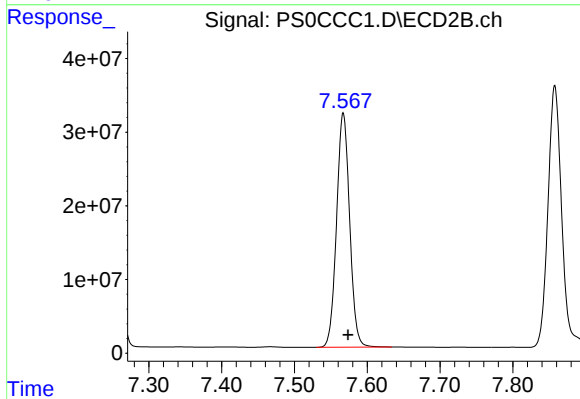

#8 DICHLORPROP


R.T.: 7.567 min
Delta R.T.: -0.007 min
Response: 396508240
Conc: 729.86 ng/ml

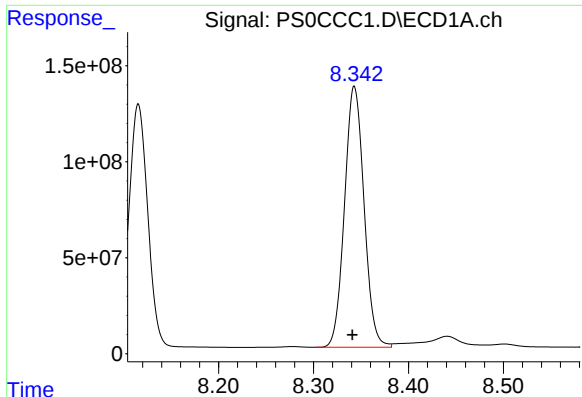

#9 2,4-D


R.T.: 8.343 min
Delta R.T.: 0.002 min
Response: 1940527398
Conc: 761.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

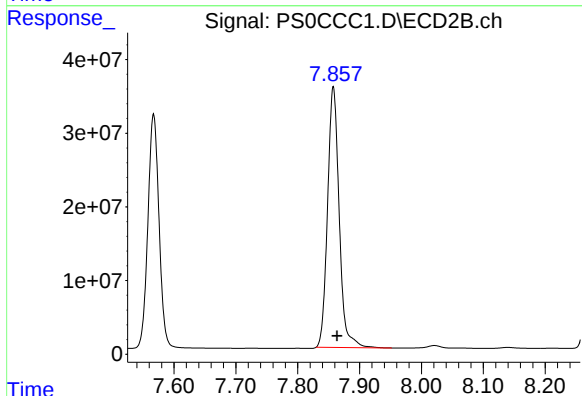


#9 2,4-D

R.T.: 7.858 min
Delta R.T.: -0.006 min
Response: 462309192
Conc: 717.84 ng/ml

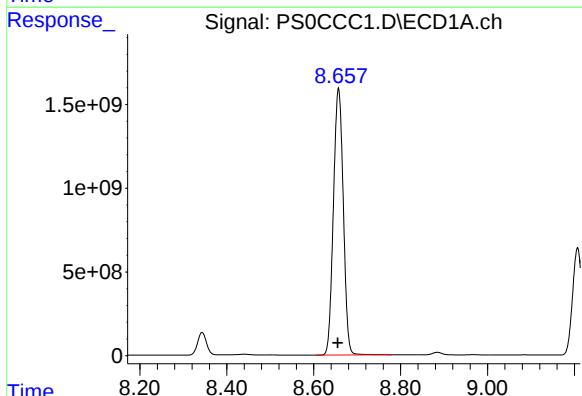


#10 Pentachlorophenol

R.T.: 8.657 min
Delta R.T.: 0.002 min
Response: 25108311373
Conc: 775.65 ng/ml

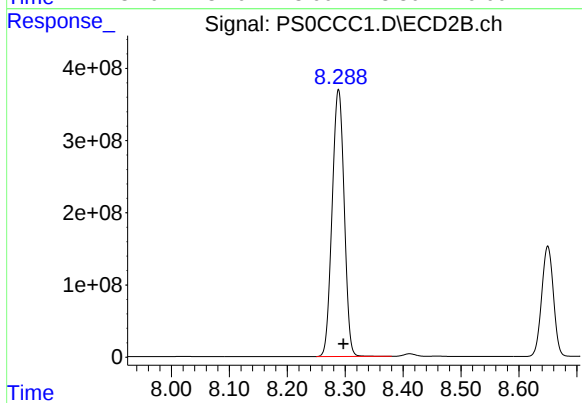

#10 Pentachlorophenol


R.T.: 8.289 min
Delta R.T.: -0.008 min
Response: 5377587331
Conc: 730.53 ng/ml

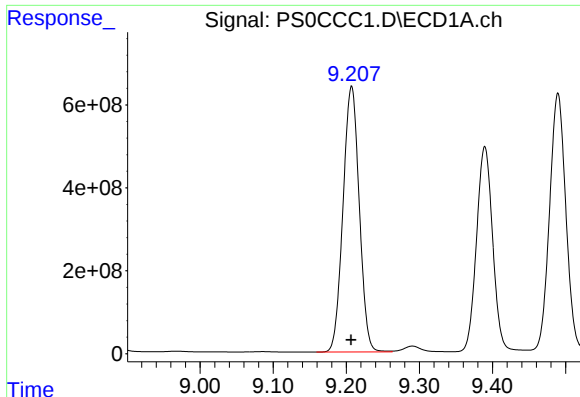

#11 2,4,5-TP (SILVEX)


R.T.: 9.207 min
Delta R.T.: 0.000 min
Response: 9886477132
Conc: 796.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

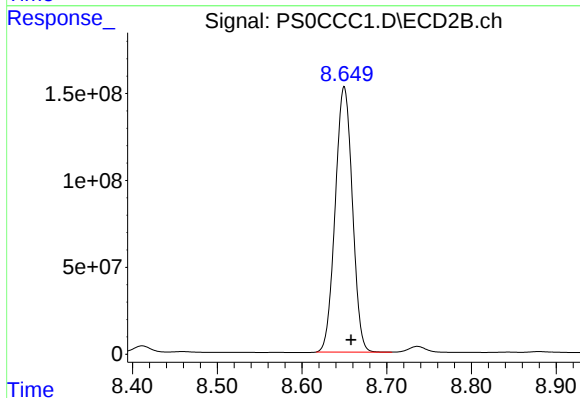


#11 2,4,5-TP (SILVEX)

R.T.: 8.650 min
Delta R.T.: -0.008 min
Response: 2147303674
Conc: 739.96 ng/ml

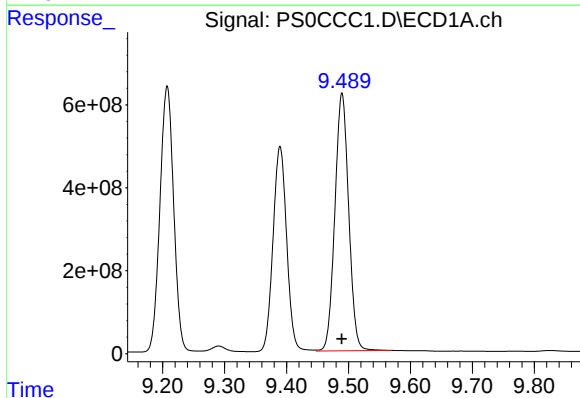


#12 2,4,5-T

R.T.: 9.490 min
Delta R.T.: 0.000 min
Response: 9630030210
Conc: 801.77 ng/ml

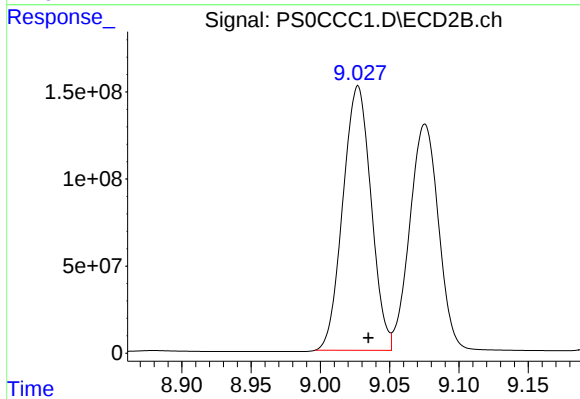

#12 2,4,5-T


R.T.: 9.027 min
Delta R.T.: -0.007 min
Response: 2148370792
Conc: 742.10 ng/ml

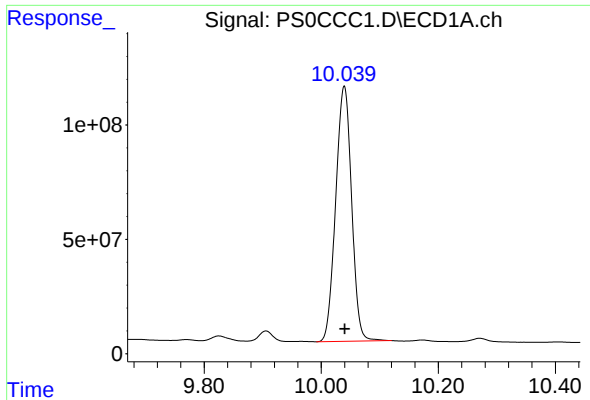

#13 2,4-DB


R.T.: 10.039 min
Delta R.T.: 0.000 min
Response: 2103614161
Conc: 826.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

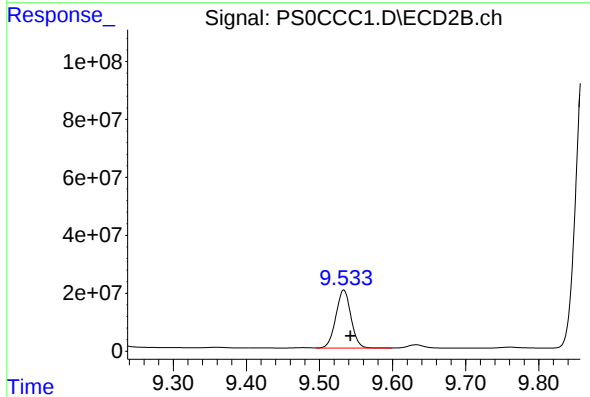


#13 2,4-DB

R.T.: 9.533 min
Delta R.T.: -0.009 min
Response: 286280788
Conc: 742.14 ng/ml

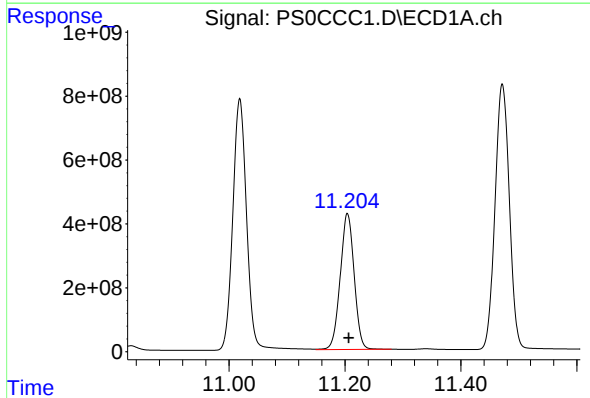


#14 DINOSEB

R.T.: 11.204 min
Delta R.T.: -0.002 min
Response: 7099764557
Conc: 888.63 ng/ml

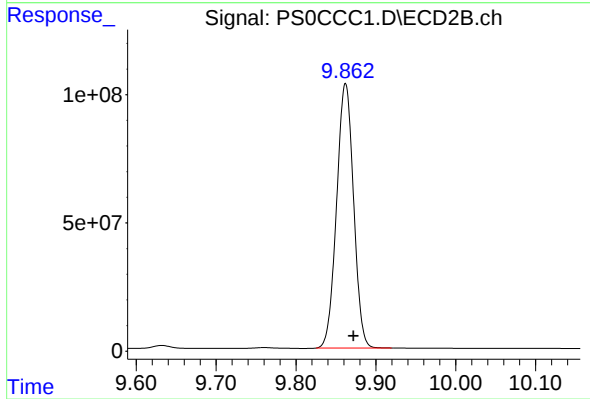

#14 DINOSEB


R.T.: 9.862 min
Delta R.T.: -0.010 min
Response: 1522886653
Conc: 833.94 ng/ml

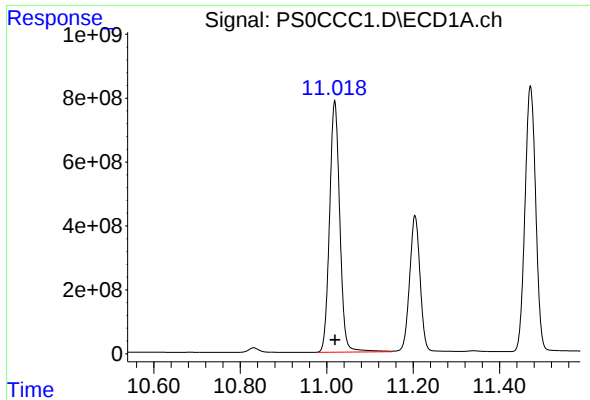

#15 Picloram


R.T.: 11.019 min
Delta R.T.: 0.000 min
Response: 12968361172
Conc: 782.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

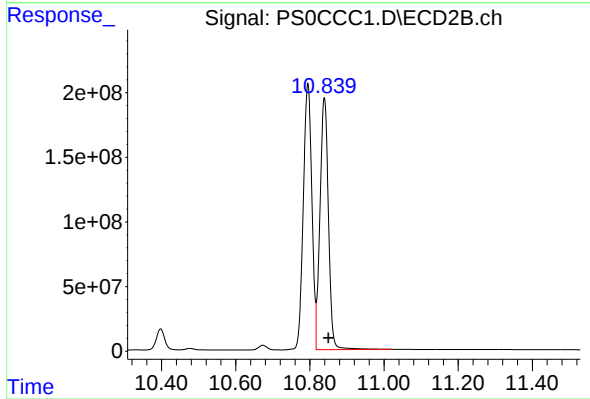


#15 Picloram

R.T.: 10.839 min
Delta R.T.: -0.011 min
Response: 3074850754
Conc: 740.41 ng/ml

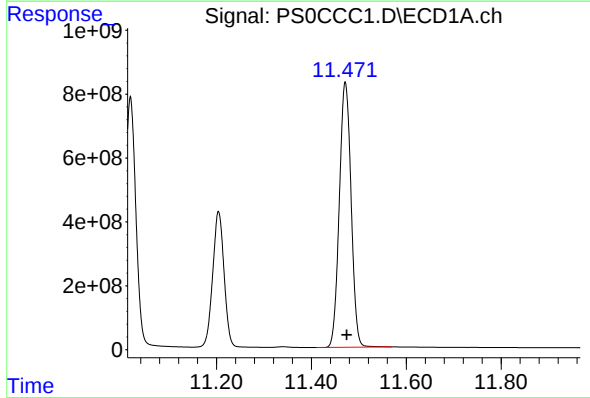

#16 DCPA

R.T.: 11.471 min
Delta R.T.: -0.004 min
Response: 14270779331
Conc: 846.32 ng/ml

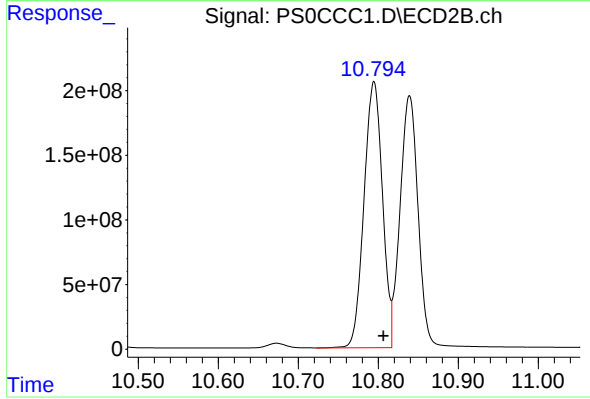

#16 DCPA

R.T.: 10.795 min
Delta R.T.: -0.012 min
Response: 3296062197
Conc: 764.57 ng/ml