

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061121\
 Data File : PS015477.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2021 05:48
 Operator : DD\AJ
 Sample : M2589-25
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 18-B8(2-4)

Manual Integrations
 APPROVED

Ankita
 6/14/2021 12:27:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 02:32:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.227	6.780	1467.4E6	277.3E6	582.206	517.485m

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061121\
Data File : PS015477.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2021 05:48
Operator : DD\AJ
Sample : M2589-25
Misc :
ALS Vial : 72 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
18-B8(2-4)


Manual Integrations
APPROVED

Ankita
6/14/2021 12:27:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 02:32:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

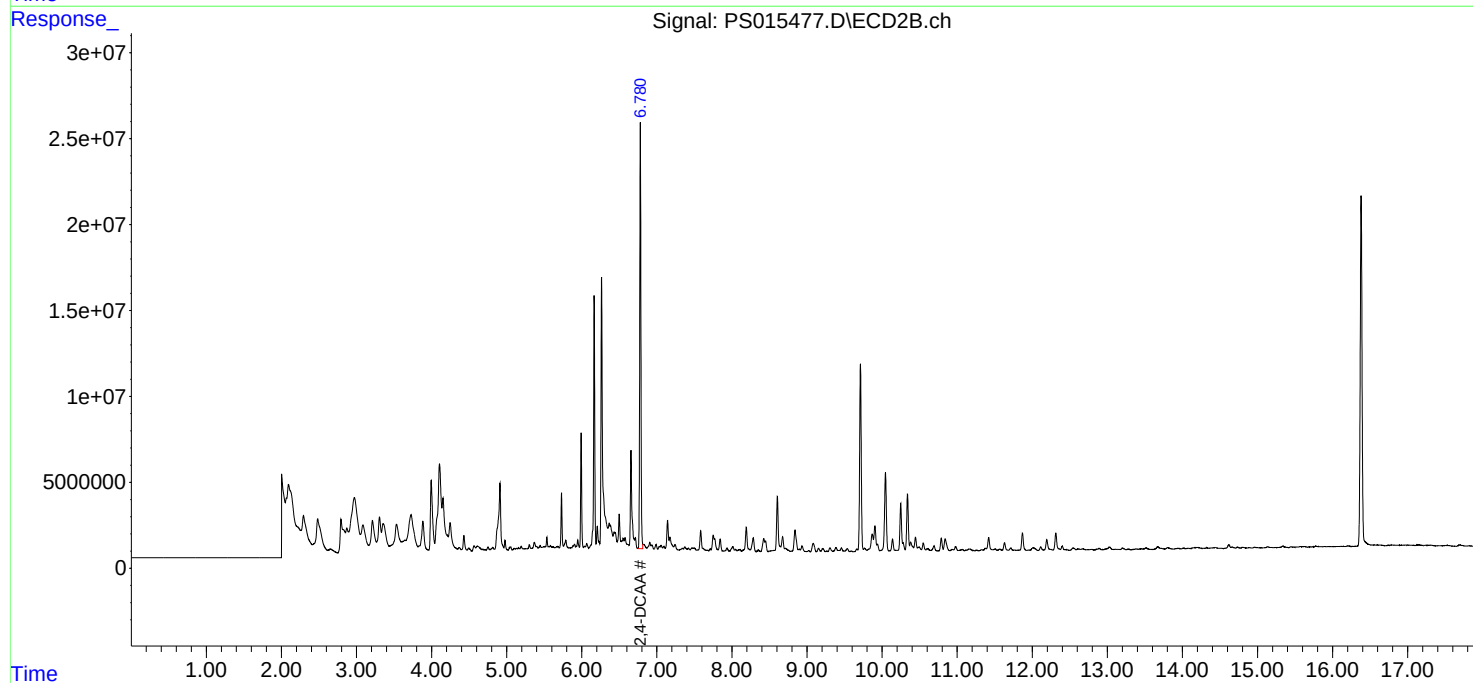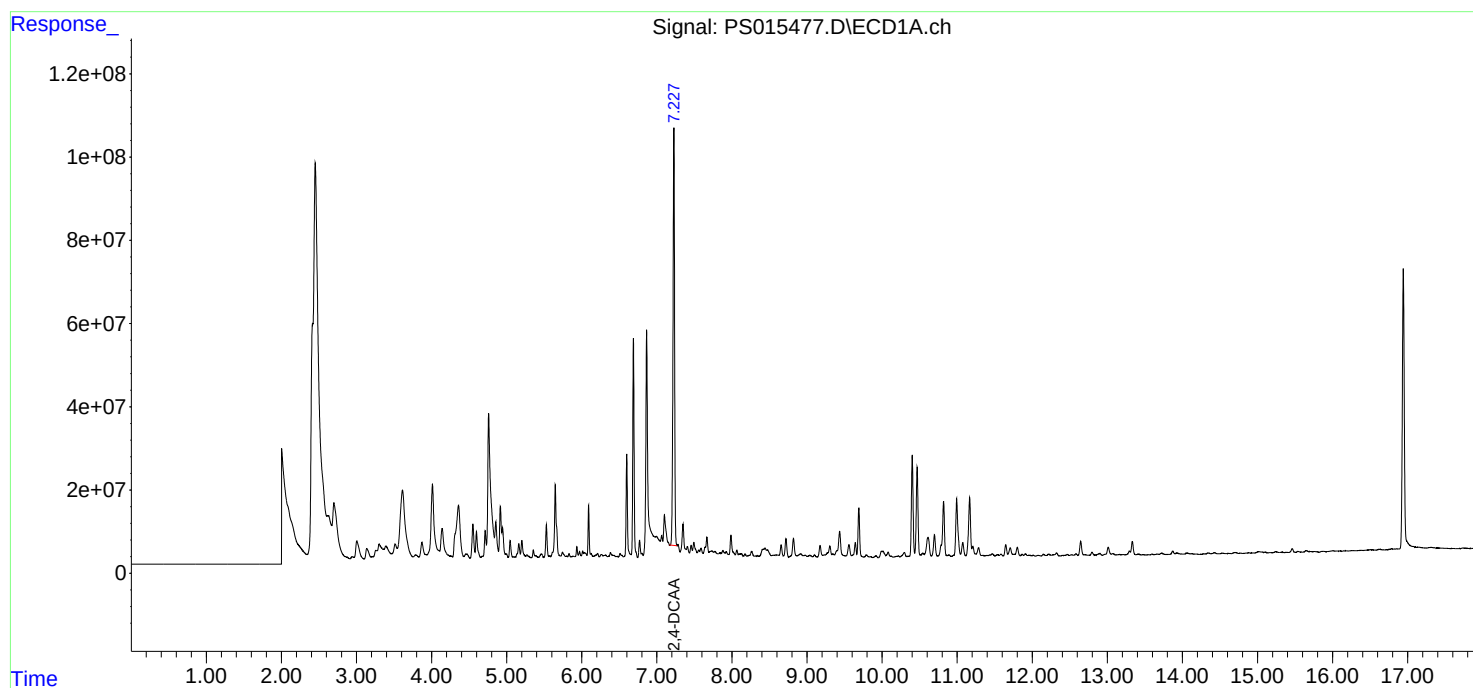

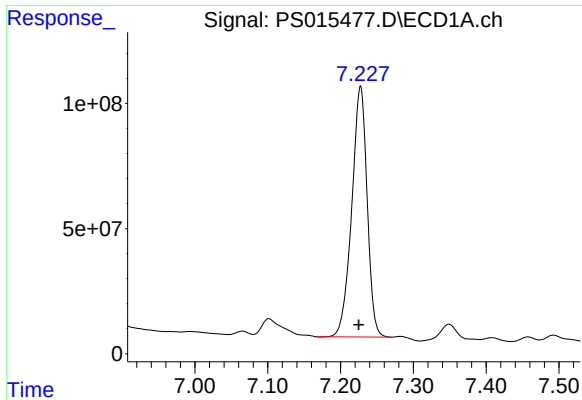


#4 2,4-DCAA

R.T.: 7.227 min
Delta R.T.: 0.002 min
Response: 1467378049
Conc: 582.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
18-B8(2-4)

Manual Integrations
APPROVED

Ankita
6/14/2021 12:27:51 PM

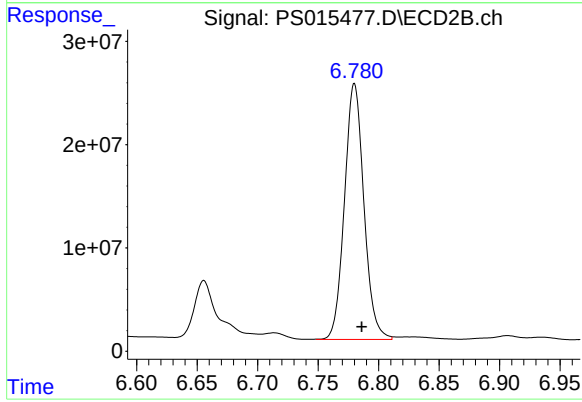

#4 2,4-DCAA

R.T.: 6.780 min
Delta R.T.: -0.007 min
Response: 277253313
Conc: 517.48 ng/ml m