

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061220\
 Data File : PS010792.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2020 09:26
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 14:39:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

2) T	3,5-DICHL...	6.485	0.000	41380871	0	37.853	N.D.	#
5) T	DICAMBA	0.000	7.154	0	29519571	N.D.	13.115	
6) T	MCP	0.000	7.154	0	29519571	N.D.	15.841	
12) T	2,4,5-T	0.000	9.237	0	8524111	N.D.	2.841	
15) T	Picloram	11.028	11.005	41522403	40522980	8.133	9.821	
16) T	DCPA	0.000	11.005	0	40522980	N.D.	10.928	



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061220\
Data File : PS010792.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2020 09:26
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 14:39:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

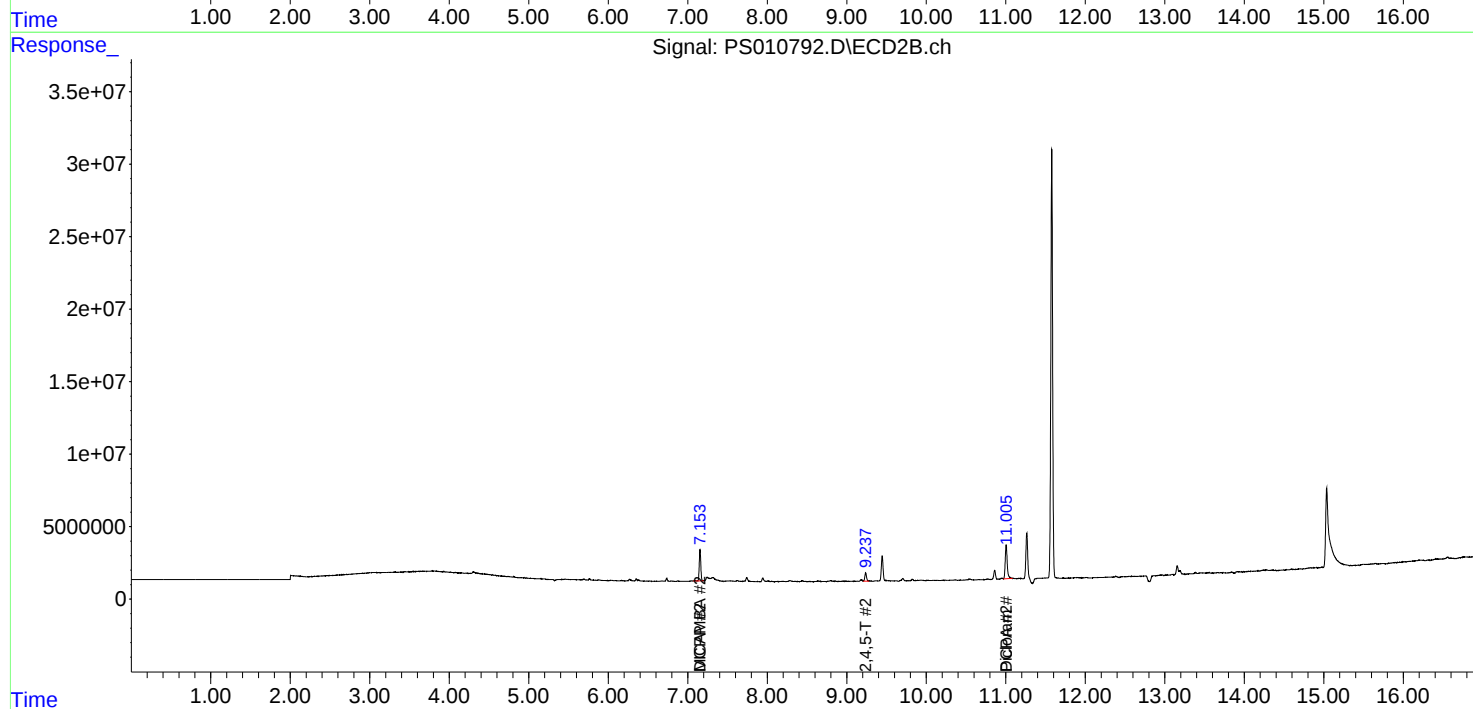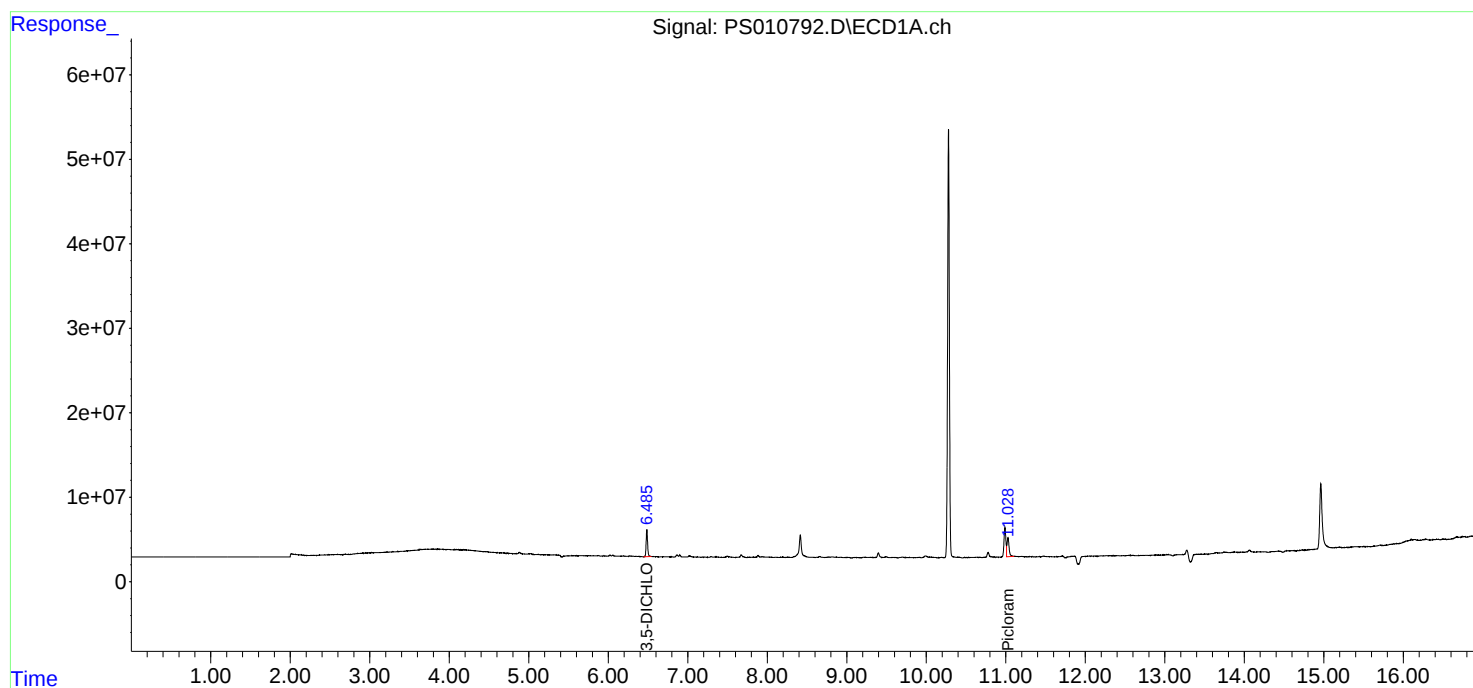


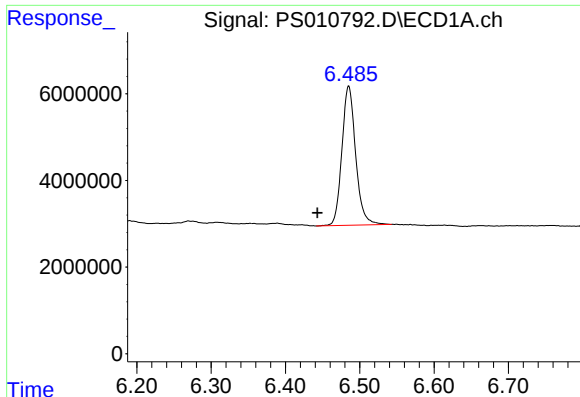

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.485 min
Delta R.T.: 0.042 min
Response: 41380871
Conc: 37.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

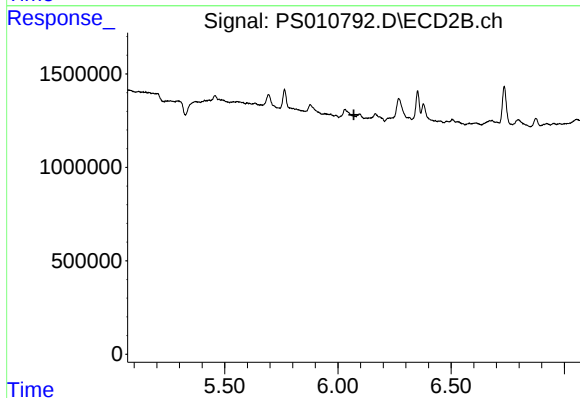


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.070 min
Response: 0
Conc: N.D.

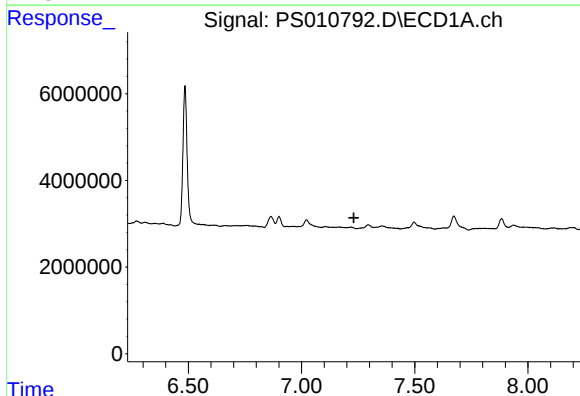


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.231 min
Response: 0
Conc: N.D.

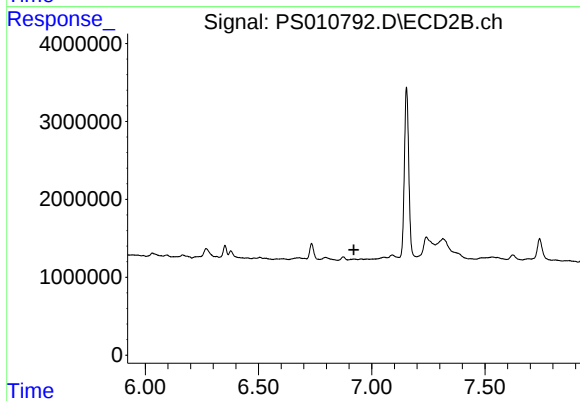

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.921 min
Response: 0
Conc: N.D.

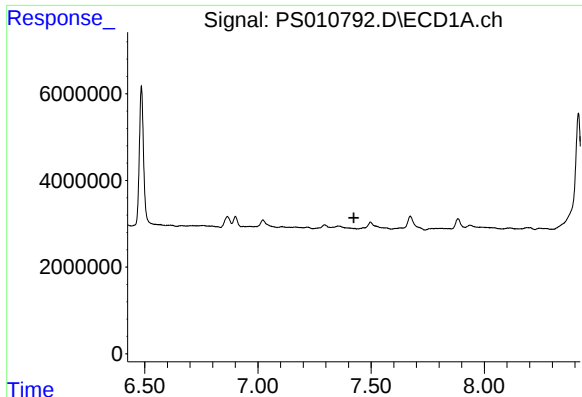

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.423 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

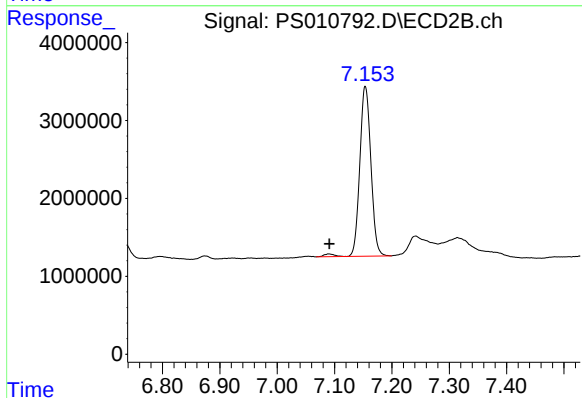


#5 DICAMBA

R.T.: 7.154 min
Delta R.T.: 0.063 min
Response: 29519571
Conc: 13.12 ng/ml

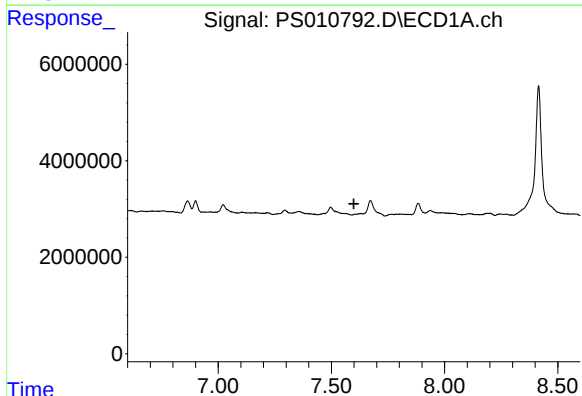


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.600 min
Response: 0
Conc: N.D.

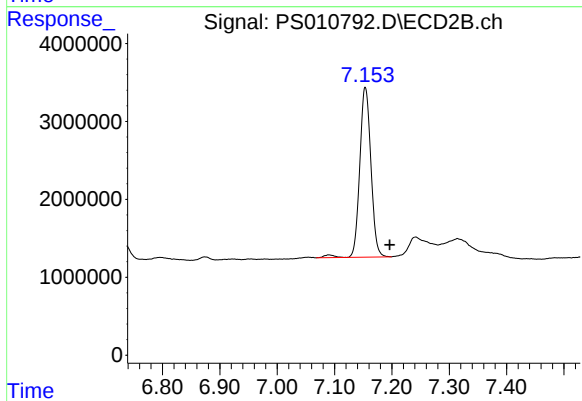

#6 MCP


R.T.: 7.154 min
Delta R.T.: -0.043 min
Response: 29519571
Conc: 15.84 ug/ml

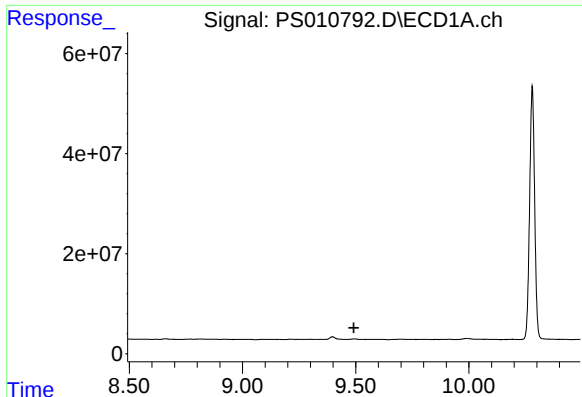

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

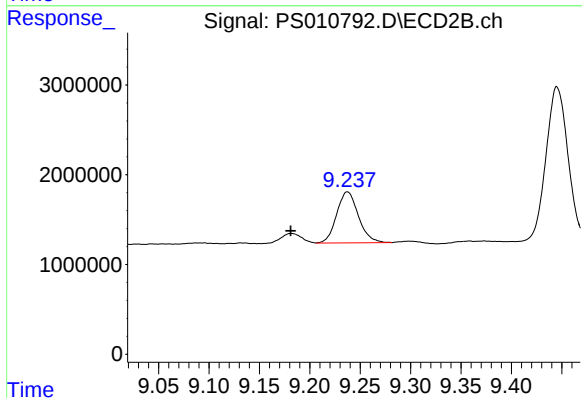


#12 2,4,5-T

R.T.: 9.237 min
Delta R.T.: 0.056 min
Response: 8524111
Conc: 2.84 ng/ml

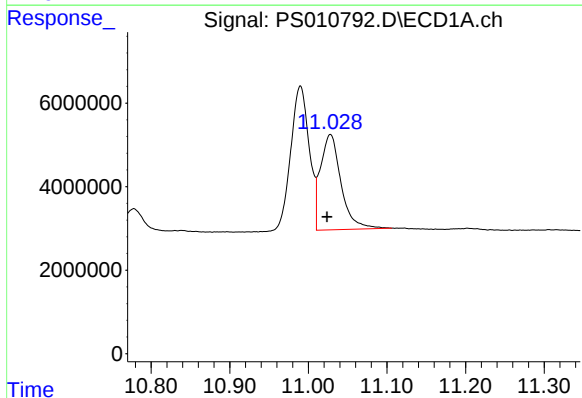


#15 Picloram

R.T.: 11.028 min
Delta R.T.: 0.004 min
Response: 41522403
Conc: 8.13 ng/ml

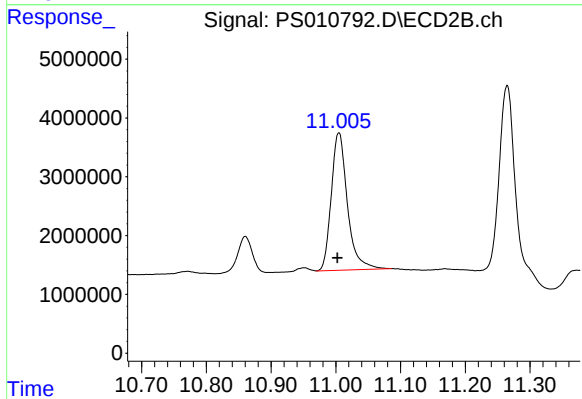

#15 Picloram


R.T.: 11.005 min
Delta R.T.: 0.002 min
Response: 40522980
Conc: 9.82 ng/ml

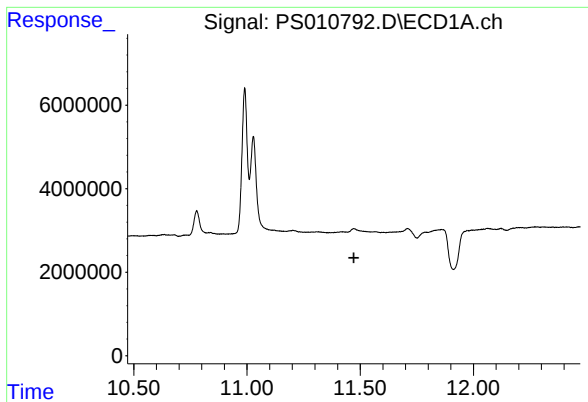

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

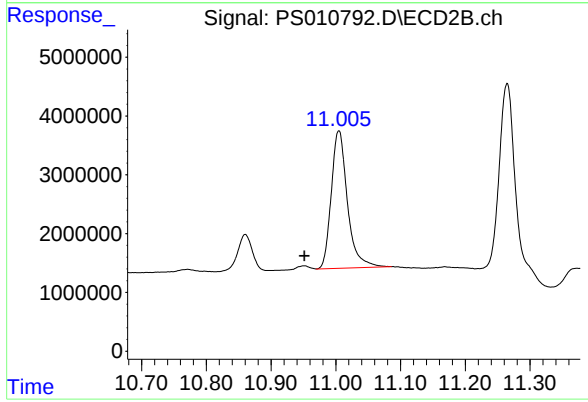

#16 DCPA

R.T.: 11.005 min
Delta R.T.: 0.054 min
Response: 40522980
Conc: 10.93 ng/ml