

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061220\
 Data File : PS010799.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2020 15:16
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 17:35:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.920	379.8E6	275.4E6	480.218	504.898
Target Compounds							
12) T	2,4,5-T	9.493	0.000	2550080	0	<MDL	N.D. #
13) T	2,4-DB	0.000	9.681	0	35601813	N.D.	87.641
15) T	Picloram	11.021	11.002	22146837	150.6E6	4.338	36.492 #
16) T	DCPA	0.000	11.002	0	150.6E6	N.D.	40.603



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061220\
Data File : PS010799.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2020 15:16
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 17:35:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

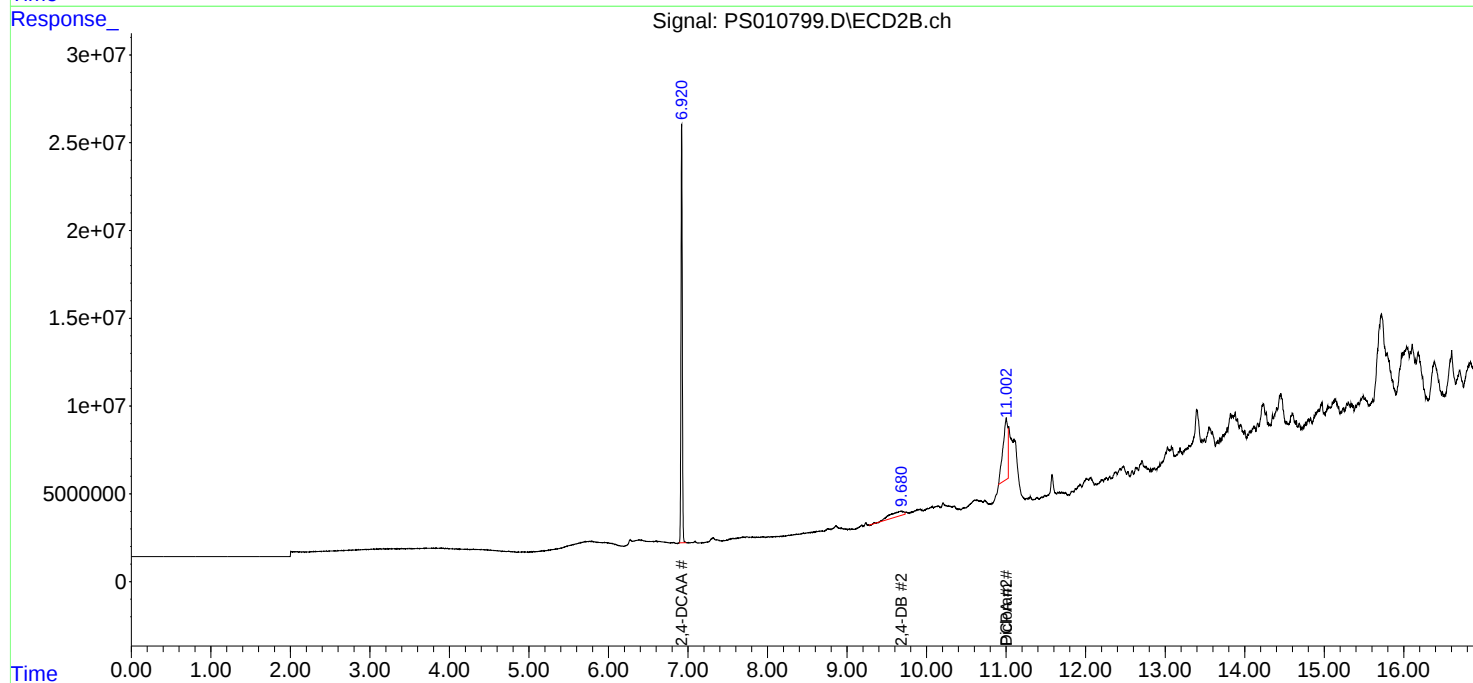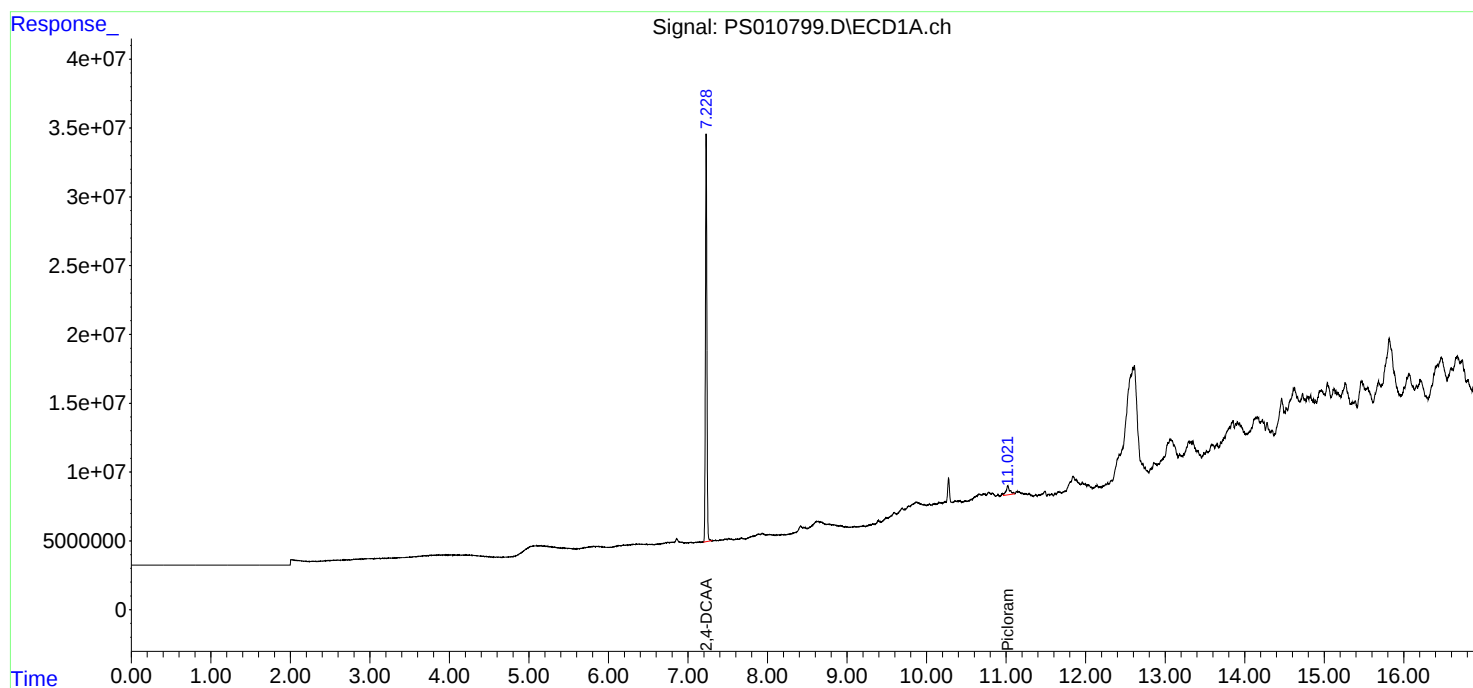


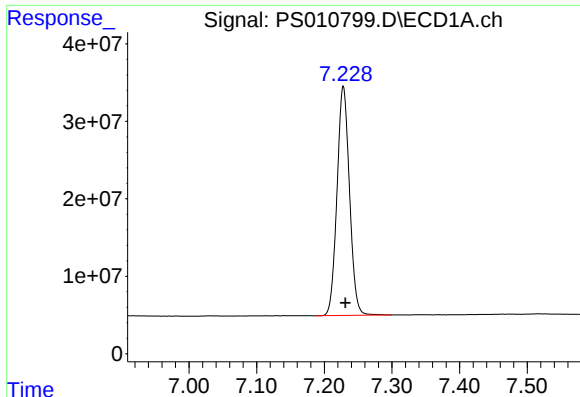

#4 2,4-DCAA


R.T.: 7.228 min
Delta R.T.: -0.003 min
Response: 379786076
Conc: 480.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

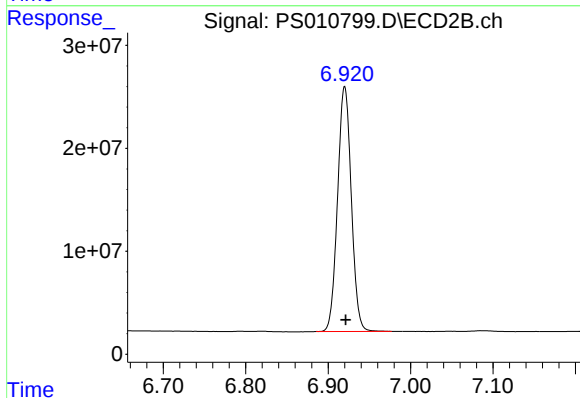


#4 2,4-DCAA

R.T.: 6.920 min
Delta R.T.: -0.001 min
Response: 275379114
Conc: 504.90 ng/ml

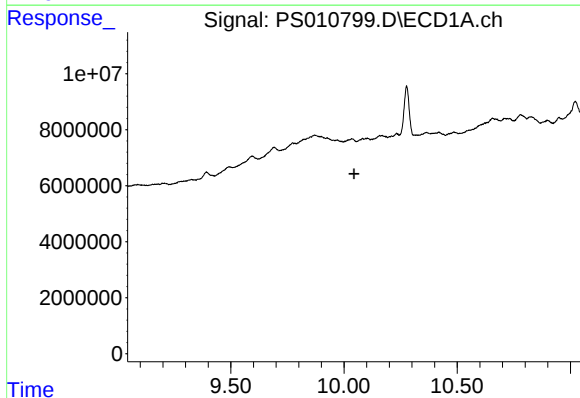


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.044 min
Response: 0
Conc: N.D.

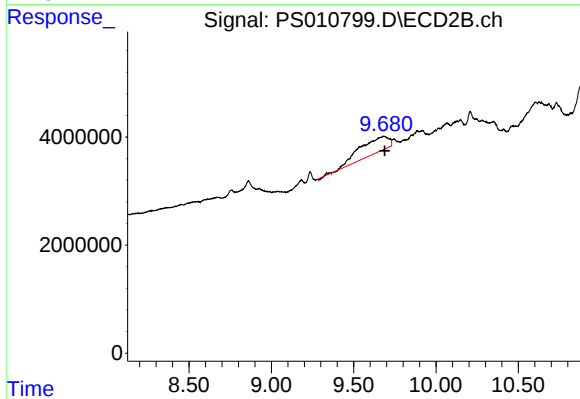

#13 2,4-DB


R.T.: 9.681 min
Delta R.T.: -0.007 min
Response: 35601813
Conc: 87.64 ng/ml

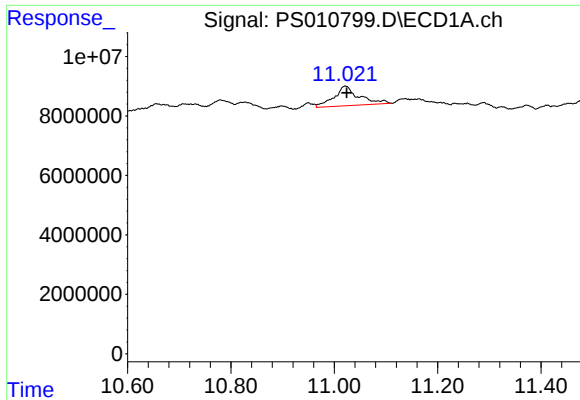

#15 Picloram


R.T.: 11.021 min
Delta R.T.: -0.003 min
Response: 22146837
Conc: 4.34 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

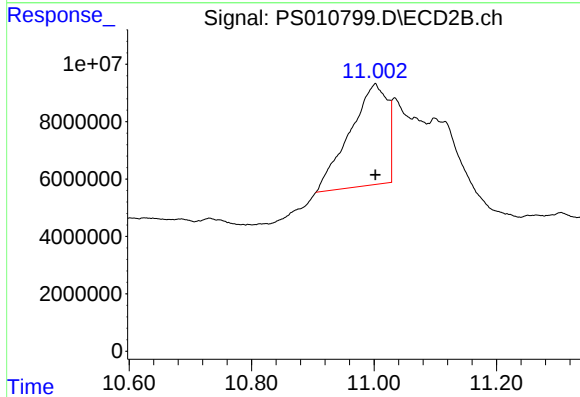


#15 Picloram

R.T.: 11.002 min
Delta R.T.: 0.000 min
Response: 150564684
Conc: 36.49 ng/ml

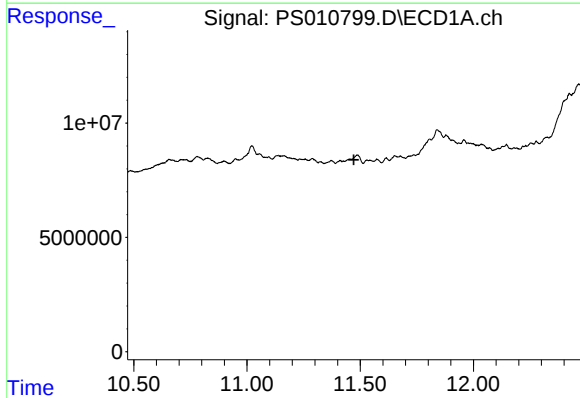

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.472 min
Response: 0
Conc: N.D.

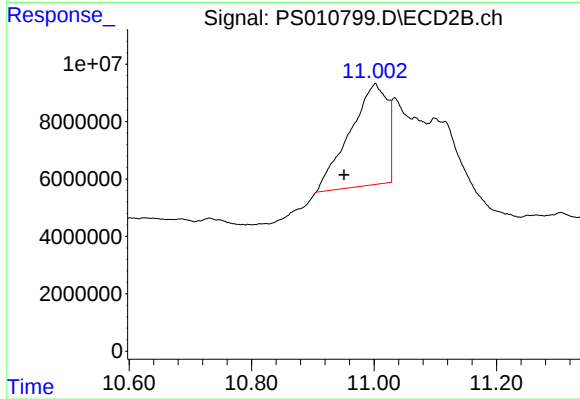

#16 DCPA

R.T.: 11.002 min
Delta R.T.: 0.051 min
Response: 150564684
Conc: 40.60 ng/ml