

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061321\
 Data File : PS015497.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2021 14:16
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 04:43:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	0.000	5192824	0	2.060	N.D. #
Target Compounds							
2) T	3,5-DICHL...	6.441	0.000	3230549	0	<MDL	N.D. #
3) T	4-Nitroph...	7.058	0.000	4106379	0	2.913	N.D. #
5) T	DICAMBA	7.421	6.945	12494770	3502740	1.311	1.583
7) T	MCPA	7.672f	0.000	24651680	0	2.456	N.D. #
8) T	DICHLORPROP	8.116	7.586	4168911	4973505	1.810	9.155 #
9) T	2,4-D	8.347	0.000	17796056	0	6.984	N.D. #
10) T	Pentachlo...	8.657	8.285	24542228	4716691	<MDL	<MDL #
11) T	2,4,5-TP ...	9.208	8.647	12072649	3238912	<MDL	1.116 #
12) T	2,4,5-T	9.490	9.026	35609586	6958604	2.965	2.404
13) T	2,4-DB	10.035	0.000	22513784	0	8.841	N.D. #
14) T	DINOSEB	11.202	0.000	12054269	0	1.509	N.D. #
15) T	Picloram	11.018	10.838	492.3E6	127.7E6	29.717	30.758
16) T	DCPA	11.470	10.792	27675119	6792389	1.641	1.576



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061321\
Data File : PS015497.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2021 14:16
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 04:43:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

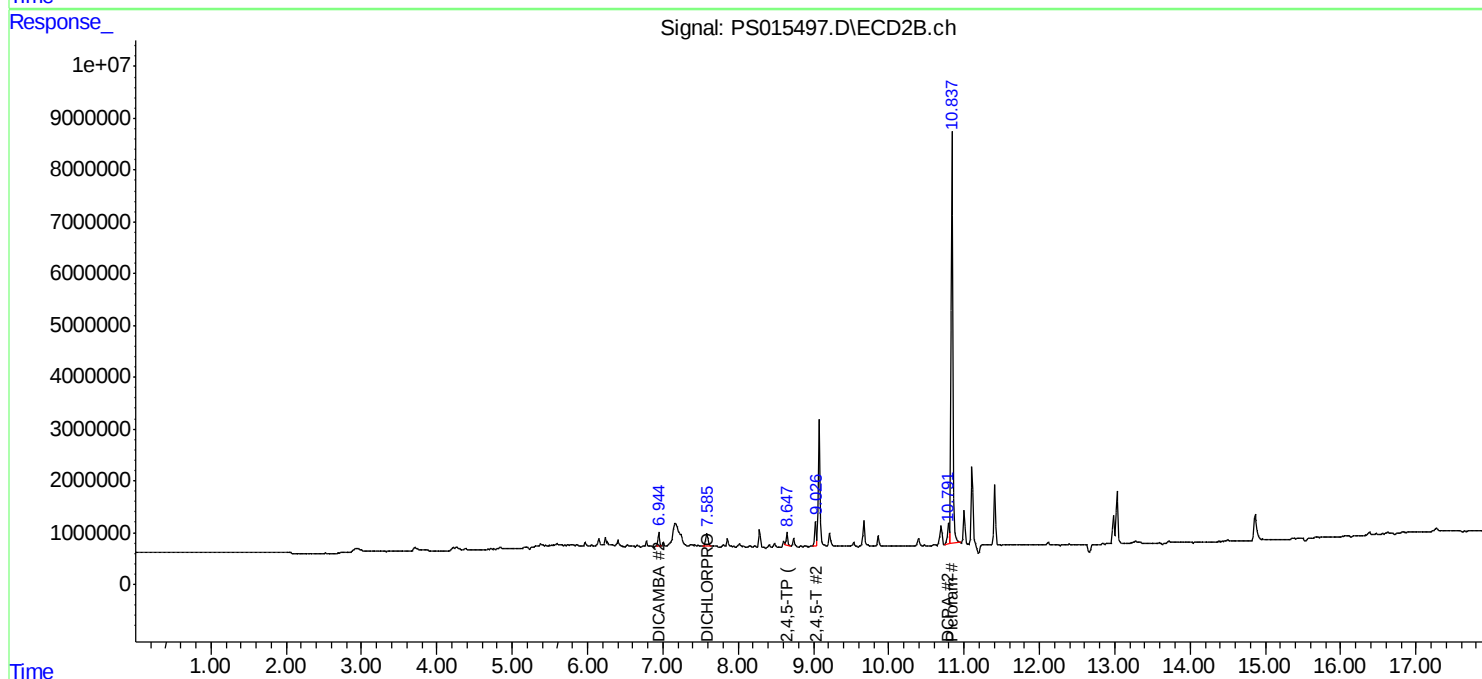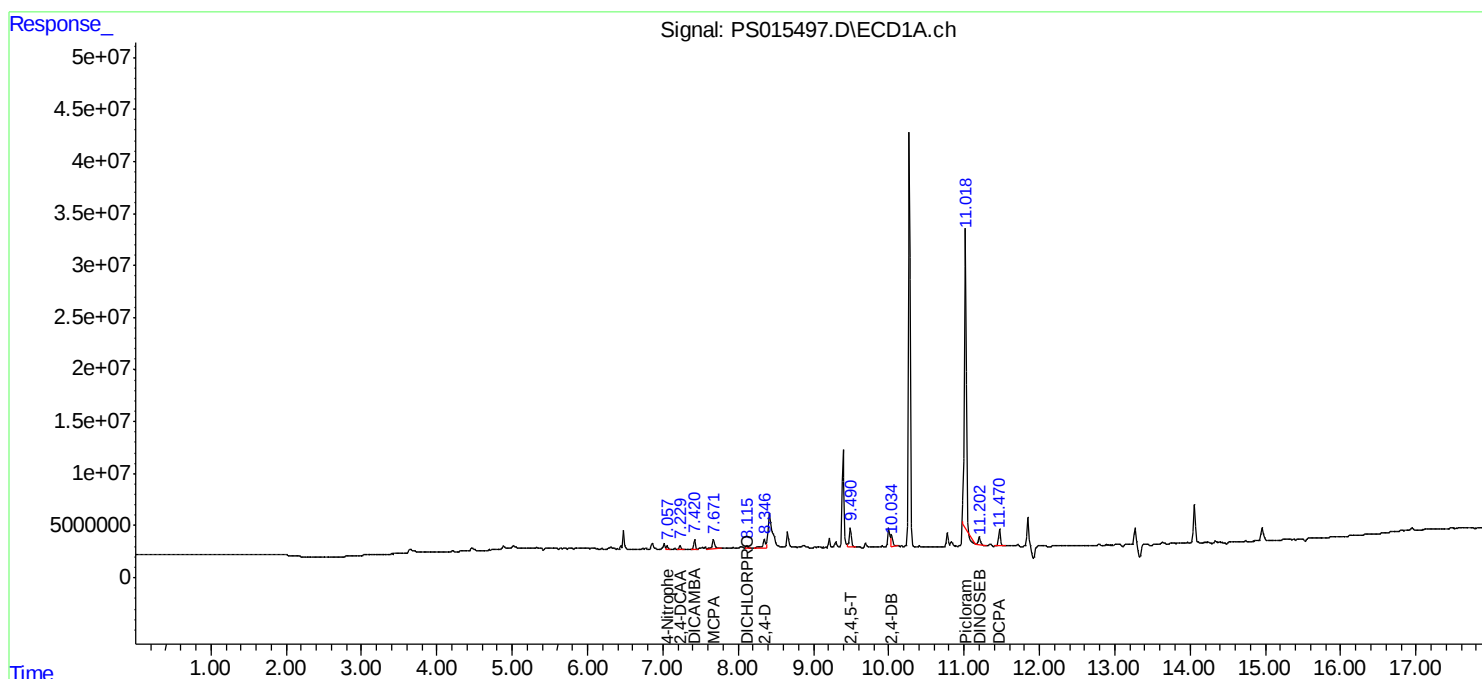


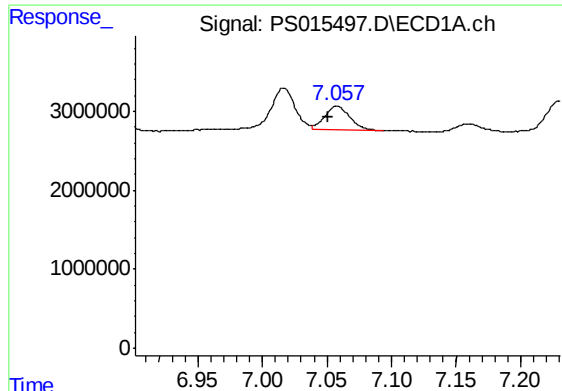

#3 4-Nitrophenol


R.T.: 7.058 min
Delta R.T.: 0.006 min
Response: 4106379
Conc: 2.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

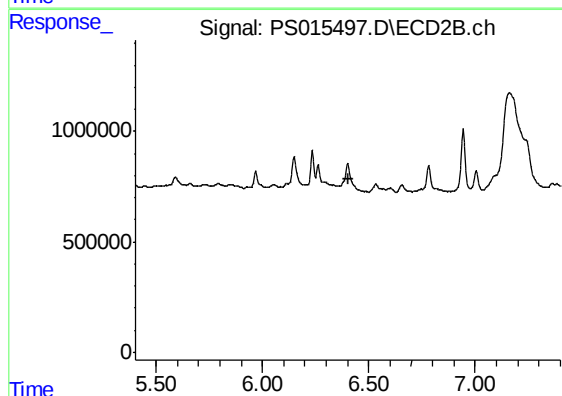


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

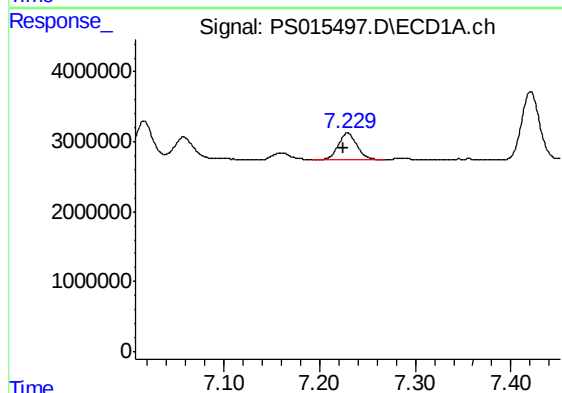


#4 2,4-DCAA

R.T.: 7.229 min
Delta R.T.: 0.004 min
Response: 5192824
Conc: 2.06 ng/ml

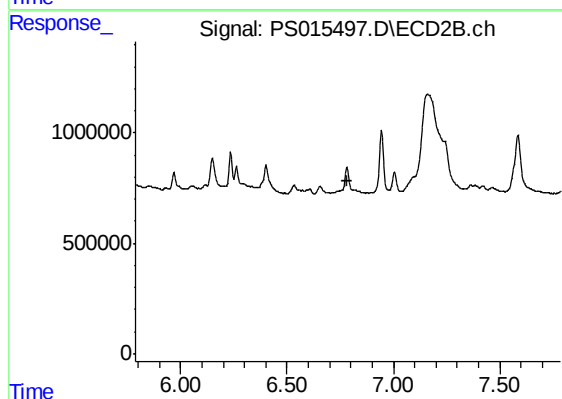

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.786 min
Response: 0
Conc: N.D.

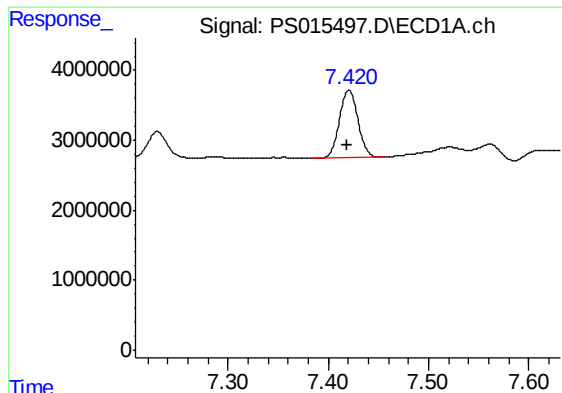

#5 DICAMBA


R.T.: 7.421 min
Delta R.T.: 0.001 min
Response: 12494770
Conc: 1.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

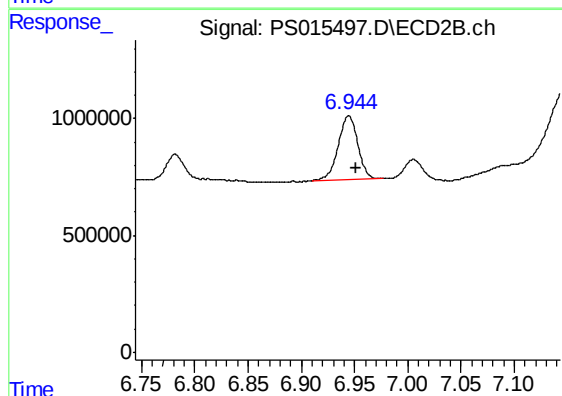


#5 DICAMBA

R.T.: 6.945 min
Delta R.T.: -0.007 min
Response: 3502740
Conc: 1.58 ng/ml

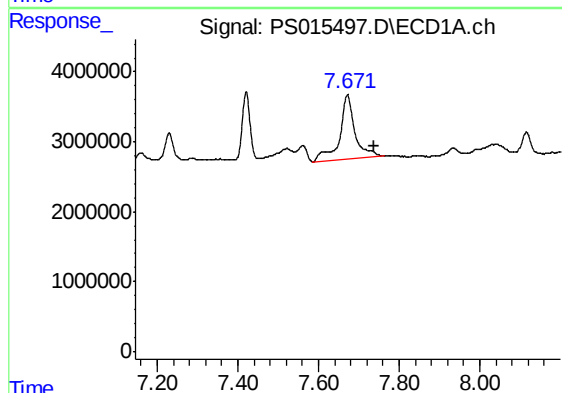


#7 MCPA

R.T.: 7.672 min
Delta R.T.: -0.067 min
Response: 24651680
Conc: 2.46 ug/ml

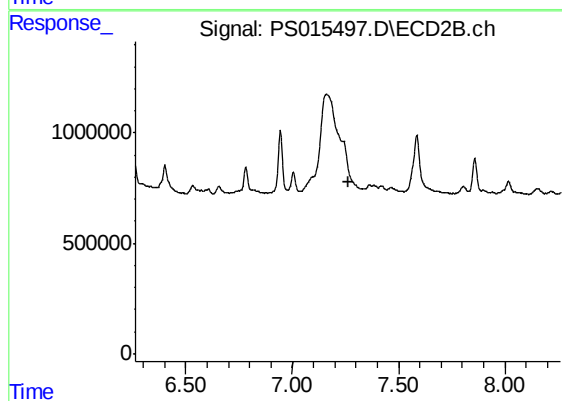

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.262 min
Response: 0
Conc: N.D.

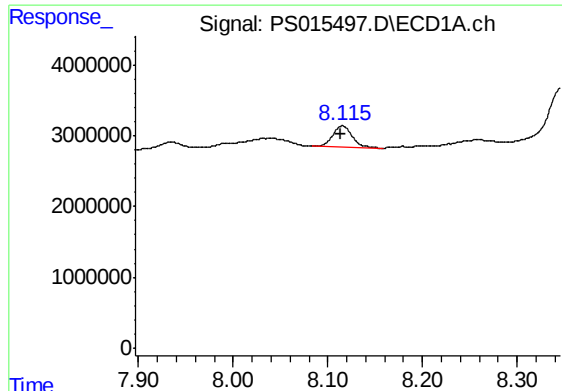

#8 DICHLORPROP


R.T.: 8.116 min
Delta R.T.: 0.002 min
Response: 4168911
Conc: 1.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

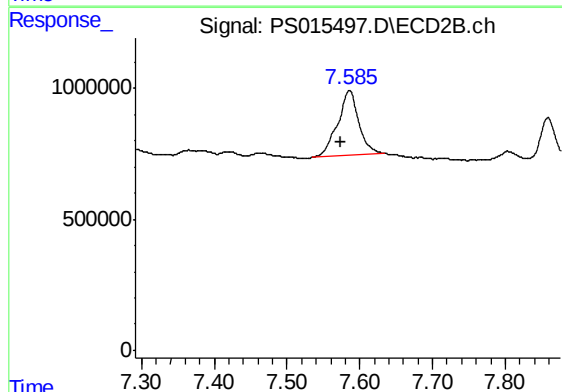


#8 DICHLORPROP

R.T.: 7.586 min
Delta R.T.: 0.012 min
Response: 4973505
Conc: 9.15 ng/ml

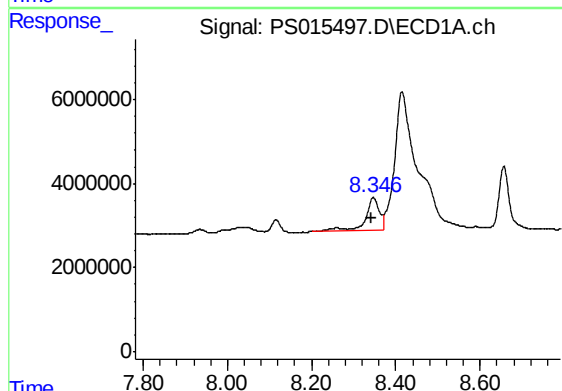


#9 2,4-D

R.T.: 8.347 min
Delta R.T.: 0.006 min
Response: 17796056
Conc: 6.98 ng/ml

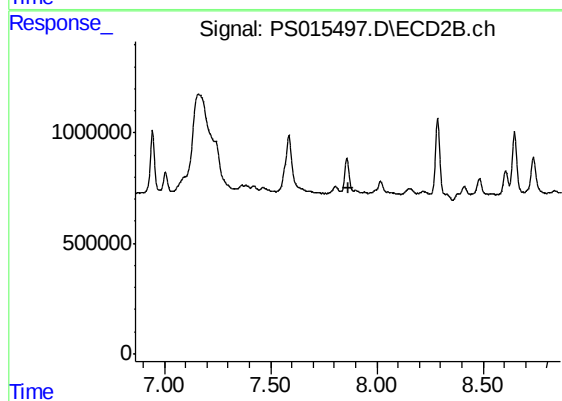

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.864 min
Response: 0
Conc: N.D.

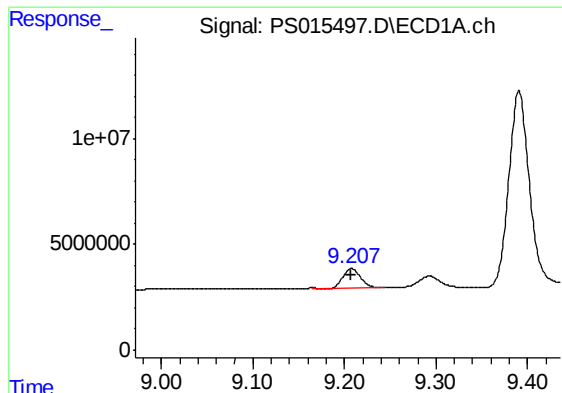

#11 2,4,5-TP (SILVEX)


R.T.: 9.208 min
Delta R.T.: 0.001 min
Response: 12072649
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

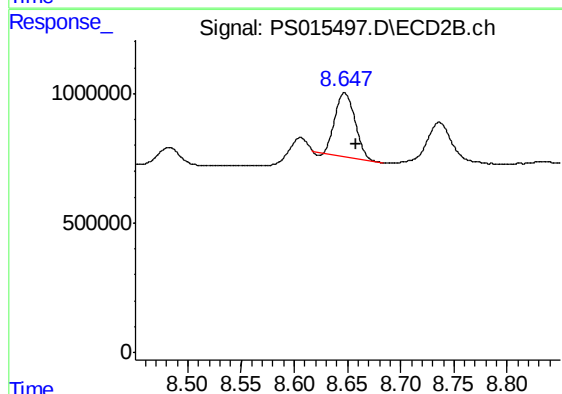


#11 2,4,5-TP (SILVEX)

R.T.: 8.647 min
Delta R.T.: -0.011 min
Response: 3238912
Conc: 1.12 ng/ml

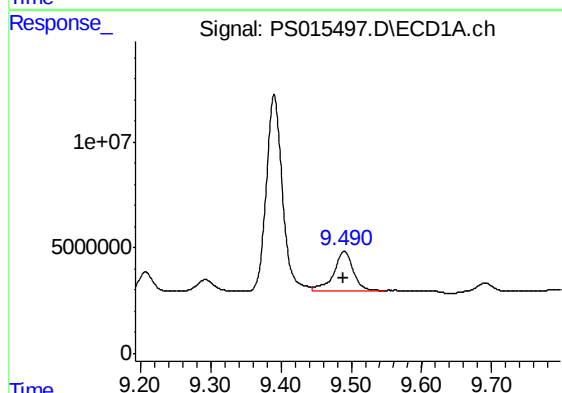


#12 2,4,5-T

R.T.: 9.490 min
Delta R.T.: 0.000 min
Response: 35609586
Conc: 2.96 ng/ml

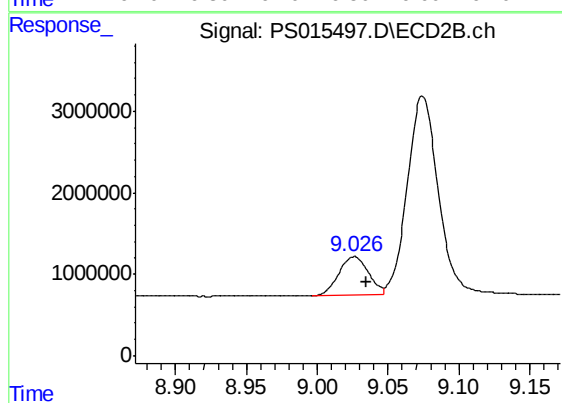

#12 2,4,5-T


R.T.: 9.026 min
Delta R.T.: -0.008 min
Response: 6958604
Conc: 2.40 ng/ml

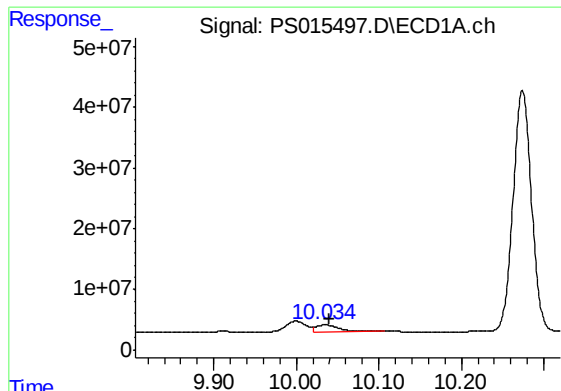

#13 2,4-DB


R.T.: 10.035 min
Delta R.T.: -0.005 min
Response: 22513784
Conc: 8.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

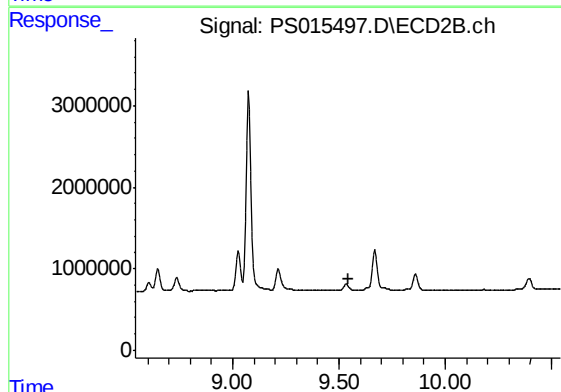


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.542 min
Response: 0
Conc: N.D.

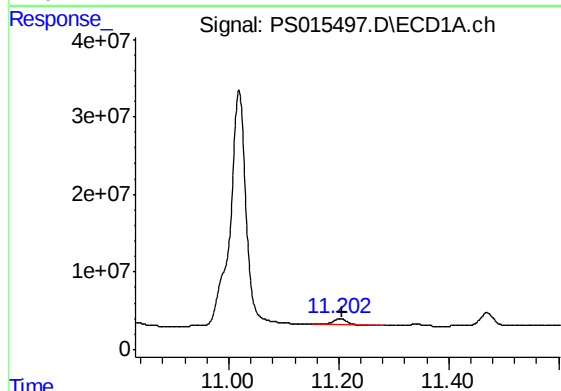


#14 DINOSEB

R.T.: 11.202 min
Delta R.T.: -0.004 min
Response: 12054269
Conc: 1.51 ng/ml

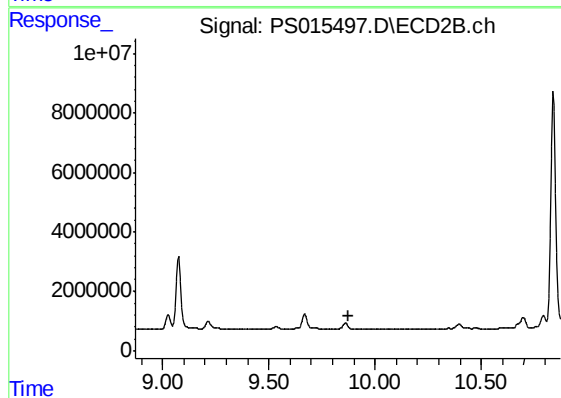

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.872 min
Response: 0
Conc: N.D.

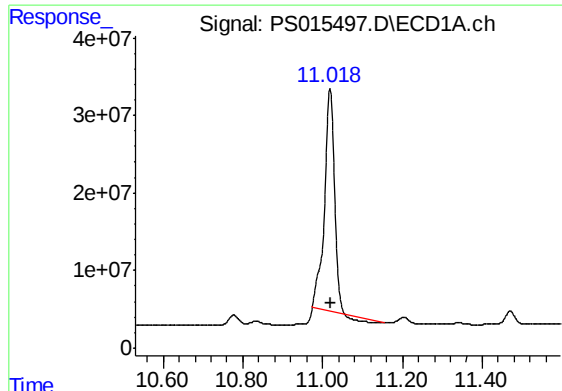

#15 Picloram


R.T.: 11.018 min
Delta R.T.: 0.000 min
Response: 492317994
Conc: 29.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

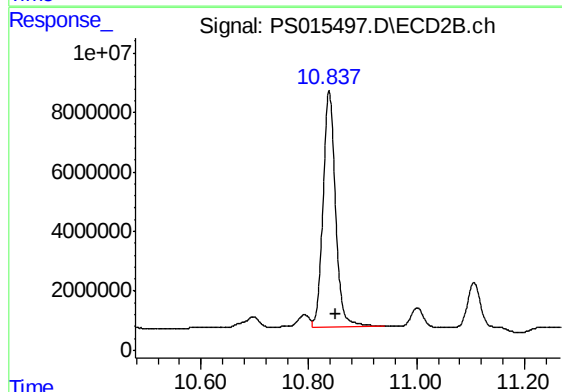


#15 Picloram

R.T.: 10.838 min
Delta R.T.: -0.012 min
Response: 127734492
Conc: 30.76 ng/ml

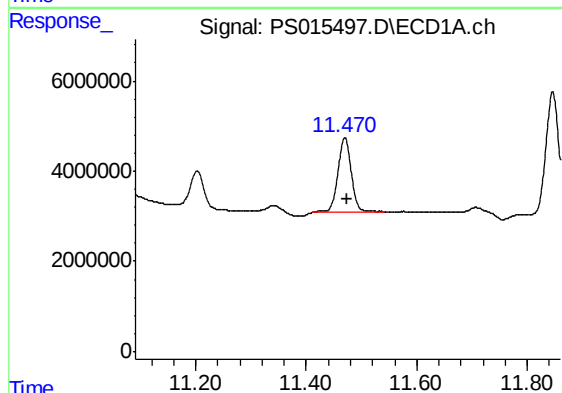

#16 DCPA

R.T.: 11.470 min
Delta R.T.: -0.005 min
Response: 27675119
Conc: 1.64 ng/ml

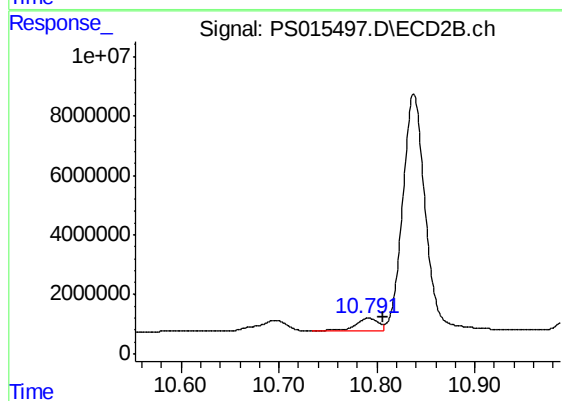

#16 DCPA

R.T.: 10.792 min
Delta R.T.: -0.015 min
Response: 6792389
Conc: 1.58 ng/ml