

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061321\
 Data File : PS015546.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2021 11:11
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 12:04:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.227	6.779	1320.8E6	293.9E6	524.063	548.479
Target Compounds							
3) T	4-Nitroph...	7.020	0.000	8827269	0	6.262	N.D. #
7) T	MCPA	7.673f	0.000	26701831	0	2.660	N.D. #
10) T	Pentachlo...	8.688	0.000	3602327	0	<MDL	N.D. #
12) T	2,4,5-T	9.461	0.000	9174965	0	<MDL	N.D. #
15) T	Picloram	11.020	10.838	18845217	4286145	1.138	1.032
16) T	DCPA	0.000	10.838	0	4286145	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061321\
Data File : PS015546.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2021 11:11
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 12:04:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

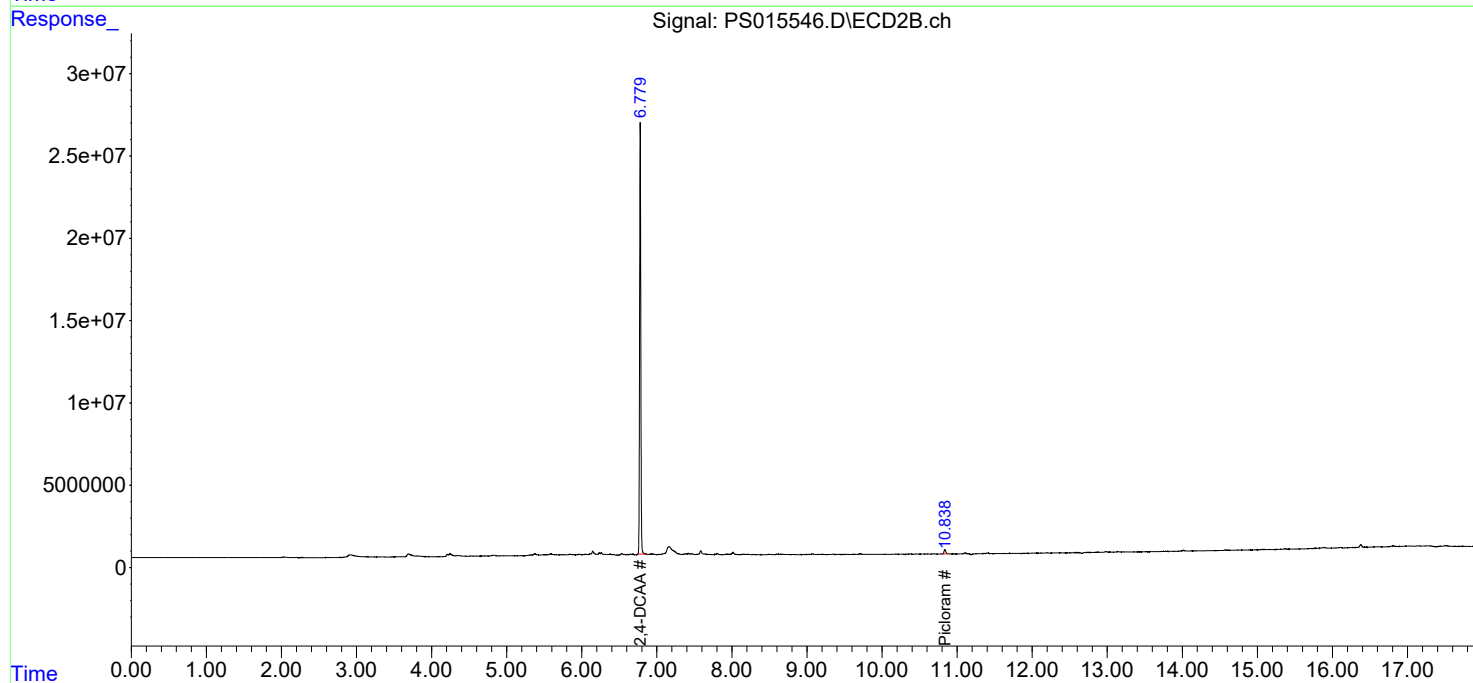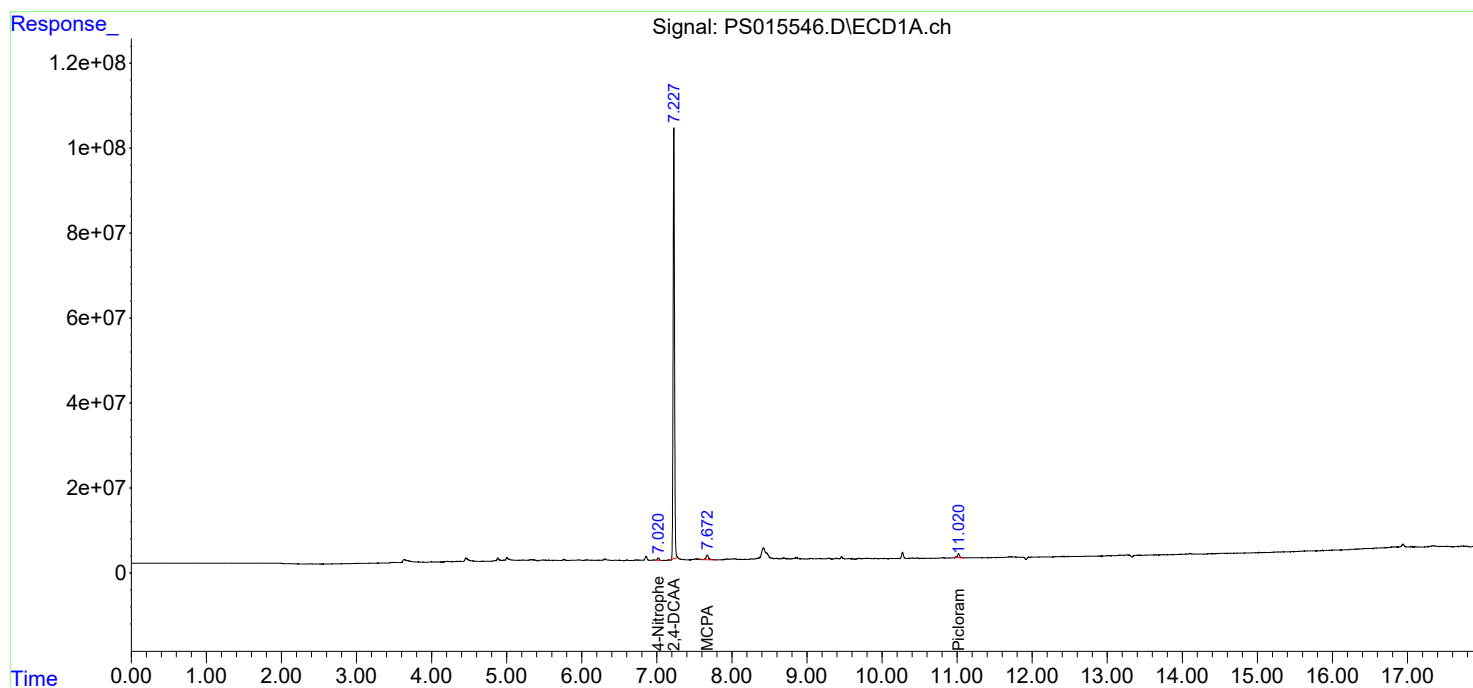


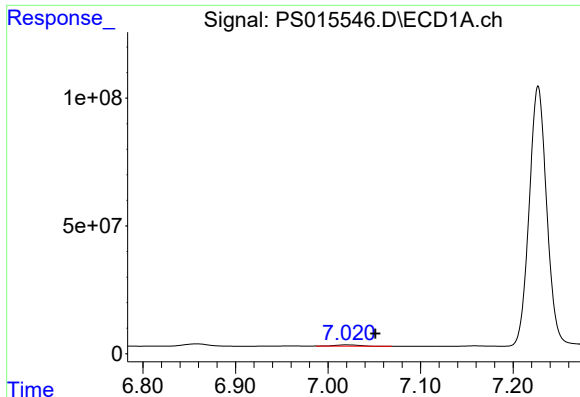

#3 4-Nitrophenol


R.T.: 7.020 min
Delta R.T.: -0.031 min
Response: 8827269
Conc: 6.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

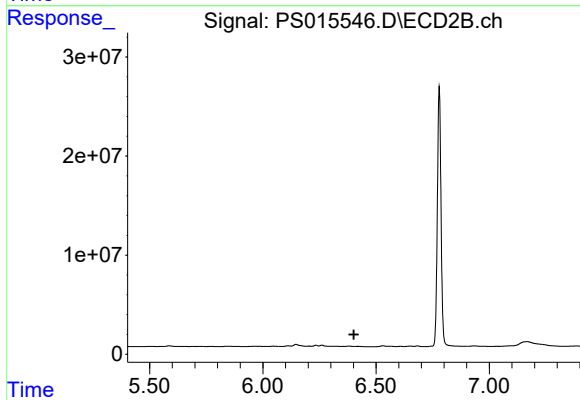


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

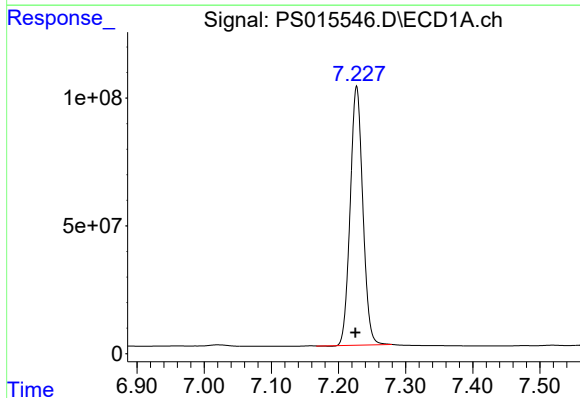


#4 2,4-DCAA

R.T.: 7.227 min
Delta R.T.: 0.002 min
Response: 1320835208
Conc: 524.06 ng/ml

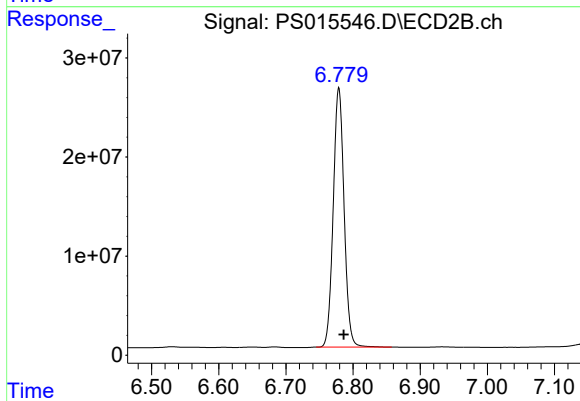

#4 2,4-DCAA


R.T.: 6.779 min
Delta R.T.: -0.007 min
Response: 293859173
Conc: 548.48 ng/ml

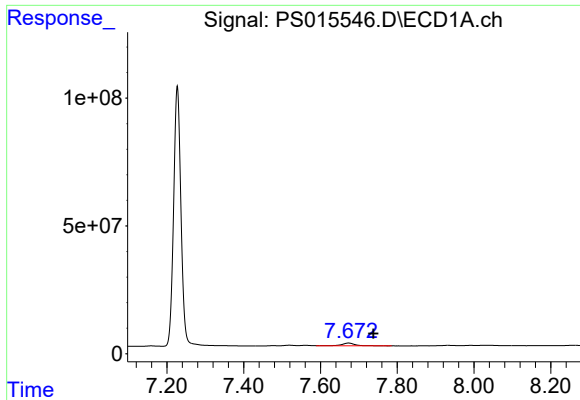

#7 MCPA


R.T.: 7.673 min
Delta R.T.: -0.065 min
Response: 26701831
Conc: 2.66 ug/ml

Instrument :
ECD_S
ClientSampleId :

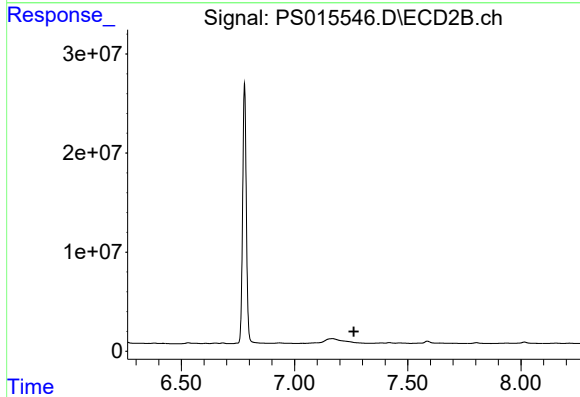


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.262 min
Response: 0
Conc: N.D.

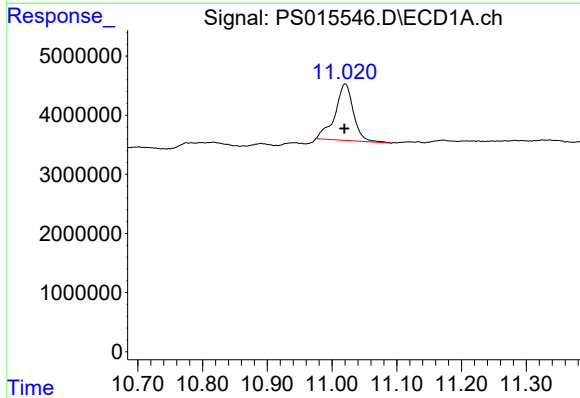

#15 Picloram

R.T.: 11.020 min
Delta R.T.: 0.001 min
Response: 18845217
Conc: 1.14 ng/ml

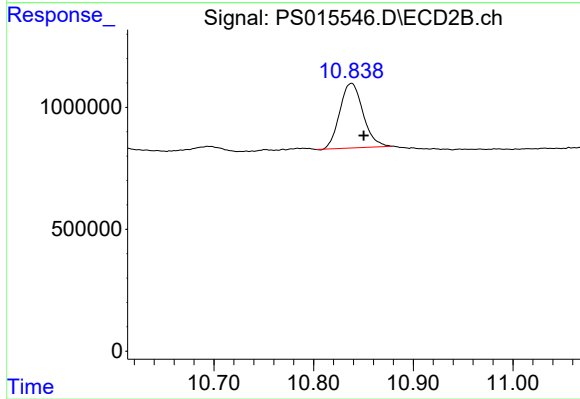

#15 Picloram

R.T.: 10.838 min
Delta R.T.: -0.012 min
Response: 4286145
Conc: 1.03 ng/ml