

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061323\
 Data File : PS023273.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2023 13:58
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 01:59:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.484	6.855	929.6E6	290.7E6	525.439	512.107
Target Compounds							
2) T	3,5-DICHL...	5.801	0.000	344660	0	<MDL	N.D. #
3) T	4-Nitroph...	6.319	0.000	6038102	0	4.685	N.D. #
5) T	DICAMBA	6.691f	7.019	92149	640742	<MDL	<MDL #
6) T	MCP	6.823	0.000	17299	0	<MDL	N.D. #
7) T	MCPA	6.859f	7.302	-1522318	12024194	N.D.	4.474
8) T	DICHLORPROP	7.191f	0.000	6506471	0	3.153	N.D. #
9) T	2,4-D	7.410	0.000	915481	0	<MDL	N.D. #
10) T	Pentachlo...	7.676	0.000	932344	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.215	0.000	5204294	0	<MDL	N.D. #
12) T	2,4,5-T	8.481	9.140f	2189948	892252	<MDL	<MDL #
13) T	2,4-DB	8.991	0.000	2443831	0	1.038	N.D. #
14) T	DINOSEB	10.064	0.000	738505	0	<MDL	N.D. #
15) T	Picloram	9.900	10.897	30862415	5321765	1.778	1.166 #
16) T	DCPA	10.342	10.897	2123586	5321765	<MDL	1.327 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061323\
Data File : PS023273.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2023 13:58
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 01:59:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

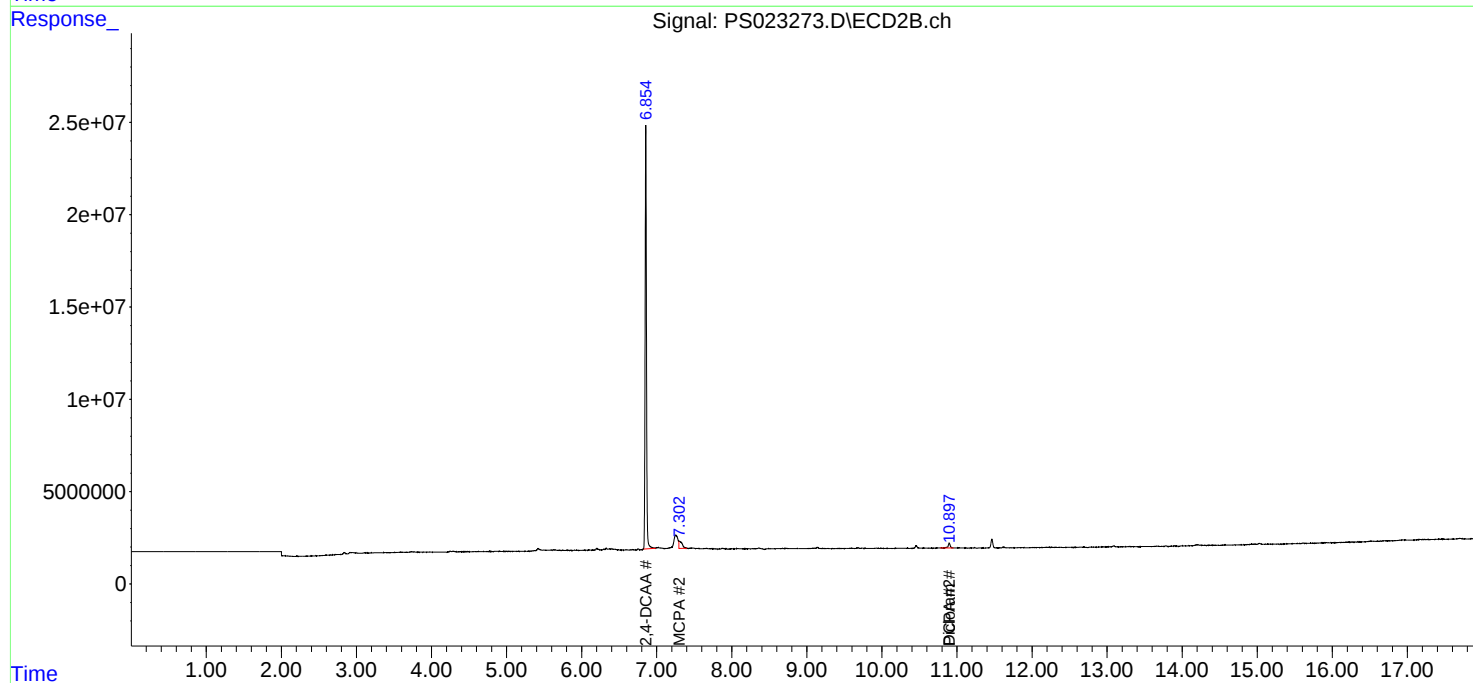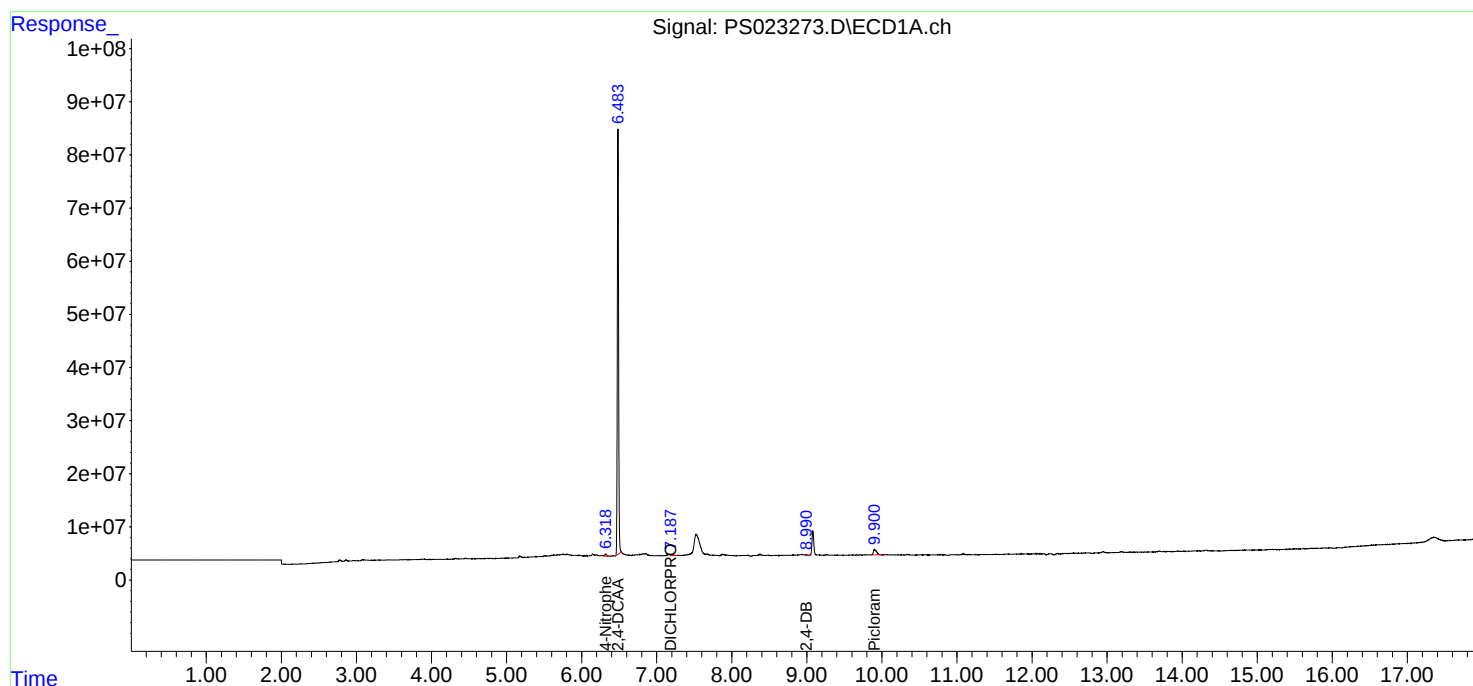


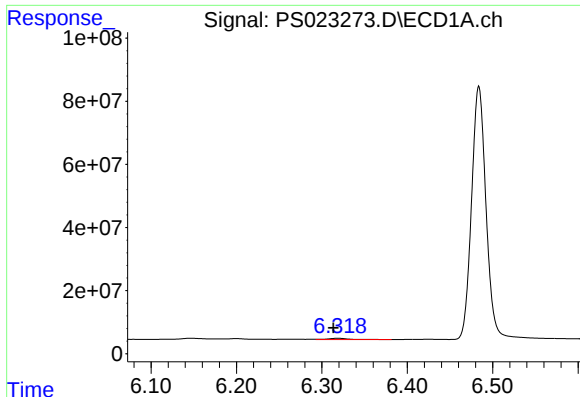

#3 4-Nitrophenol


R.T.: 6.319 min
Delta R.T.: 0.005 min
Response: 6038102
Conc: 4.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

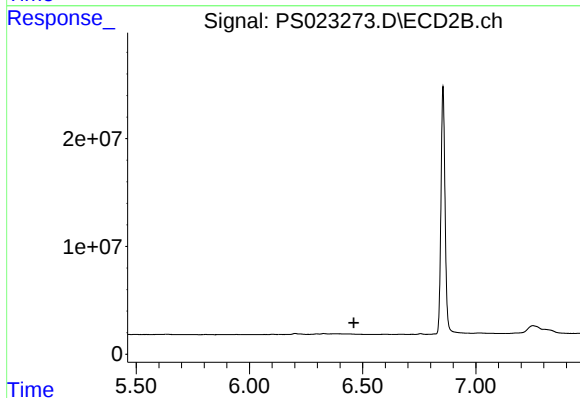


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

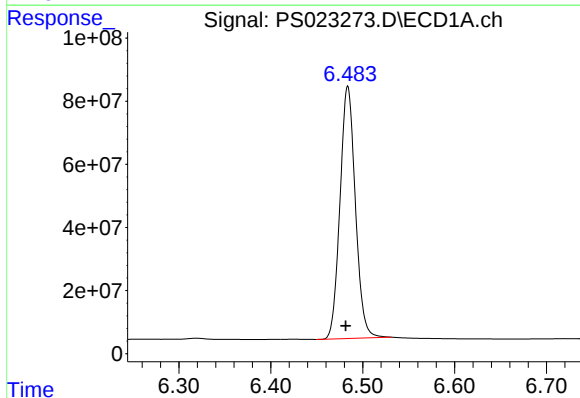


#4 2,4-DCAA

R.T.: 6.484 min
Delta R.T.: 0.002 min
Response: 929636978
Conc: 525.44 ng/ml

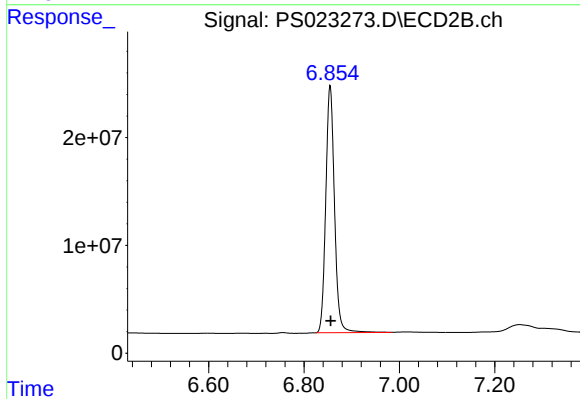

#4 2,4-DCAA


R.T.: 6.855 min
Delta R.T.: -0.001 min
Response: 290720698
Conc: 512.11 ng/ml

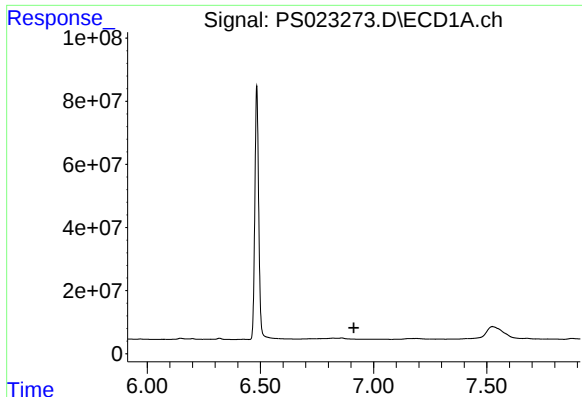

#7 MCPA


R.T.: 6.859 min
Delta R.T.: -0.054 min
Response: -1522318
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

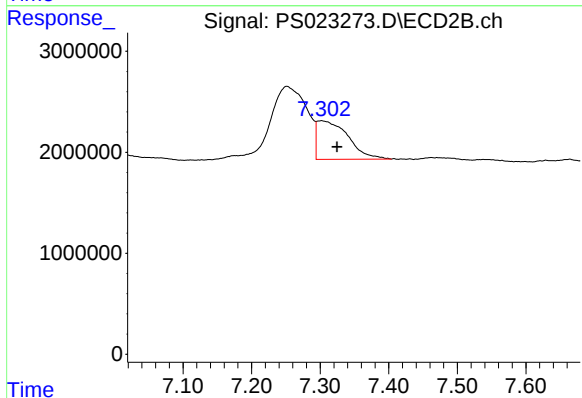


#7 MCPA

R.T.: 7.302 min
Delta R.T.: -0.023 min
Response: 12024194
Conc: 4.47 ug/ml

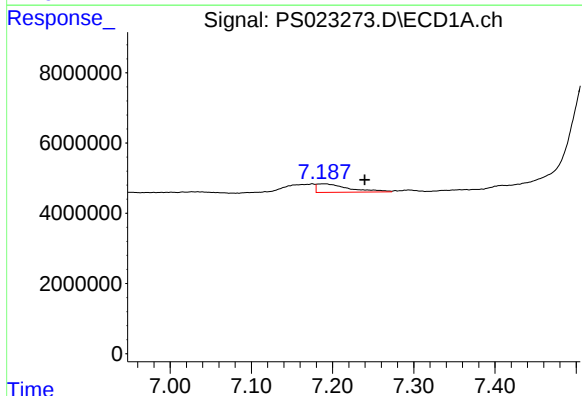


#8 DICHLORPROP

R.T.: 7.191 min
Delta R.T.: -0.049 min
Response: 6506471
Conc: 3.15 ng/ml

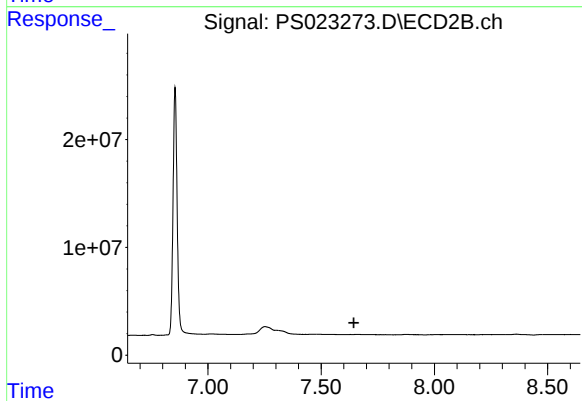

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.645 min
Response: 0
Conc: N.D.

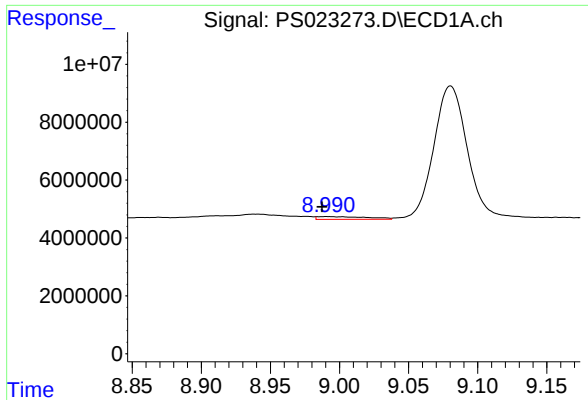

#13 2,4-DB


R.T.: 8.991 min
Delta R.T.: 0.003 min
Response: 2443831
Conc: 1.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

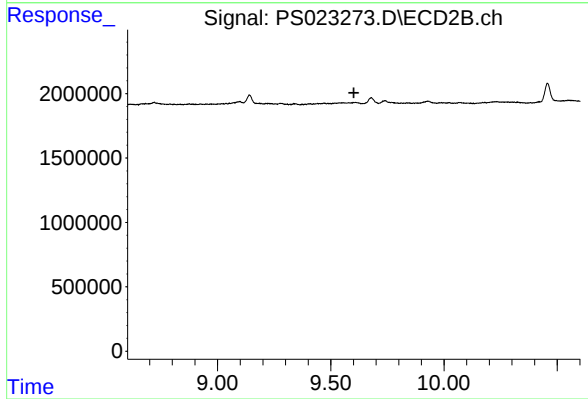


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.602 min
Response: 0
Conc: N.D.

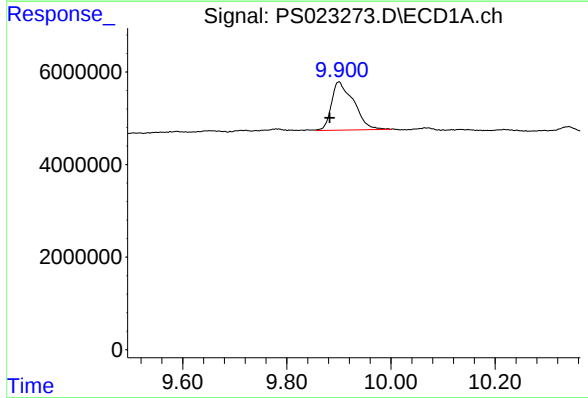


#15 Picloram

R.T.: 9.900 min
Delta R.T.: 0.018 min
Response: 30862415
Conc: 1.78 ng/ml

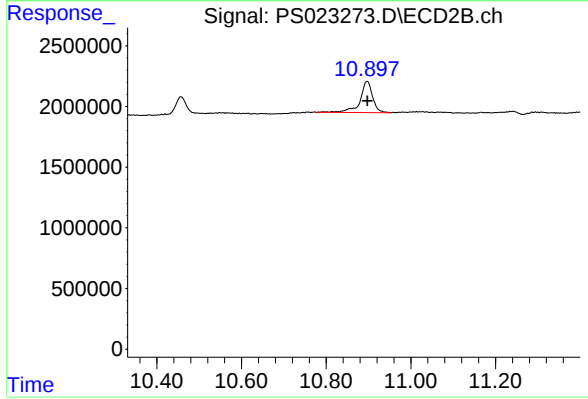

#15 Picloram


R.T.: 10.897 min
Delta R.T.: 0.000 min
Response: 5321765
Conc: 1.17 ng/ml

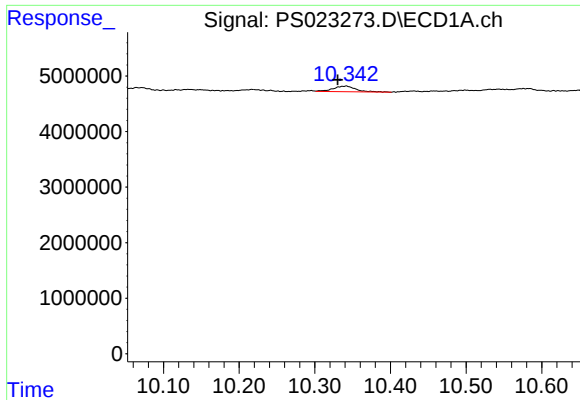

#16 DCPA

R.T.: 10.342 min
Delta R.T.: 0.011 min
Response: 2123586
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

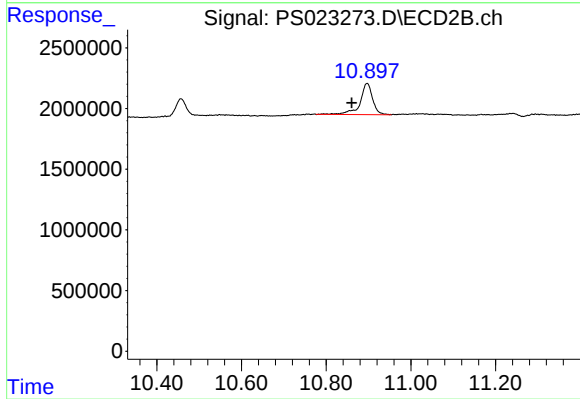

#16 DCPA

R.T.: 10.897 min
Delta R.T.: 0.036 min
Response: 5321765
Conc: 1.33 ng/ml