

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061421\
 Data File : PS015549.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2021 12:33
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 08:50:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061421.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 08:41:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.780	1368.3E6	298.6E6	492.010	554.504
Target Compounds							
3) T	4-Nitroph...	7.022	0.000	7830725	0	5.178	N.D. #
8) T	DICHLORPROP	8.165f	0.000	3246024	0	1.245	N.D. #
9) T	2,4-D	8.347	0.000	7981847	0	2.753	N.D. #
10) T	Pentachlo...	8.688	0.000	3342098	0	<MDL	N.D. #
12) T	2,4,5-T	9.489	9.074f	7887776	11372771	<MDL	3.861 #
13) T	2,4-DB	10.025	0.000	28511353	0	9.025	N.D. #
15) T	Picloram	11.019	10.838	244.8E6	52341909	12.742	12.629
16) T	DCPA	11.476	10.838f	-1220867	52341909	N.D.	11.619



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061421\
Data File : PS015549.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2021 12:33
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 08:50:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061421.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 08:41:47 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

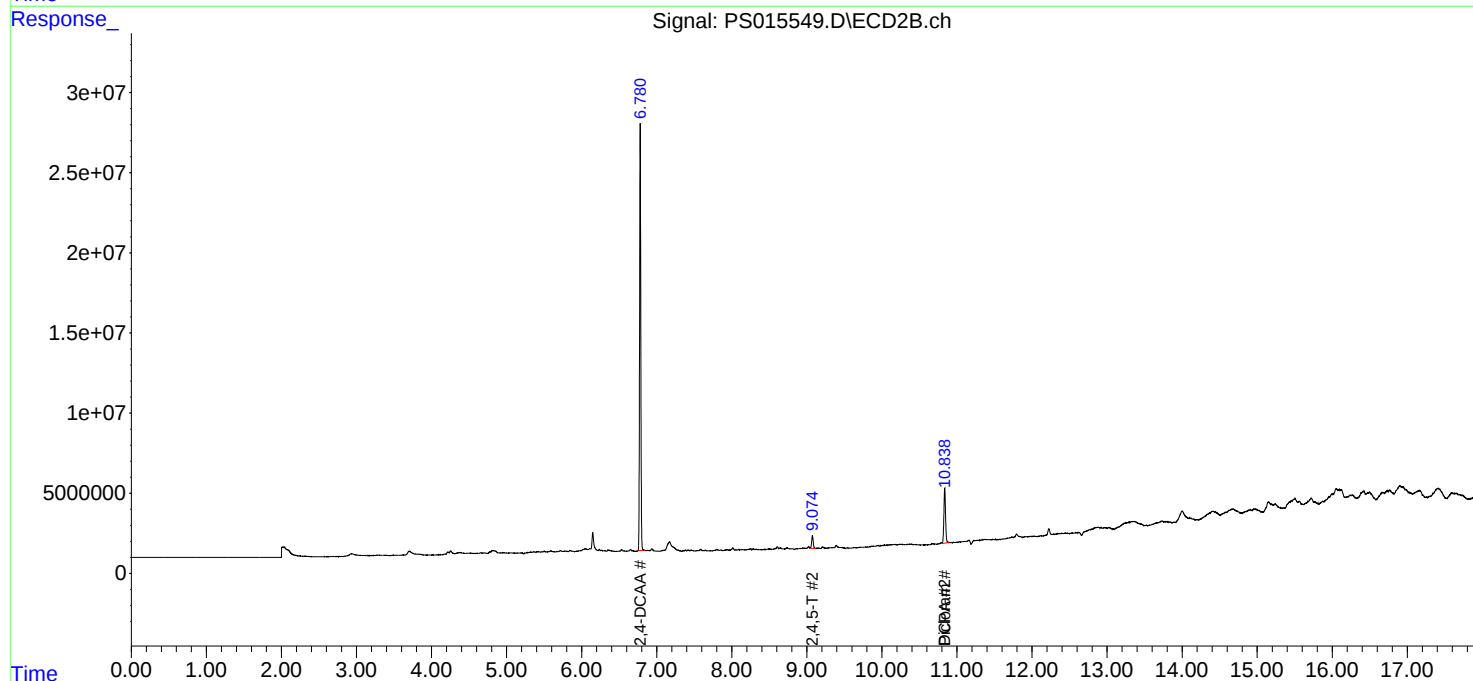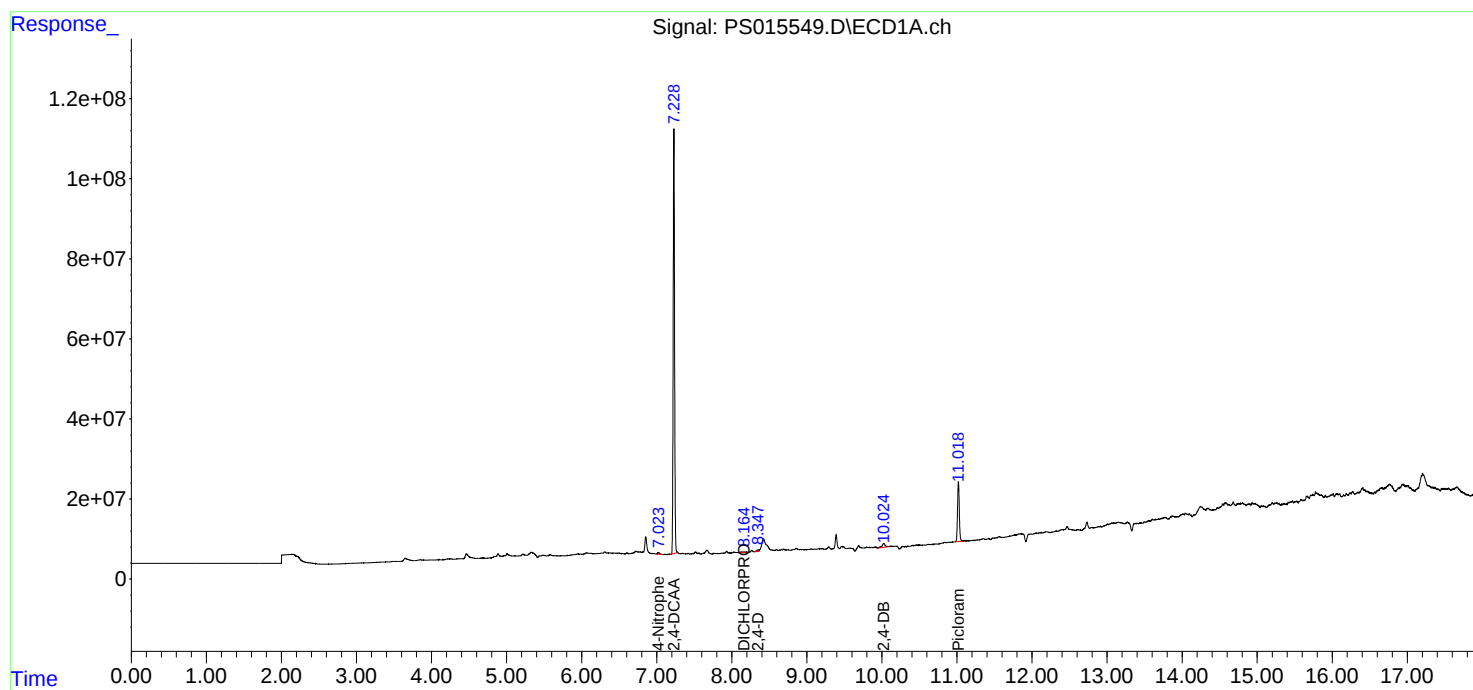


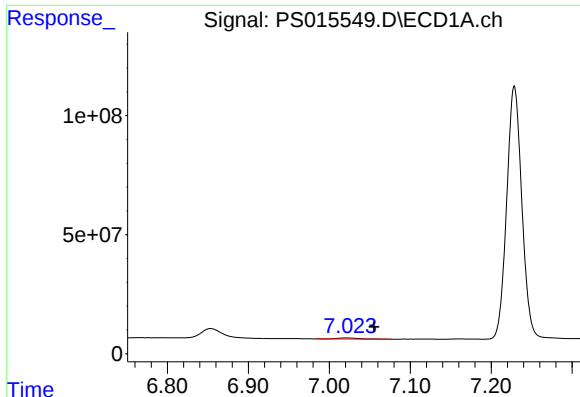

#3 4-Nitrophenol


R.T.: 7.022 min
Delta R.T.: -0.034 min
Response: 7830725
Conc: 5.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

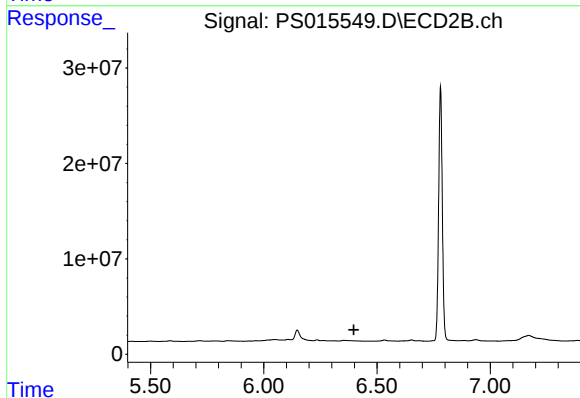


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.398 min
Response: 0
Conc: N.D.

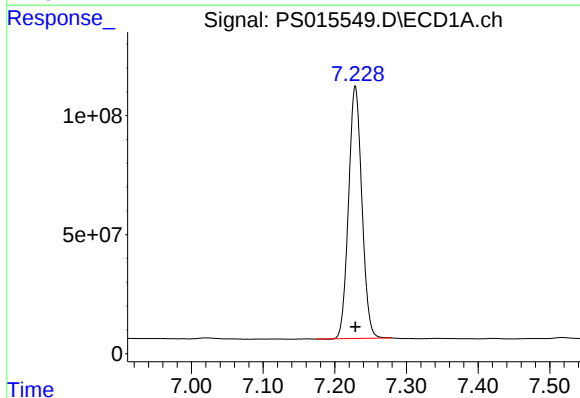


#4 2,4-DCAA

R.T.: 7.229 min
Delta R.T.: 0.000 min
Response: 1368341055
Conc: 492.01 ng/ml

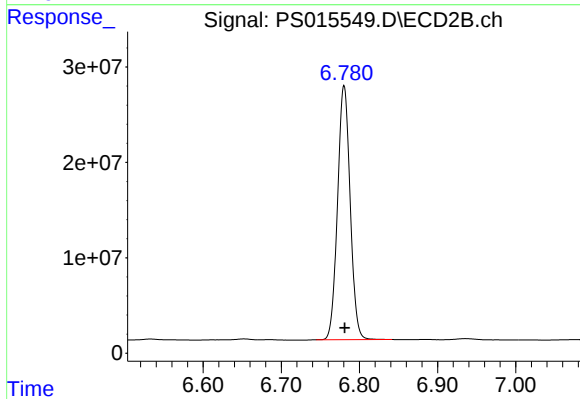

#4 2,4-DCAA


R.T.: 6.780 min
Delta R.T.: 0.000 min
Response: 298620047
Conc: 554.50 ng/ml

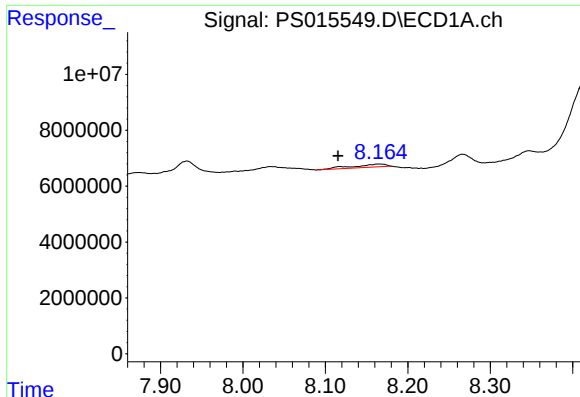

#8 DICHLORPROP


R.T.: 8.165 min
Delta R.T.: 0.049 min
Response: 3246024
Conc: 1.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

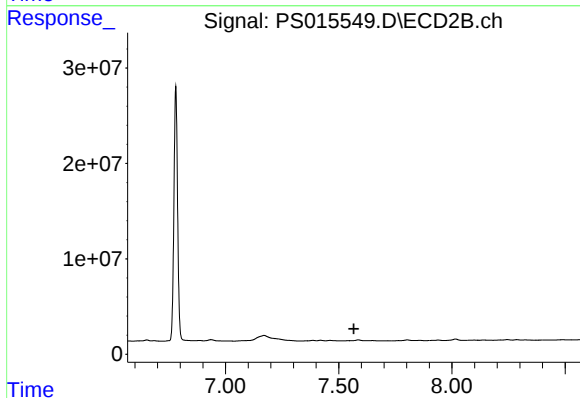


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.567 min
Response: 0
Conc: N.D.

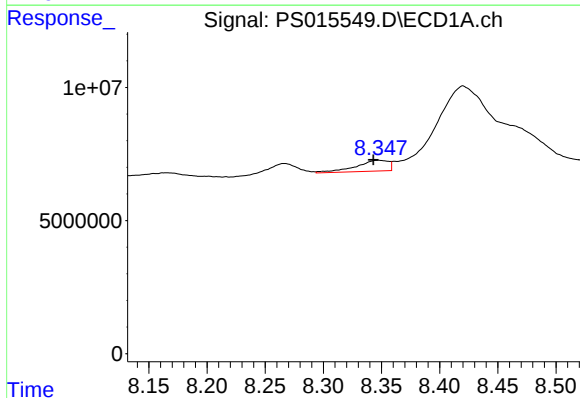


#9 2,4-D

R.T.: 8.347 min
Delta R.T.: 0.004 min
Response: 7981847
Conc: 2.75 ng/ml

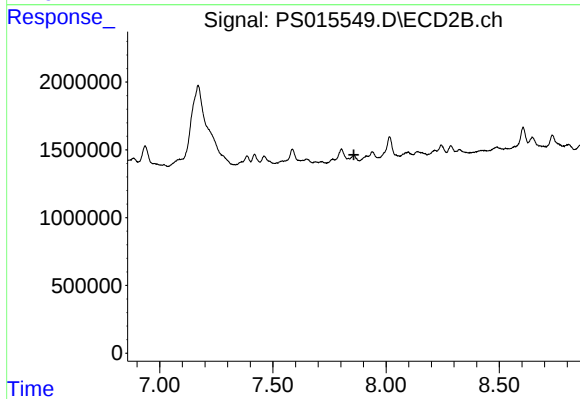

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.858 min
Response: 0
Conc: N.D.

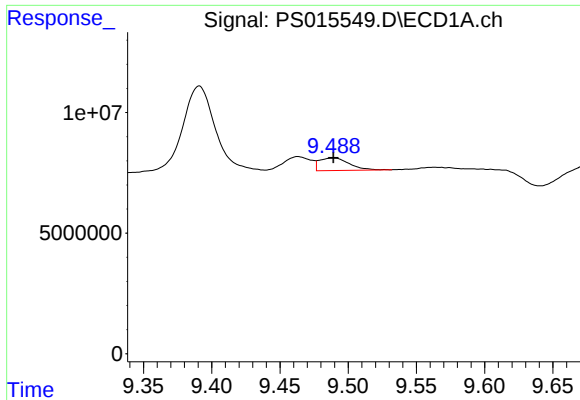

#12 2,4,5-T


R.T.: 9.489 min
Delta R.T.: 0.000 min
Response: 7887776
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

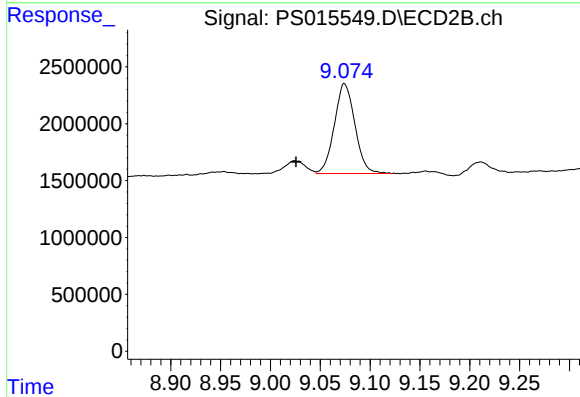


#12 2,4,5-T

R.T.: 9.074 min
Delta R.T.: 0.049 min
Response: 11372771
Conc: 3.86 ng/ml

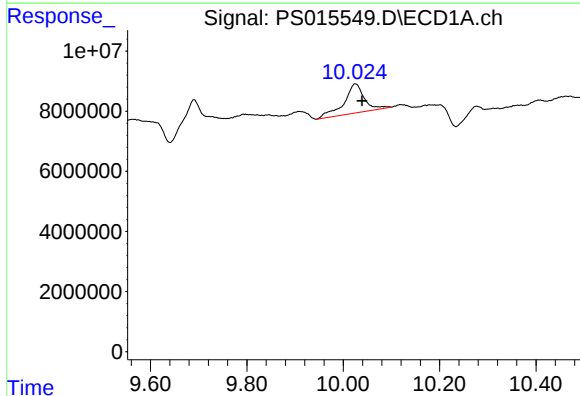


#13 2,4-DB

R.T.: 10.025 min
Delta R.T.: -0.014 min
Response: 28511353
Conc: 9.03 ng/ml

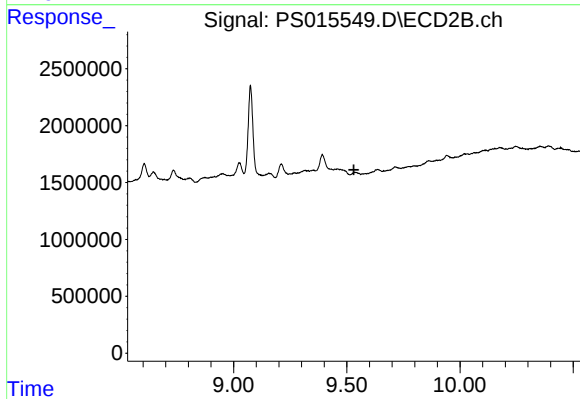

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.531 min
Response: 0
Conc: N.D.

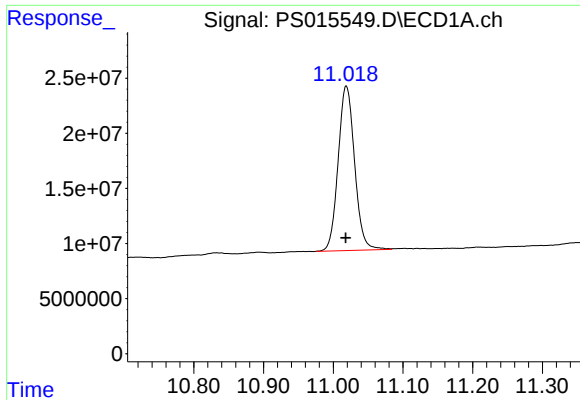

#15 Picloram


R.T.: 11.019 min
Delta R.T.: 0.000 min
Response: 244768676
Conc: 12.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

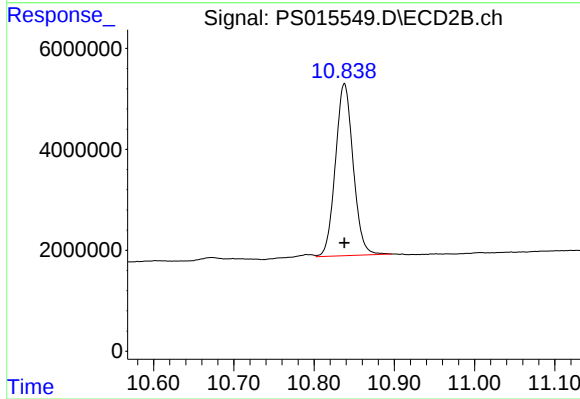


#15 Picloram

R.T.: 10.838 min
Delta R.T.: 0.000 min
Response: 52341909
Conc: 12.63 ng/ml

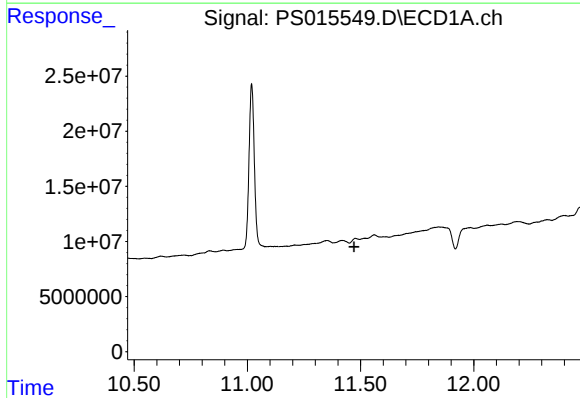

#16 DCPA

R.T.: 11.476 min
Delta R.T.: 0.005 min
Response: -1220867
Conc: N.D.

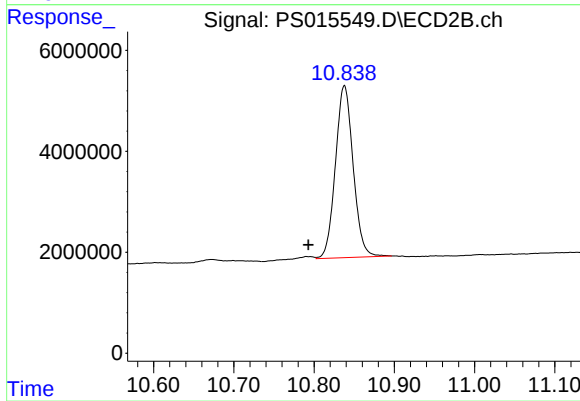

#16 DCPA

R.T.: 10.838 min
Delta R.T.: 0.045 min
Response: 52341909
Conc: 11.62 ng/ml