

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061421\
 Data File : PS015567.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2021 20:12
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 09:06:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061421.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 08:41:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.230	6.780	1626.2E6	303.4E6	584.740	563.375
Target Compounds							
3) T	4-Nitroph...	7.022	0.000	11944996	0	7.898	N.D. #
9) T	2,4-D	8.356	0.000	13677031	0	4.717	N.D. #
10) T	Pentachlo...	8.658	0.000	3700411	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.209	0.000	4726938	0	<MDL	N.D. #
12) T	2,4,5-T	9.495	9.077f	13649146	6421829	<MDL	2.180 #
13) T	2,4-DB	10.042	0.000	14529817	0	4.599	N.D. #
15) T	Picloram	11.026	10.841	157.7E6	27248339	8.208	6.575
16) T	DCPA	11.471	10.841f	6860094	27248339	<MDL	6.049 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061421\
Data File : PS015567.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2021 20:12
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 09:06:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061421.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 08:41:47 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

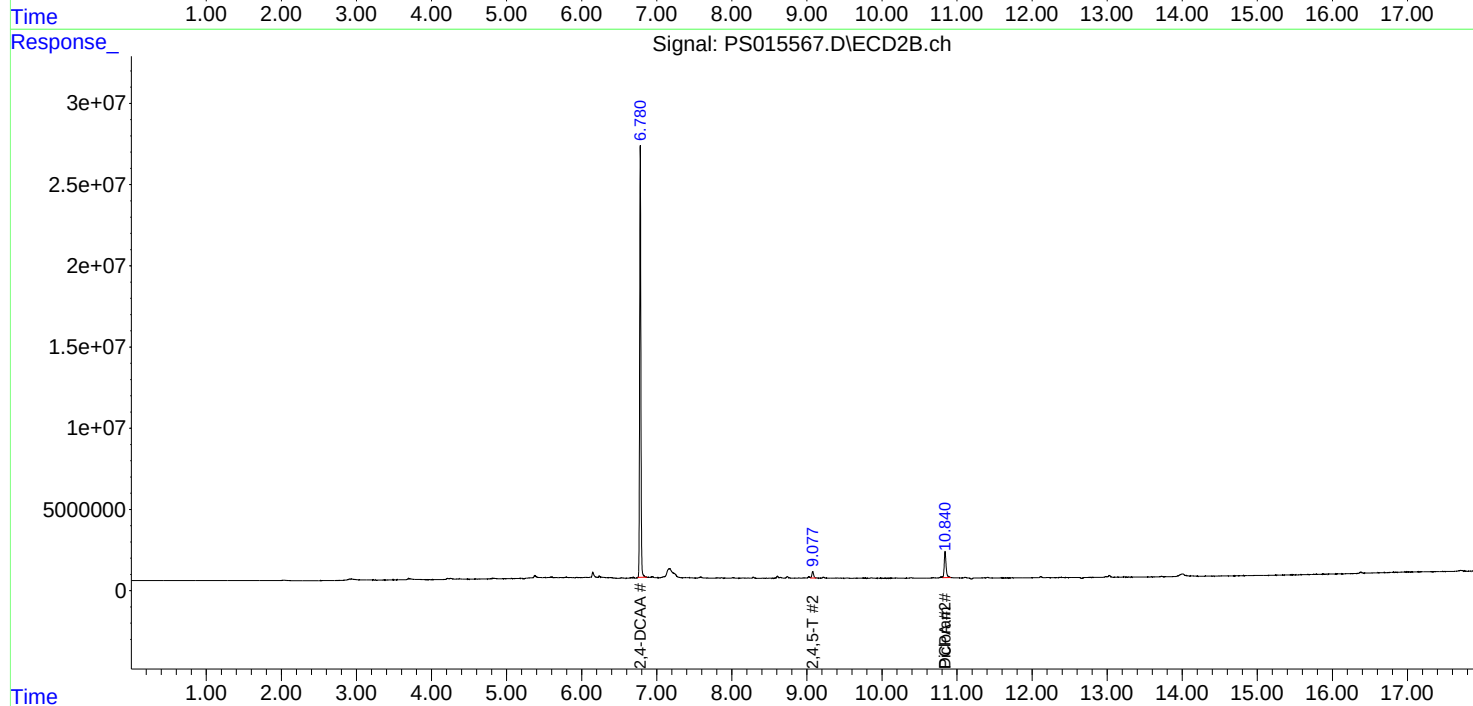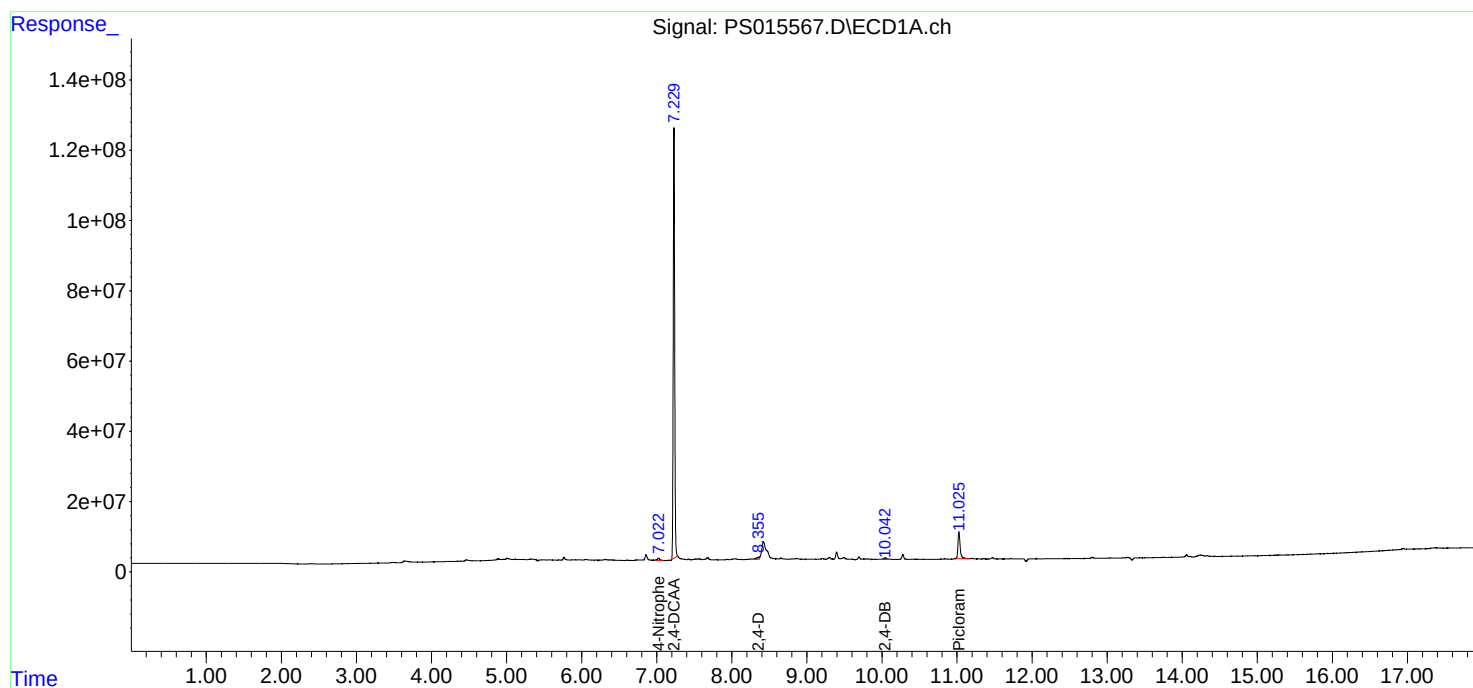


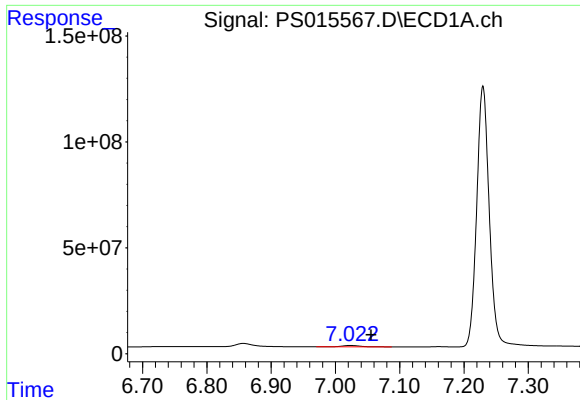

#3 4-Nitrophenol


R.T.: 7.022 min
Delta R.T.: -0.033 min
Response: 11944996
Conc: 7.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

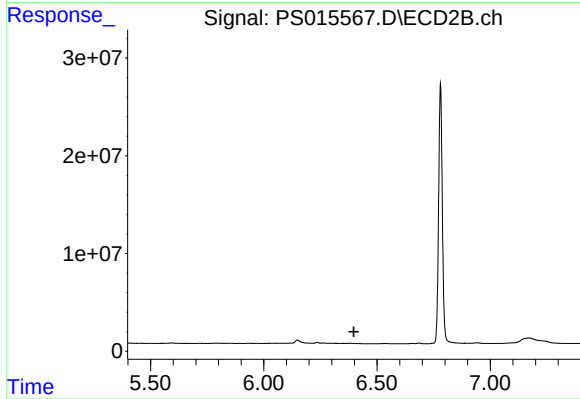


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.398 min
Response: 0
Conc: N.D.

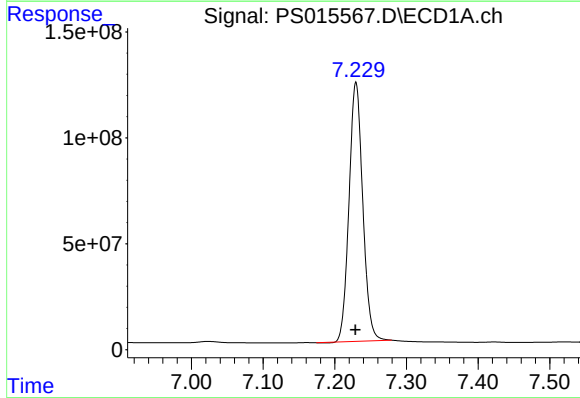


#4 2,4-DCAA

R.T.: 7.230 min
Delta R.T.: 0.000 min
Response: 1626235340
Conc: 584.74 ng/ml

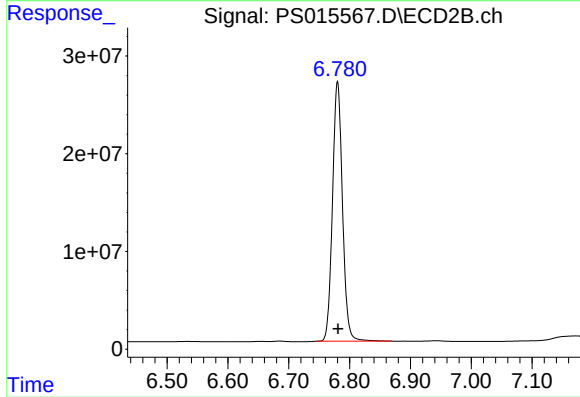

#4 2,4-DCAA


R.T.: 6.780 min
Delta R.T.: 0.000 min
Response: 303397227
Conc: 563.37 ng/ml

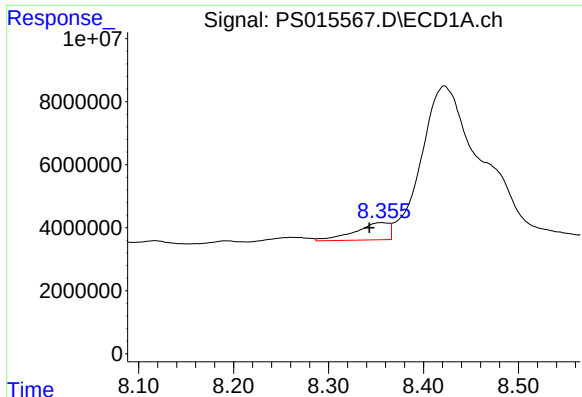

#9 2,4-D


R.T.: 8.356 min
Delta R.T.: 0.013 min
Response: 13677031
Conc: 4.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

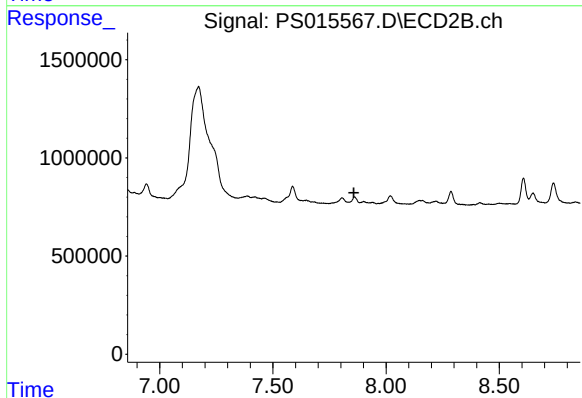


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.858 min
Response: 0
Conc: N.D.

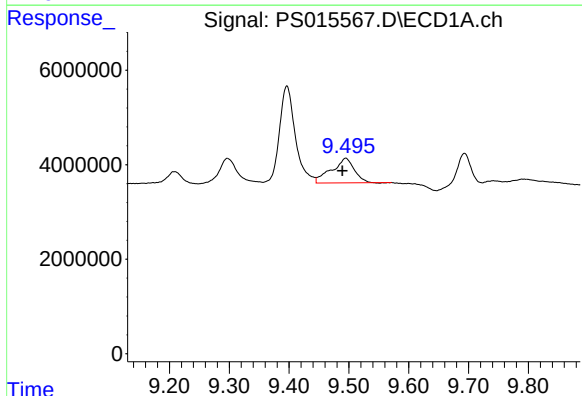


#12 2,4,5-T

R.T.: 9.495 min
Delta R.T.: 0.006 min
Response: 13649146
Conc: N.D.

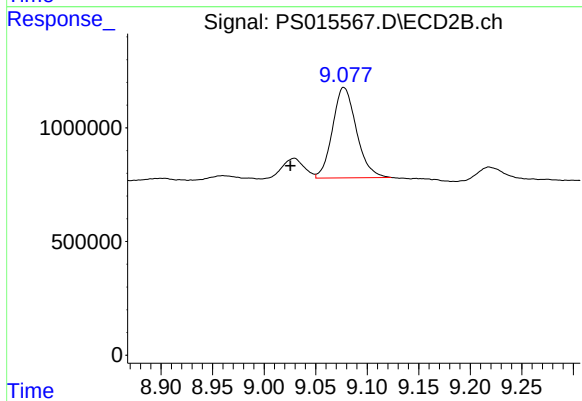

#12 2,4,5-T


R.T.: 9.077 min
Delta R.T.: 0.052 min
Response: 6421829
Conc: 2.18 ng/ml

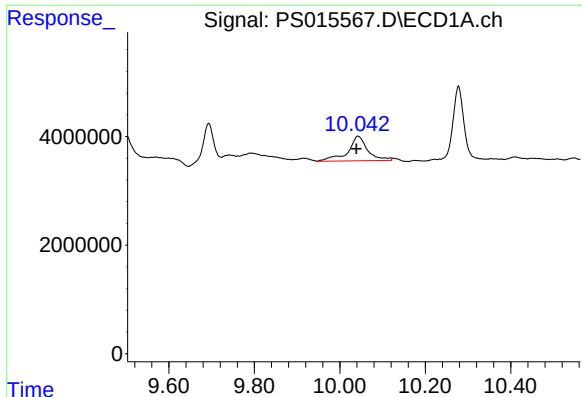

#13 2,4-DB


R.T.: 10.042 min
Delta R.T.: 0.003 min
Response: 14529817
Conc: 4.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

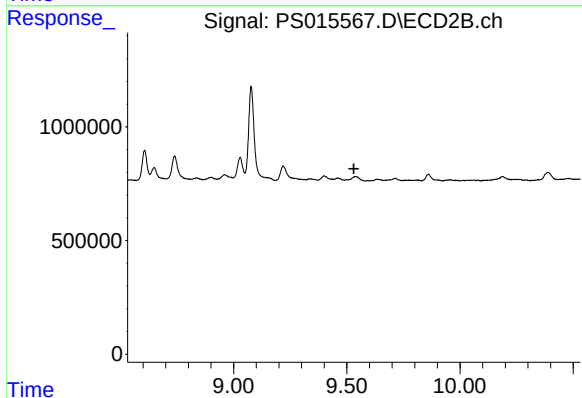


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.531 min
Response: 0
Conc: N.D.

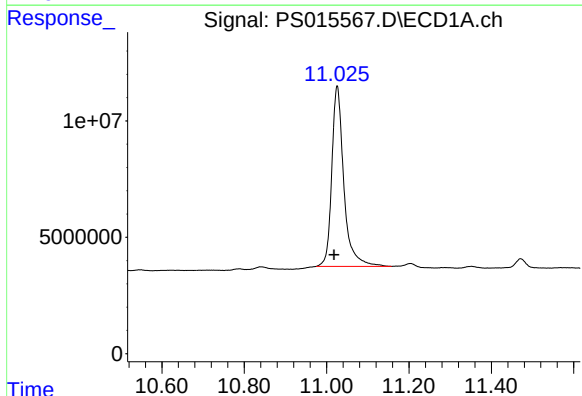


#15 Picloram

R.T.: 11.026 min
Delta R.T.: 0.008 min
Response: 157675041
Conc: 8.21 ng/ml

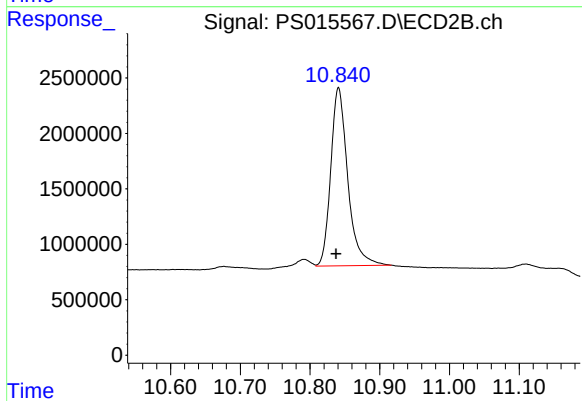

#15 Picloram


R.T.: 10.841 min
Delta R.T.: 0.003 min
Response: 27248339
Conc: 6.57 ng/ml

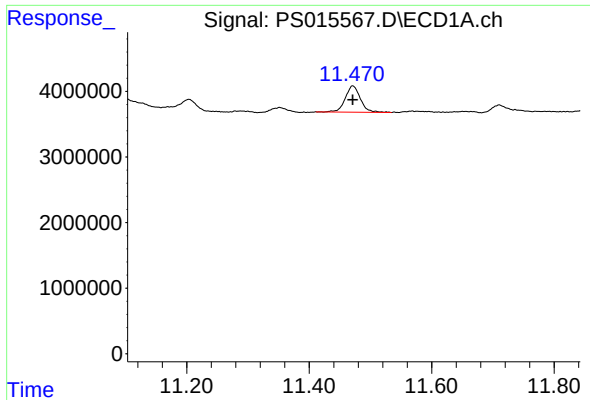

#16 DCPA

R.T.: 11.471 min
Delta R.T.: 0.000 min
Response: 6860094
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

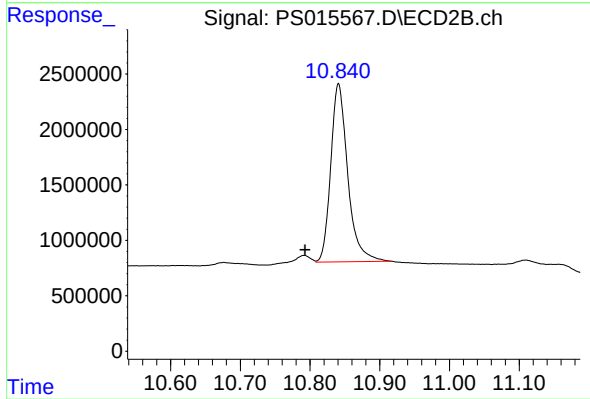

#16 DCPA

R.T.: 10.841 min
Delta R.T.: 0.048 min
Response: 27248339
Conc: 6.05 ng/ml