

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061421\
 Data File : PS015579.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2021 01:02
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 09:10:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061421.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 08:41:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.230	6.780	1670.4E6	304.2E6	600.608	564.852
Target Compounds							
3) T	4-Nitroph...	7.022	0.000	11384709	0	7.528	N.D. #
12) T	2,4,5-T	9.493	0.000	6959124	0	<MDL	N.D. #
13) T	2,4-DB	10.028	0.000	9601869	0	3.039	N.D. #
15) T	Picloram	11.024	10.841	53599737	8404575	2.790	2.028 #
16) T	DCPA	11.474	10.841f	3444474	8404575	<MDL	1.866 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061421\
Data File : PS015579.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2021 01:02
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 09:10:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061421.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 08:41:47 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

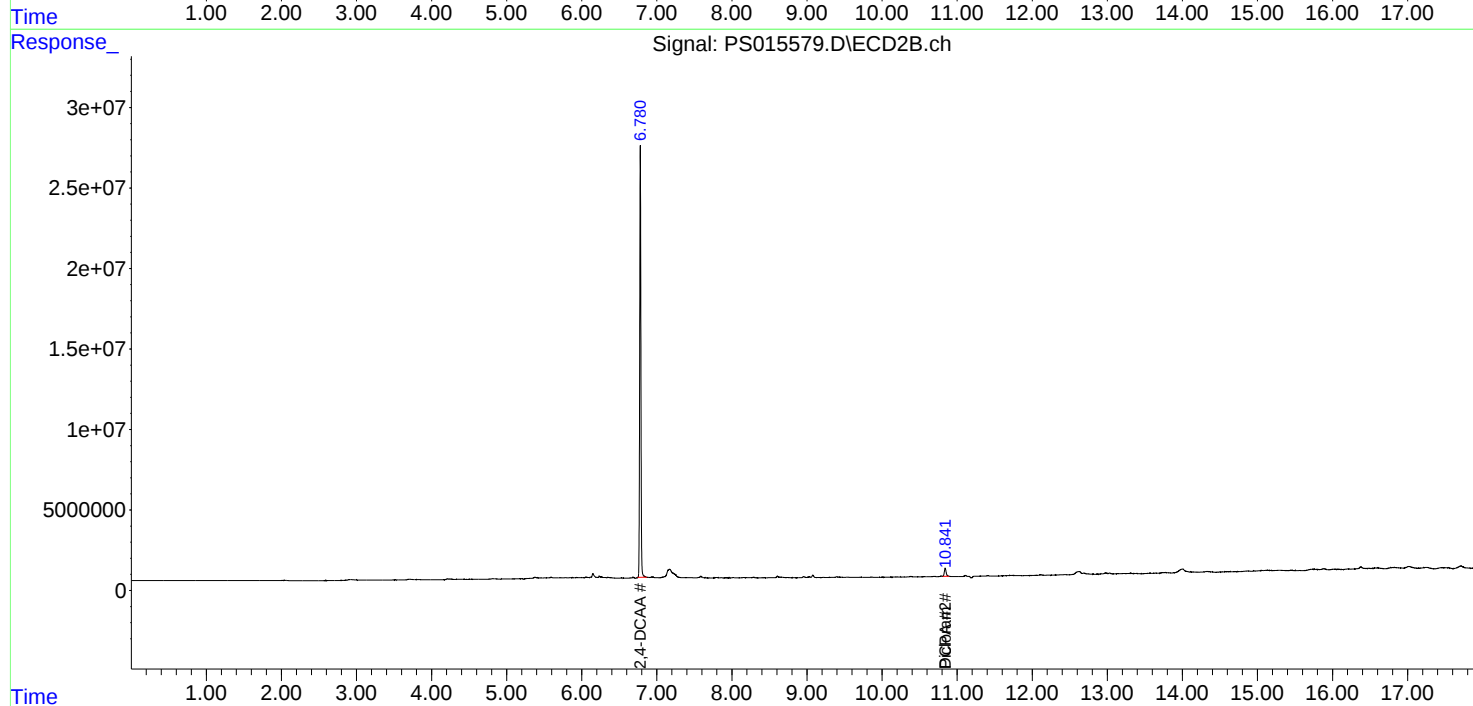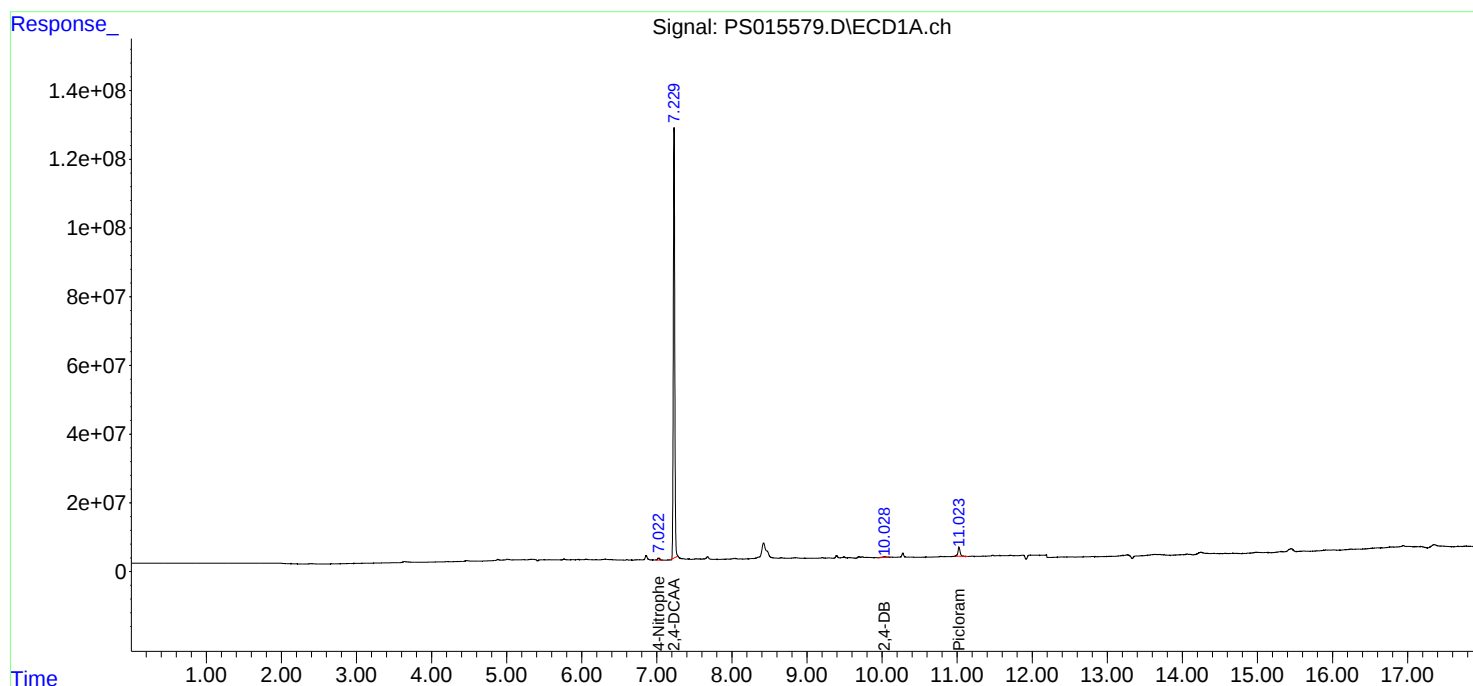


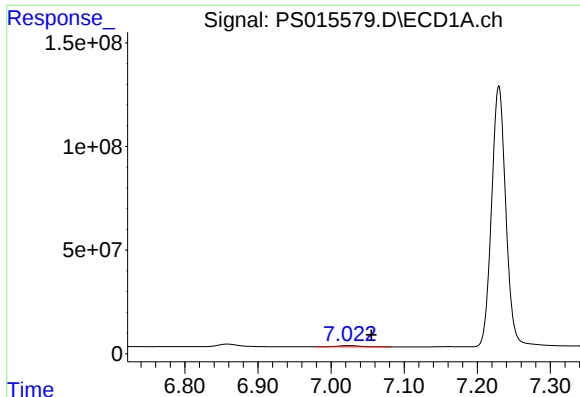

#3 4-Nitrophenol


R.T.: 7.022 min
Delta R.T.: -0.033 min
Response: 11384709
Conc: 7.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

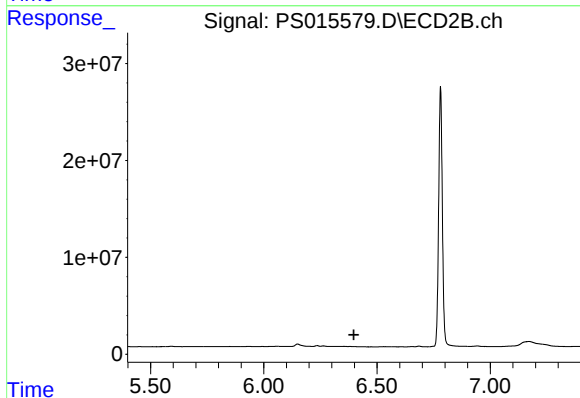


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.398 min
Response: 0
Conc: N.D.

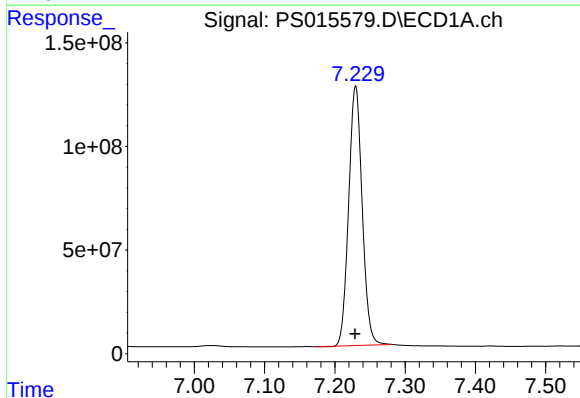


#4 2,4-DCAA

R.T.: 7.230 min
Delta R.T.: 0.000 min
Response: 1670365907
Conc: 600.61 ng/ml

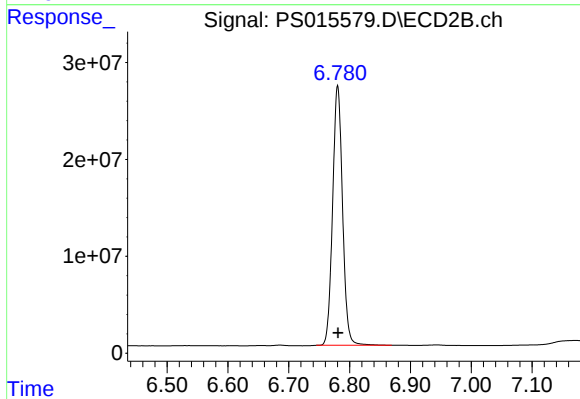

#4 2,4-DCAA


R.T.: 6.780 min
Delta R.T.: 0.000 min
Response: 304192671
Conc: 564.85 ng/ml

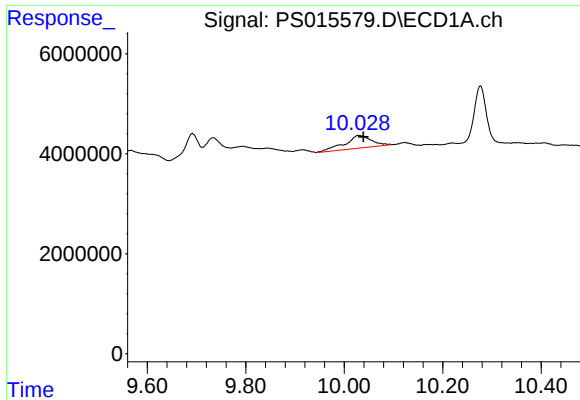

#13 2,4-DB


R.T.: 10.028 min
Delta R.T.: -0.011 min
Response: 9601869
Conc: 3.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

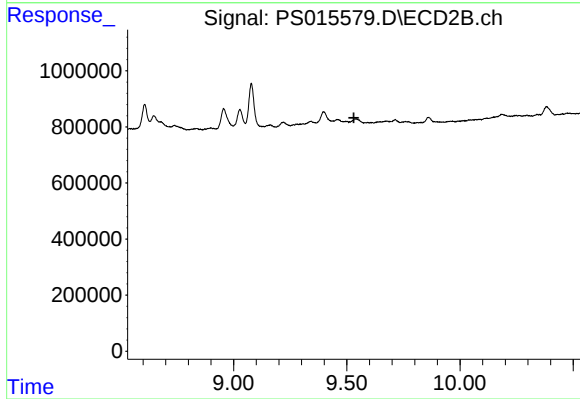


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.531 min
Response: 0
Conc: N.D.

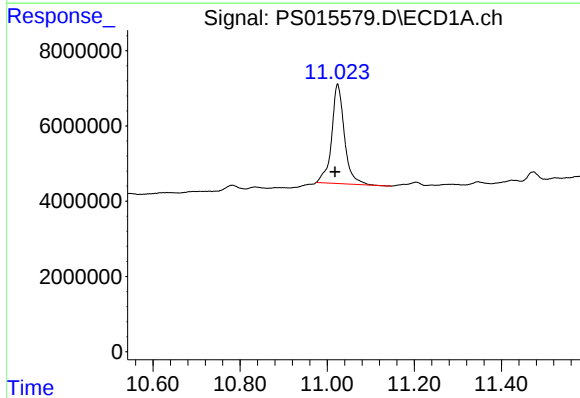


#15 Picloram

R.T.: 11.024 min
Delta R.T.: 0.006 min
Response: 53599737
Conc: 2.79 ng/ml

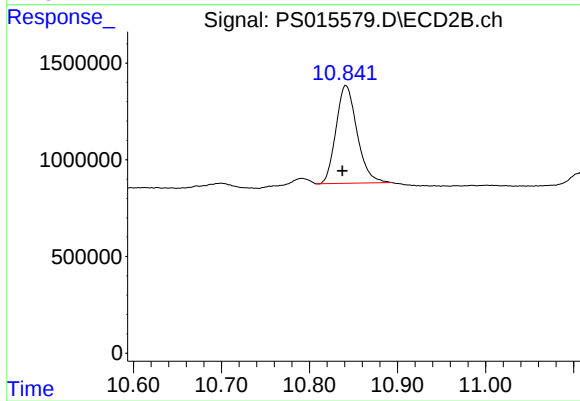

#15 Picloram


R.T.: 10.841 min
Delta R.T.: 0.004 min
Response: 8404575
Conc: 2.03 ng/ml

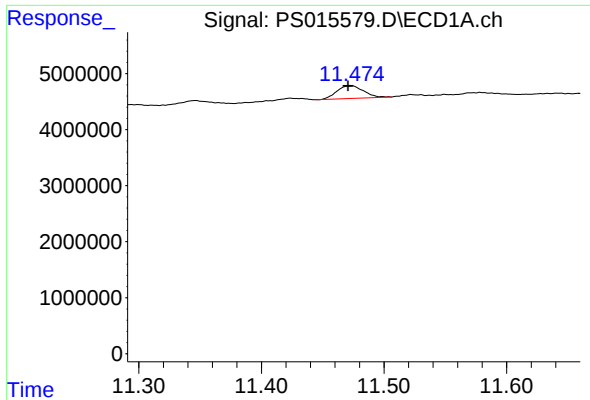

#16 DCPA

R.T.: 11.474 min
Delta R.T.: 0.003 min
Response: 3444474
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

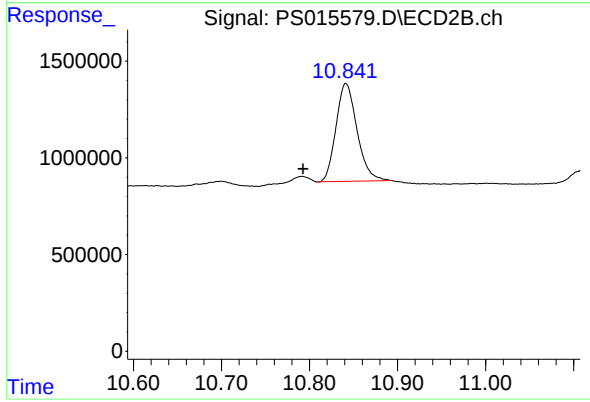

#16 DCPA

R.T.: 10.841 min
Delta R.T.: 0.048 min
Response: 8404575
Conc: 1.87 ng/ml