

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061421\
 Data File : PS015596.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2021 07:53
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 09:14:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061421.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 08:41:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.781	1688.9E6	304.3E6	607.262	565.075
Target Compounds							
3) T	4-Nitroph...	7.021	0.000	15717184	0	10.392	N.D. #
9) T	2,4-D	8.351	0.000	10331916	0	3.563	N.D. #
10) T	Pentachlo...	8.657	0.000	3653335	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.207	0.000	5397193	0	<MDL	N.D. #
12) T	2,4,5-T	9.491	9.078f	15492432	8945027	1.093	3.036 #
13) T	2,4-DB	10.039	0.000	15138518	0	4.792	N.D. #
15) T	Picloram	11.023	10.840	262.8E6	43456008	13.680	10.485
16) T	DCPA	11.470	10.840f	6706575	43456008	<MDL	9.647 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061421\
Data File : PS015596.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2021 07:53
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 09:14:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061421.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 08:41:47 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

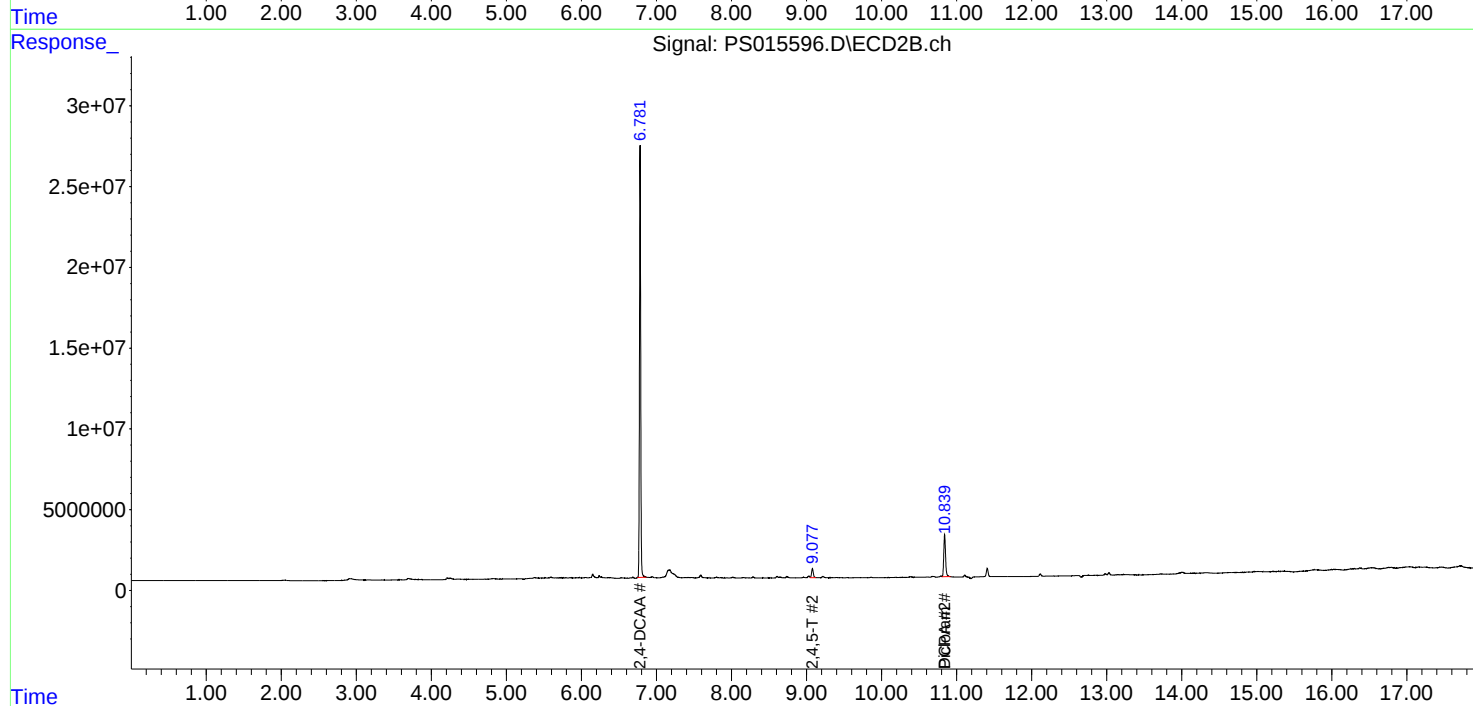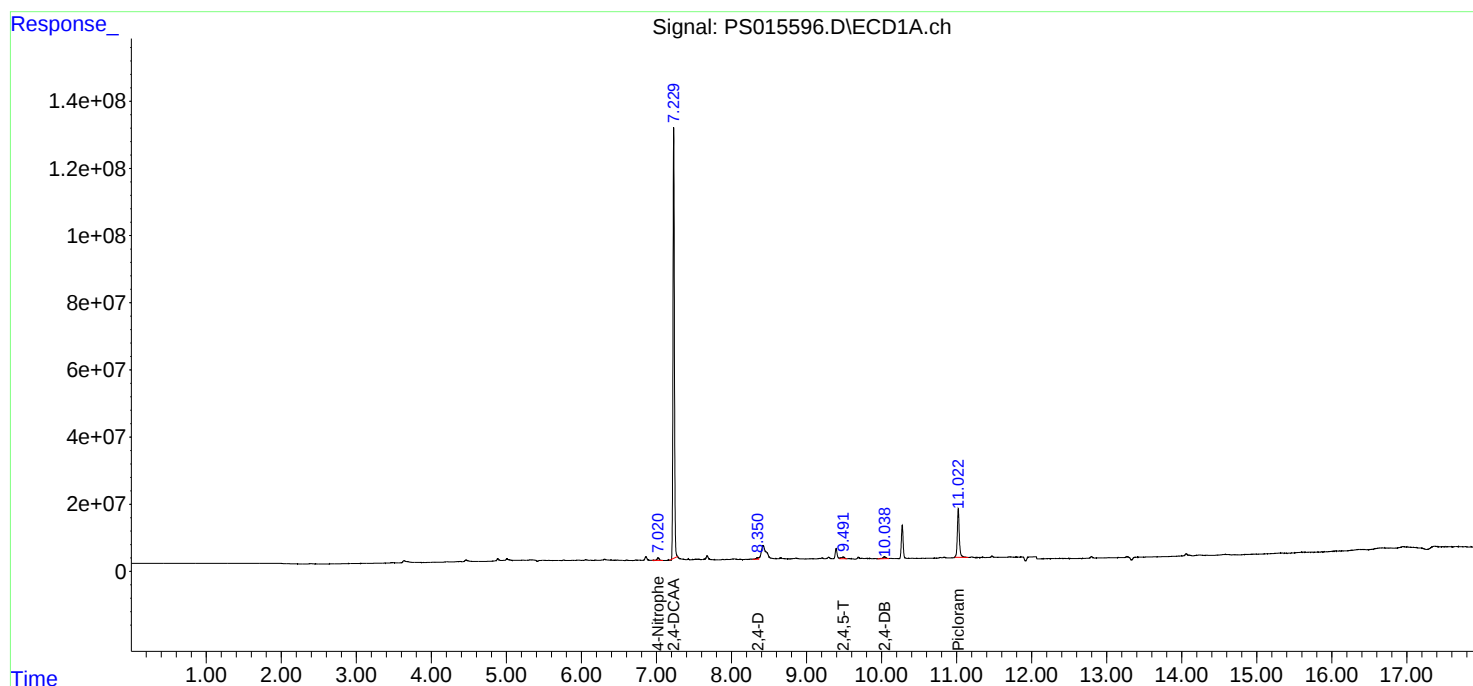


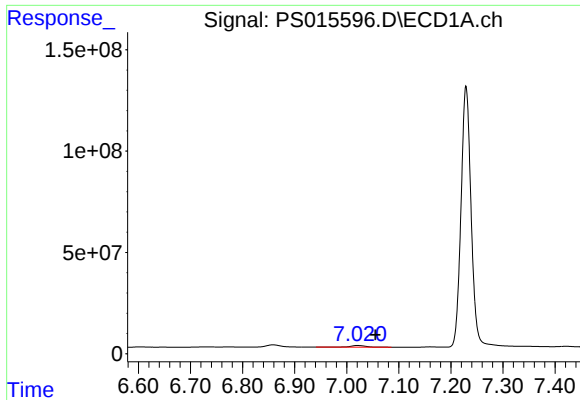

#3 4-Nitrophenol


R.T.: 7.021 min
Delta R.T.: -0.035 min
Response: 15717184
Conc: 10.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

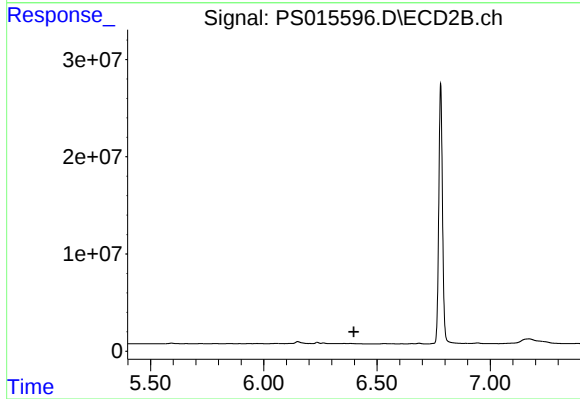


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.398 min
Response: 0
Conc: N.D.

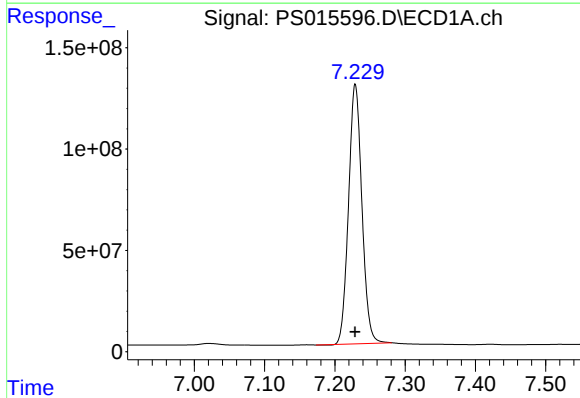


#4 2,4-DCAA

R.T.: 7.229 min
Delta R.T.: 0.000 min
Response: 1688872428
Conc: 607.26 ng/ml

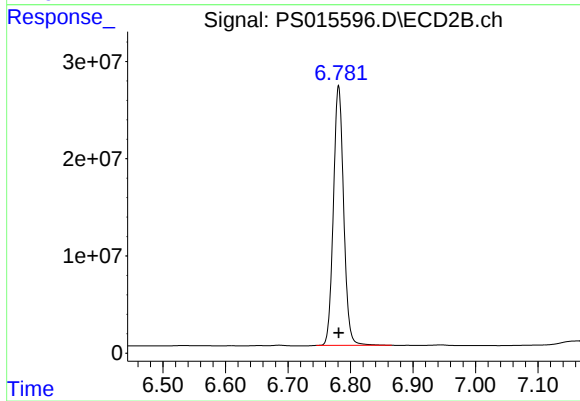

#4 2,4-DCAA


R.T.: 6.781 min
Delta R.T.: 0.000 min
Response: 304312918
Conc: 565.07 ng/ml

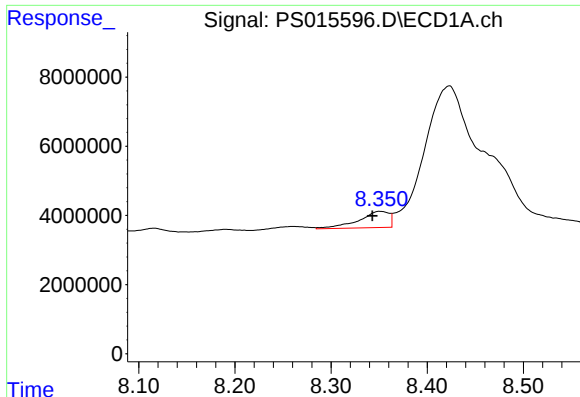

#9 2,4-D


R.T.: 8.351 min
Delta R.T.: 0.007 min
Response: 10331916
Conc: 3.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

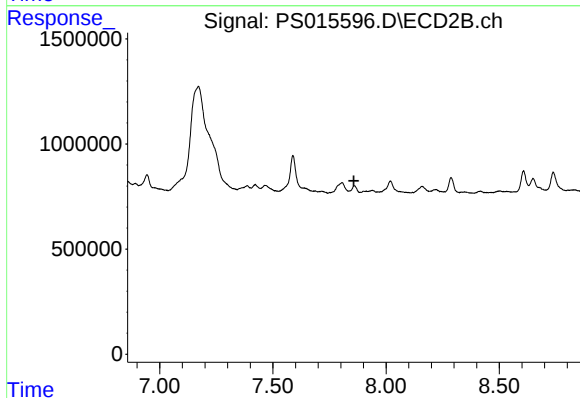


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.858 min
Response: 0
Conc: N.D.

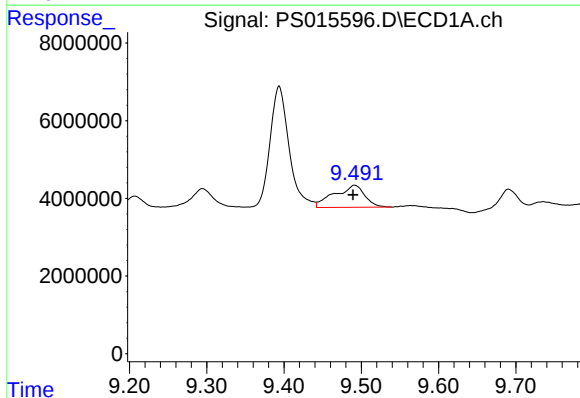


#12 2,4,5-T

R.T.: 9.491 min
Delta R.T.: 0.002 min
Response: 15492432
Conc: 1.09 ng/ml

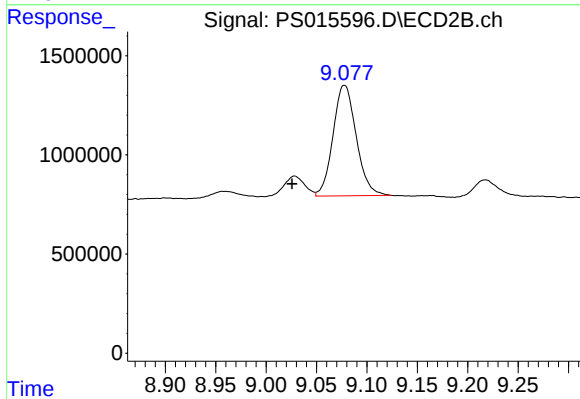

#12 2,4,5-T


R.T.: 9.078 min
Delta R.T.: 0.052 min
Response: 8945027
Conc: 3.04 ng/ml

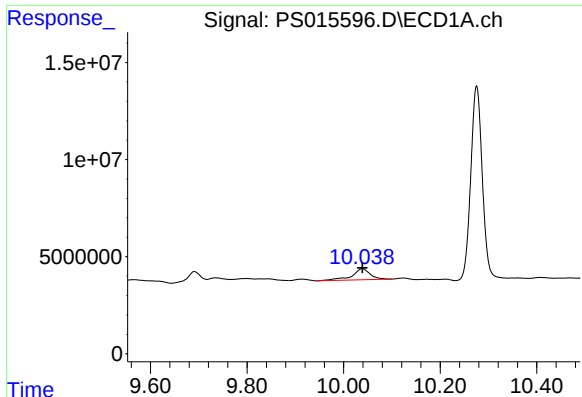

#13 2,4-DB


R.T.: 10.039 min
Delta R.T.: 0.000 min
Response: 15138518
Conc: 4.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

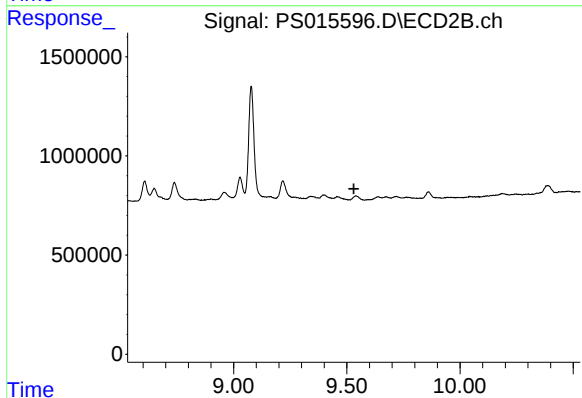


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.531 min
Response: 0
Conc: N.D.

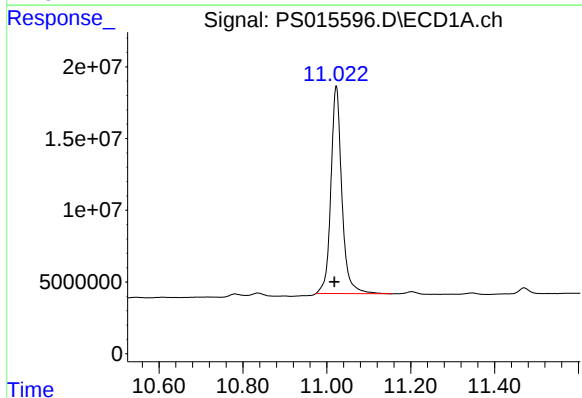


#15 Picloram

R.T.: 11.023 min
Delta R.T.: 0.005 min
Response: 262781012
Conc: 13.68 ng/ml

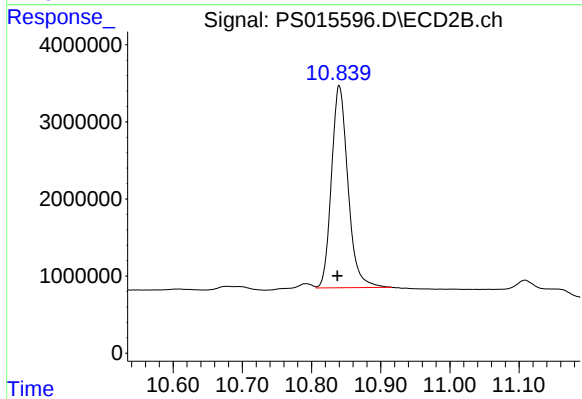

#15 Picloram


R.T.: 10.840 min
Delta R.T.: 0.002 min
Response: 43456008
Conc: 10.49 ng/ml

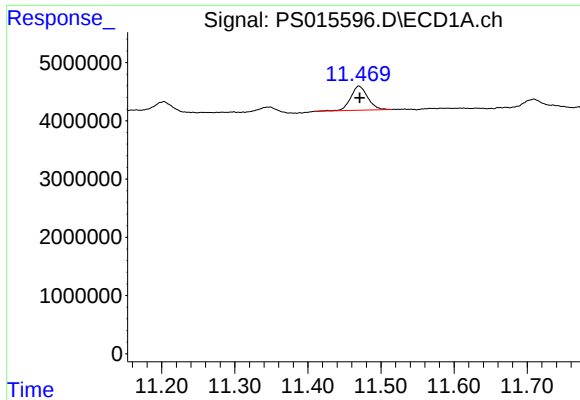

#16 DCPA

R.T.: 11.470 min
Delta R.T.: -0.001 min
Response: 6706575
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

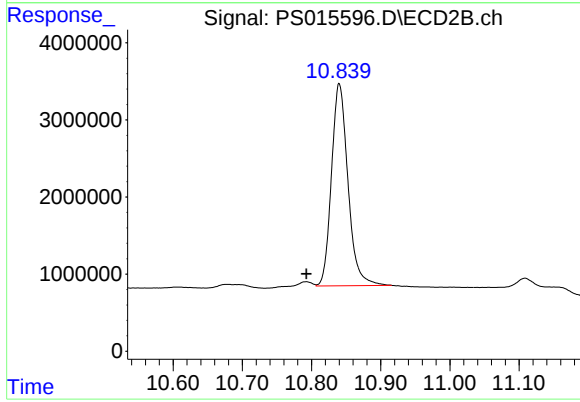

#16 DCPA

R.T.: 10.840 min
Delta R.T.: 0.047 min
Response: 43456008
Conc: 9.65 ng/ml