

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061521\
 Data File : PS015654.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jun 2021 14:04
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 16:48:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.191	6.770	786.5E6	245.9E6	473.385	488.028
Target Compounds							
11) T	2,4,5-TP ...	9.198	0.000	5298175	0	<MDL	N.D. #
14) T	DINOSEB	11.164	0.000	8704191	0	1.344	N.D. #
15) T	Picloram	10.976	10.823	61934143	10502710	4.530	2.497 #
16) T	DCPA	11.436	10.753	23455085	65631137	1.773	15.611 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061521\
Data File : PS015654.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jun 2021 14:04
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 16:48:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

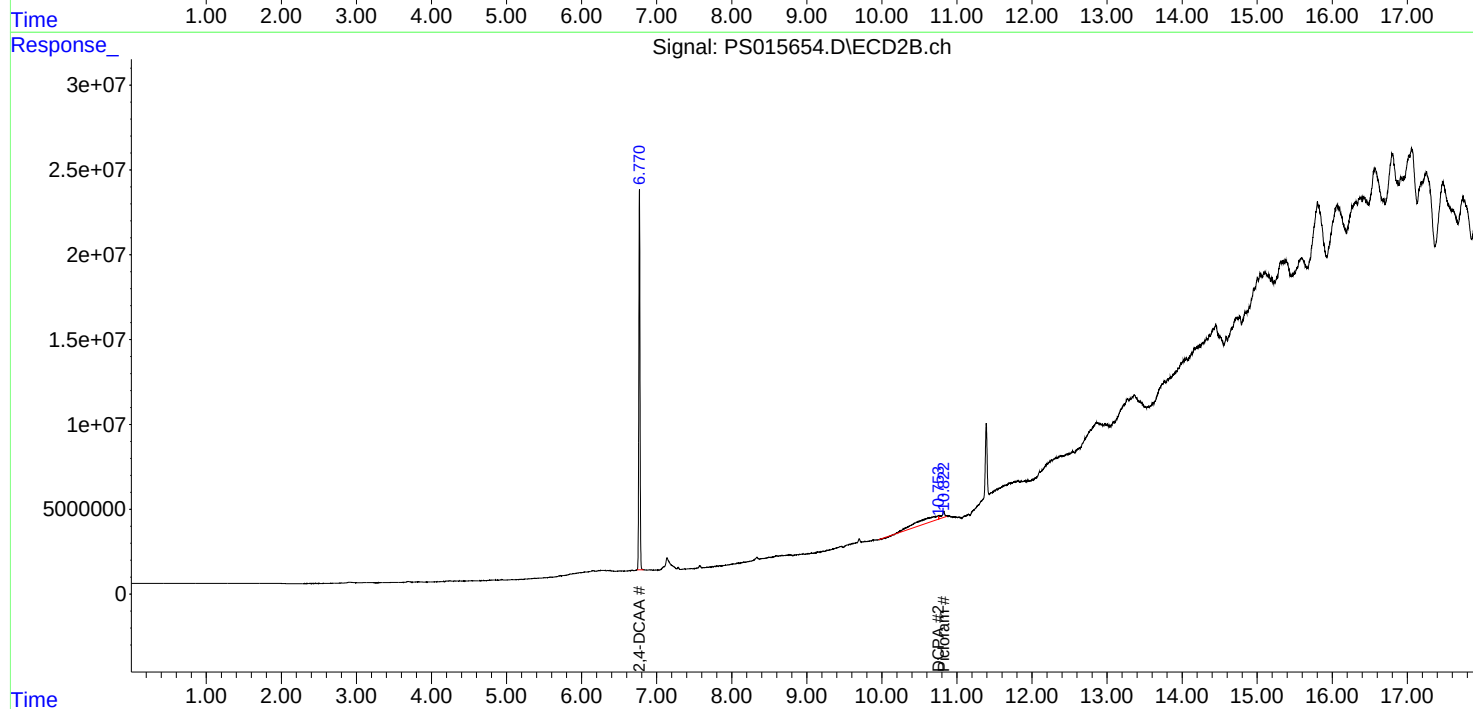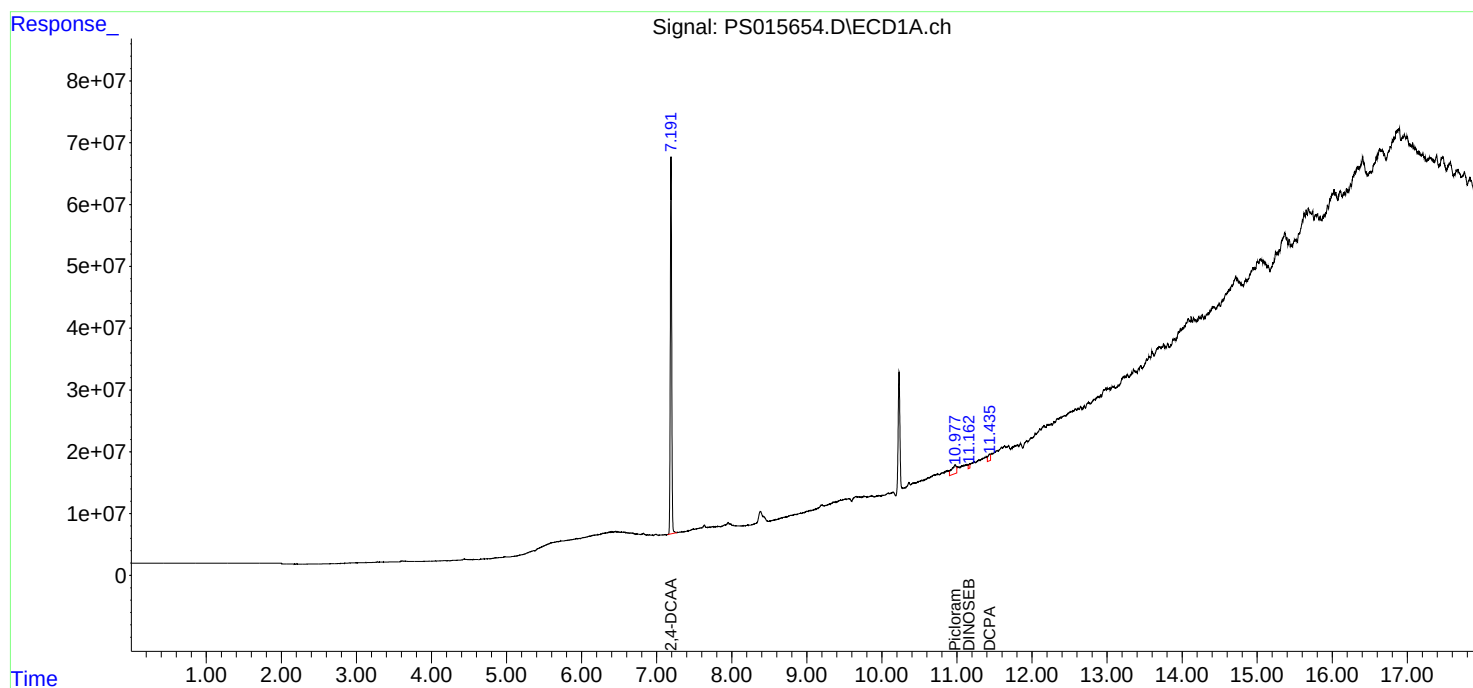


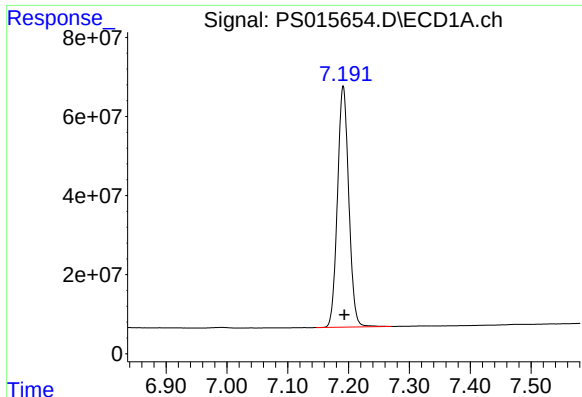

#4 2,4-DCAA


R.T.: 7.191 min
Delta R.T.: -0.002 min
Response: 786504647
Conc: 473.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

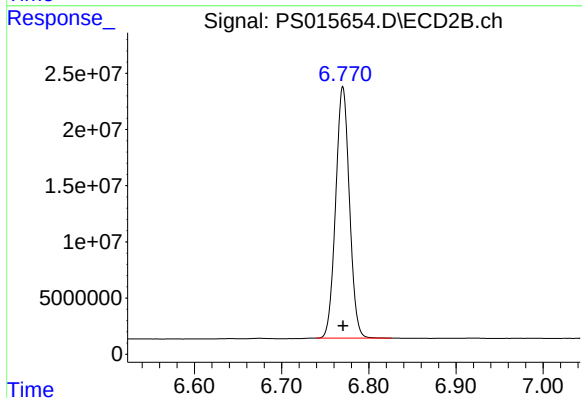


#4 2,4-DCAA

R.T.: 6.770 min
Delta R.T.: 0.000 min
Response: 245893932
Conc: 488.03 ng/ml

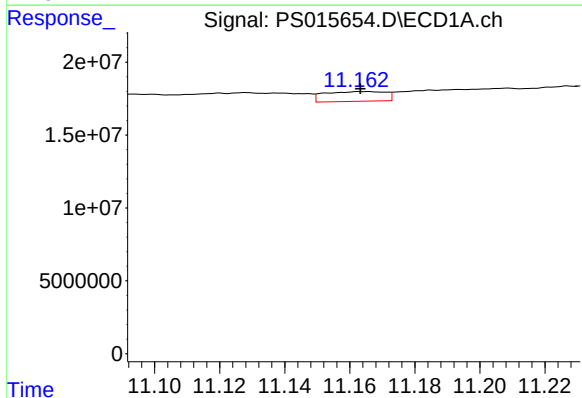


#14 DINOSEB

R.T.: 11.164 min
Delta R.T.: 0.000 min
Response: 8704191
Conc: 1.34 ng/ml

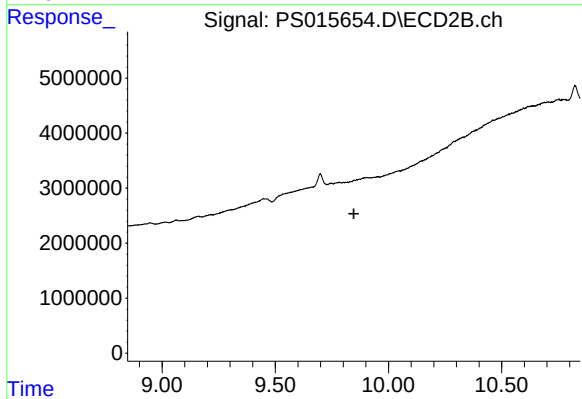

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.847 min
Response: 0
Conc: N.D.

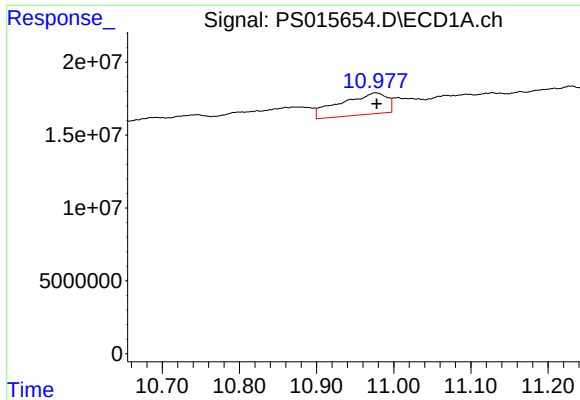

#15 Picloram


R.T.: 10.976 min
Delta R.T.: -0.002 min
Response: 61934143
Conc: 4.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

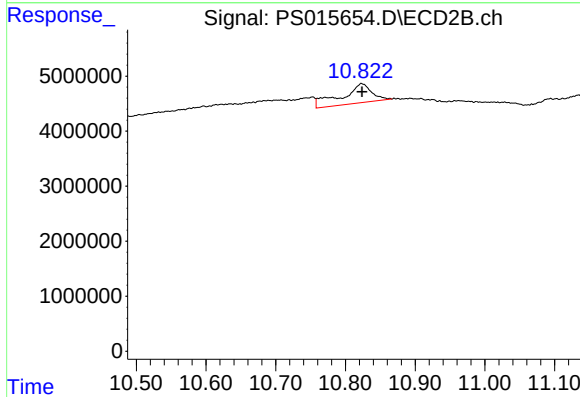


#15 Picloram

R.T.: 10.823 min
Delta R.T.: 0.000 min
Response: 10502710
Conc: 2.50 ng/ml

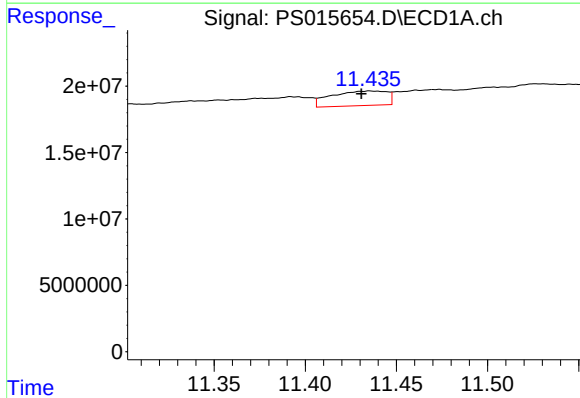

#16 DCPA

R.T.: 11.436 min
Delta R.T.: 0.005 min
Response: 23455085
Conc: 1.77 ng/ml

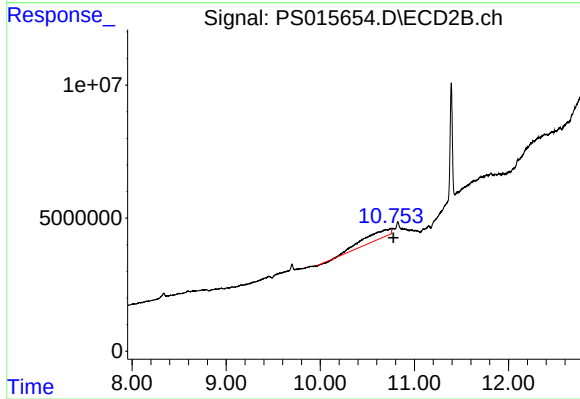

#16 DCPA

R.T.: 10.753 min
Delta R.T.: -0.026 min
Response: 65631137
Conc: 15.61 ng/ml