

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061521\
 Data File : PS015693.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2021 06:33
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 06:56:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.191	6.769	809.2E6	267.5E6	487.018	530.835
Target Compounds							
9) T	2,4-D	8.372f	0.000	43500131	0	24.821	N.D. #
10) T	Pentachlo...	8.614	0.000	7608963	0	<MDL	N.D. #
15) T	Picloram	10.977	10.823	46886899	17235982	3.430	4.098
16) T	DCPA	0.000	10.823f	0	17235982	N.D.	4.100



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061521\
Data File : PS015693.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2021 06:33
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 06:56:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

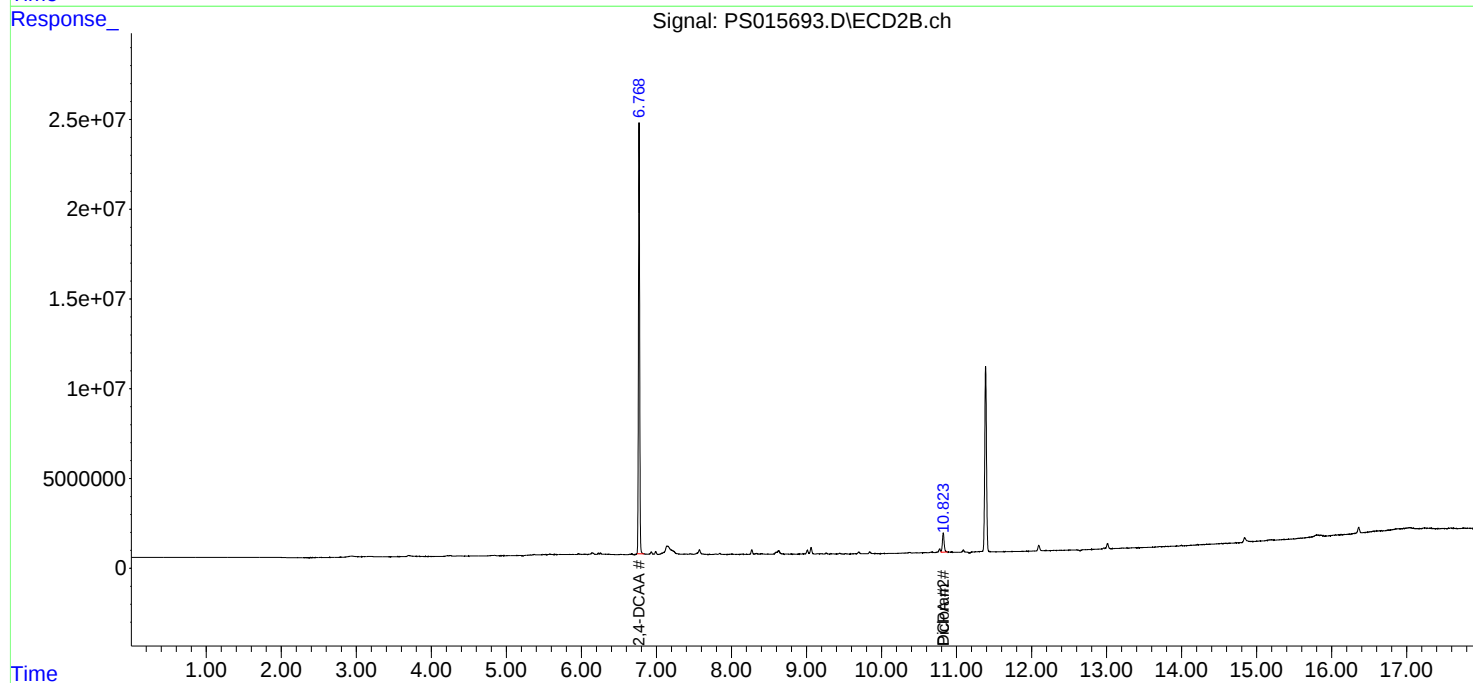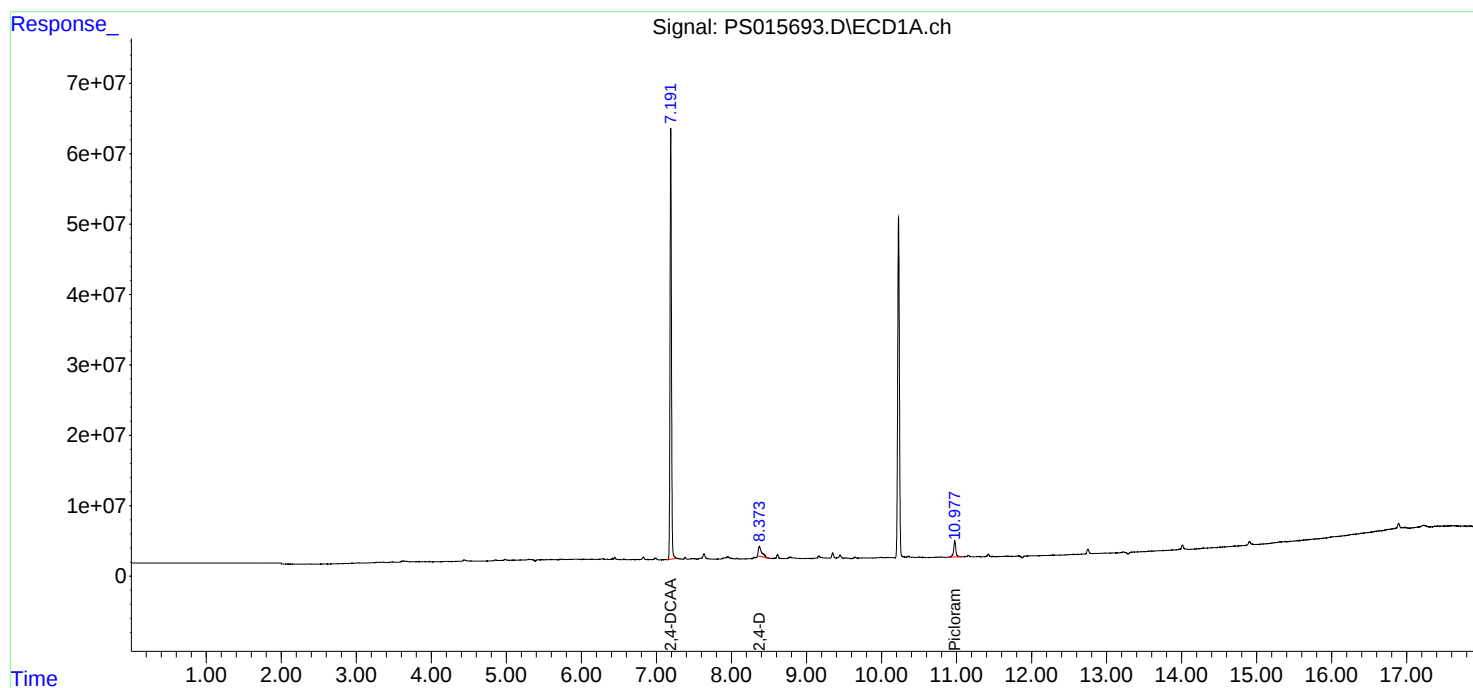


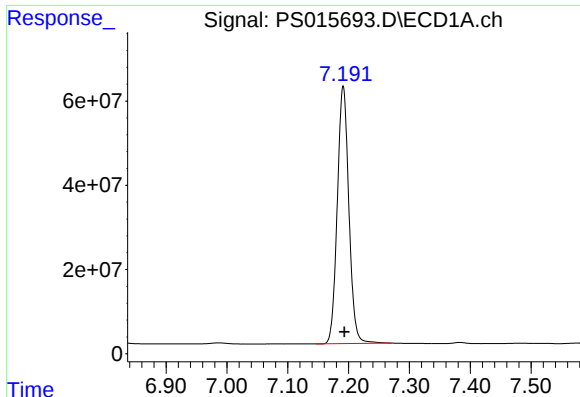

#4 2,4-DCAA


R.T.: 7.191 min
Delta R.T.: -0.002 min
Response: 809154118
Conc: 487.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

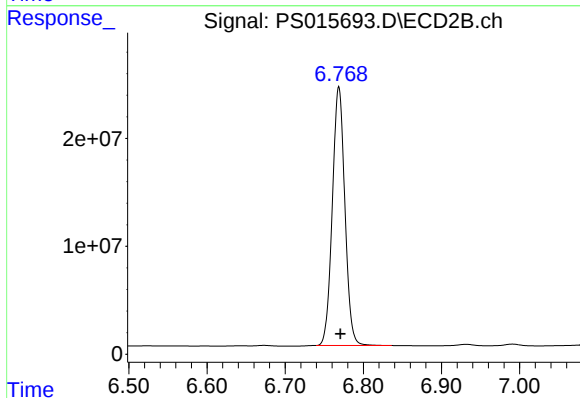


#4 2,4-DCAA

R.T.: 6.769 min
Delta R.T.: -0.002 min
Response: 267462057
Conc: 530.83 ng/ml

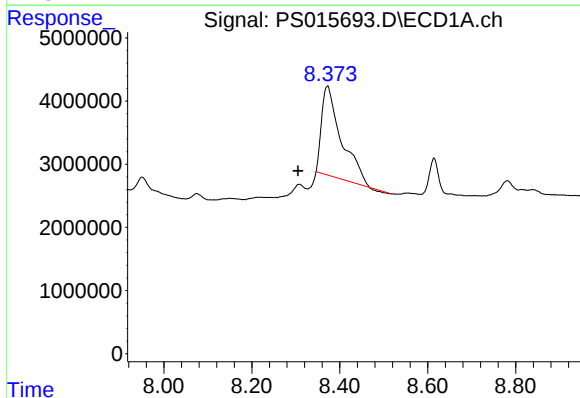


#9 2,4-D

R.T.: 8.372 min
Delta R.T.: 0.067 min
Response: 43500131
Conc: 24.82 ng/ml

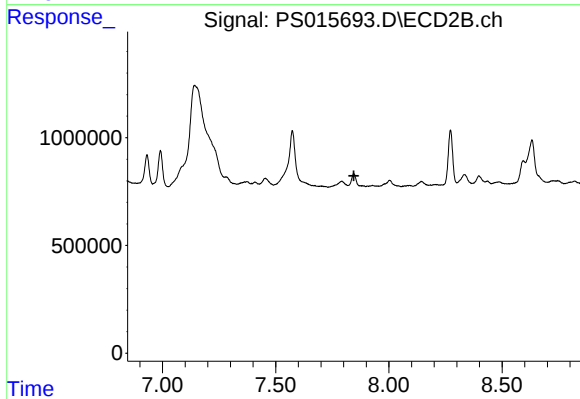

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.845 min
Response: 0
Conc: N.D.

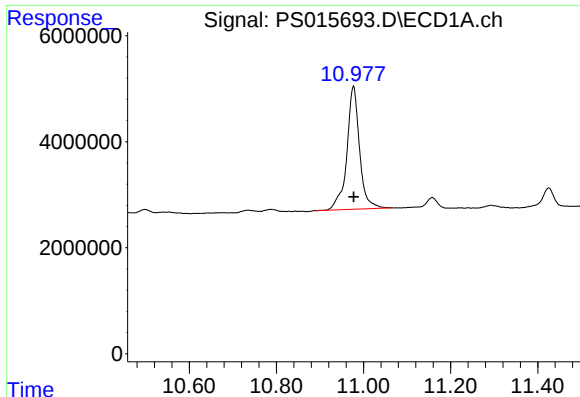

#15 Picloram


R.T.: 10.977 min
Delta R.T.: 0.000 min
Response: 46886899
Conc: 3.43 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

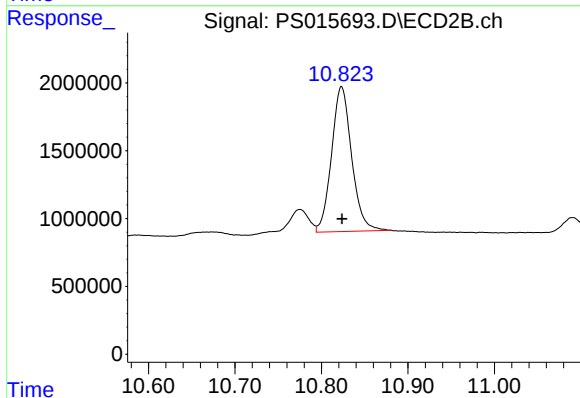


#15 Picloram

R.T.: 10.823 min
Delta R.T.: 0.000 min
Response: 17235982
Conc: 4.10 ng/ml

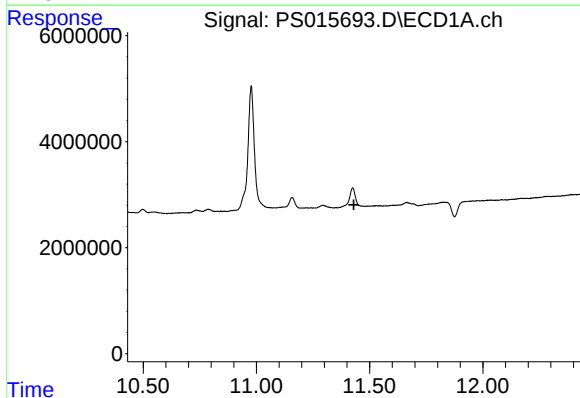

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.431 min
Response: 0
Conc: N.D.

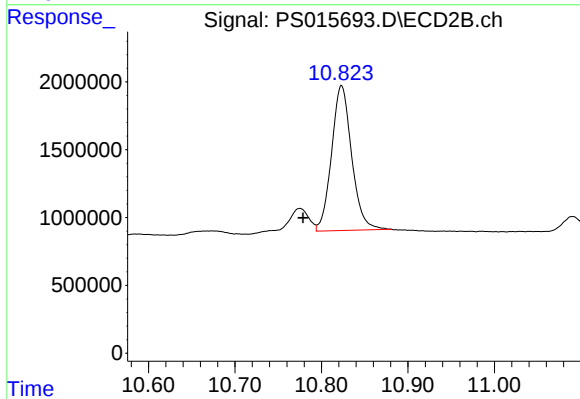

#16 DCPA

R.T.: 10.823 min
Delta R.T.: 0.045 min
Response: 17235982
Conc: 4.10 ng/ml