

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061521\
 Data File : PS015651.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jun 2021 12:51
 Operator : DD\AJ
 Sample : M2674-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TMR-DS-02-060921

Manual Integrations
 APPROVED

Ankita
 6/17/2021 9:01:56 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 16:47:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.191	6.770	828.0E6	245.8E6	498.372m	487.895m

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061521\
Data File : PS015651.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jun 2021 12:51
Operator : DD\AJ
Sample : M2674-02
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
TMR-DS-02-060921


Manual Integrations
APPROVED

Ankita
6/17/2021 9:01:56 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 16:47:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

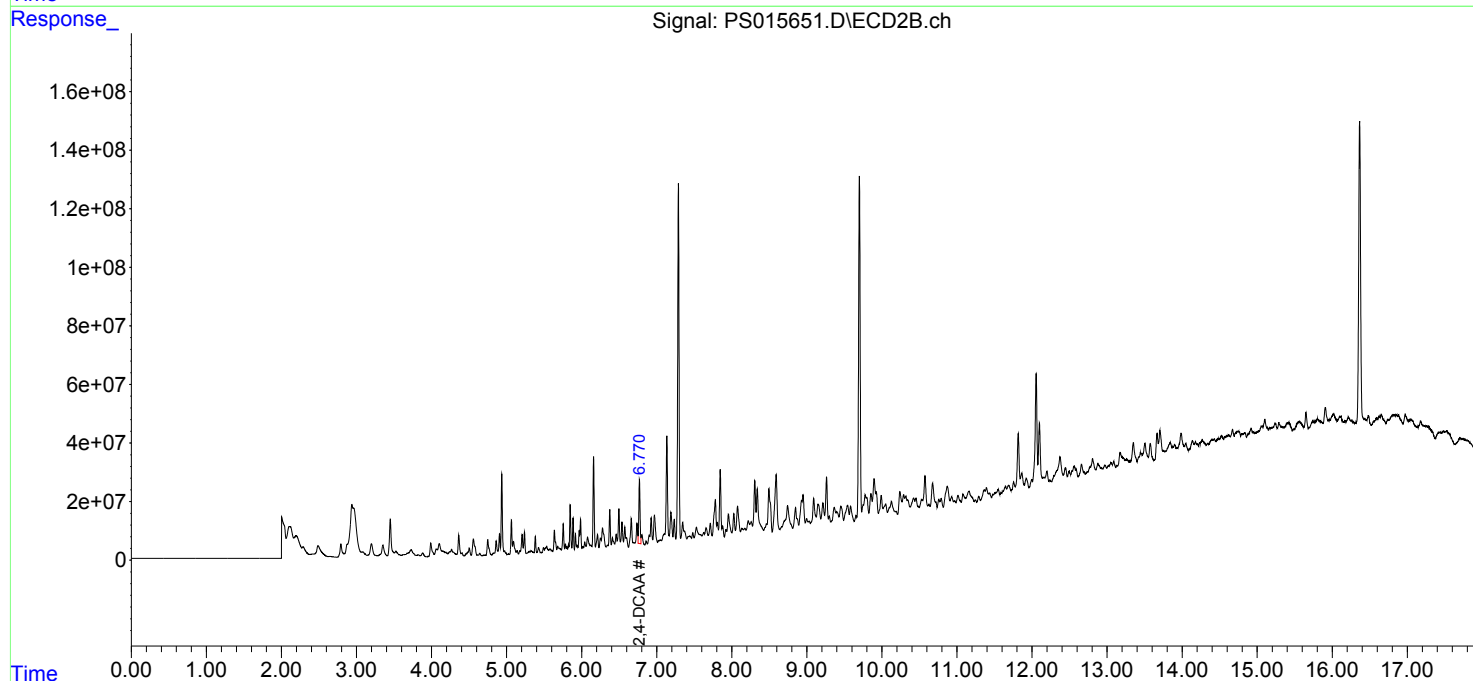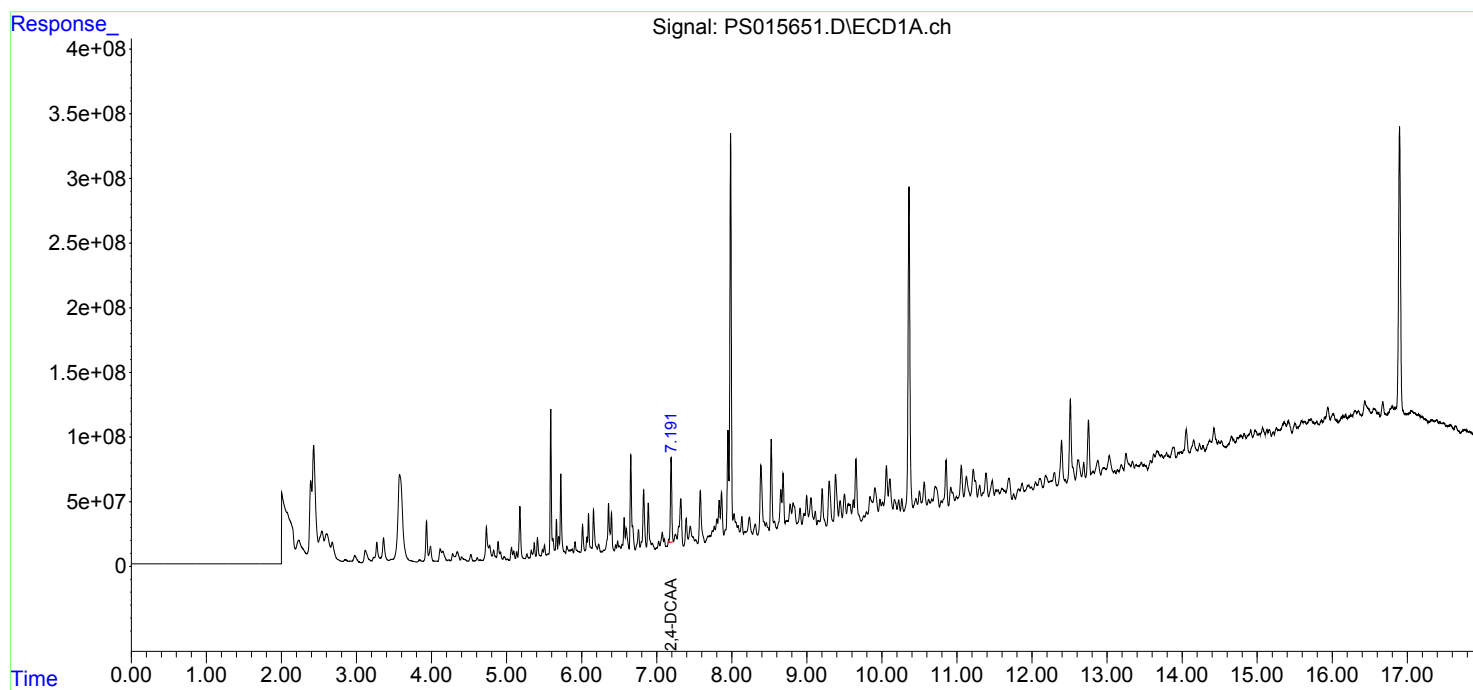

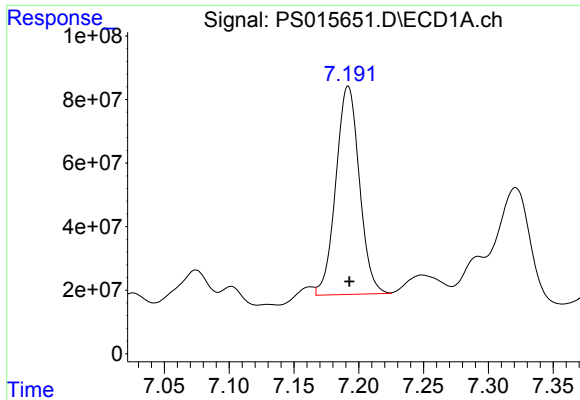


#4 2,4-DCAA

R.T.: 7.191 min
Delta R.T.: -0.001 min
Response: 828018179
Conc: 498.37 ng/ml m

Instrument :
ECD_S
ClientSampleId :
TMR-DS-02-060921

Manual Integrations
APPROVED

Ankita
6/17/2021 9:01:56 AM

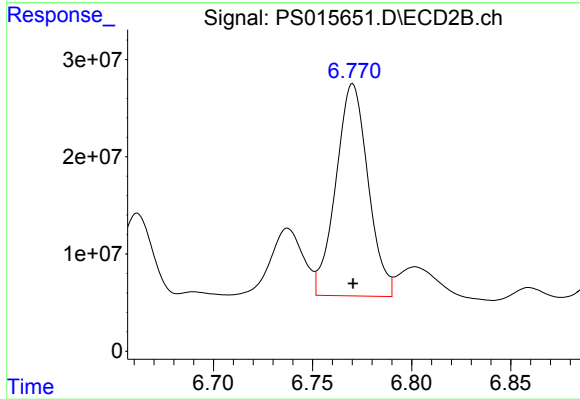

#4 2,4-DCAA

R.T.: 6.770 min
Delta R.T.: 0.000 min
Response: 245826697
Conc: 487.89 ng/ml m