

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061522\
 Data File : PS019701.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2022 08:37
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 12:09:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.215	6.815	717536	219035	<MDL	<MDL	#
Target Compounds								
2) T	3,5-DICHL...	6.407	5.942	3661304	183139	1.158	<MDL	#
3) T	4-Nitroph...	7.053	6.423	4618535	330011	4.706	<MDL	#
5) T	DICAMBA	7.393	6.971	1569631	617306	<MDL	<MDL	#
6) T	MCP	7.578	7.039	952996	641364	<MDL	<MDL	#
7) T	MCPA	7.675	0.000	8228113	0	<MDL	N.D.	#
8) T	DICHLORPROP	8.075	0.000	1261789	0	<MDL	N.D.	#
9) T	2,4-D	8.312	0.000	20114825	0	7.034	N.D.	#
11) T	2,4,5-TP ...	9.170	8.607	219669	1565662	<MDL	<MDL	#
12) T	2,4,5-T	9.450	9.037	3076052	122137	<MDL	<MDL	#
13) T	2,4-DB	9.999	9.541	1234324	27770	<MDL	<MDL	#
14) T	DINOSEB	11.146	0.000	4578171	0	<MDL	N.D.	#
15) T	Picloram	10.968	10.858	5236592	3595555	<MDL	<MDL	#
16) T	DCPA	11.433	10.779	504377	412217	<MDL	<MDL	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061522\
Data File : PS019701.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2022 08:37
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 12:09:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

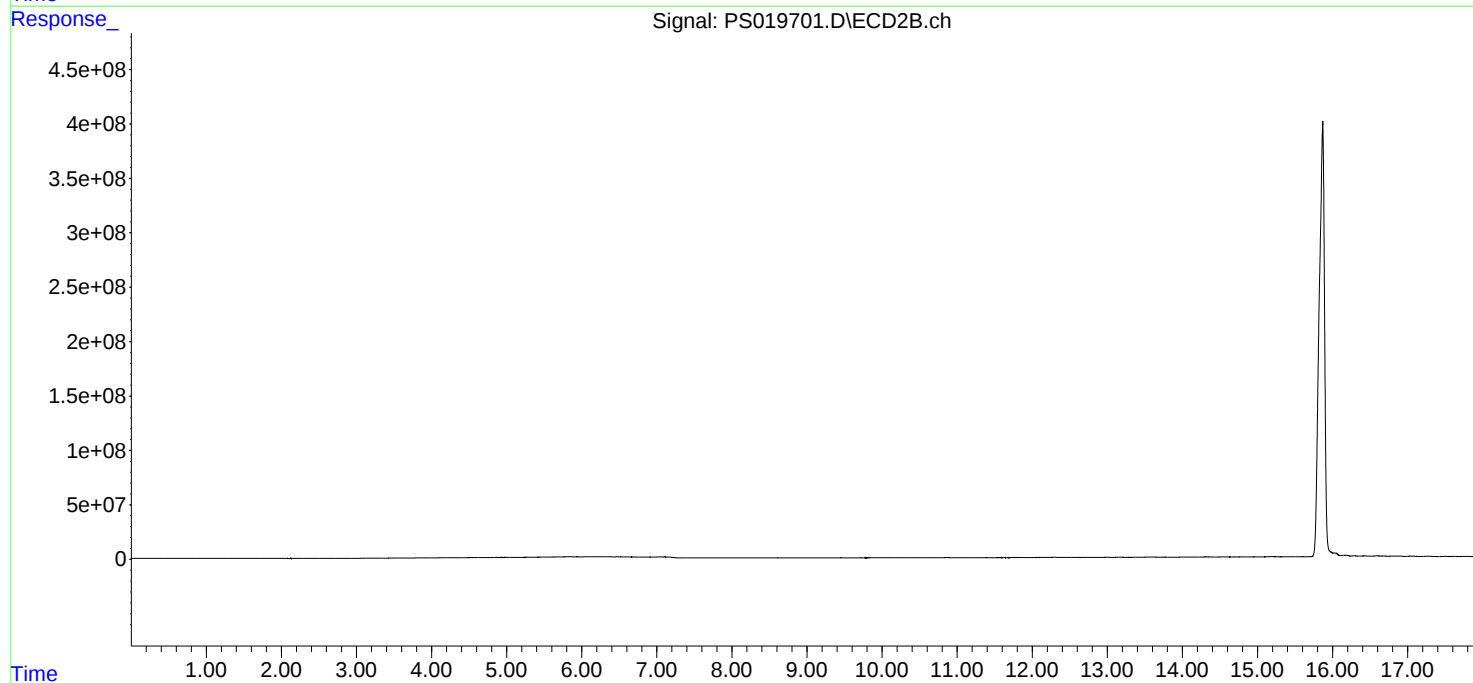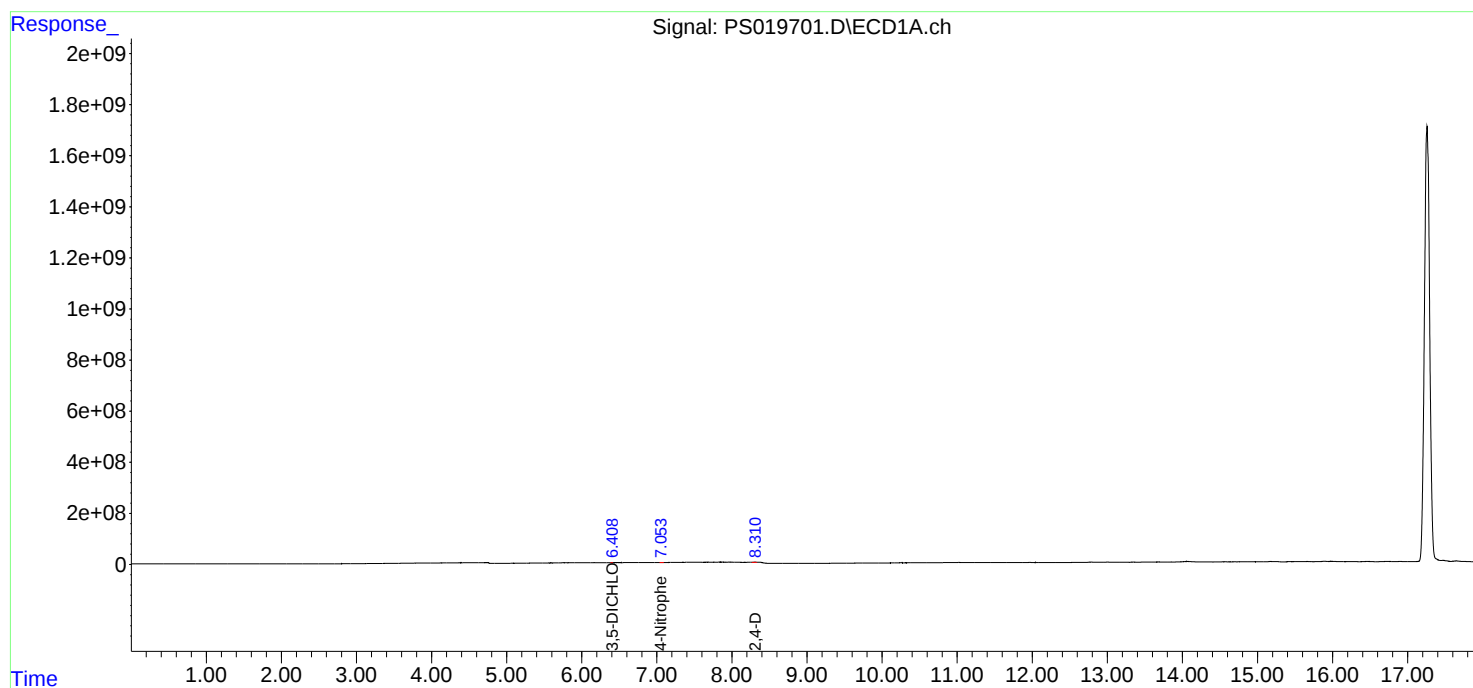


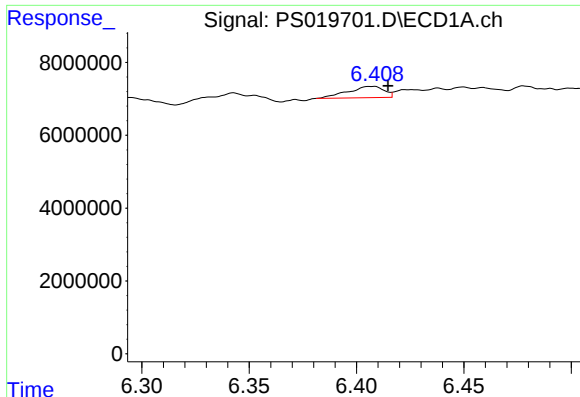

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.407 min
Delta R.T.: -0.007 min
Response: 3661304
Conc: 1.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

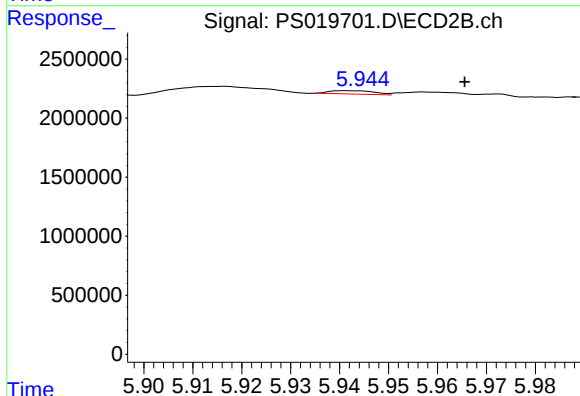


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.942 min
Delta R.T.: -0.024 min
Response: 183139
Conc: N.D.

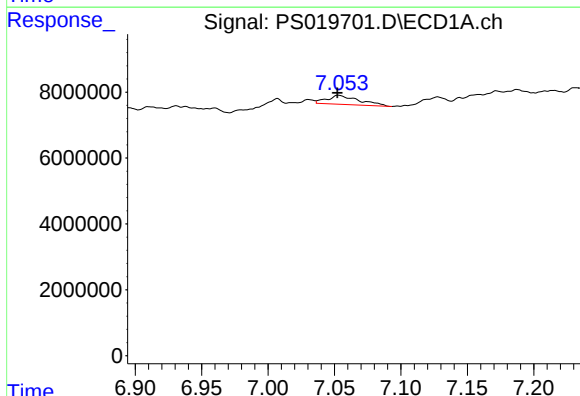


#3 4-Nitrophenol

R.T.: 7.053 min
Delta R.T.: 0.001 min
Response: 4618535
Conc: 4.71 ng/ml

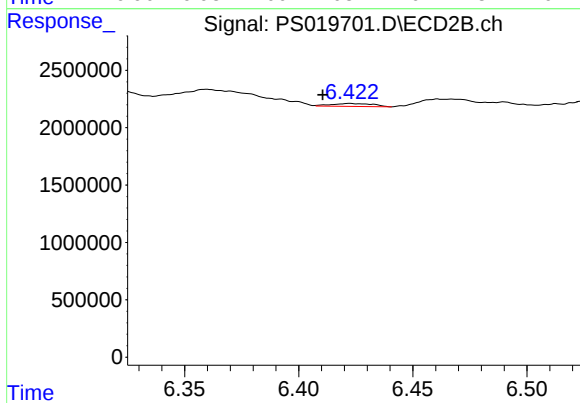

#3 4-Nitrophenol


R.T.: 6.423 min
Delta R.T.: 0.012 min
Response: 330011
Conc: N.D.

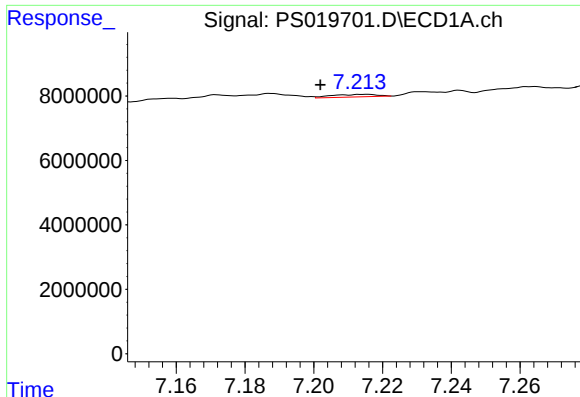

#4 2,4-DCAA


R.T.: 7.215 min
Delta R.T.: 0.013 min
Response: 717536
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

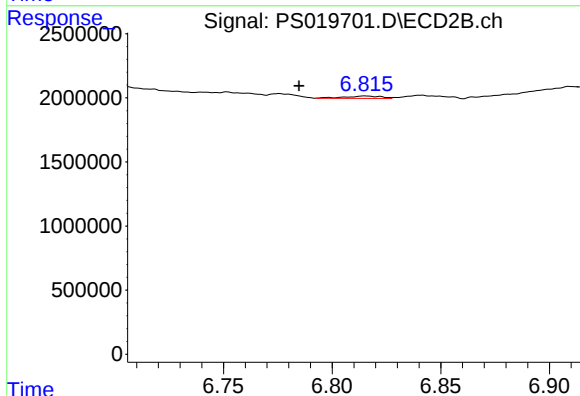


#4 2,4-DCAA

R.T.: 6.815 min
Delta R.T.: 0.030 min
Response: 219035
Conc: N.D.

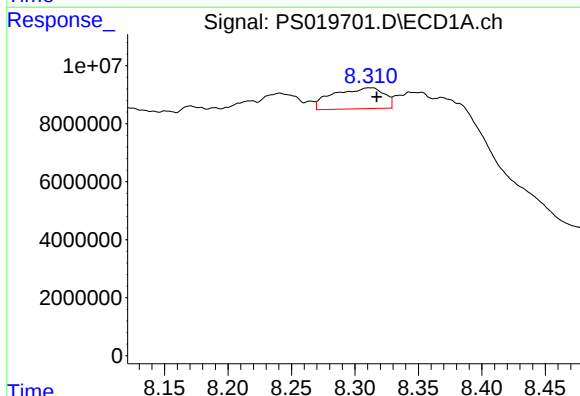

#9 2,4-D

R.T.: 8.312 min
Delta R.T.: -0.005 min
Response: 20114825
Conc: 7.03 ng/ml

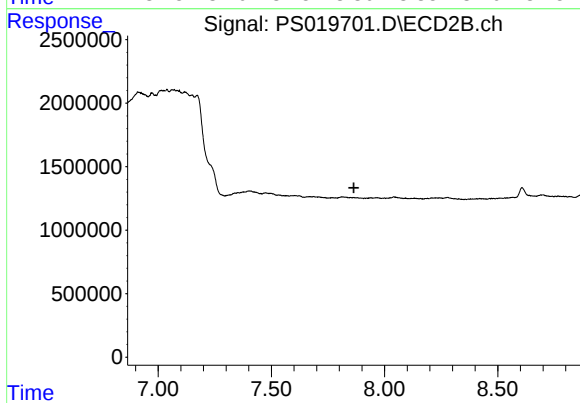

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.864 min
Response: 0
Conc: N.D.