

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061522\
 Data File : PS019714.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2022 13:46
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 14:04:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.197	6.781	1082.0E6	412.9E6	450.996	532.920
Target Compounds							
1) T	Dalapon	2.993	0.000	114984	0	<MDL	N.D. #
6) T	MCP	7.616f	0.000	95961	0	<MDL	N.D. #
7) T	MCPA	7.653f	0.000	3305733	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.612f	0	827506	N.D.	<MDL
10) T	Pentachlo...	8.616	8.284	470675	798563	<MDL	<MDL #
11) T	2,4,5-TP ...	9.129	8.685	1760498	1995968	<MDL	<MDL #
12) T	2,4,5-T	9.470	9.036	8636700	286742	<MDL	<MDL #
13) T	2,4-DB	9.999	9.541	7104464	456893	1.756	<MDL #
14) T	DINOSEB	11.128	9.861	32858407	345797	2.124	<MDL #
15) T	Picloram	10.959	10.861	1919783	9773469	<MDL	1.519 #
16) T	DCPA	11.421	10.789	961670	793504	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061522\
Data File : PS019714.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2022 13:46
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 14:04:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

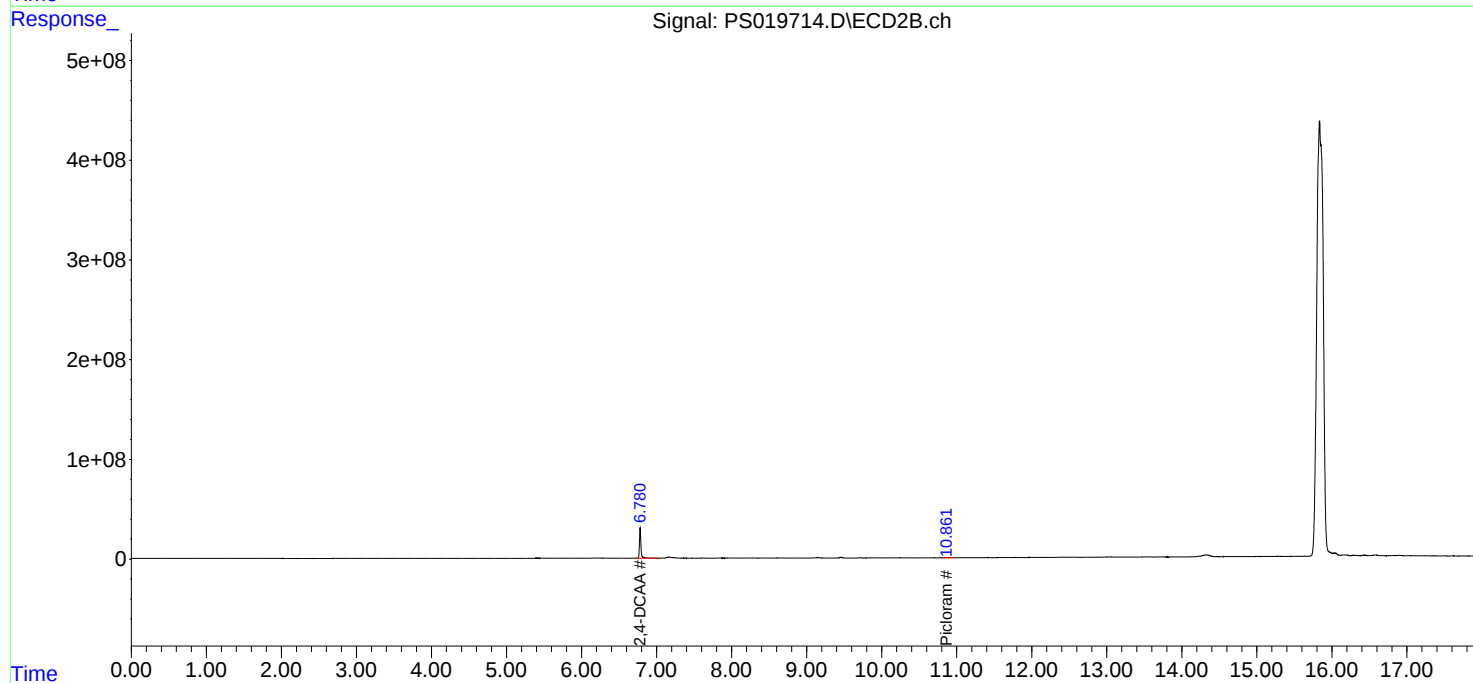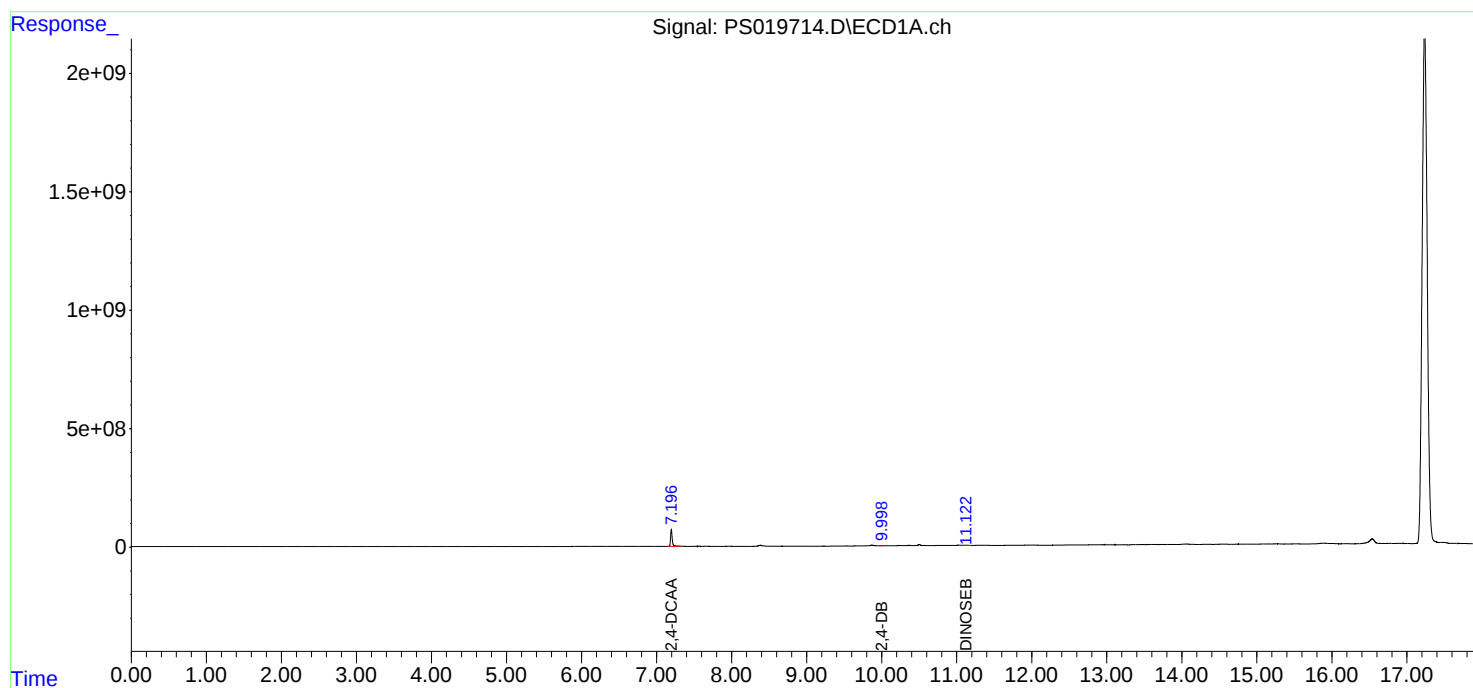


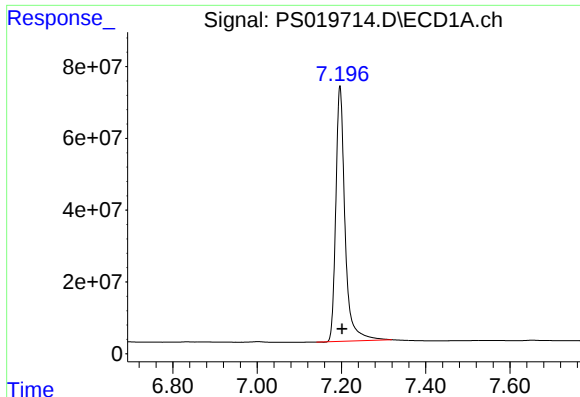

#4 2,4-DCAA


R.T.: 7.197 min
Delta R.T.: -0.005 min
Response: 1082014497
Conc: 451.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

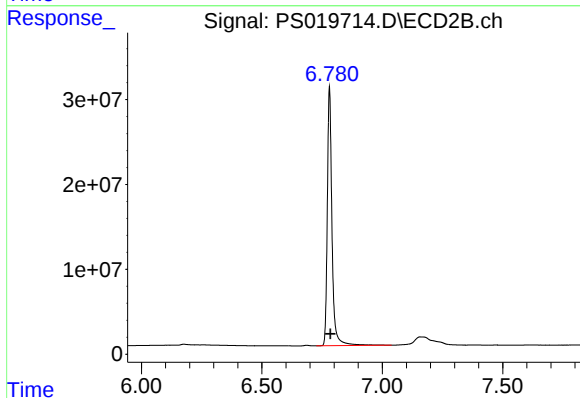


#4 2,4-DCAA

R.T.: 6.781 min
Delta R.T.: -0.004 min
Response: 412944299
Conc: 532.92 ng/ml

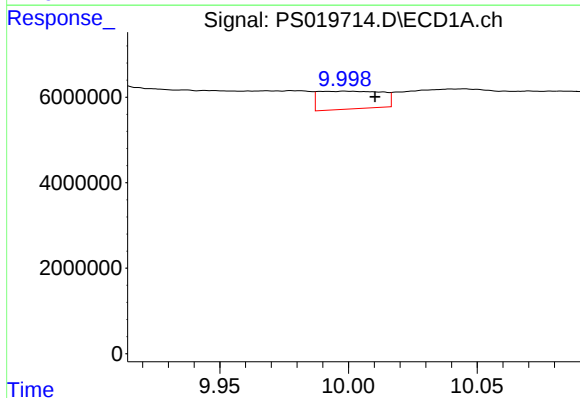


#13 2,4-DB

R.T.: 9.999 min
Delta R.T.: -0.011 min
Response: 7104464
Conc: 1.76 ng/ml

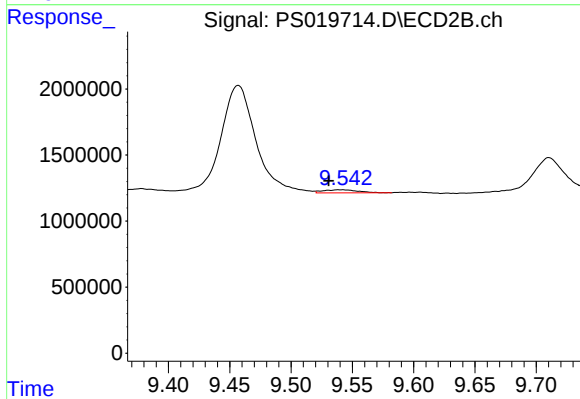

#13 2,4-DB


R.T.: 9.541 min
Delta R.T.: 0.010 min
Response: 456893
Conc: N.D.

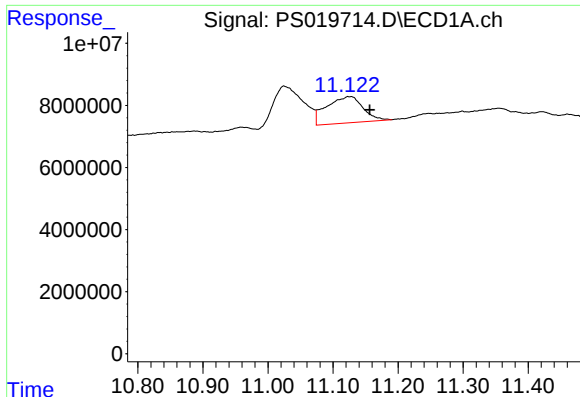

#14 DINOSEB


R.T.: 11.128 min
Delta R.T.: -0.029 min
Response: 32858407
Conc: 2.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

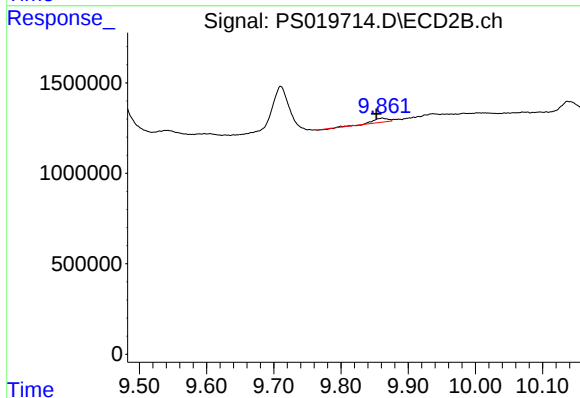


#14 DINOSEB

R.T.: 9.861 min
Delta R.T.: 0.008 min
Response: 345797
Conc: N.D.

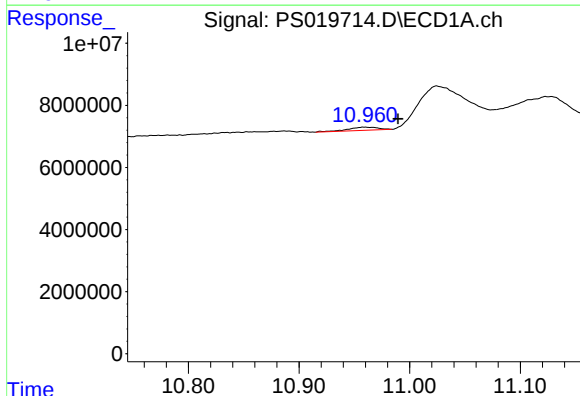

#15 Picloram

R.T.: 10.959 min
Delta R.T.: -0.030 min
Response: 1919783
Conc: N.D.

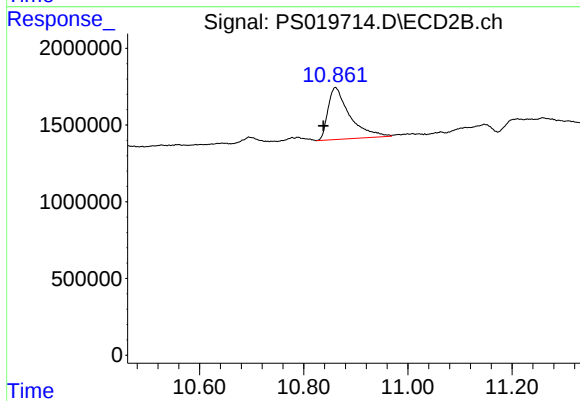

#15 Picloram

R.T.: 10.861 min
Delta R.T.: 0.024 min
Response: 9773469
Conc: 1.52 ng/ml