

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061522\
 Data File : PS019735.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2022 22:57
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 01:09:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.198	6.781	1059.8E6	419.4E6	441.738	541.218
Target Compounds							
1) T	Dalapon	3.024	0.000	1195407	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.356f	0.000	581811	0	<MDL	N.D. #
6) T	MCP	7.511f	0.000	20194	0	<MDL	N.D. #
7) T	MCPA	7.657f	0.000	3021195	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.621f	0	1615871	N.D.	1.829
10) T	Pentachlo...	8.619	8.283	839960	1553791	<MDL	<MDL #
11) T	2,4,5-TP ...	9.181	8.608	1644854	2076392	<MDL	<MDL #
12) T	2,4,5-T	9.429	9.046	12717287	456323	<MDL	<MDL #
13) T	2,4-DB	9.997	9.546	2201386	249278	<MDL	<MDL #
14) T	DINOSEB	11.125	9.857	25200298	681674	1.629	<MDL #
15) T	Picloram	10.972	10.876	3916927	7069195	<MDL	1.099 #
16) T	DCPA	11.427	10.779	703231	1948252	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061522\
Data File : PS019735.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2022 22:57
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 01:09:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

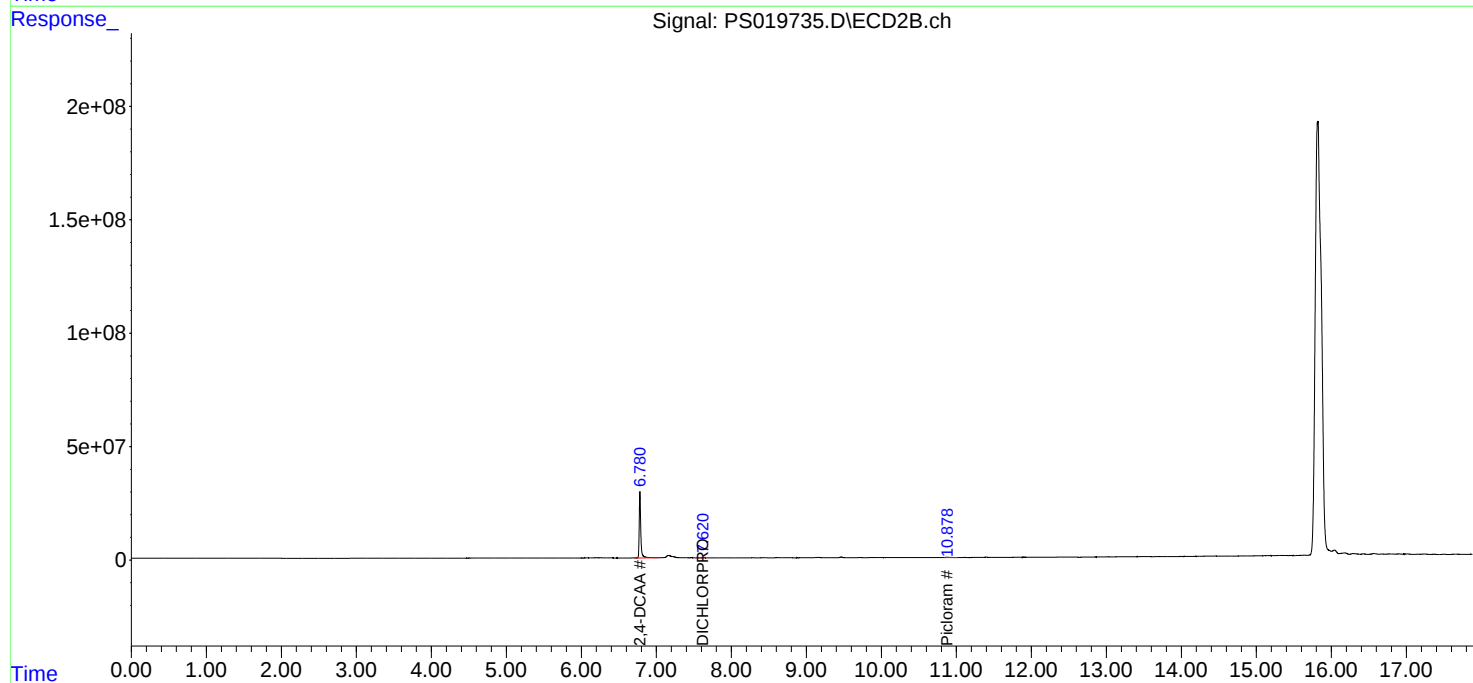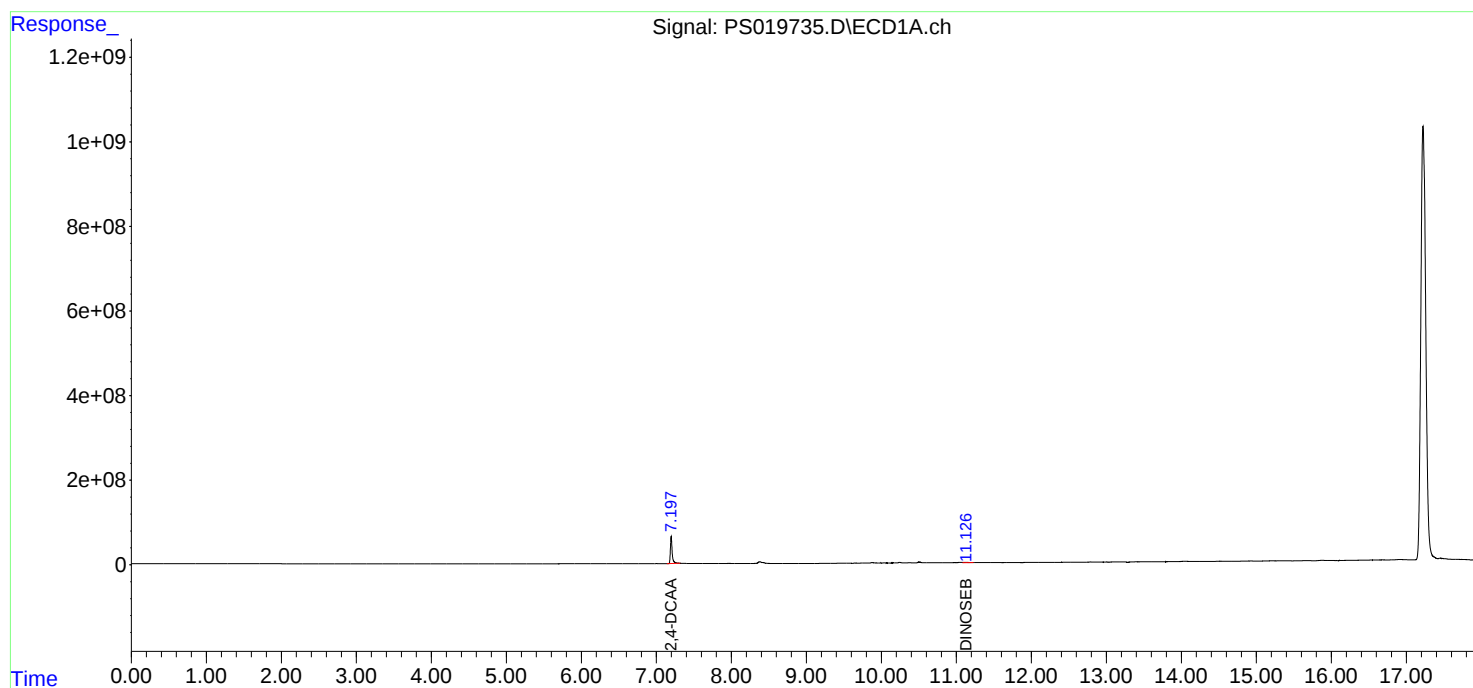


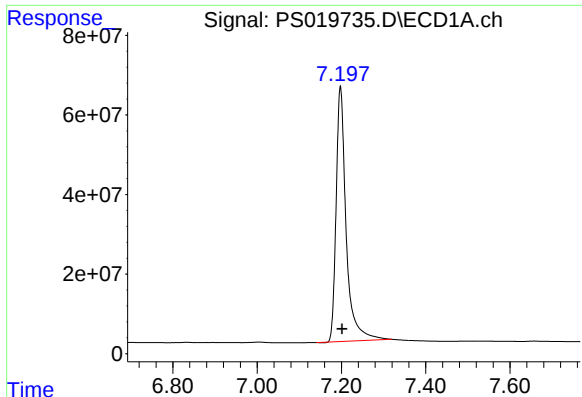

#4 2,4-DCAA


R.T.: 7.198 min
Delta R.T.: -0.004 min
Response: 1059804191
Conc: 441.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

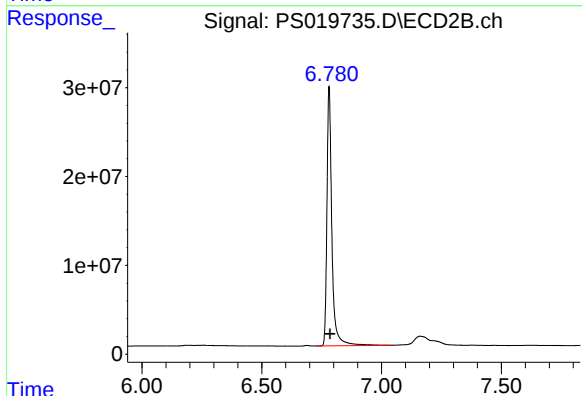


#4 2,4-DCAA

R.T.: 6.781 min
Delta R.T.: -0.004 min
Response: 419373771
Conc: 541.22 ng/ml

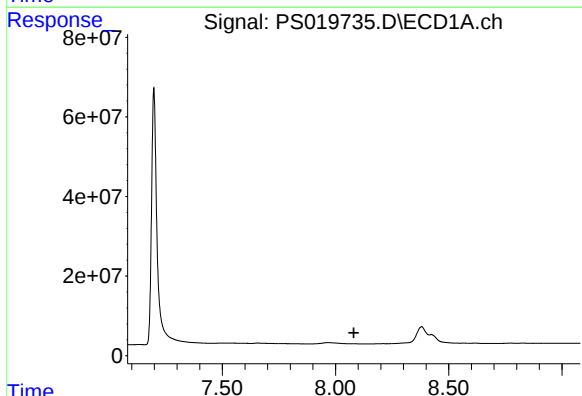


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.081 min
Response: 0
Conc: N.D.

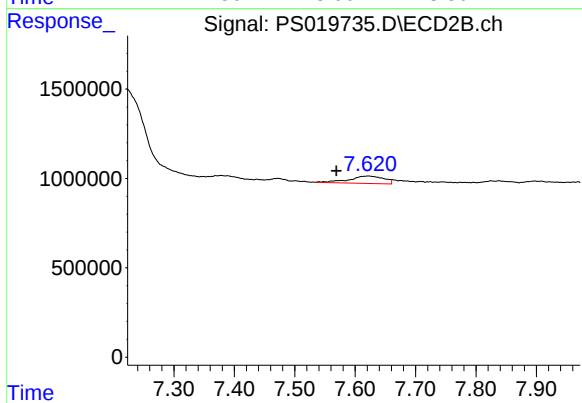

#8 DICHLORPROP


R.T.: 7.621 min
Delta R.T.: 0.052 min
Response: 1615871
Conc: 1.83 ng/ml

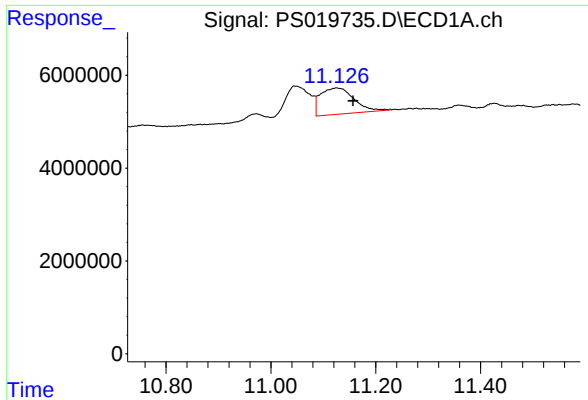

#14 DINOSEB


R.T.: 11.125 min
Delta R.T.: -0.031 min
Response: 25200298
Conc: 1.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

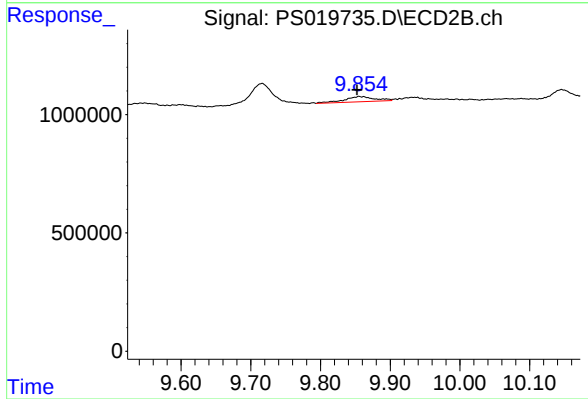


#14 DINOSEB

R.T.: 9.857 min
Delta R.T.: 0.004 min
Response: 681674
Conc: N.D.

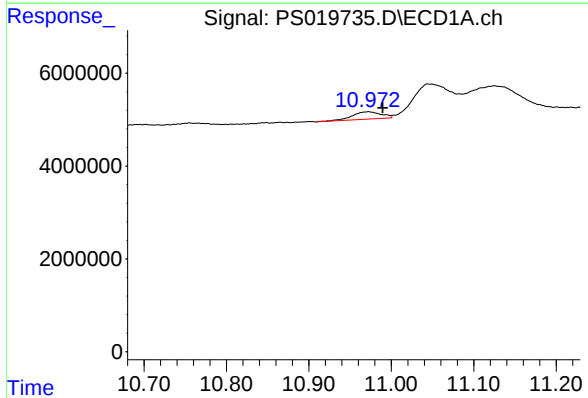

#15 Picloram

R.T.: 10.972 min
Delta R.T.: -0.017 min
Response: 3916927
Conc: N.D.

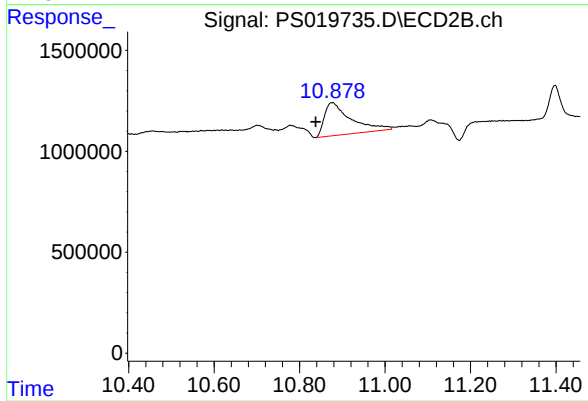

#15 Picloram

R.T.: 10.876 min
Delta R.T.: 0.039 min
Response: 7069195
Conc: 1.10 ng/ml