

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061523\
 Data File : PS023297.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2023 08:42
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 12:22:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.518	0.000	88539	0	<MDL	N.D. #
Target Compounds							
2) T	3,5-DICHL...	5.801	0.000	267595	0	<MDL	N.D. #
3) T	4-Nitroph...	6.313	0.000	4790973	0	3.717	N.D. #
5) T	DICAMBA	6.584f	0.000	175864	0	<MDL	N.D. #
6) T	MCP	6.753	0.000	605771	0	<MDL	N.D. #
7) T	MCPA	0.000	7.302	0	14098913	N.D.	5.246
8) T	DICHLORPROP	7.259	7.659	738759	771599	<MDL	1.247 #
9) T	2,4-D	7.408	0.000	2346955	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.210	0.000	1522916	0	<MDL	N.D. #
12) T	2,4,5-T	8.486	9.140f	1246826	1366818	<MDL	<MDL #
13) T	2,4-DB	8.984	0.000	4295875	0	1.825	N.D. #
15) T	Picloram	9.898	10.894	29070114	5572842	1.675	1.221 #
16) T	DCPA	10.331	10.894	516756	5572842	<MDL	1.389 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061523\
Data File : PS023297.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2023 08:42
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 12:22:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

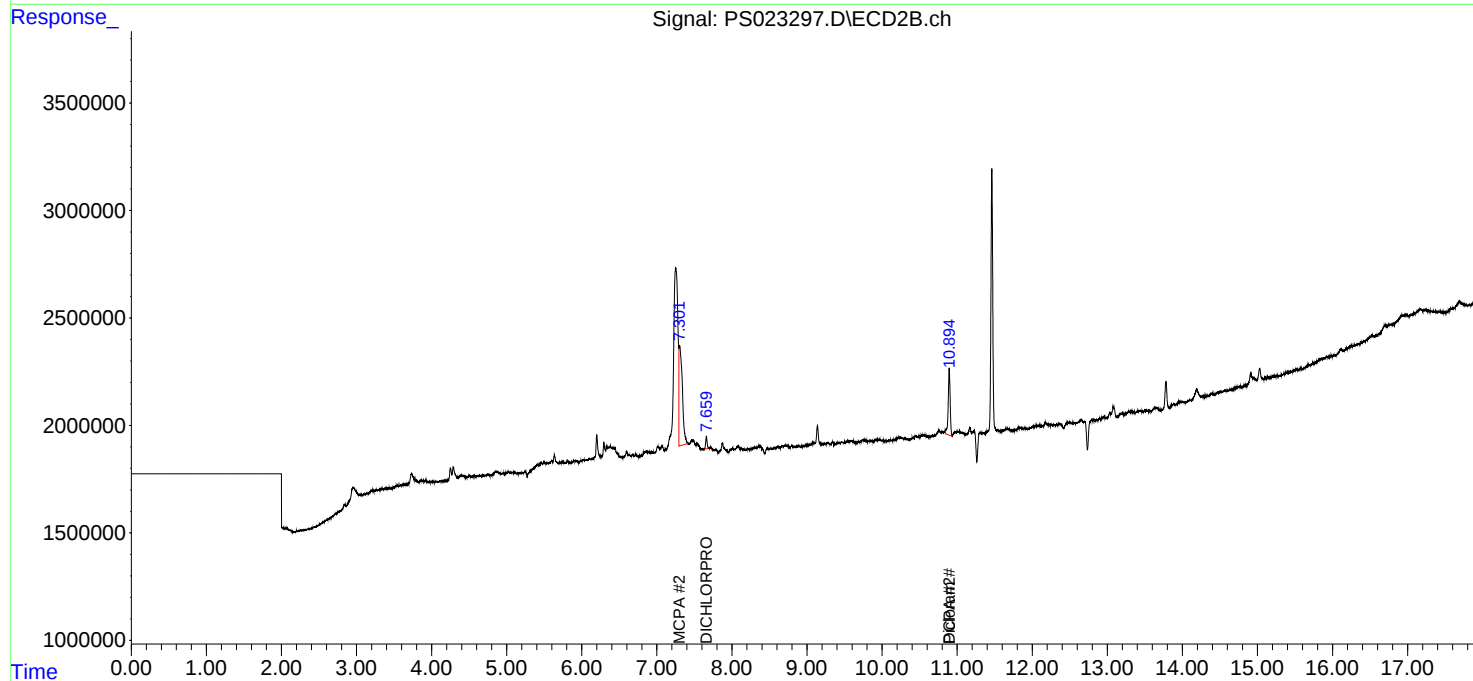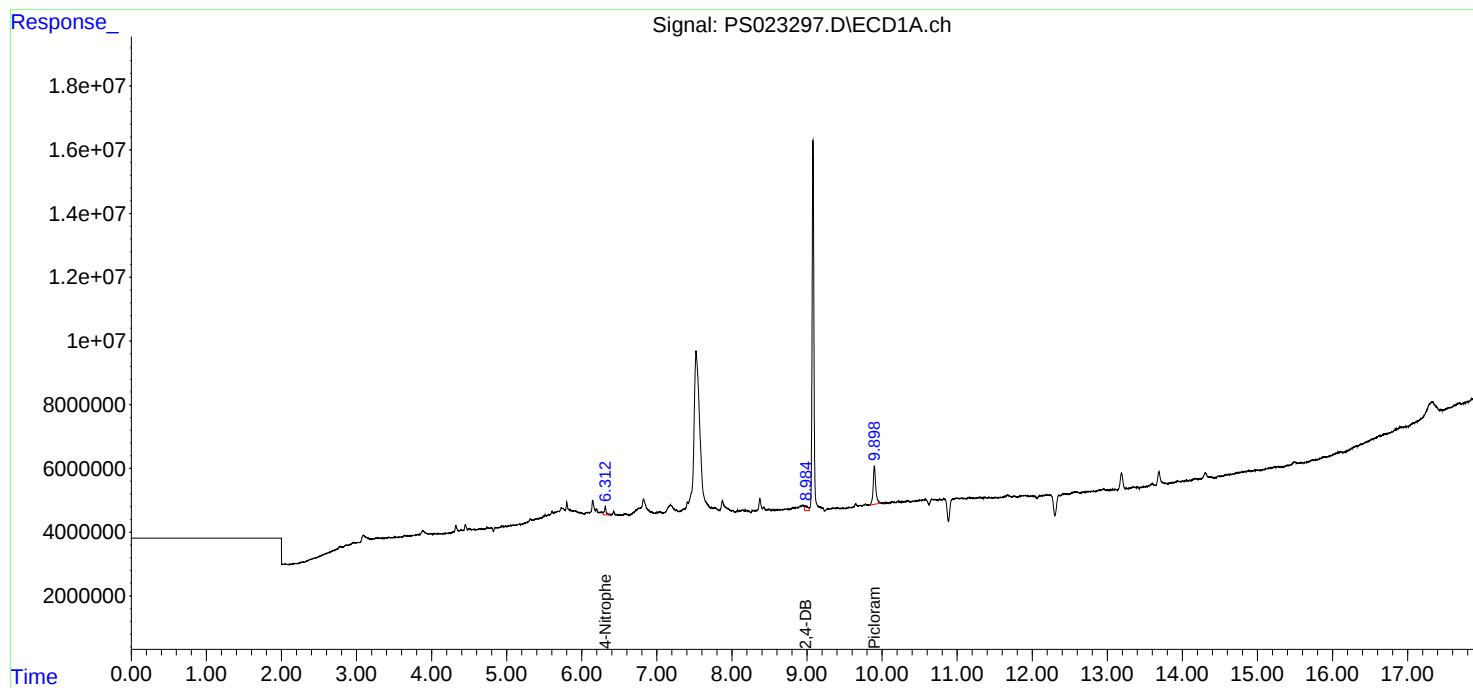


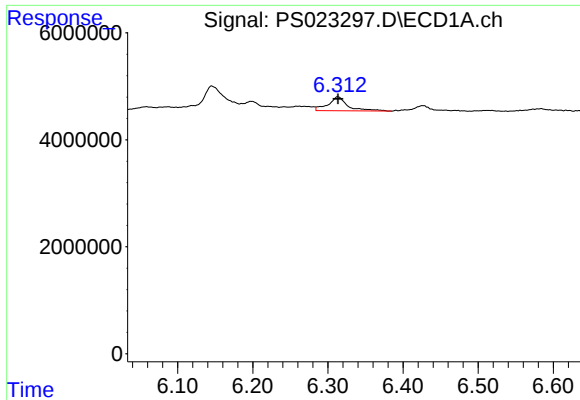

#3 4-Nitrophenol


R.T.: 6.313 min
Delta R.T.: 0.000 min
Response: 4790973
Conc: 3.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

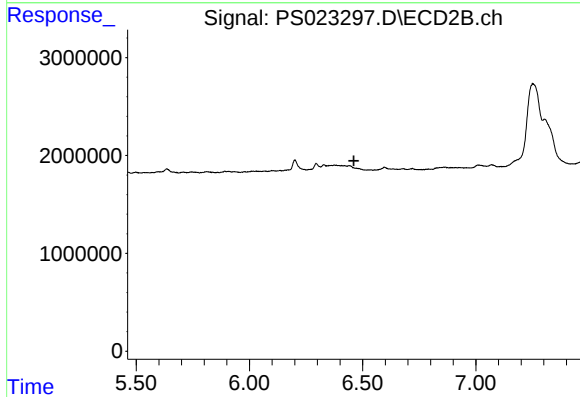


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

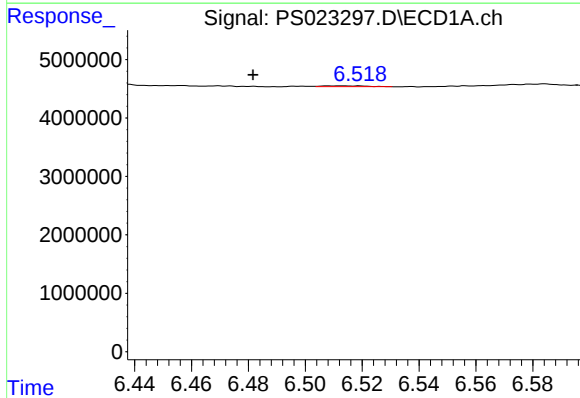


#4 2,4-DCAA

R.T.: 6.518 min
Delta R.T.: 0.037 min
Response: 88539
Conc: N.D.

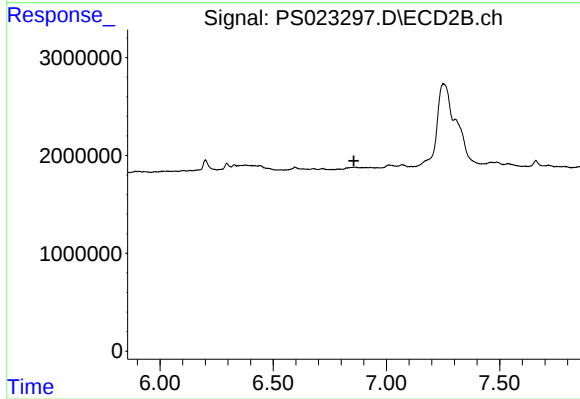

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.856 min
Response: 0
Conc: N.D.

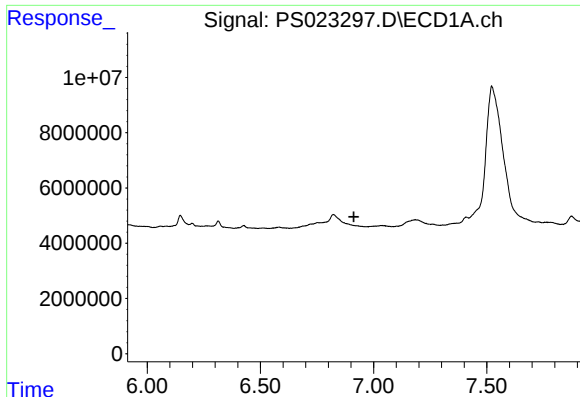

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.913 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

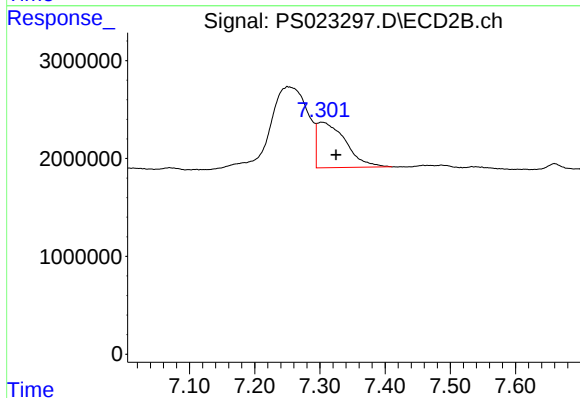


#7 MCPA

R.T.: 7.302 min
Delta R.T.: -0.023 min
Response: 14098913
Conc: 5.25 ug/ml

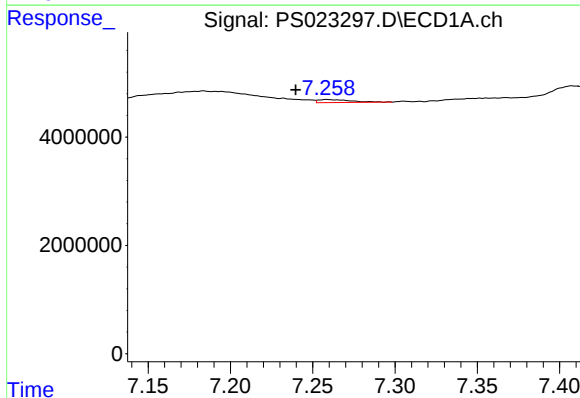


#8 DICHLORPROP

R.T.: 7.259 min
Delta R.T.: 0.019 min
Response: 738759
Conc: N.D.

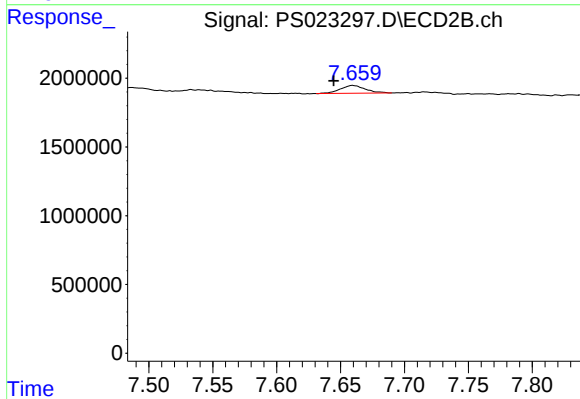

#8 DICHLORPROP


R.T.: 7.659 min
Delta R.T.: 0.015 min
Response: 771599
Conc: 1.25 ng/ml

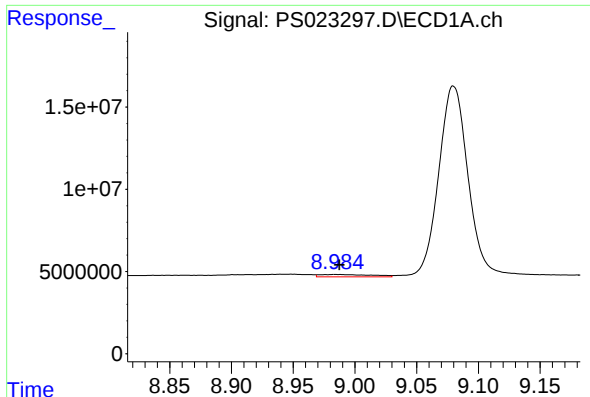

#13 2,4-DB


R.T.: 8.984 min
Delta R.T.: -0.003 min
Response: 4295875
Conc: 1.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

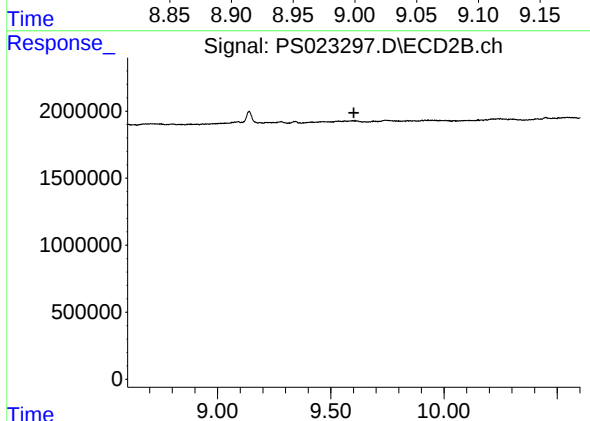


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.602 min
Response: 0
Conc: N.D.

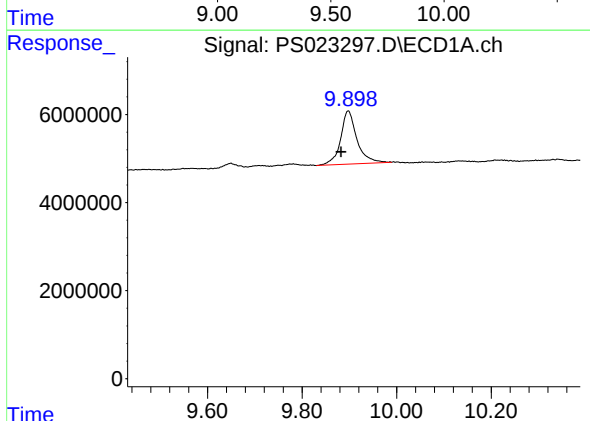


#15 Picloram

R.T.: 9.898 min
Delta R.T.: 0.015 min
Response: 29070114
Conc: 1.68 ng/ml

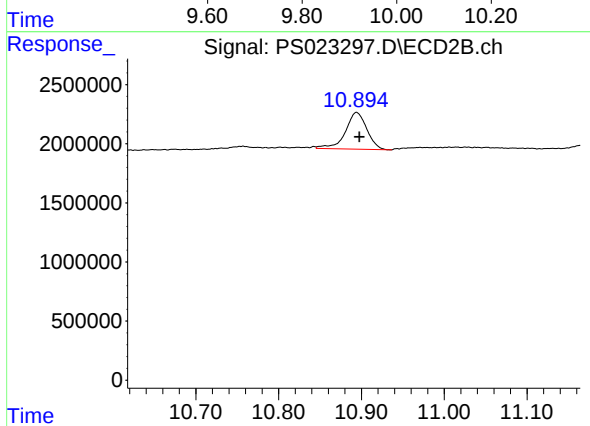

#15 Picloram


R.T.: 10.894 min
Delta R.T.: -0.003 min
Response: 5572842
Conc: 1.22 ng/ml

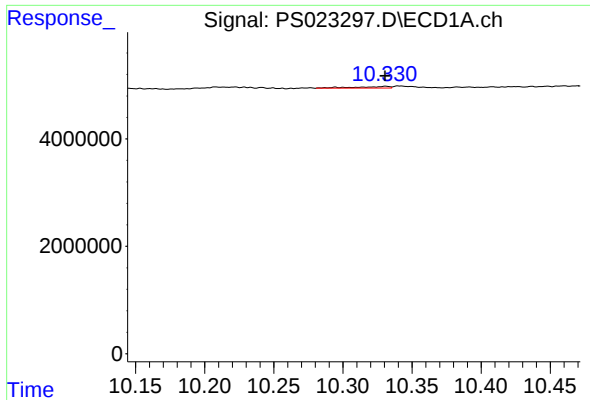

#16 DCPA

R.T.: 10.331 min
Delta R.T.: 0.000 min
Response: 516756
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

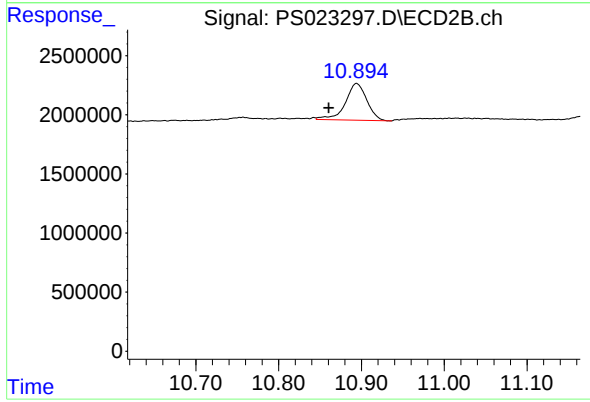

#16 DCPA

R.T.: 10.894 min
Delta R.T.: 0.034 min
Response: 5572842
Conc: 1.39 ng/ml