

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061523\
 Data File : PS023298.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2023 09:06
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 12:23:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.481	6.854	963.3E6	302.6E6	544.451	533.067
Target Compounds							
1) T	Dalapon	2.588f	0.000	1821781	0	<MDL	N.D. #
3) T	4-Nitroph...	6.317	0.000	6392506	0	4.960	N.D. #
5) T	DICAMBA	6.628	7.013	-33729	758862	N.D.	<MDL
6) T	MCP	6.818	0.000	654542	0	<MDL	N.D. #
7) T	MCPA	6.856f	7.303	-1340064	13866343	N.D.	5.159
8) T	DICHLORPROP	7.290f	0.000	463223	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.211	0.000	8348775	0	<MDL	N.D. #
12) T	2,4,5-T	8.479	9.140f	2526364	1048998	<MDL	<MDL #
13) T	2,4-DB	8.935f	0.000	14579294	0	6.193	N.D. #
14) T	DINOSEB	10.056	0.000	803021	0	<MDL	N.D. #
15) T	Picloram	9.892	10.895	32502327	3801863	1.873	<MDL #
16) T	DCPA	10.331	10.895	2244054	3801863	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061523\
Data File : PS023298.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2023 09:06
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 12:23:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

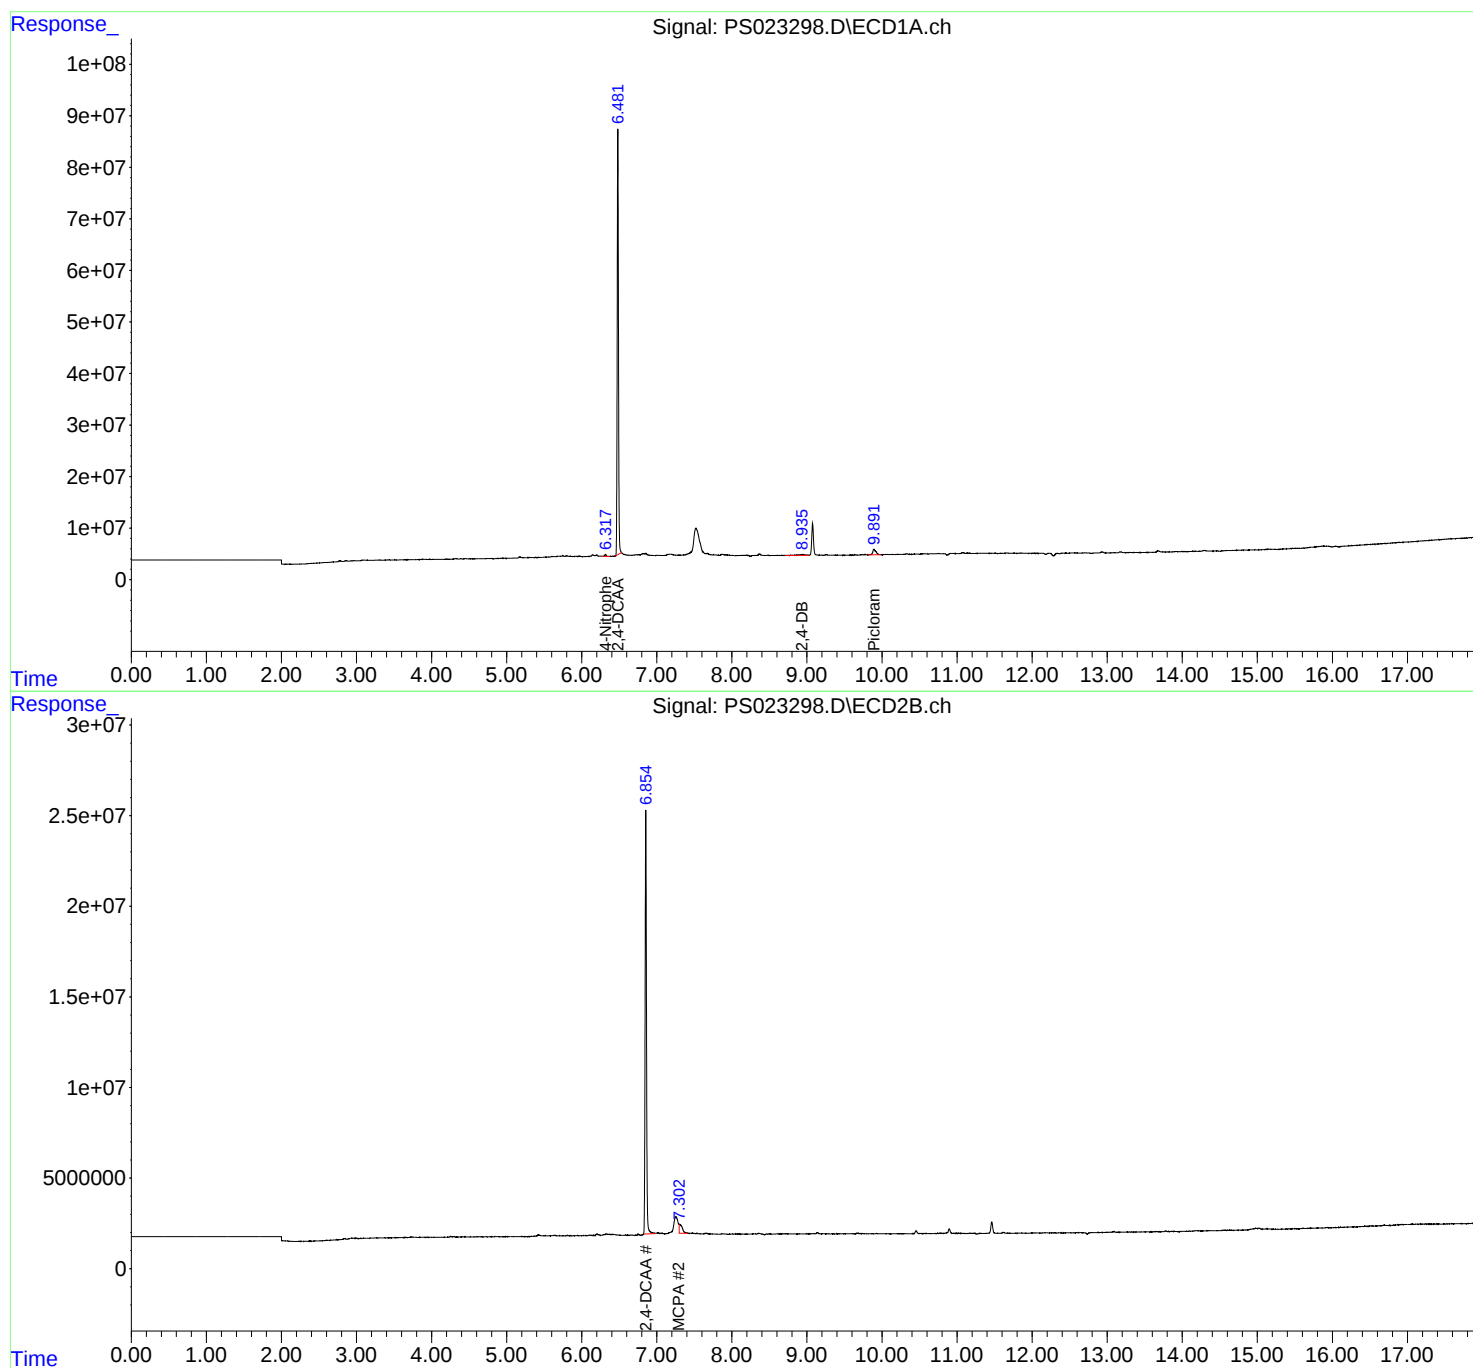


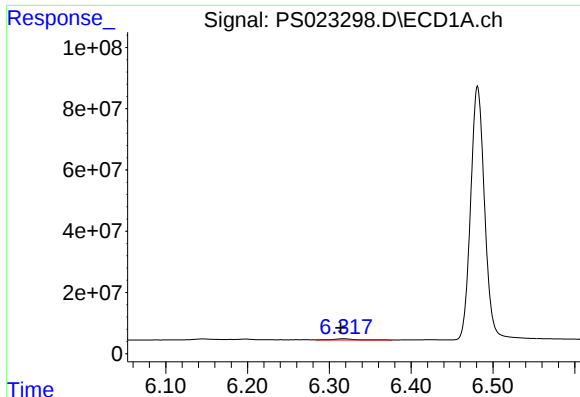

#3 4-Nitrophenol


R.T.: 6.317 min
Delta R.T.: 0.004 min
Response: 6392506
Conc: 4.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

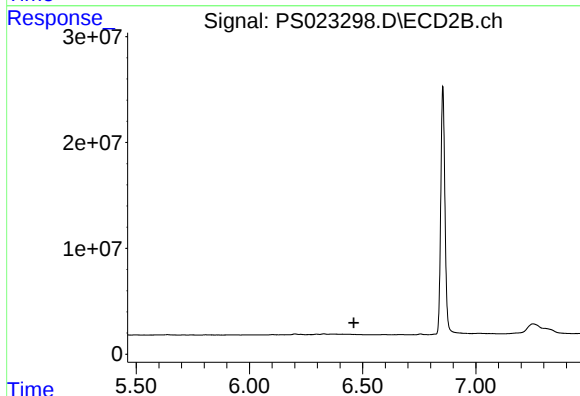


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

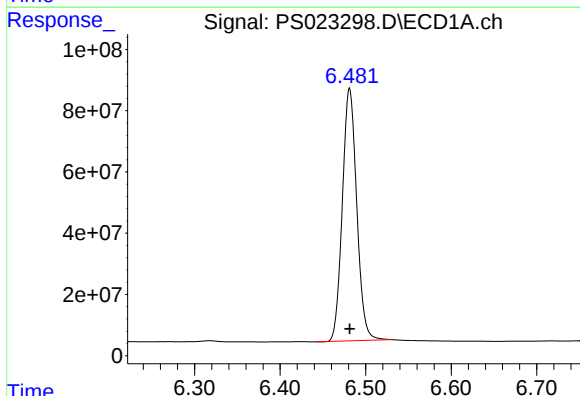


#4 2,4-DCAA

R.T.: 6.481 min
Delta R.T.: 0.000 min
Response: 963272439
Conc: 544.45 ng/ml

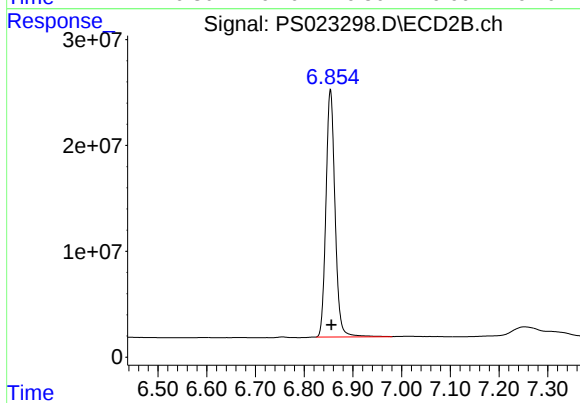

#4 2,4-DCAA


R.T.: 6.854 min
Delta R.T.: -0.002 min
Response: 302619550
Conc: 533.07 ng/ml

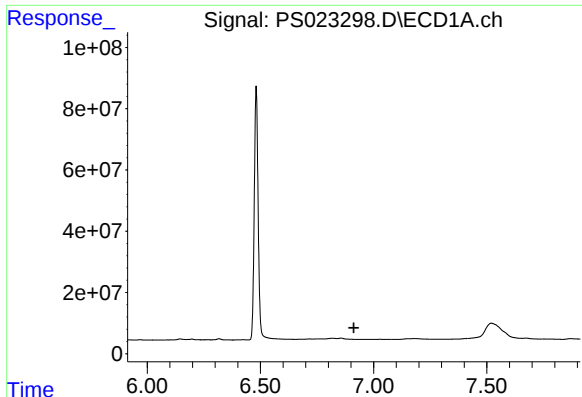

#7 MCPA


R.T.: 6.856 min
Delta R.T.: -0.057 min
Response: -1340064
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

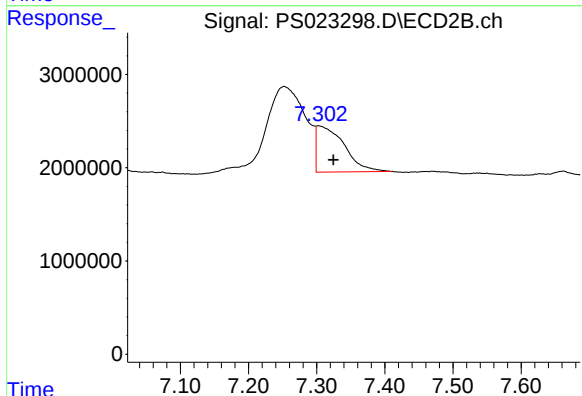


#7 MCPA

R.T.: 7.303 min
Delta R.T.: -0.022 min
Response: 13866343
Conc: 5.16 ug/ml

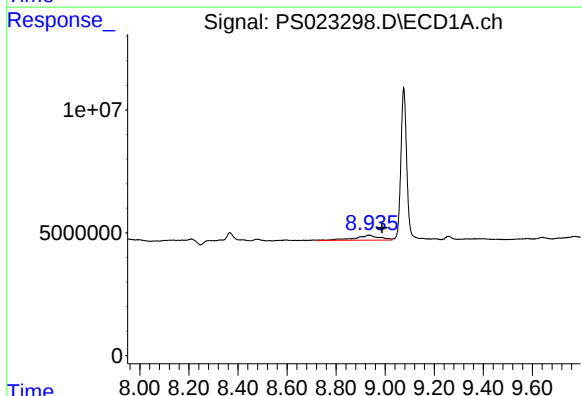


#13 2,4-DB

R.T.: 8.935 min
Delta R.T.: -0.052 min
Response: 14579294
Conc: 6.19 ng/ml

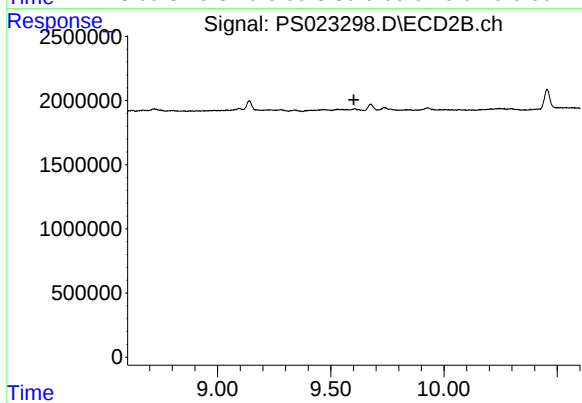

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.602 min
Response: 0
Conc: N.D.

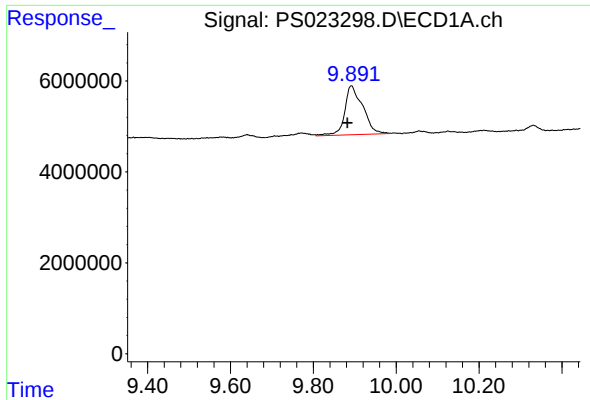

#15 Picloram

R.T.: 9.892 min
Delta R.T.: 0.009 min
Response: 32502327
Conc: 1.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

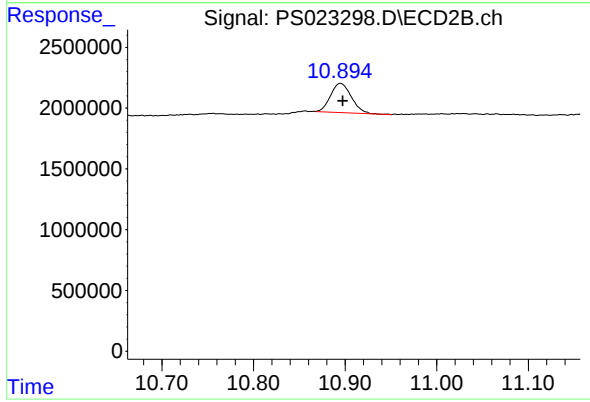

#15 Picloram

R.T.: 10.895 min
Delta R.T.: -0.003 min
Response: 3801863
Conc: N.D.