

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061625\
 Data File : PS030680.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jun 2025 09:32
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 11:54:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061625.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 16 11:52:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.352	7.768	1489.3E6	510.0E6	395.991	472.390
Target Compounds							
1) T	Dalapon	0.000	2.672f	0	29889310	N.D.	10.621
2) T	3,5-DICHL...	6.509	0.000	214278	0	<MDL	N.D. #
3) T	4-Nitroph...	7.148	0.000	5684034	0	3.487	N.D. #
5) T	DICAMBA	7.542	0.000	1097558	0	<MDL	N.D. #
7) T	MCPA	7.863	8.278f	142583	22141176	<MDL	6.906 #
8) T	DICHLORPROP	8.254	0.000	1743075	0	<MDL	N.D. #
10) T	Pentachlo...	8.798	9.549	6269861	3726641	<MDL	<MDL #
11) T	2,4,5-TP ...	9.381	9.931	3746900	5071993	<MDL	<MDL #
12) T	2,4,5-T	9.678	10.362	2570760	1390310	<MDL	<MDL #
13) T	2,4-DB	10.244	10.963f	1404648	4185879	<MDL	3.528 #
14) T	DINOSEB	11.472	0.000	1463156	0	<MDL	N.D. #
15) T	Picloram	11.286	12.422	32679620	55769407	1.957	2.326
16) T	DCPA	11.767	0.000	3432380	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061625\
Data File : PS030680.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jun 2025 09:32
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 11:54:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061625.M
Quant Title : 8080.M
QLast Update : Mon Jun 16 11:52:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

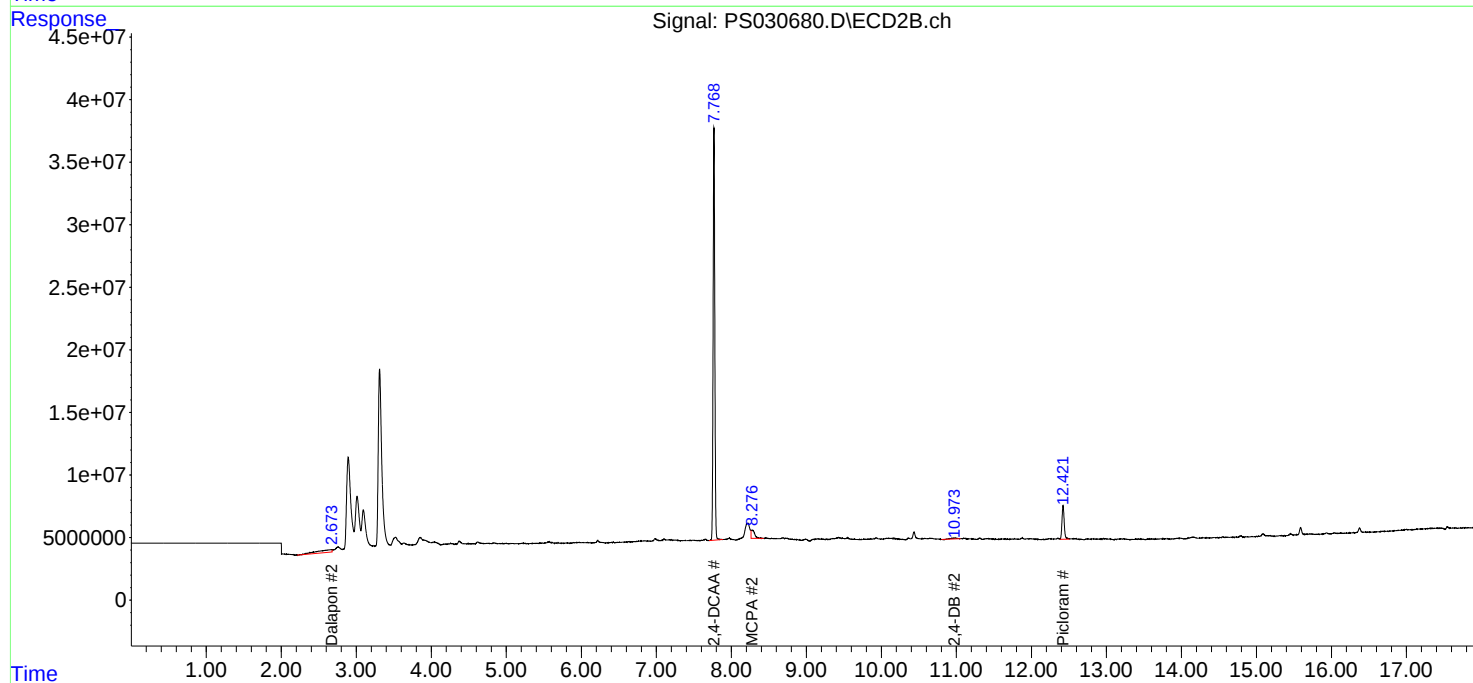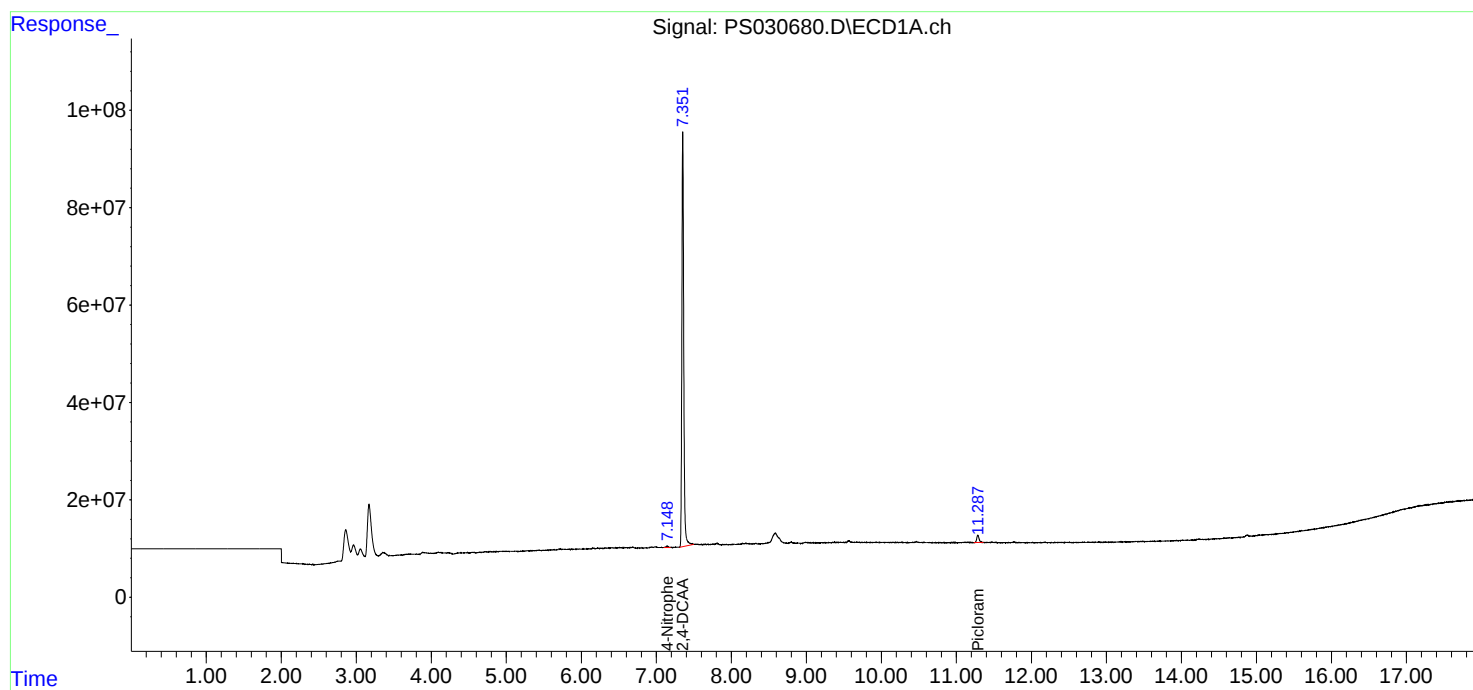


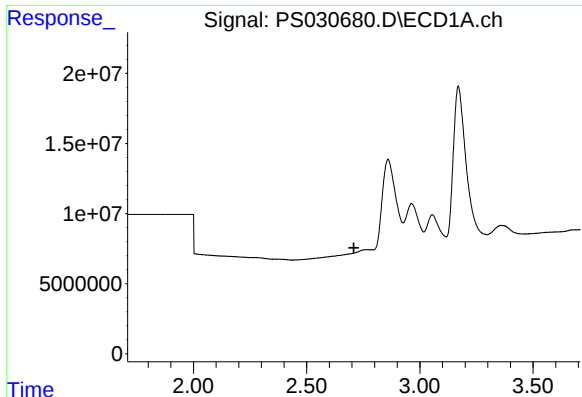

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.709 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

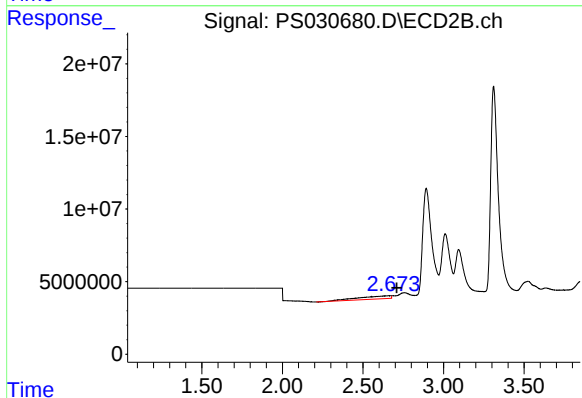


#1 Dalapon

R.T.: 2.672 min
Delta R.T.: -0.038 min
Response: 29889310
Conc: 10.62 ng/ml

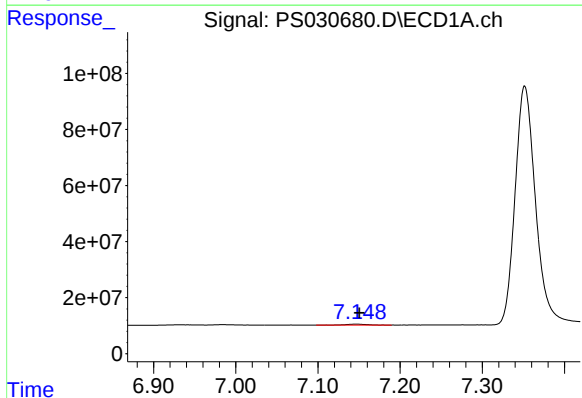


#3 4-Nitrophenol

R.T.: 7.148 min
Delta R.T.: -0.002 min
Response: 5684034
Conc: 3.49 ng/ml

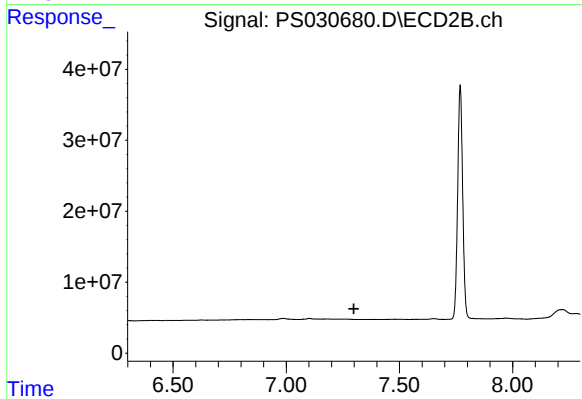

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.299 min
Response: 0
Conc: N.D.

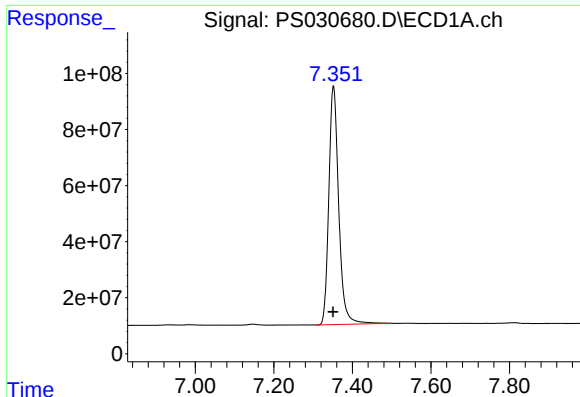

#4 2,4-DCAA


R.T.: 7.352 min
Delta R.T.: 0.001 min
Response: 1489250686
Conc: 395.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

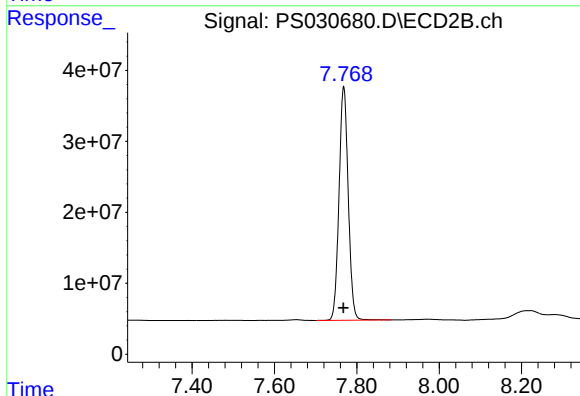


#4 2,4-DCAA

R.T.: 7.768 min
Delta R.T.: 0.000 min
Response: 510035415
Conc: 472.39 ng/ml

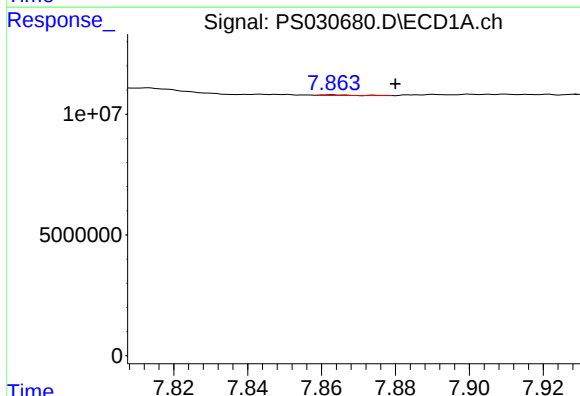


#7 MCPA

R.T.: 7.863 min
Delta R.T.: -0.017 min
Response: 142583
Conc: N.D.

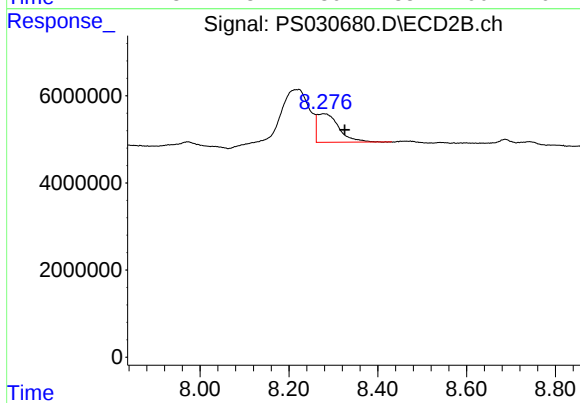

#7 MCPA


R.T.: 8.278 min
Delta R.T.: -0.047 min
Response: 22141176
Conc: 6.91 ug/ml

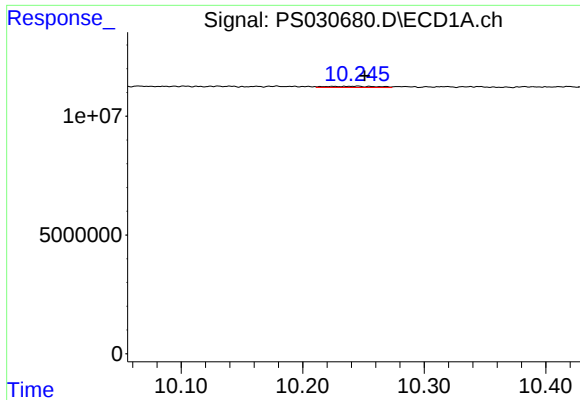

#13 2,4-DB


R.T.: 10.244 min
Delta R.T.: -0.006 min
Response: 1404648
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

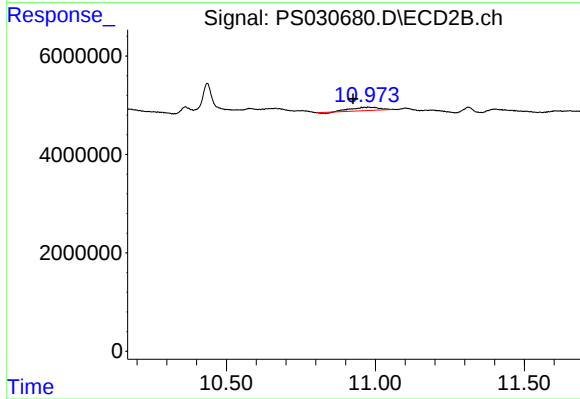


#13 2,4-DB

R.T.: 10.963 min
Delta R.T.: 0.039 min
Response: 4185879
Conc: 3.53 ng/ml

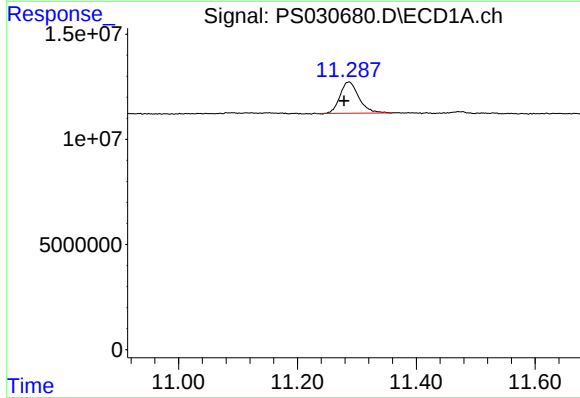

#15 Picloram

R.T.: 11.286 min
Delta R.T.: 0.008 min
Response: 32679620
Conc: 1.96 ng/ml

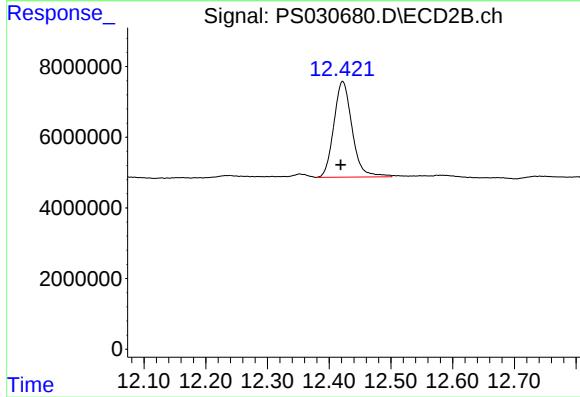

#15 Picloram

R.T.: 12.422 min
Delta R.T.: 0.003 min
Response: 55769407
Conc: 2.33 ng/ml