

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061718\
 Data File : PS000419.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2018 20:36
 Operator : UA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 12:02:55 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.850	11.225	179.8E6	151.5E6	477.253	445.115
Target Compounds							
3) T	4-Nitroph...	11.474	0.000	527001	0	2.242	N.D. #
6) T	MCP	12.530	0.000	535036	0	0.472	N.D. #
8) T	DICHLORPROP	0.000	12.548	0	2138423	N.D.	6.642 #
10) T	Pentachlo...	14.117	13.673	614780	521801	0.117	0.110
11) T	2,4,5-TP ...	14.983	14.284	476203	224375	0.219	0.115 #
12) T	2,4,5-T	15.381	14.856	390849	401275	0.182	0.237 #
14) T	DINOSEB	17.648	15.932	417789	216107	0.281	0.166 #
15) T	Picloram	17.367	17.178	596141	494062	0.204	0.198
16) T	DCPA	17.984	17.120	368187	357404	0.144	0.155



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061718\
Data File : PS000419.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2018 20:36
Operator : UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 12:02:55 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

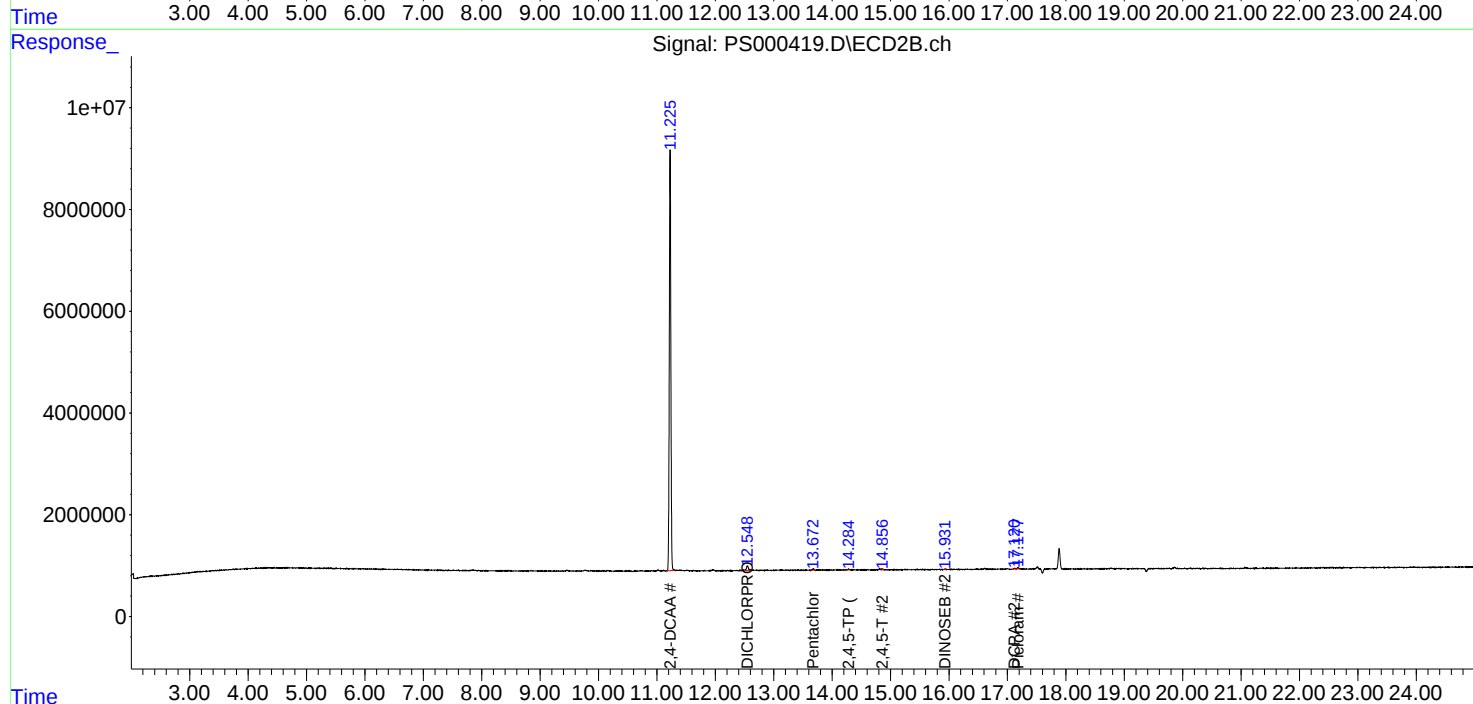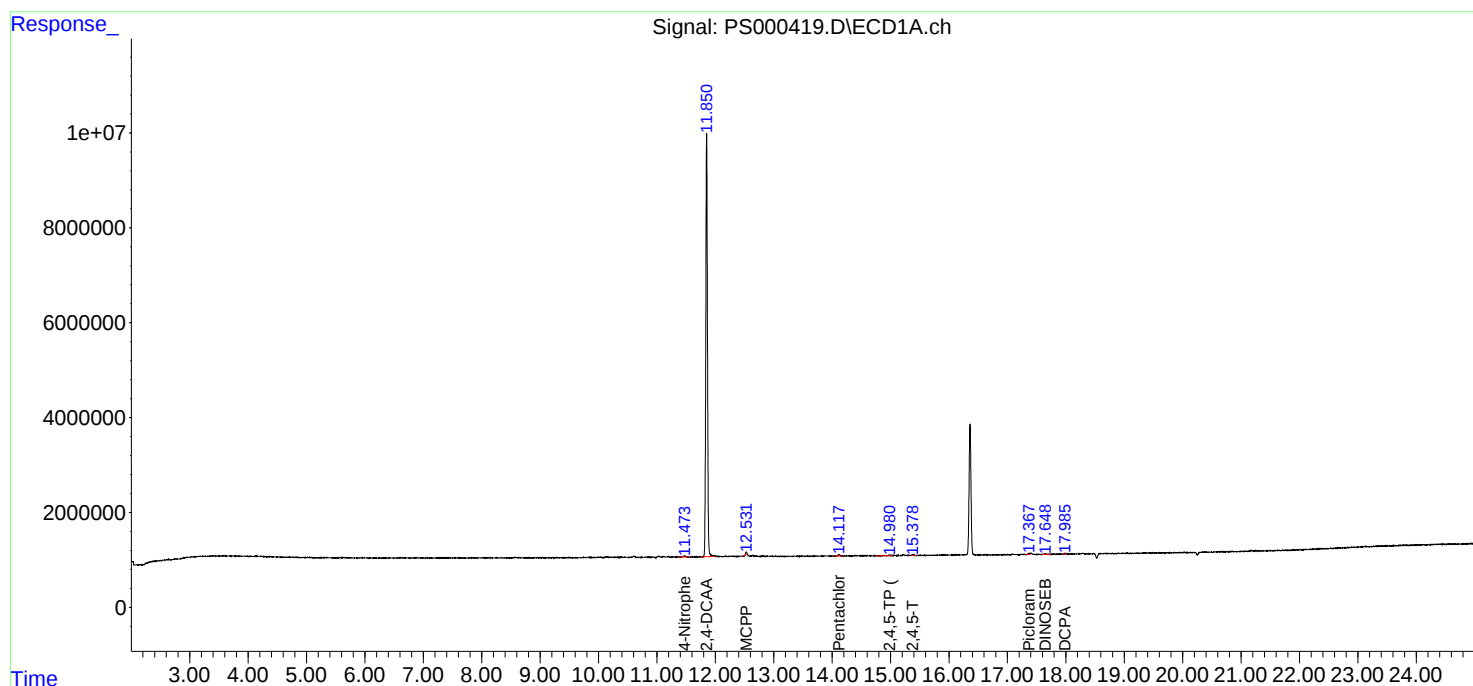


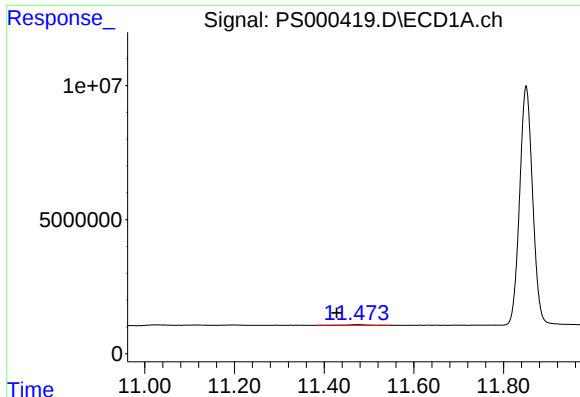

#3 4-Nitrophenol


R.T.: 11.474 min
Delta R.T.: 0.047 min
Response: 527001
Conc: 2.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

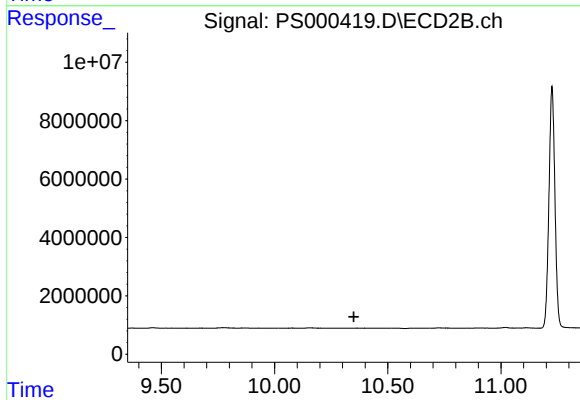


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 10.350 min
Response: 0
Conc: N.D.

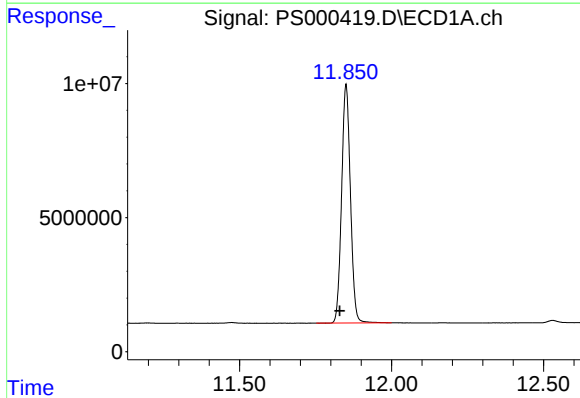


#4 2,4-DCAA

R.T.: 11.850 min
Delta R.T.: 0.021 min
Response: 179759710
Conc: 477.25 ng/ml

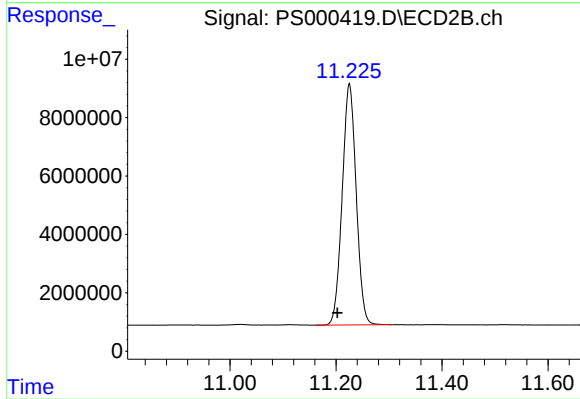

#4 2,4-DCAA


R.T.: 11.225 min
Delta R.T.: 0.022 min
Response: 151476617
Conc: 445.12 ng/ml

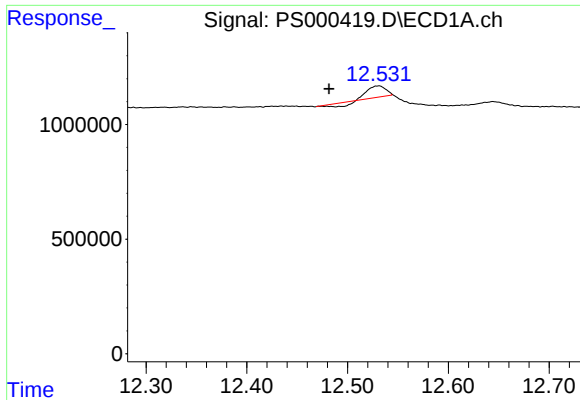

#6 MCP


R.T.: 12.530 min
Delta R.T.: 0.049 min
Response: 535036
Conc: 0.47 ug/ml

Instrument :
ECD_S
ClientSampleId :

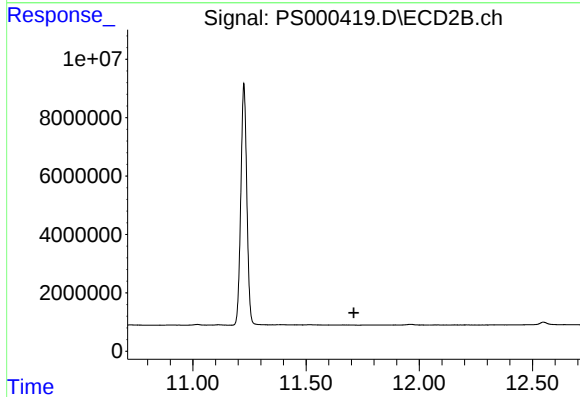


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.711 min
Response: 0
Conc: N.D.

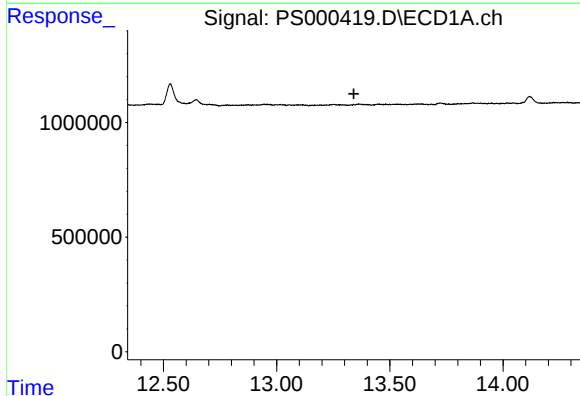


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.341 min
Response: 0
Conc: N.D.

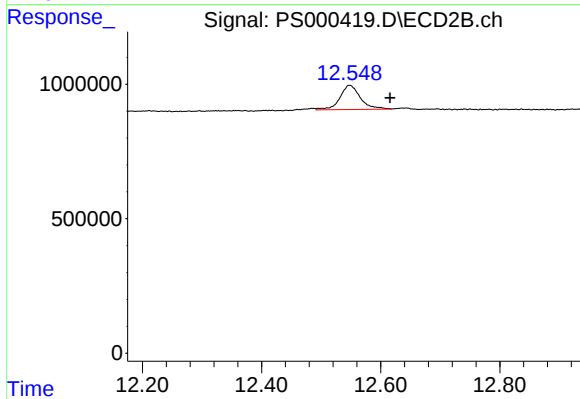

#8 DICHLORPROP


R.T.: 12.548 min
Delta R.T.: -0.068 min
Response: 2138423
Conc: 6.64 ng/ml

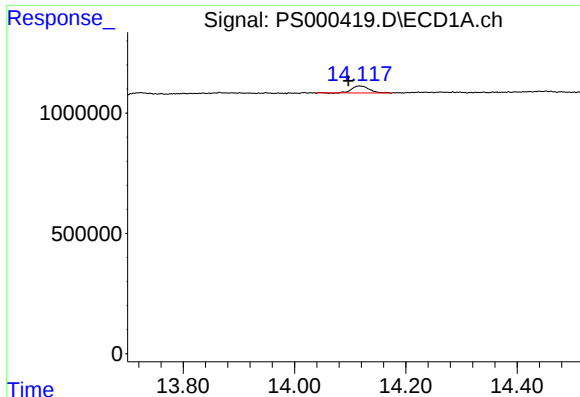

#10 Pentachlorophenol


R.T.: 14.117 min
Delta R.T.: 0.020 min
Response: 614780
Conc: 0.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

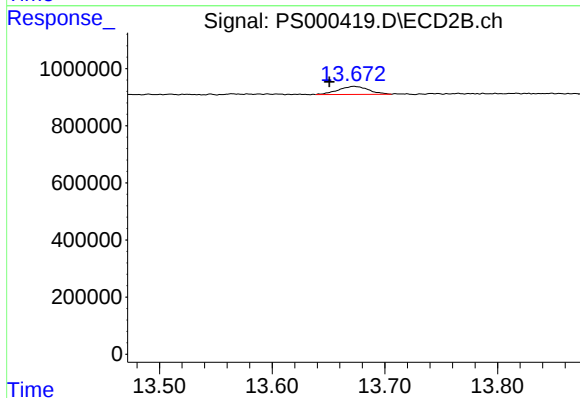


#10 Pentachlorophenol

R.T.: 13.673 min
Delta R.T.: 0.022 min
Response: 521801
Conc: 0.11 ng/ml

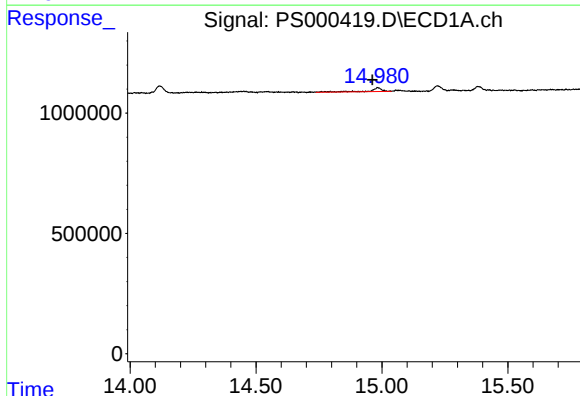


#11 2,4,5-TP (SILVEX)

R.T.: 14.983 min
Delta R.T.: 0.021 min
Response: 476203
Conc: 0.22 ng/ml

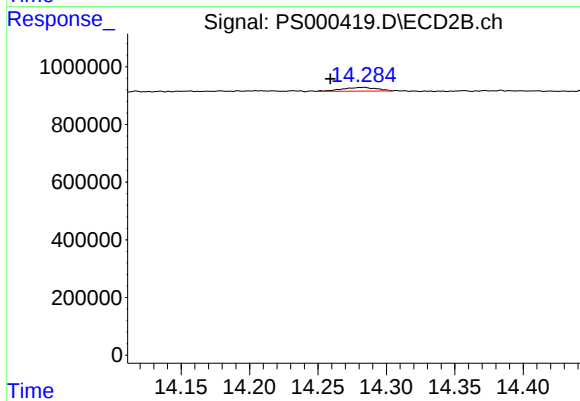

#11 2,4,5-TP (SILVEX)


R.T.: 14.284 min
Delta R.T.: 0.025 min
Response: 224375
Conc: 0.12 ng/ml

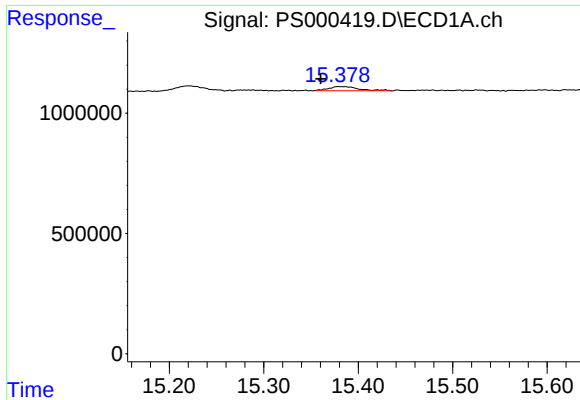

#12 2,4,5-T


R.T.: 15.381 min
Delta R.T.: 0.021 min
Response: 390849
Conc: 0.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

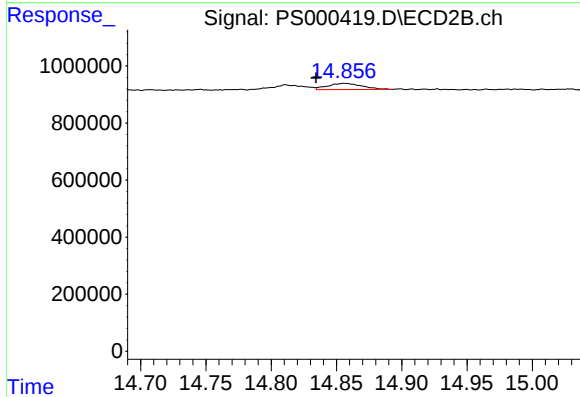


#12 2,4,5-T

R.T.: 14.856 min
Delta R.T.: 0.022 min
Response: 401275
Conc: 0.24 ng/ml

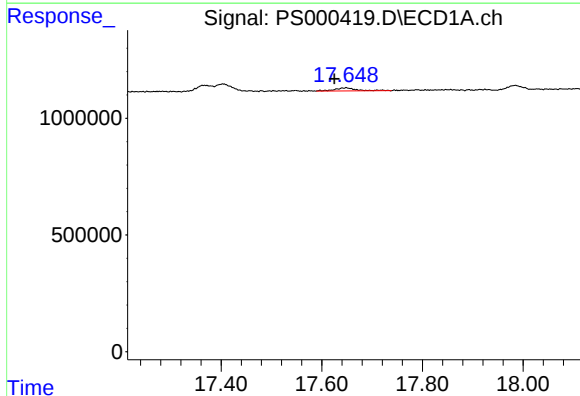


#14 DINOSEB

R.T.: 17.648 min
Delta R.T.: 0.023 min
Response: 417789
Conc: 0.28 ng/ml

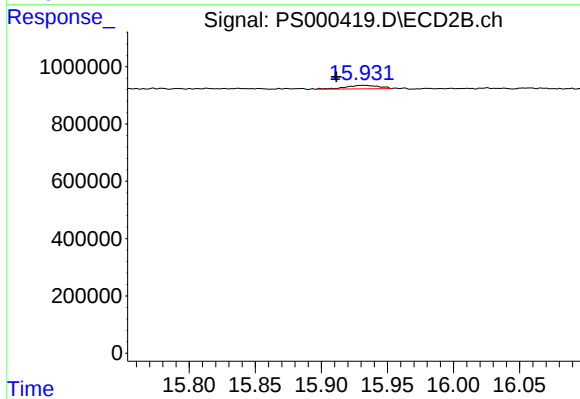

#14 DINOSEB


R.T.: 15.932 min
Delta R.T.: 0.020 min
Response: 216107
Conc: 0.17 ng/ml

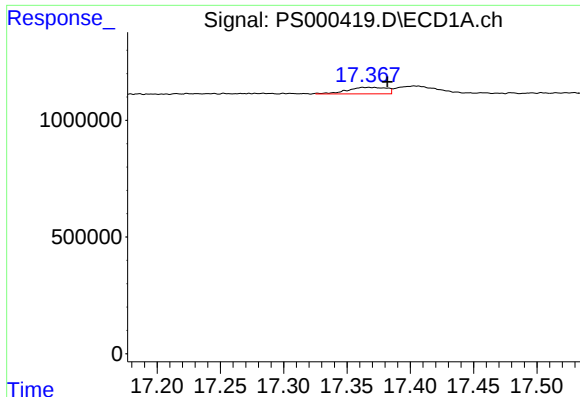

#15 Picloram


R.T.: 17.367 min
Delta R.T.: -0.015 min
Response: 596141
Conc: 0.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

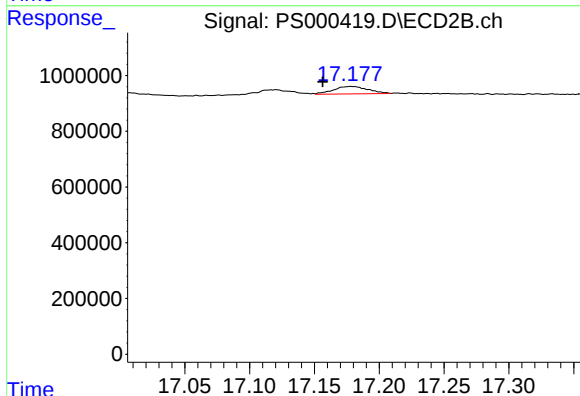


#15 Picloram

R.T.: 17.178 min
Delta R.T.: 0.022 min
Response: 494062
Conc: 0.20 ng/ml

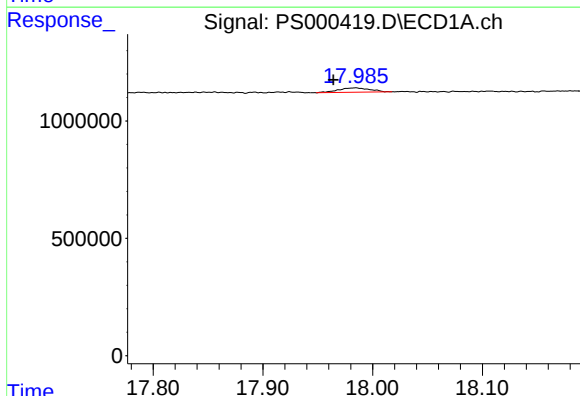

#16 DCPA

R.T.: 17.984 min
Delta R.T.: 0.020 min
Response: 368187
Conc: 0.14 ng/ml

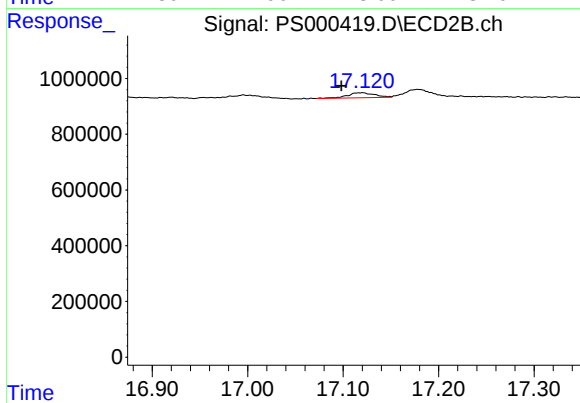

#16 DCPA

R.T.: 17.120 min
Delta R.T.: 0.022 min
Response: 357404
Conc: 0.15 ng/ml